

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021249.D
 Acq On : 29 Jun 2019 01:57
 Operator : HP/JU
 Sample : K3381-06DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCM4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	19	rVB	489116	578309	19.13%	2.577%
2	3.240	41	43	48	rVB	58437	69559	2.30%	0.310%
3	3.310	52	55	61	rVB	68316	90124	2.98%	0.402%
4	4.404	238	241	248	rVB	55196	73051	2.42%	0.325%
5	6.863	655	659	665	rVB2	29877	43322	1.43%	0.193%
6	6.928	666	670	683	rVB	39242	73719	2.44%	0.328%
7	7.098	695	699	707	rBV	117771	192769	6.38%	0.859%
8	7.293	726	732	745	rVB	143816	244371	8.08%	1.089%
9	7.757	805	811	821	rVB	682504	1099900	36.38%	4.901%
10	8.463	925	931	944	rVB	109420	188778	6.24%	0.841%
11	8.922	1003	1009	1017	rBV	165554	290429	9.61%	1.294%
12	9.292	1067	1072	1076	rVB2	16152	25054	0.83%	0.112%
13	9.639	1124	1131	1138	rBV	130165	216325	7.16%	0.964%
14	10.175	1216	1222	1234	rBV	169348	350786	11.60%	1.563%
15	10.545	1278	1285	1298	rVB	1005141	1684793	55.73%	7.507%
16	11.775	1490	1494	1499	rVB2	12812	18340	0.61%	0.082%
17	12.151	1554	1558	1565	rVB6	3974	6523	0.22%	0.029%
18	13.816	1831	1841	1854	rBV	484855	721080	23.85%	3.213%
19	14.092	1882	1888	1897	rBV	561781	806674	26.68%	3.594%
20	14.398	1934	1940	1952	rBV2	1672110	2616295	86.54%	11.658%
21	14.651	1979	1983	1987	rBV3	5699	8973	0.30%	0.040%
22	15.351	2097	2102	2104	rBV2	7572	8741	0.29%	0.039%
23	15.398	2104	2110	2120	rVV	741877	1096964	36.28%	4.888%
24	15.527	2128	2132	2143	rBV2	49224	78770	2.61%	0.351%
25	15.639	2148	2151	2154	rVB4	7269	8334	0.28%	0.037%
26	16.351	2268	2272	2275	rBV3	4247	5214	0.17%	0.023%
27	16.592	2310	2313	2317	rVB3	5406	6496	0.21%	0.029%
28	16.933	2366	2371	2376	rBV3	6305	9992	0.33%	0.045%
29	17.151	2401	2408	2417	rVV	2173274	3023212	100.00%	13.471%
30	17.245	2418	2424	2438	rVB	738691	1074104	35.53%	4.786%
31	17.668	2493	2496	2499	rVB4	3498	4217	0.14%	0.019%
32	17.727	2503	2506	2508	rBV3	2808	3910	0.13%	0.017%
33	18.045	2557	2560	2561	rBV3	4000	3757	0.12%	0.017%
34	18.609	2653	2656	2659	rBV4	6901	8221	0.27%	0.037%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021249.D
Acq On : 29 Jun 2019 01:57
Operator : HP/JU
Sample : K3381-06DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM4DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION

35	19.180	2750	2753	2758	rBV5	7373	9639	0.32%	0.043%
36	19.545	2809	2815	2825	rBV	808742	1127626	37.30%	5.024%
37	21.333	3114	3119	3126	rBV	2055286	2691520	89.03%	11.993%
38	23.456	3474	3480	3490	rVB	629490	1236476	40.90%	5.509%
39	23.597	3498	3504	3514	rVB2	1399746	2646642	87.54%	11.793%


Sum of corrected areas: 22443009

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021249.D
Acq On : 29 Jun 2019 01:57
Operator : HP/JU
Sample : K3381-06DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM4DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

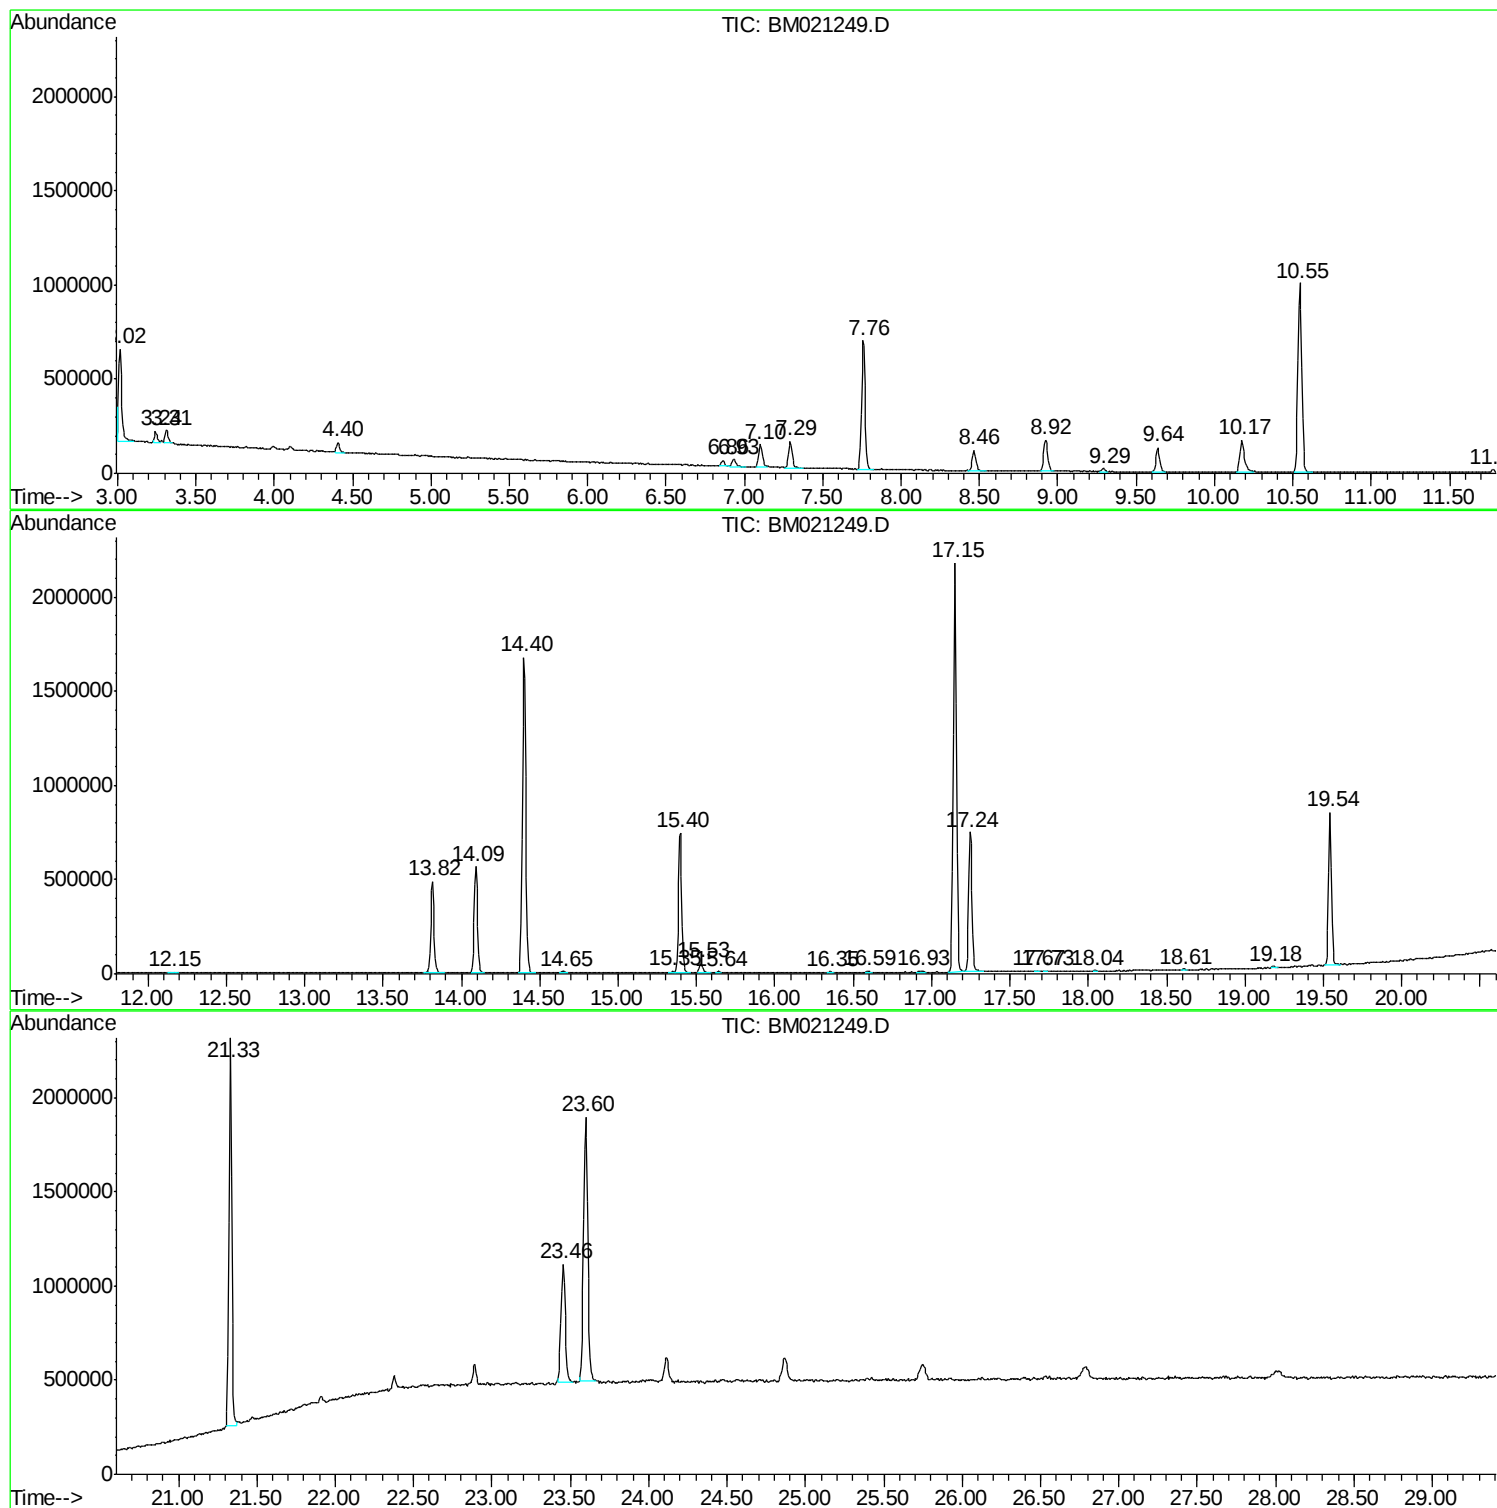

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021249.D
Acq On : 29 Jun 2019 01:57
Operator : HP/JU
Sample : K3381-06DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM4DL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.02	10.52 ng/ul	578309	1,4-Dichlorobenzene-d4	7.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	50
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

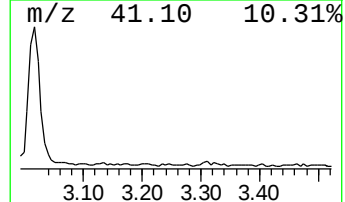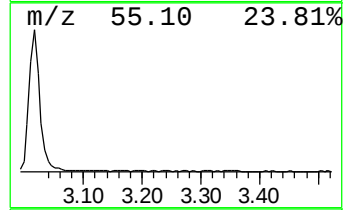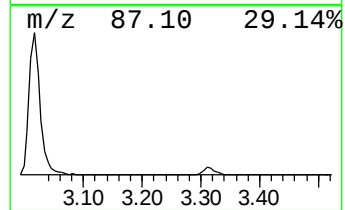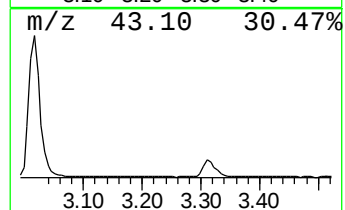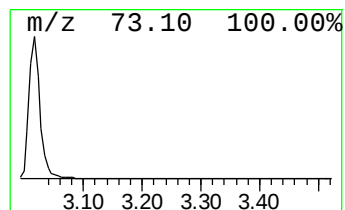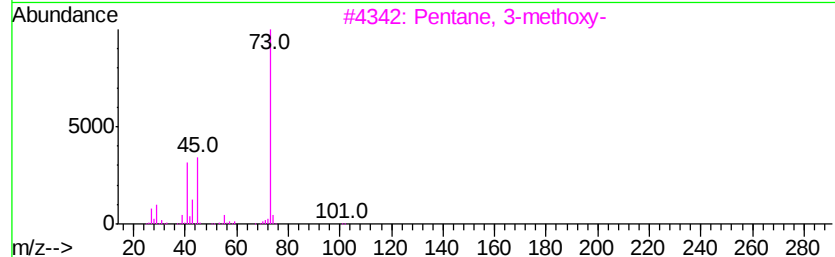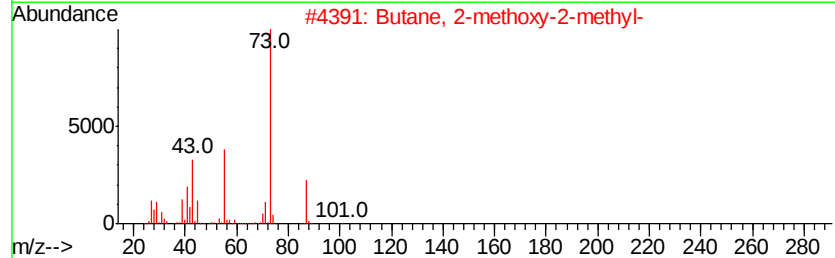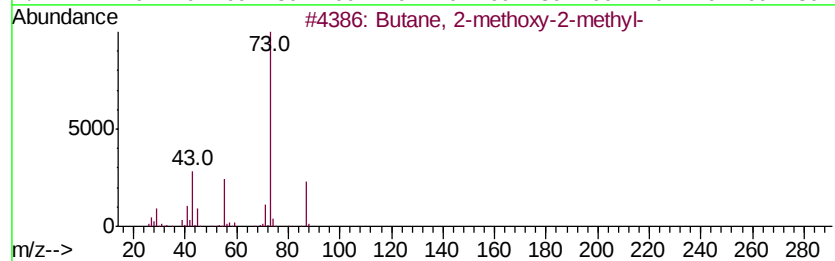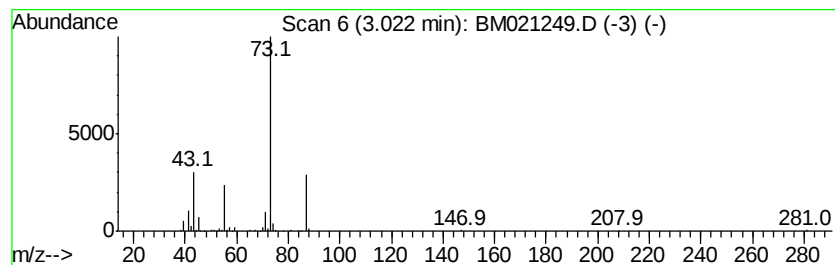

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062819\
Data File : BM021249.D
Acq On : 29 Jun 2019 01:57
Operator : HP/JU
Sample : K3381-06DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM4DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.02	10.5	ng/ul	578309	1	7.76	1099900	20.0