


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
Data File : BM030656.D
Acq On : 28 Jun 2021 16:08
Operator : CG/JU
Sample : PB137370BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK370

Manual Integrations
APPROVED

mohammad
6/29/2021 2:31:24 PM

Quant Time: Jun 28 16:41:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 14:33:12 2021
Response via : Initial Calibration

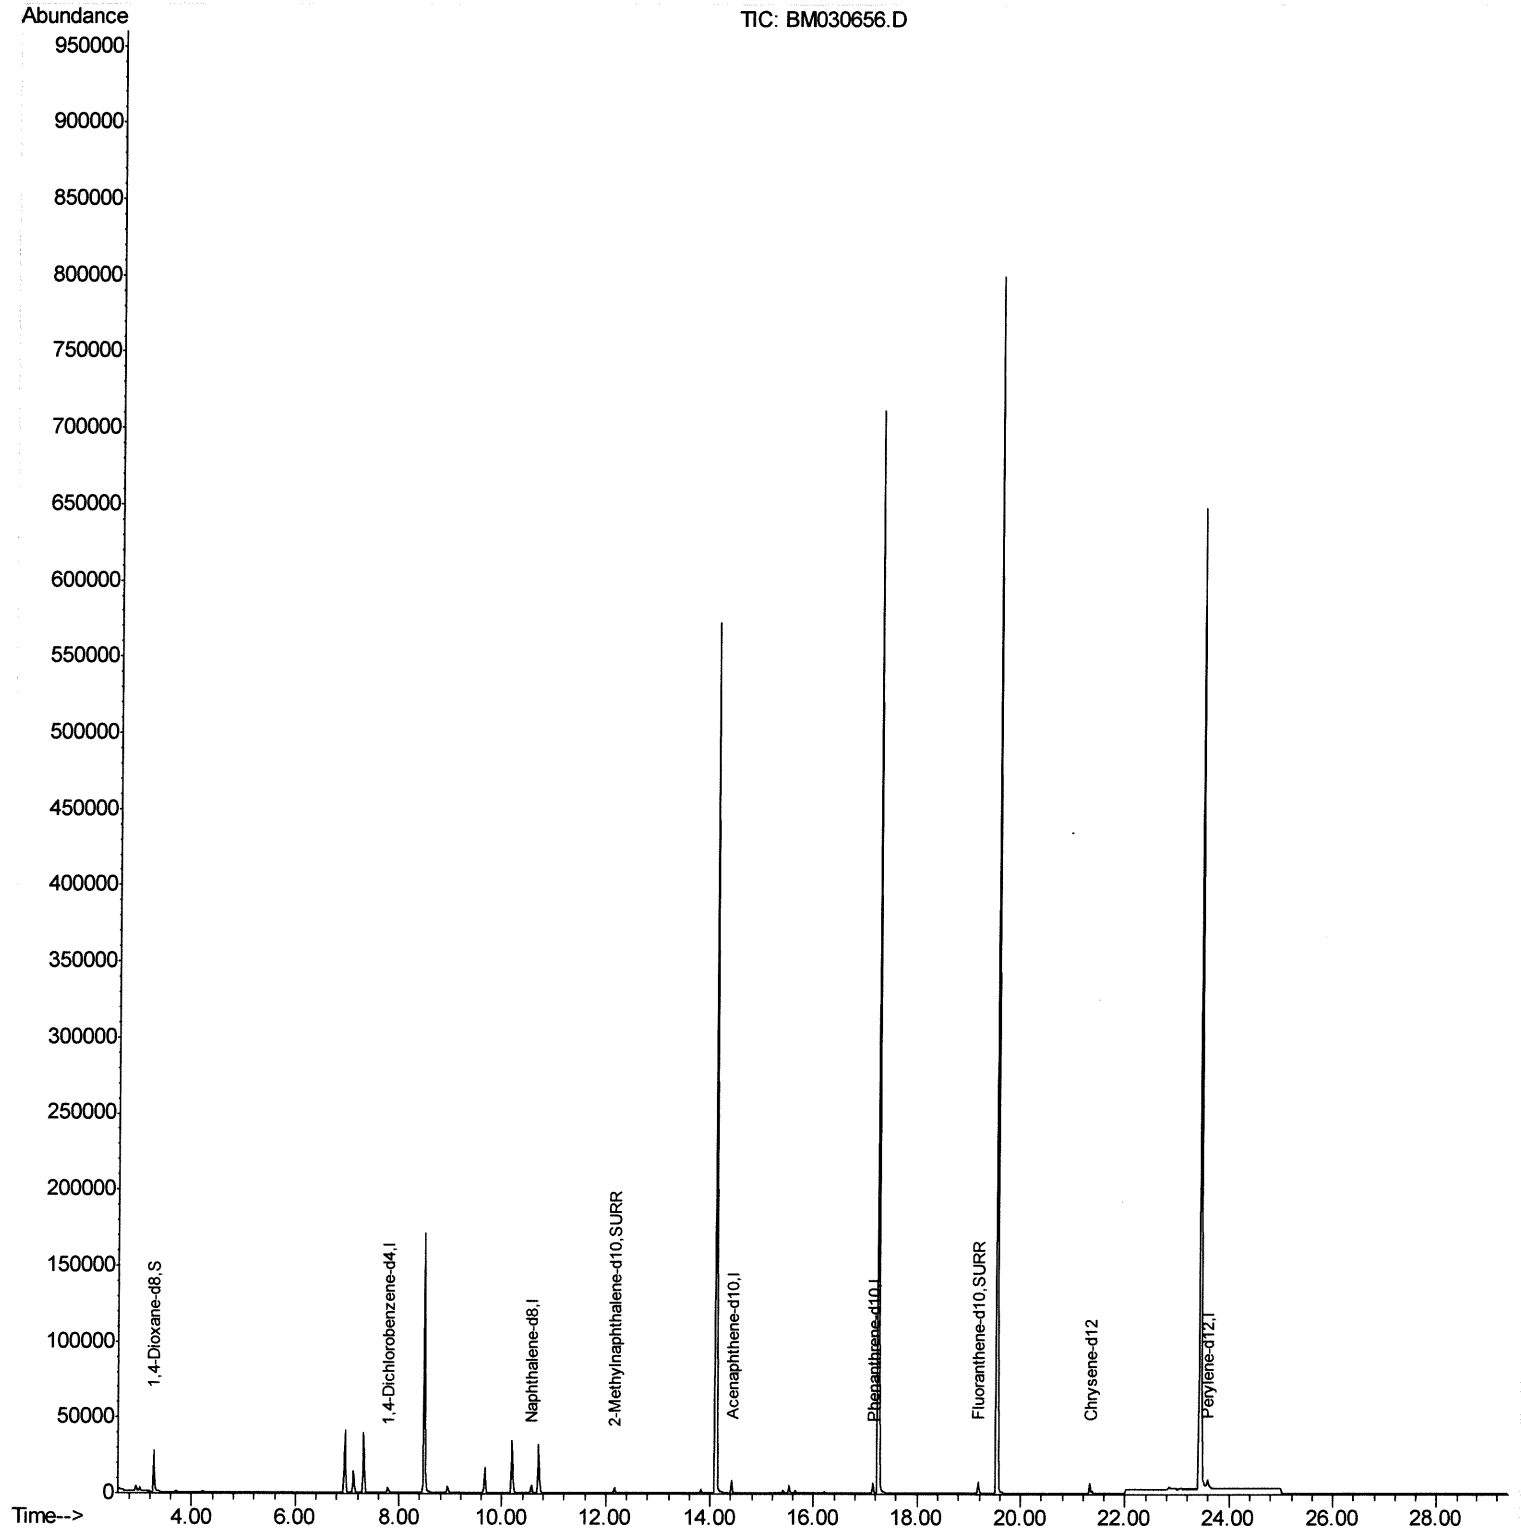




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030656.D
 Acq On : 28 Jun 2021 16:08
 Operator : CG/JU
 Sample : PB137370BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:31:24 PM

Quant Time: Jun 28 16:39:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

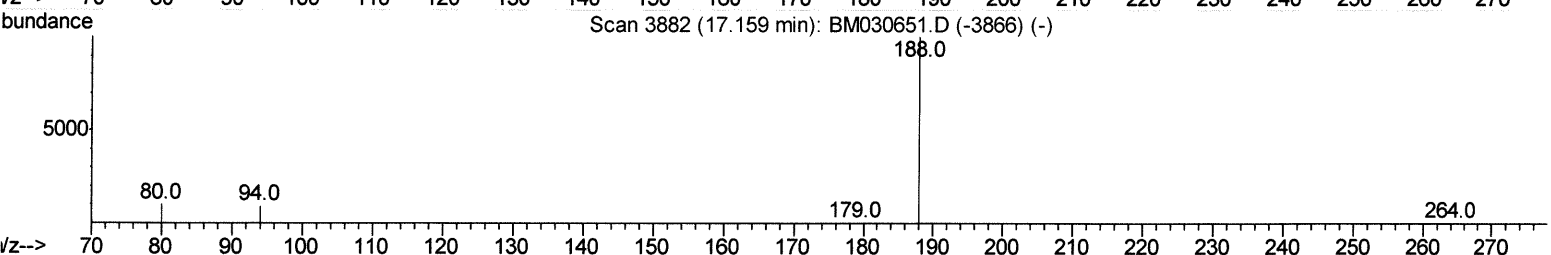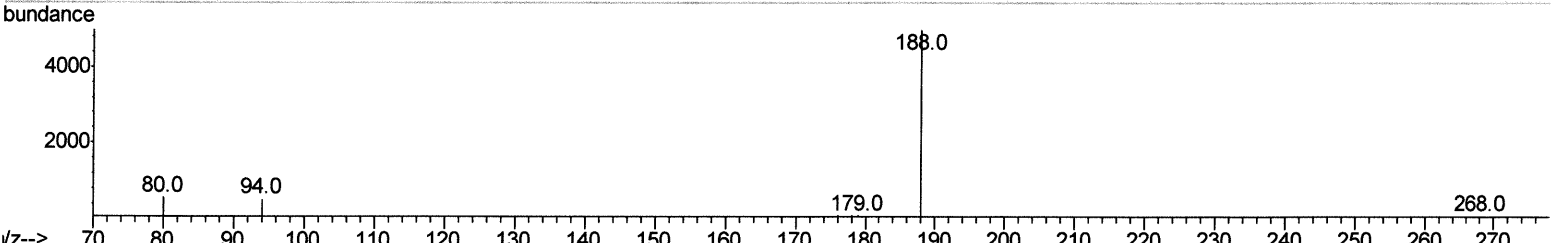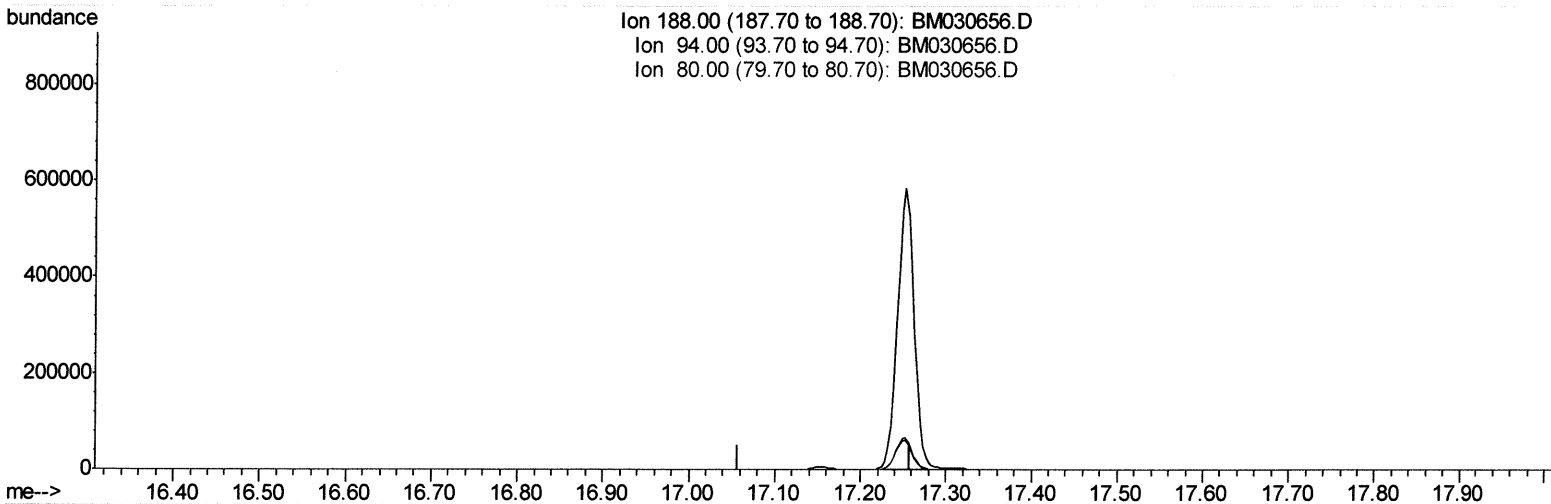

TIC: BM030656.D

(13) Phenanthrene-d10 (I)

17.159min (-17.159) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.80	0.00#
80.00	11.40	0.00#
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030656.D
 Acq On : 28 Jun 2021 16:08
 Operator : CG/JU
 Sample : PB137370BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:31:24 PM

Quant Time: Jun 28 16:39:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

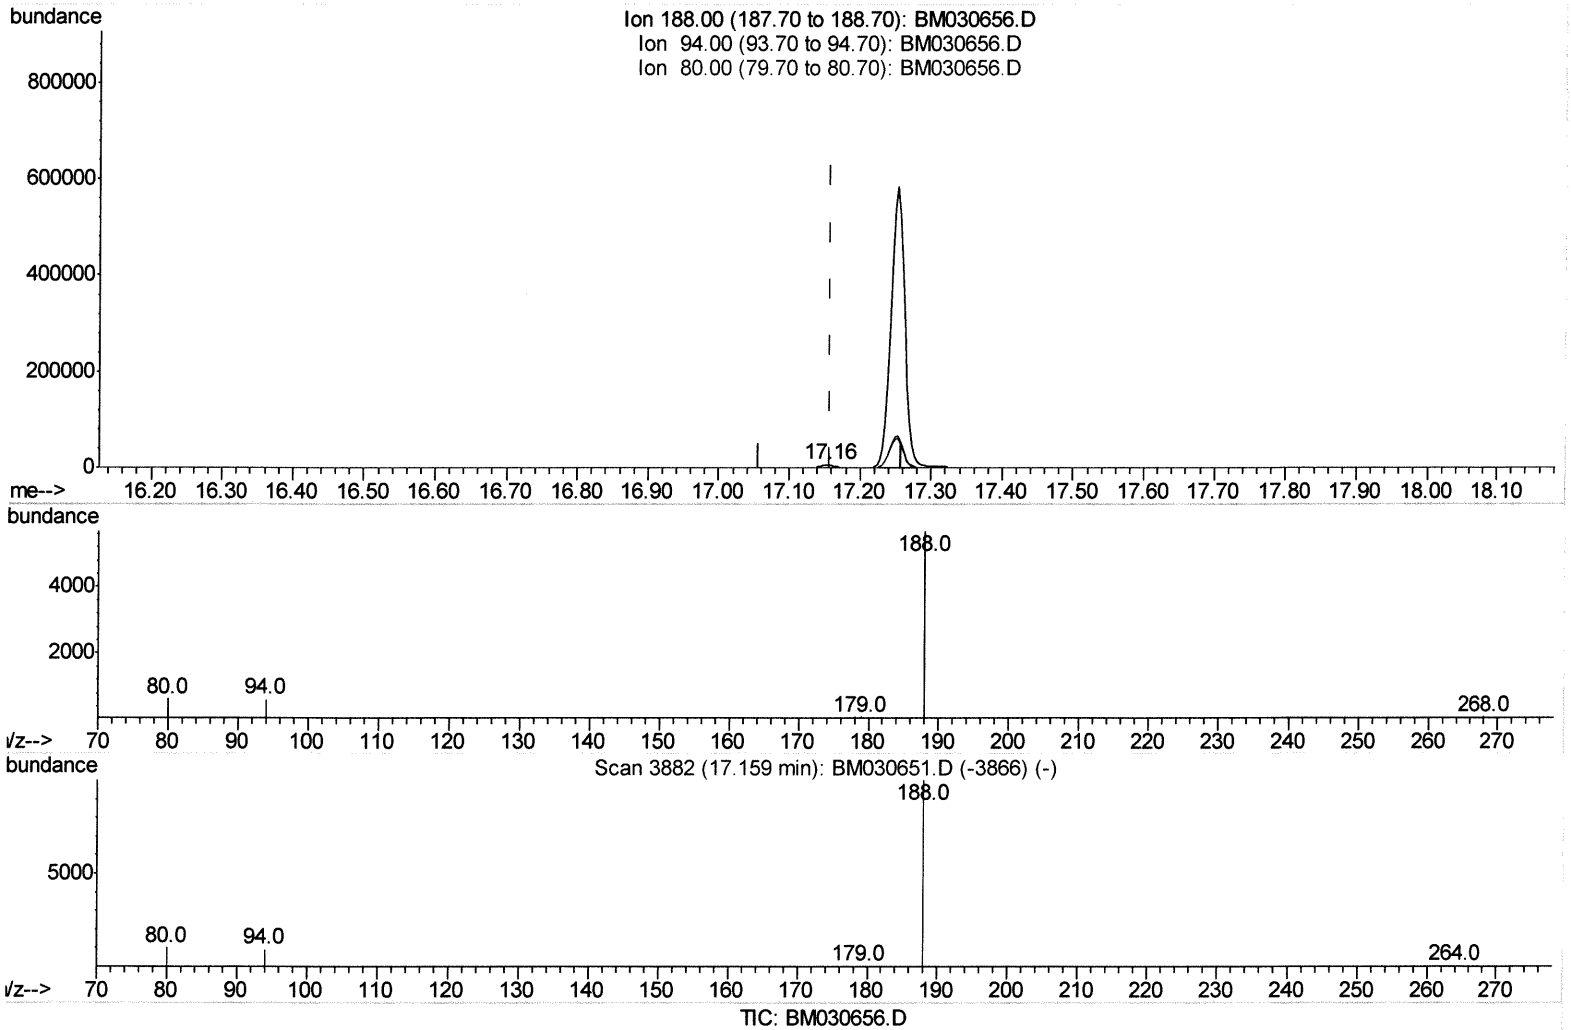

(13) Phenanthrene-d10 (I)

17.155min (-0.003) 0.40ng/ul m

response 8143

Ion	Exp%	Act%
188.00	100	100
94.00	10.80	10.40
80.00	11.40	11.00
0.00	0.00	0.00

JU 6/29/21

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030656.D
 Acq On : 28 Jun 2021 16:08
 Operator : CG/JU
 Sample : PB137370BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:31:24 PM

Quant Time: Jun 28 16:41:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1944	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	7199	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	4452	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.16	188	8143m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	7146	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	8496	0.40	ng/ul	0.00

74 6/30/21

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	16821	7.94	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.17	152	4919	0.43	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	9326	0.46	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed