


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062821\
Data File : BM030674.D
Acq On : 29 Jun 2021 04:32
Operator : CG/JU
Sample : PB137262BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual Integrations
APPROVED

mohammad
6/29/2021 2:32:12 PM

Quant Time: Jun 29 05:58:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 02:23:03 2021
Response via : Initial Calibration

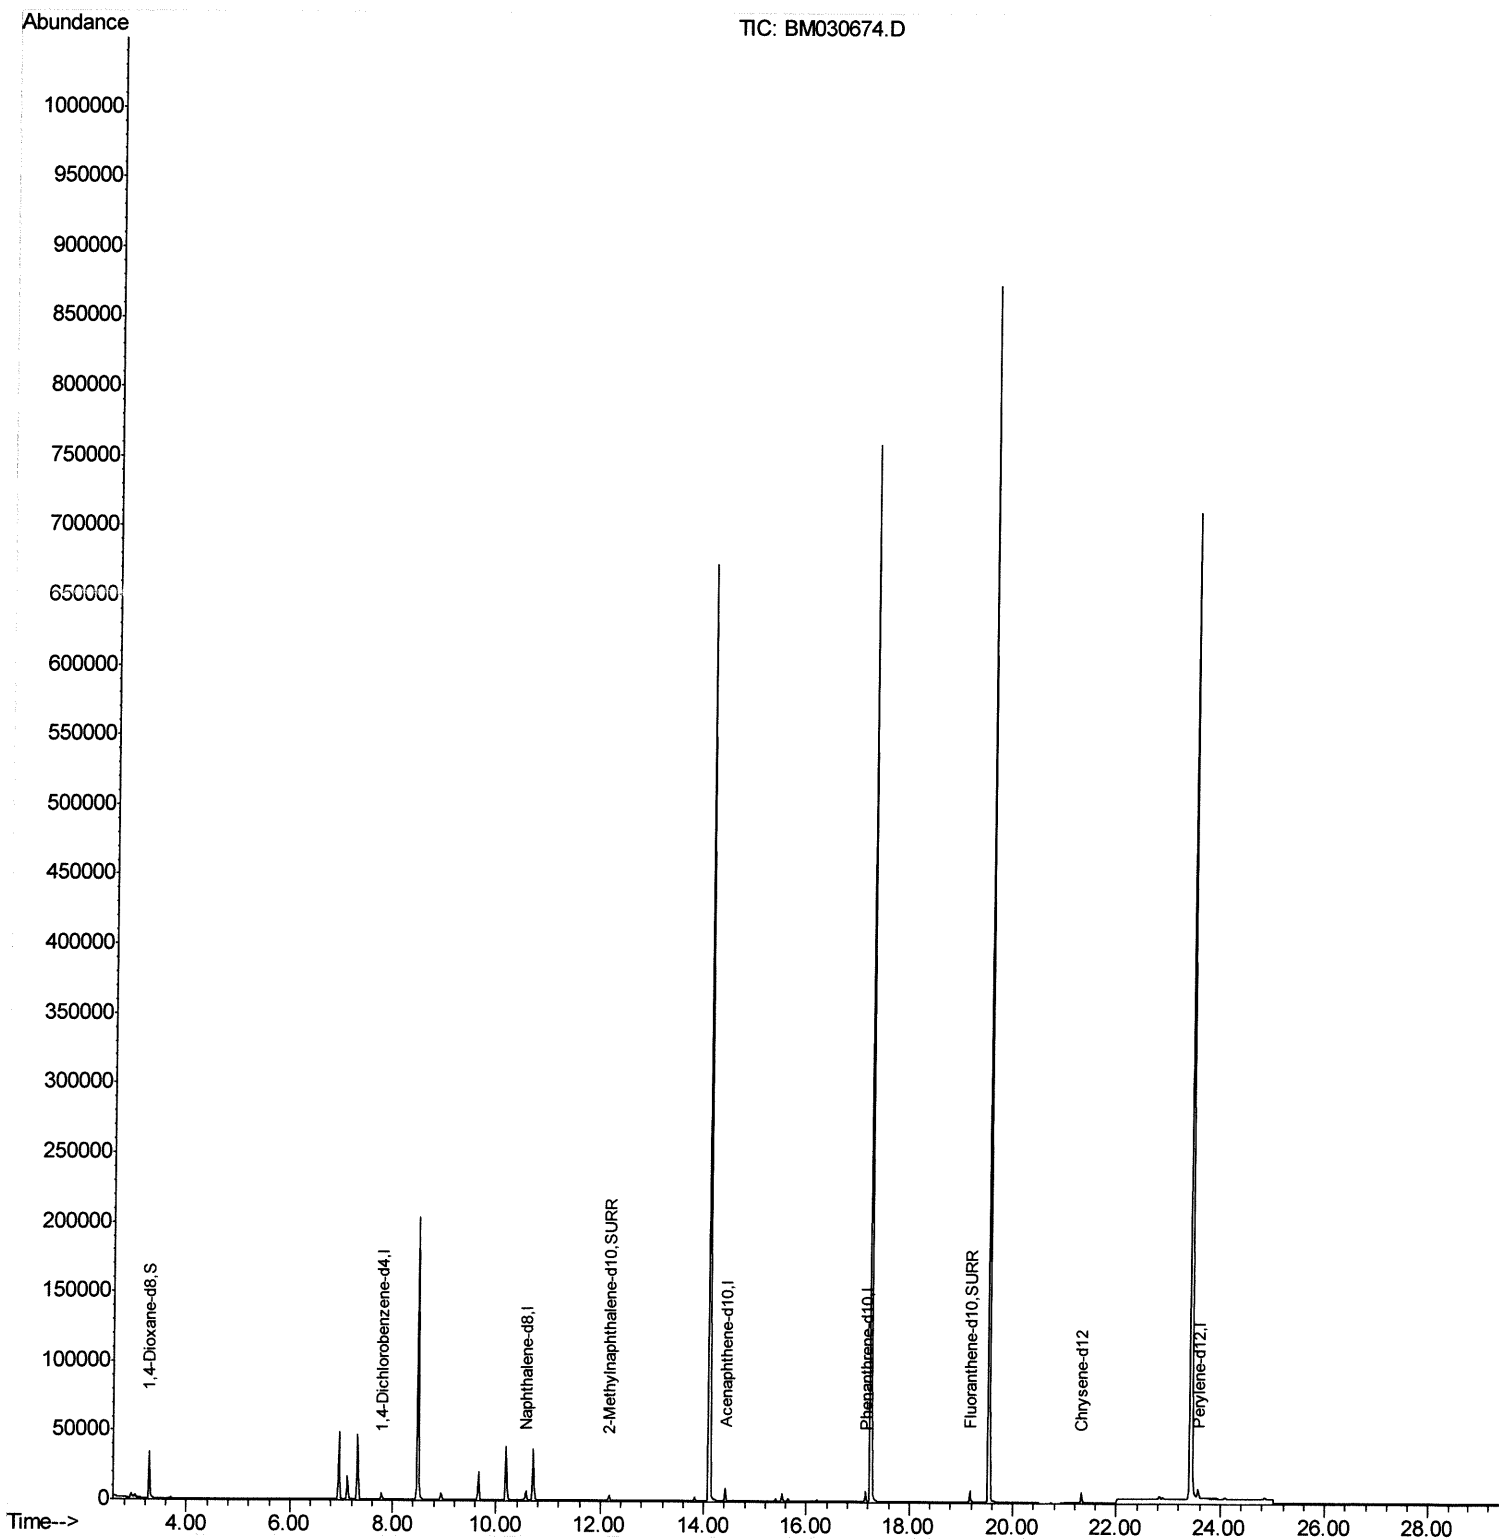


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062821\
 Data File : BM030674.D
 Acq On : 29 Jun 2021 04:32
 Operator : CG/JU
 Sample : PB137262BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK262

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:32:12 PM

Quant Time: Jun 29 05:55:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 02:23:03 2021
 Response via : Initial Calibration

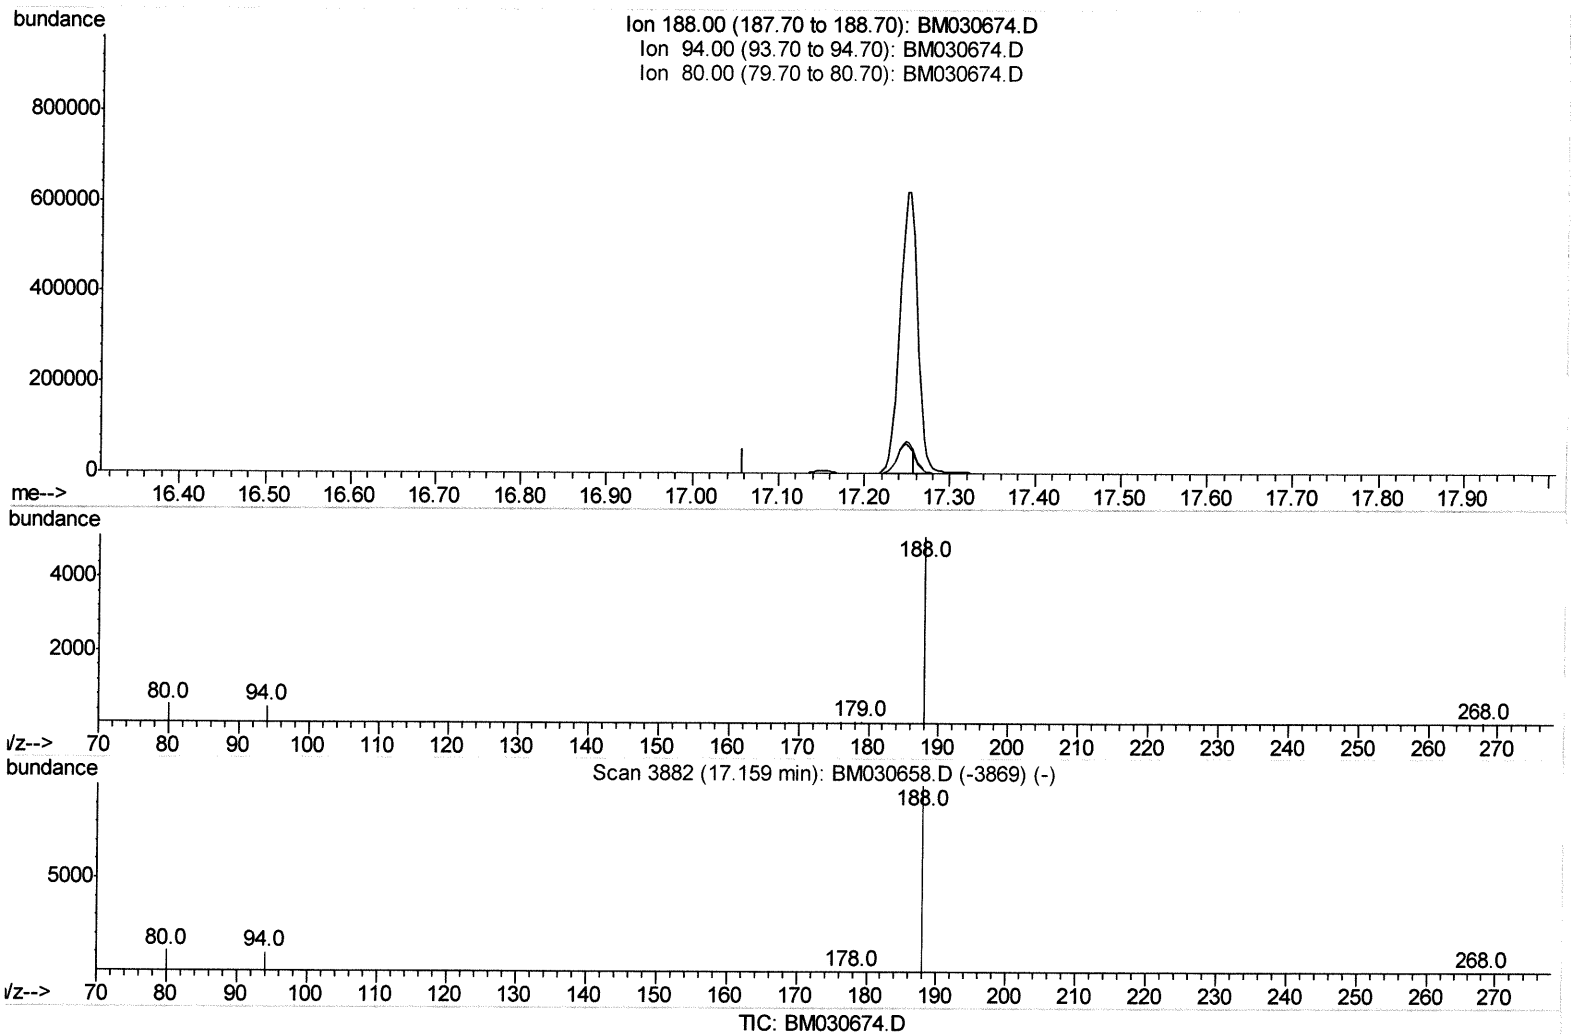

(13) Phenanthrene-d10 (I)

17.159min (-17.159) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.80	0.00#
80.00	11.40	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062821\
 Data File : BM030674.D
 Acq On : 29 Jun 2021 04:32
 Operator : CG/JU
 Sample : PB137262BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK262

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:32:12 PM

Quant Time: Jun 29 05:55:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 02:23:03 2021
 Response via : Initial Calibration

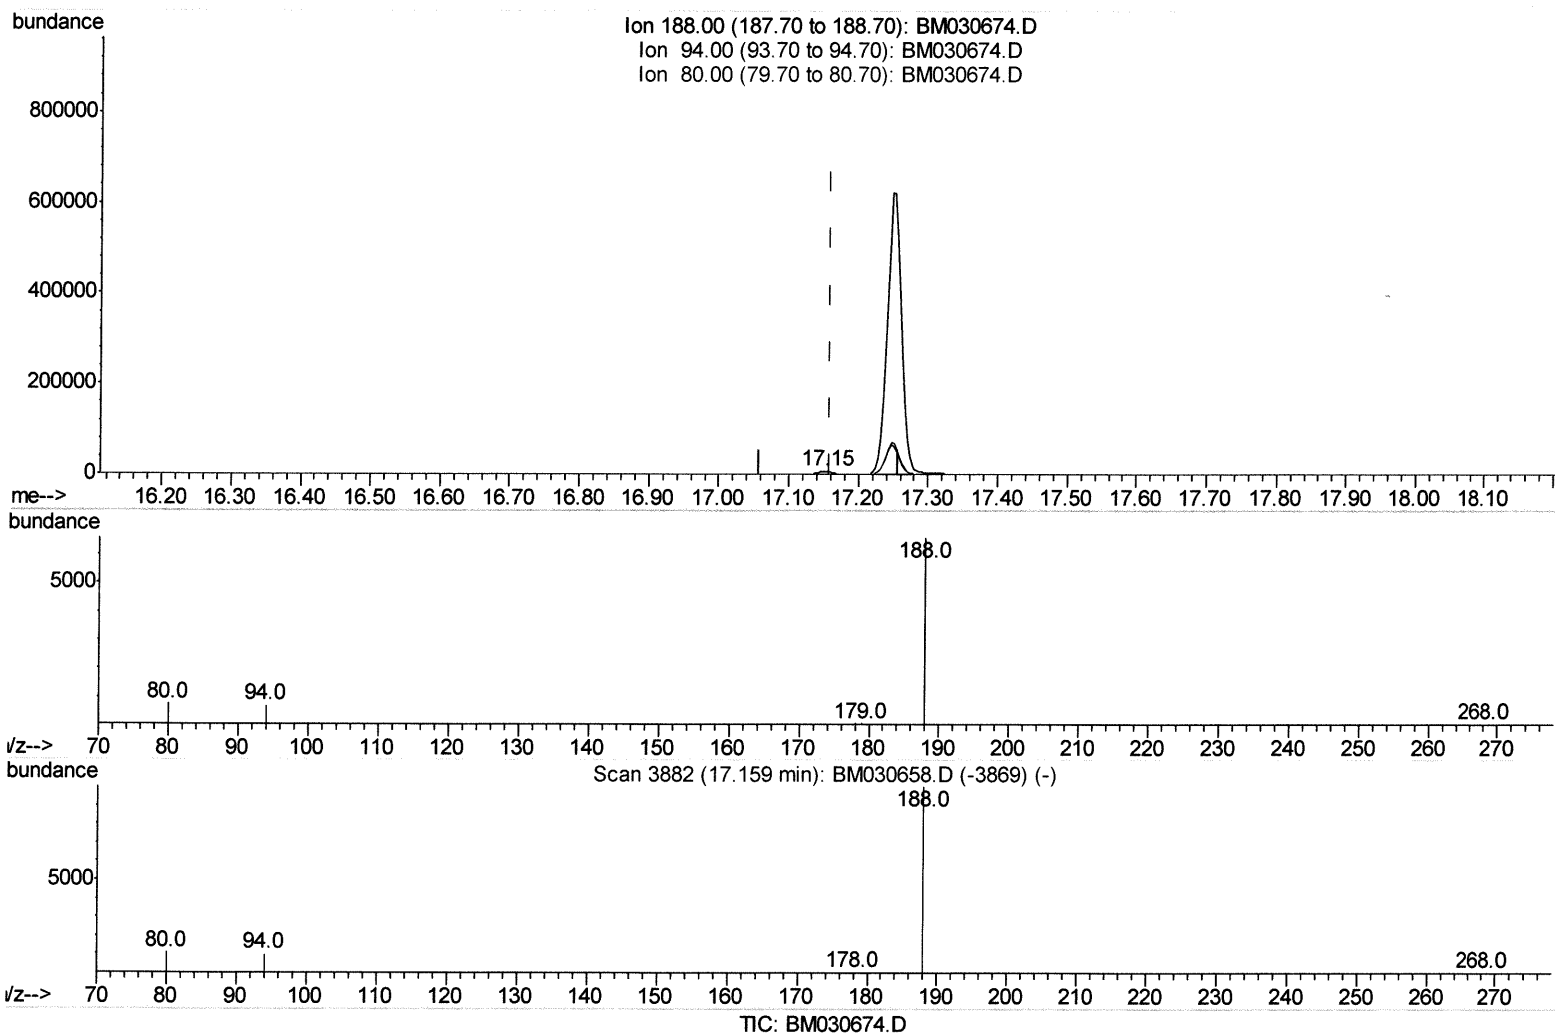

(13) Phenanthrene-d10 (I)

17.152min (-0.007) 0.40ng/ul m

JK 6/30/21

response 9123

Ion	Exp%	Act%
188.00	100	100
94.00	10.80	10.50
80.00	11.40	11.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062821\
 Data File : BM030674.D
 Acq On : 29 Jun 2021 04:32
 Operator : CG/JU
 Sample : PB137262BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK262

Manual Integrations
 APPROVED

mohammad
 6/29/2021 2:32:12 PM

Quant Time: Jun 29 05:58:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 02:23:03 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	2369	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	8682	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	5114	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.15	188	9123m	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	7354	0.40	ng/ul	0.00
23) Perylene-d12	23.57	264	9734	0.40	ng/ul	0.00

Handwritten: > 0.00 > Ju 6/30/21

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	20411	7.91	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.17	152	5828	0.43	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	10272	0.49	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed