


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
Data File : BM030683.D
Acq On : 29 Jun 2021 10:02
Operator : CG/JU
Sample : M2761-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLX83

Manual Integrations
APPROVED

mohammad
6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:12:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 14:33:12 2021
Response via : Initial Calibration

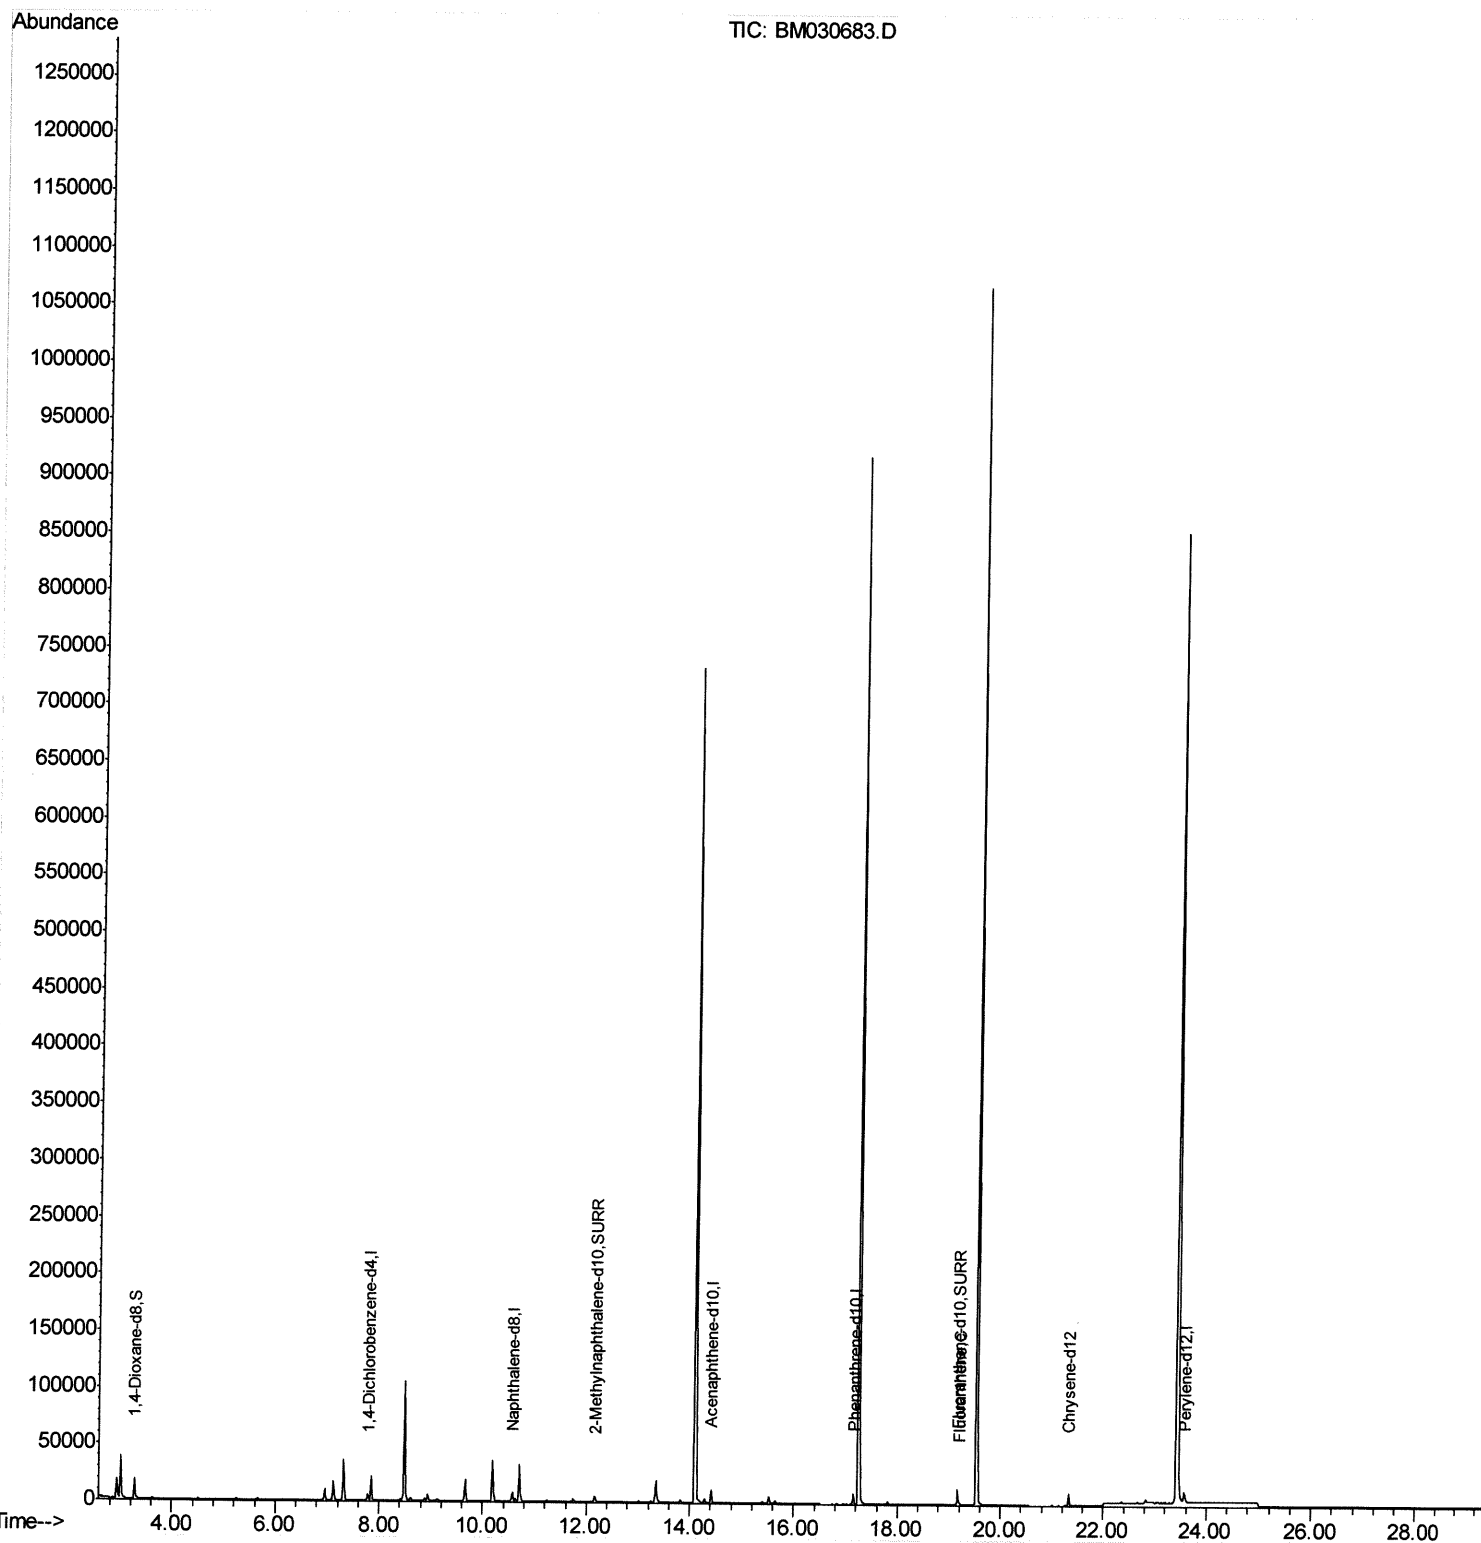




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030683.D
 Acq On : 29 Jun 2021 10:02
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX83

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:11:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

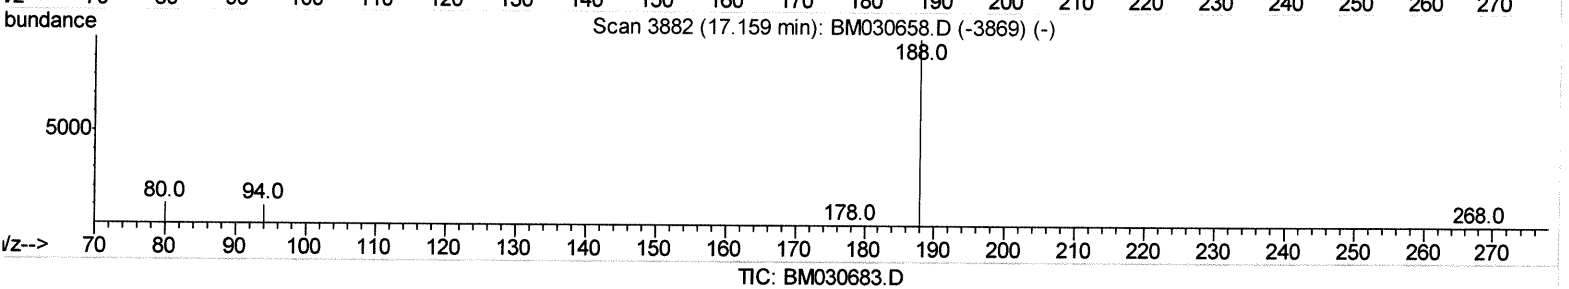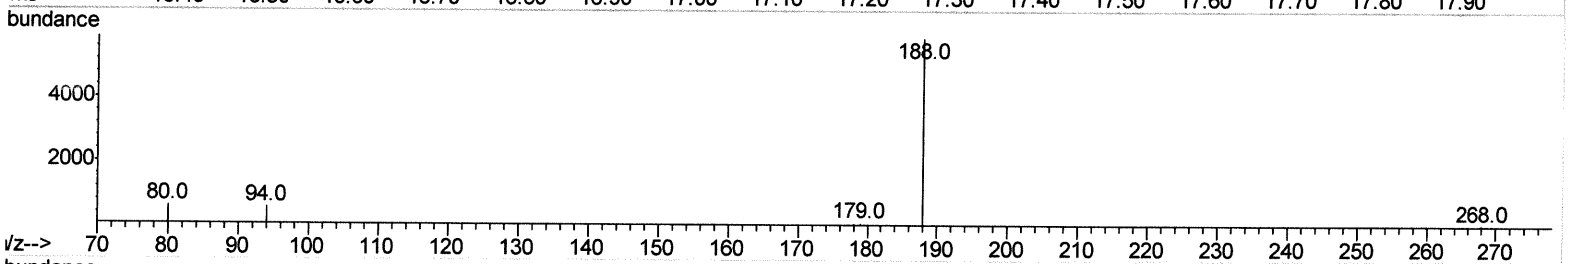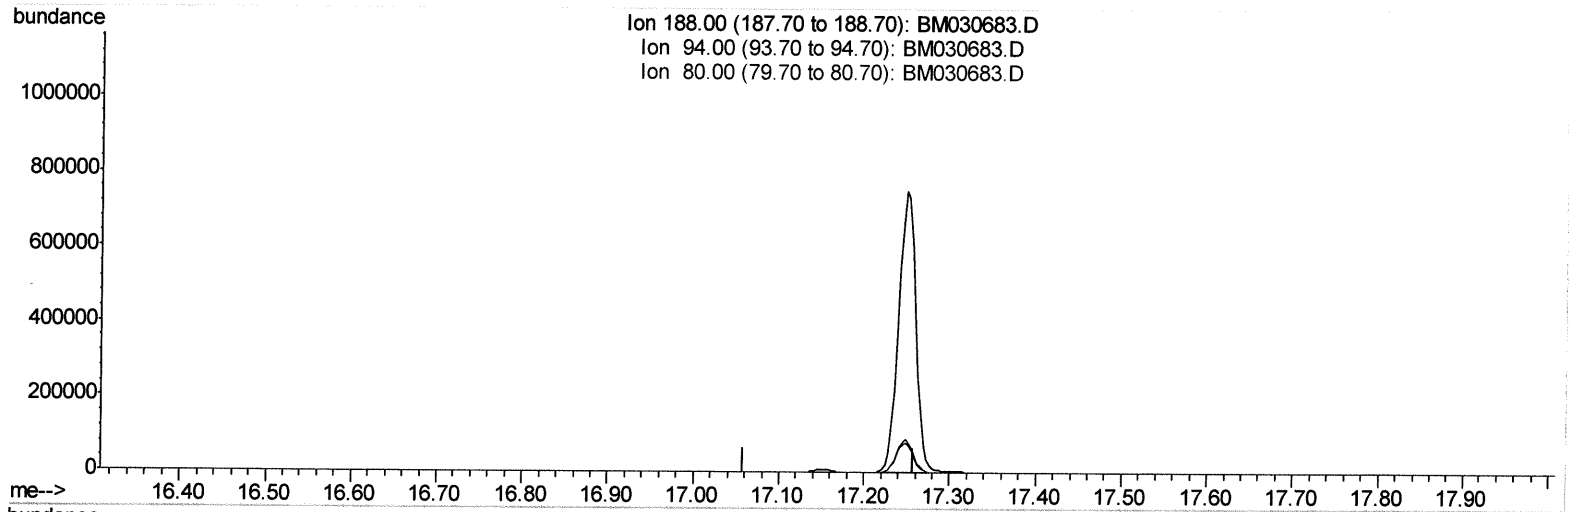

(13) Phenanthrene-d10 (I)

17.159min (-17.159) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.80	0.00#
80.00	11.40	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030683.D
 Acq On : 29 Jun 2021 10:02
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX83

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:11:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

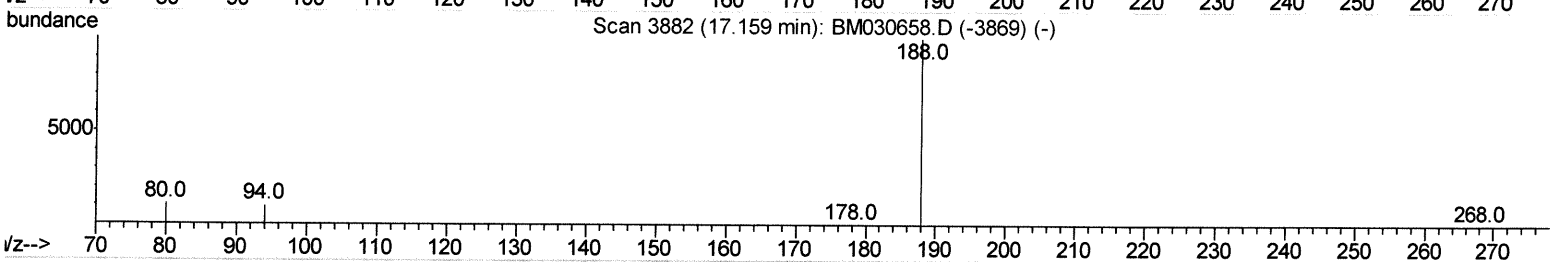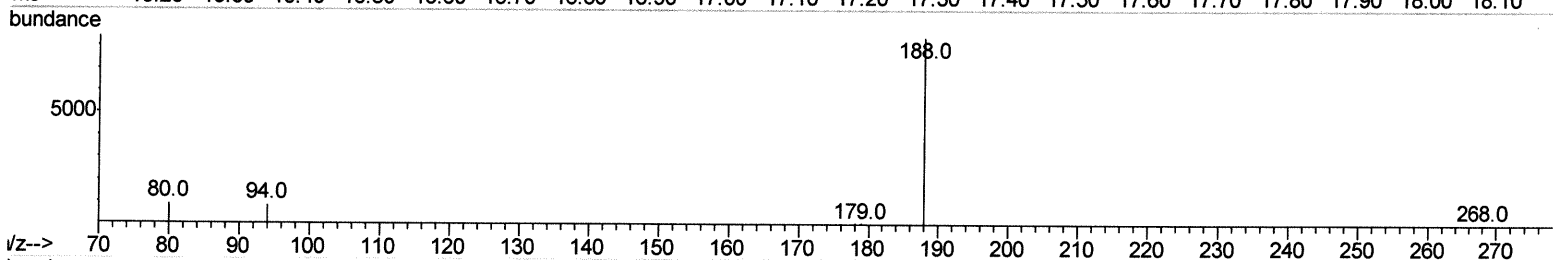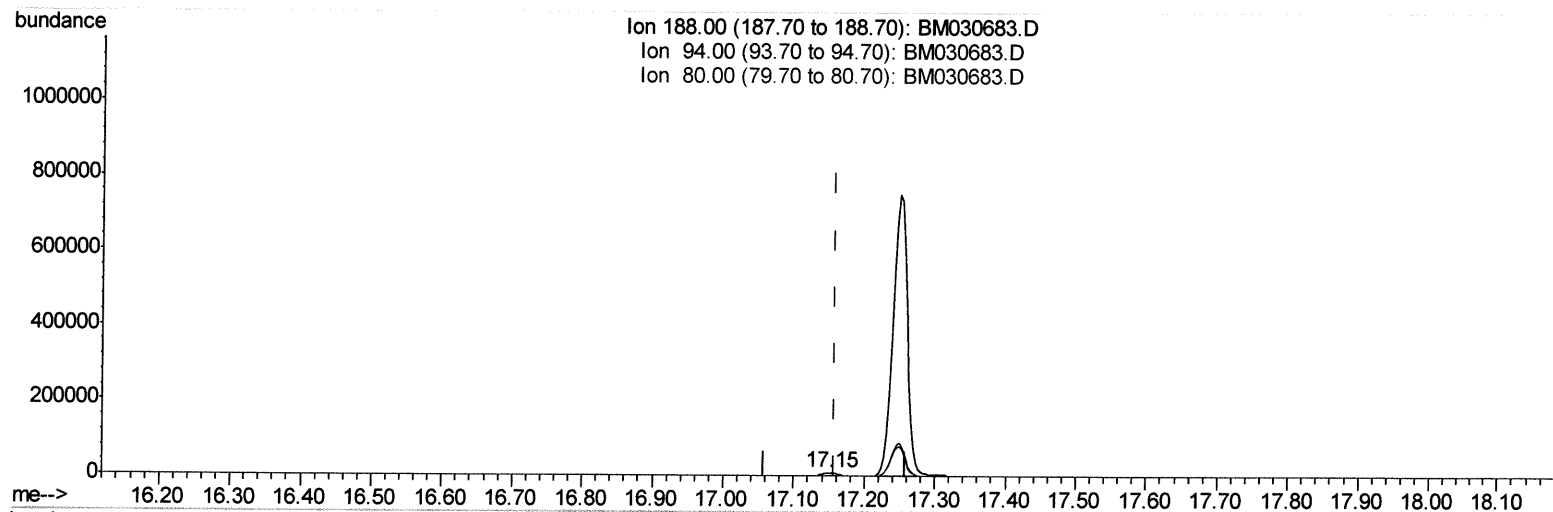

TIC: BM030683.D

(13) Phenanthrene-d10 (I)

17.152min (-0.007) 0.40ng/ul m

response 12016

Ion	Exp%	Act%
188.00	100	100
94.00	10.80	10.37
80.00	11.40	10.85
0.00	0.00	0.00

ju 6/30/21

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030683.D
 Acq On : 29 Jun 2021 10:02
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX83

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:12:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	3000	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	11000	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.41	164	6581	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.15	188	12016m	0.40	ng/ul	0.00
17) Chrysene-d12	21.32	240	9954	0.40	ng/ul	0.00
23) Perylene-d12	23.57	264	12623	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	11421	3.49	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.16	152	7297	0.42	ng/ul	0.00
18) Fluoranthene-d10	19.17	212	14954	0.52	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.20	202	1082	0.025	ng/ul#	Ovalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JP 6/30/21