


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
Data File : BM030685.D
Acq On : 29 Jun 2021 11:16
Operator : CG/JU
Sample : PB137232BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Manual Integrations
APPROVED

mohammad
6/30/2021 10:24:44 AM

Quant Time: Jun 29 11:58:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 14:33:12 2021
Response via : Initial Calibration

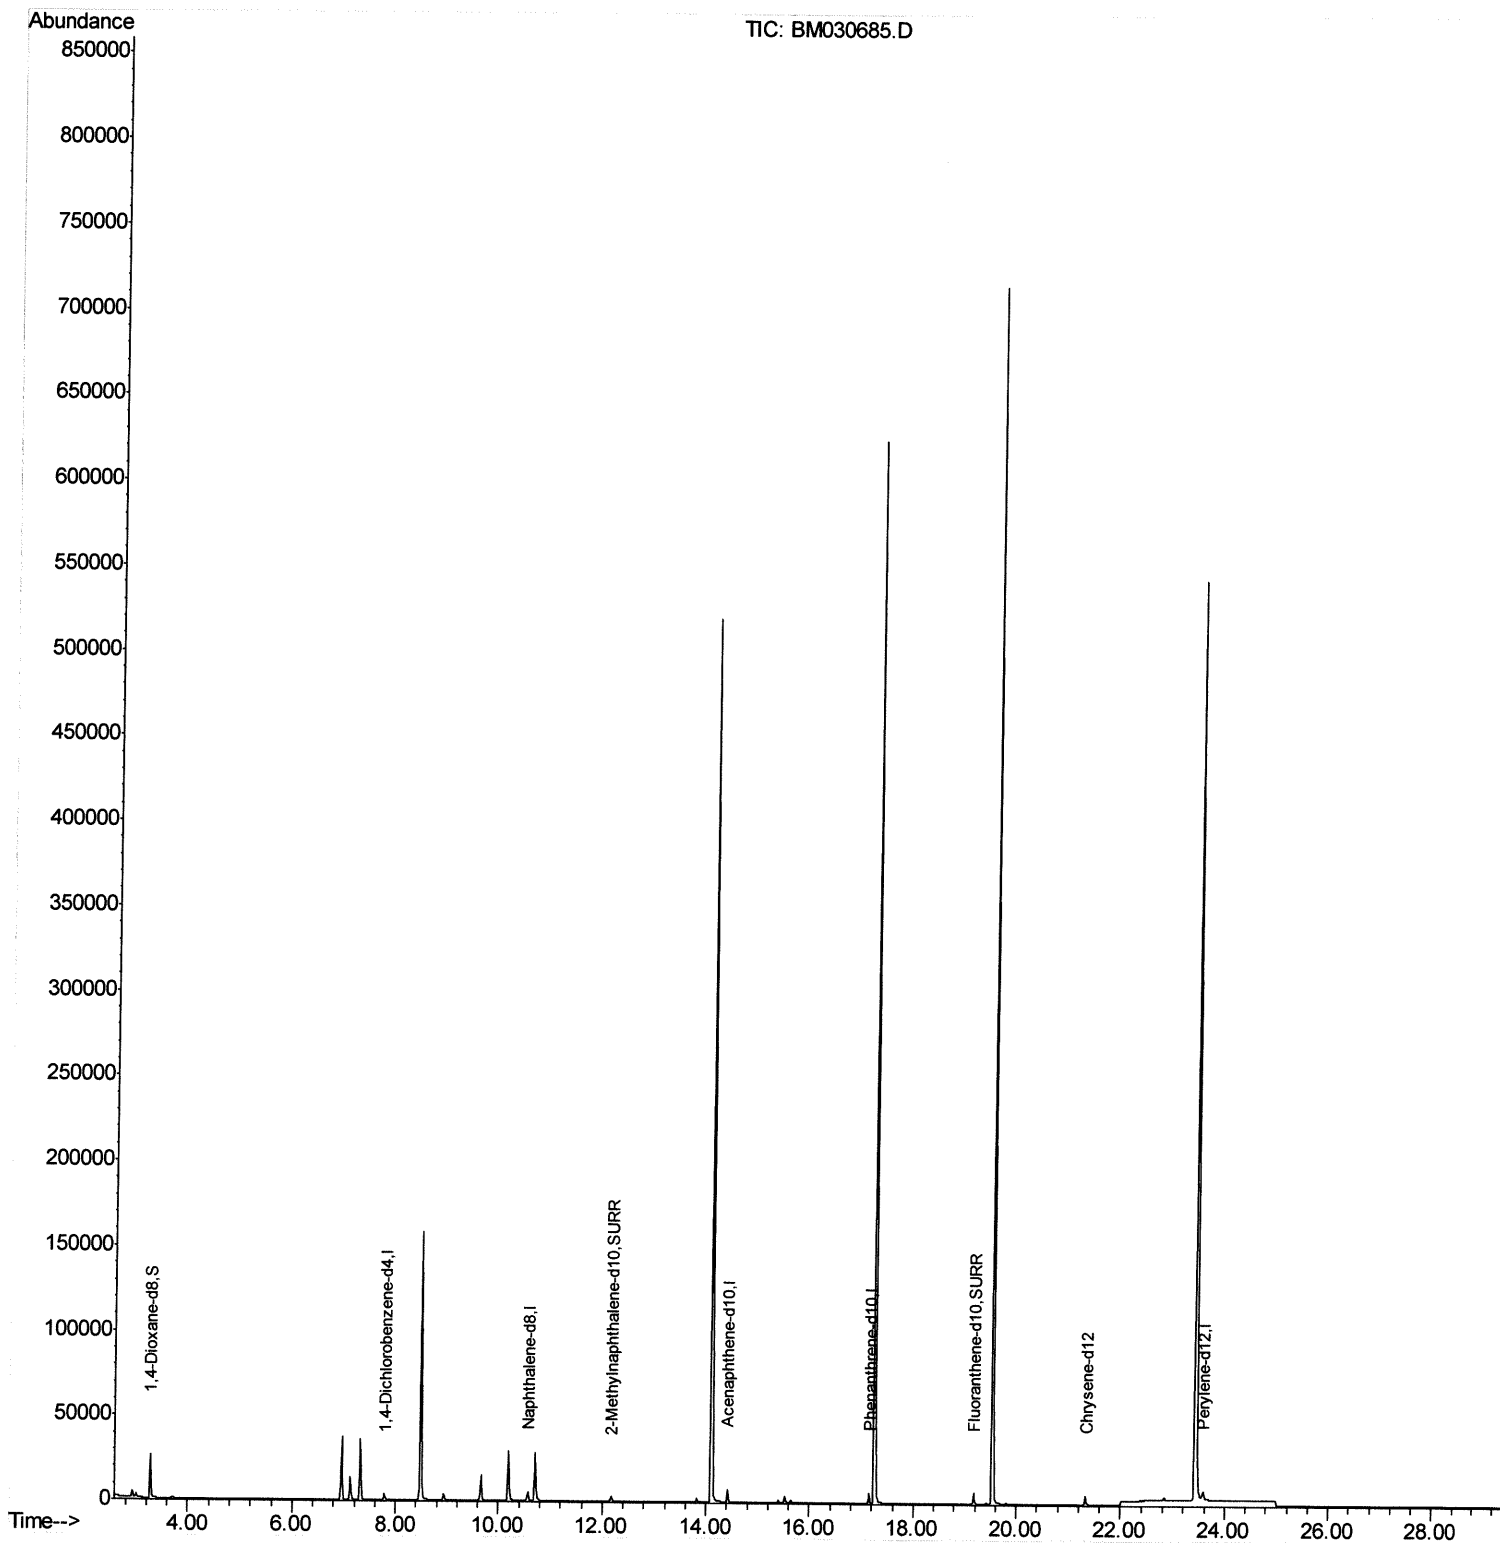




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030685.D
 Acq On : 29 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB137232BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:44 AM

Quant Time: Jun 29 11:54:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

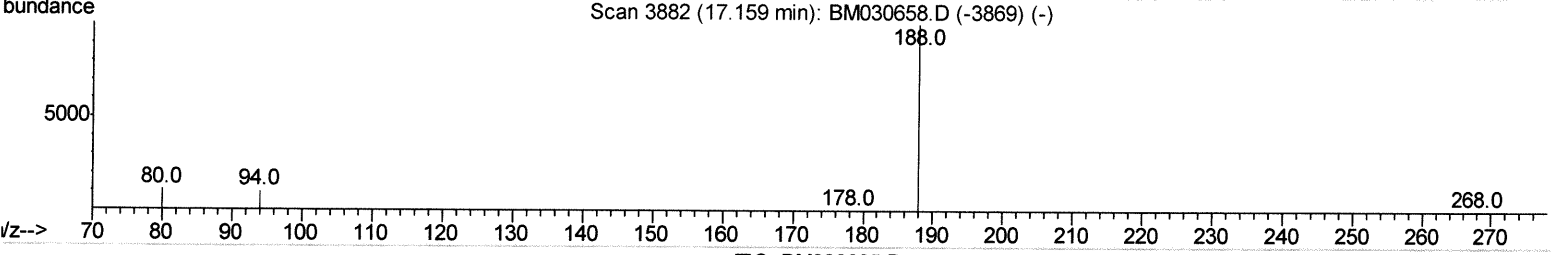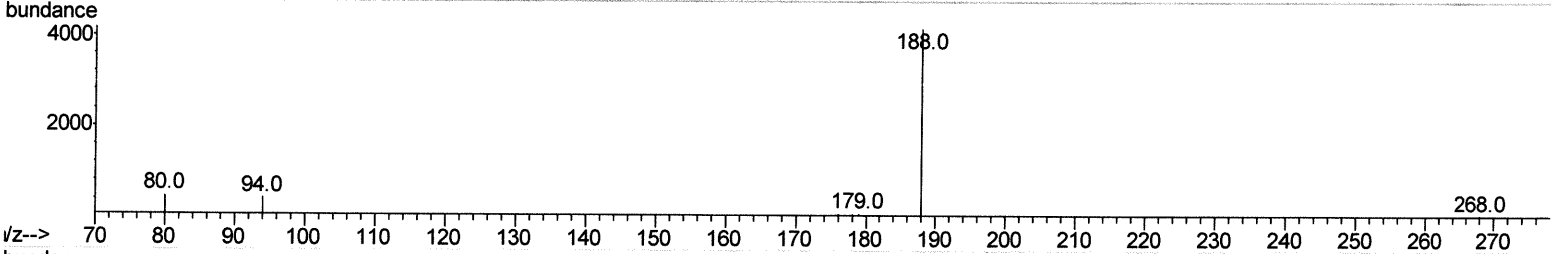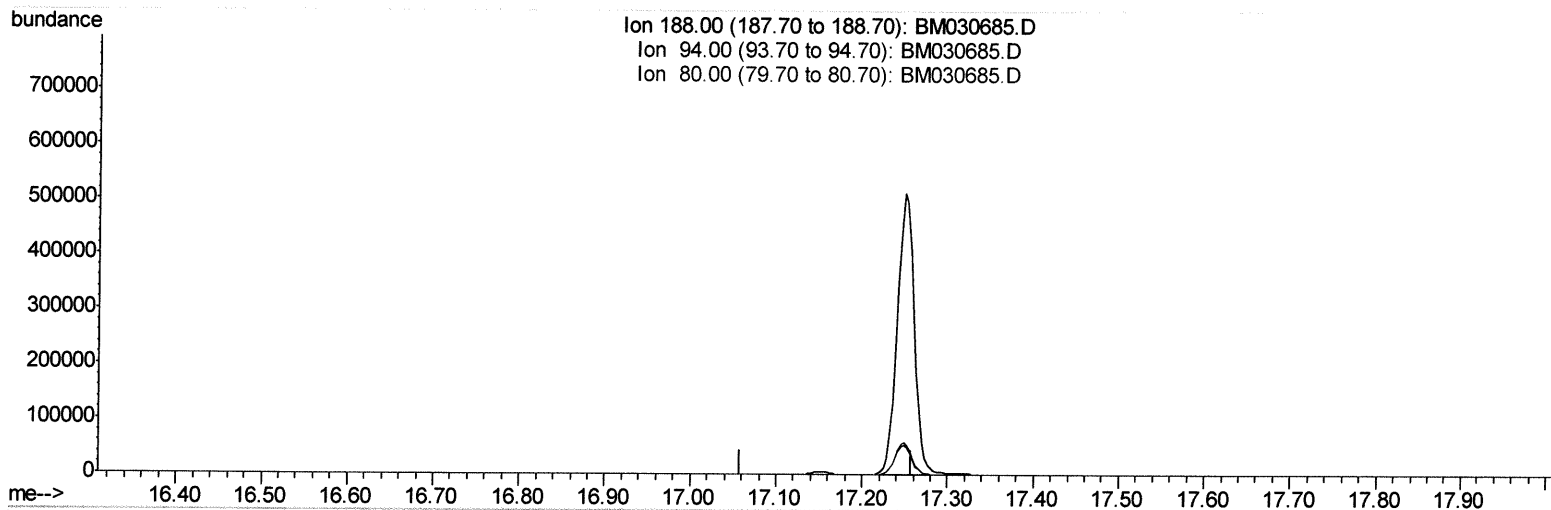

TIC: BM030685.D

(13) Phenanthrene-d10 (I)

17.159min (-17.159) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.80	0.00#
80.00	11.40	0.00#
0.00	0.00	0.00


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
 Data File : BM030685.D
 Acq On : 29 Jun 2021 11:16
 Operator : CG/JU
 Sample : PB137232BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:44 AM

Quant Time: Jun 29 11:54:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

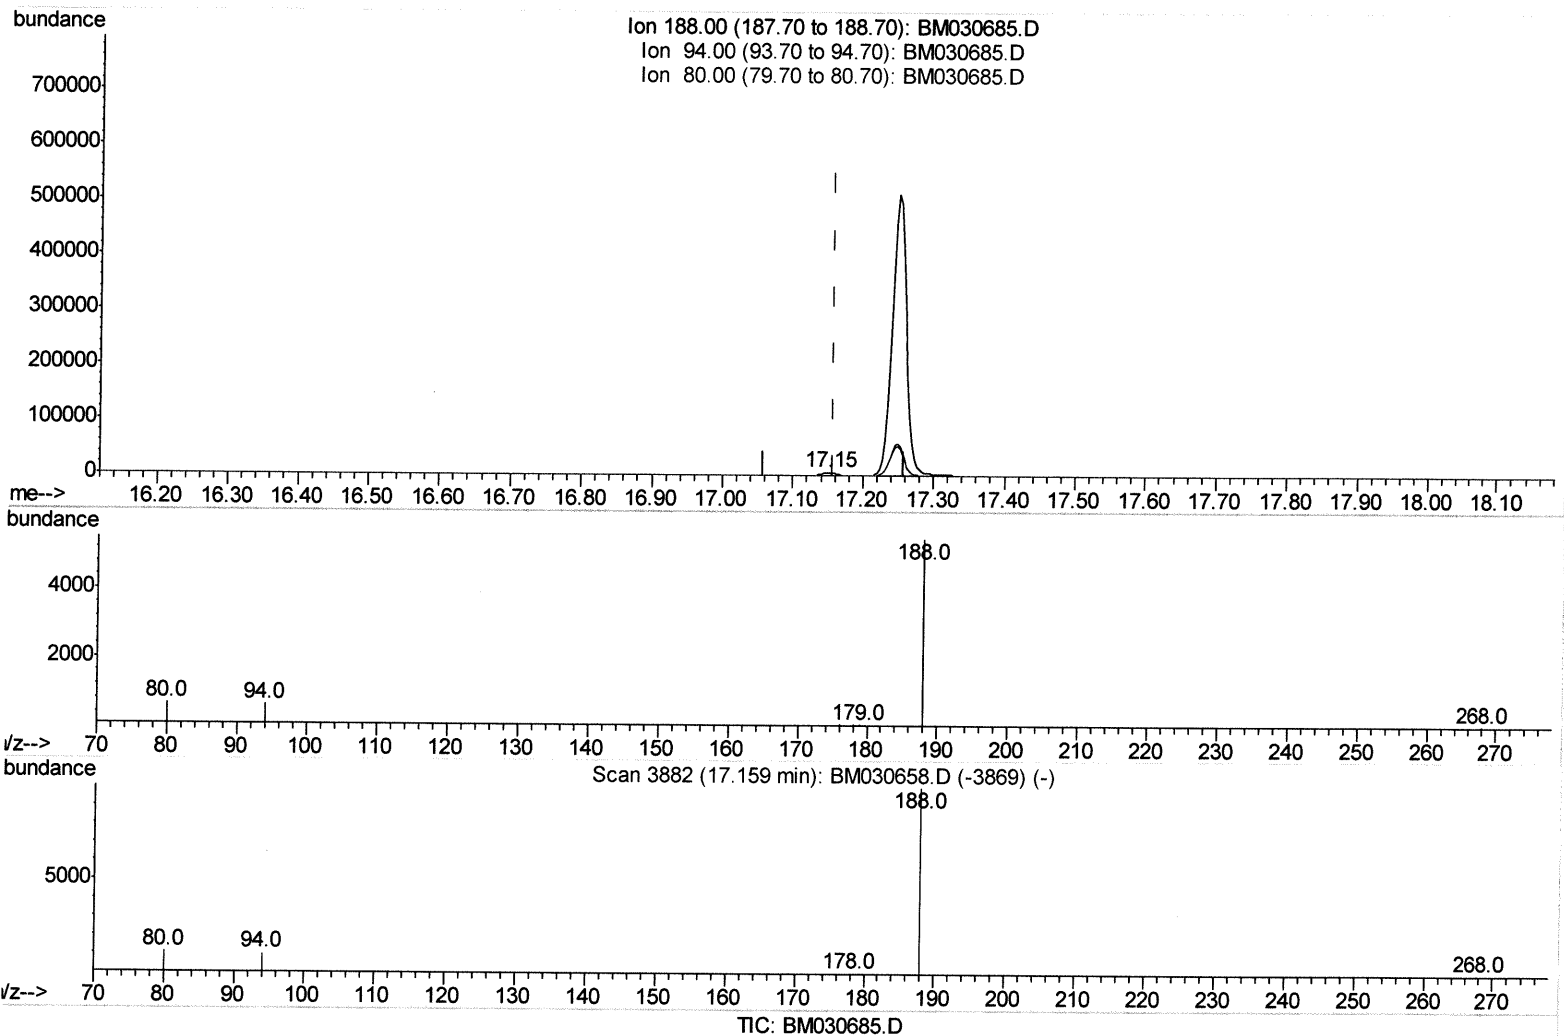

(13) Phenanthrene-d10 (I)

17.152min (-0.007) 0.40ng/ul m

response 7779

Ion	Exp%	Act%
188.00	100	100
94.00	10.80	10.80
80.00	11.40	11.66
0.00	0.00	0.00

36 6/30/21

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062821\
Data File : BM030685.D
Acq On : 29 Jun 2021 11:16
Operator : CG/JU
Sample : PB137232BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Manual Integrations
APPROVED

mohammad
6/30/2021 10:24:44 AM

Quant Time: Jun 29 11:58:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 14:33:12 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	2006	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	7358	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.41	164	4294	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.15	188	7779m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	6022	0.40	ng/ul	0.00
23) Perylene-d12	23.58	264	8015	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	15838	7.25	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.17	152	4534	0.39	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	8067	0.47	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 6/30/21