

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062821\
 Data File : BM030683.D
 Acq On : 29 Jun 2021 10:02
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX83

Manual Integrations
 APPROVED

mohammad
 6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:11:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 28 14:33:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	3000	0.400	ng/ul	0.00
4) Naphthalene-d8	10.572	136	11000	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.413	164	6581	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.152	188	12016m	0.400	ng/ul	0.00
17) Chrysene-d12	21.323	240	9954	0.400	ng/ul	0.00
23) Perylene-d12	23.571	264	12623	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	11421	3.494	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.164	152	7297	0.422	ng/ul	0.00
18) Fluoranthene-d10	19.172	212	14954	0.524	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.203	202	1082	0.025	ng/ul#	Qvalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062821\
Data File : BM030683.D
Acq On : 29 Jun 2021 10:02
Operator : CG/JU
Sample : M2761-01
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JLX83

Manual Integrations
APPROVED


mohammad
6/30/2021 10:24:40 AM

Quant Time: Jun 29 11:11:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 28 14:33:12 2021
Response via : Initial Calibration


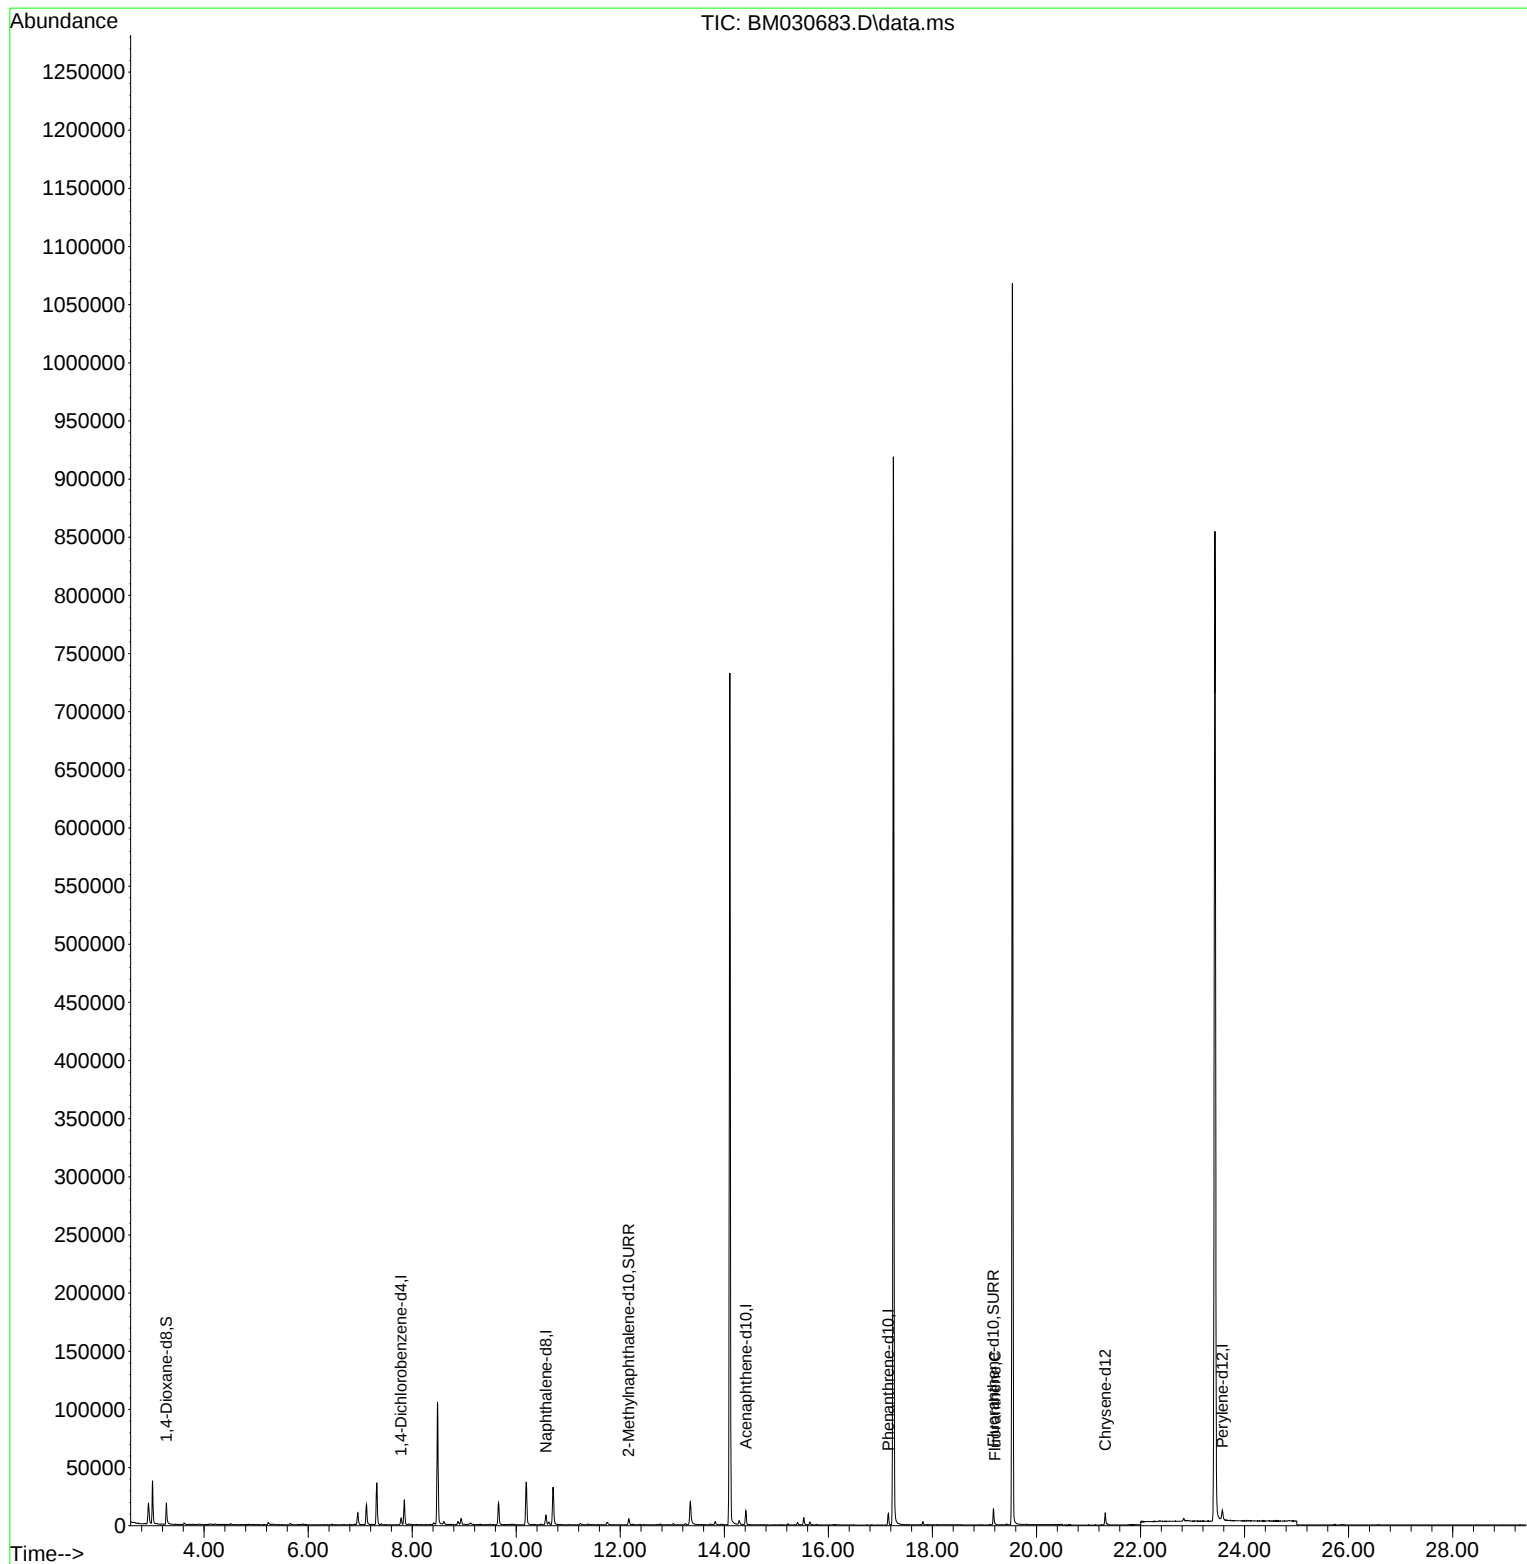


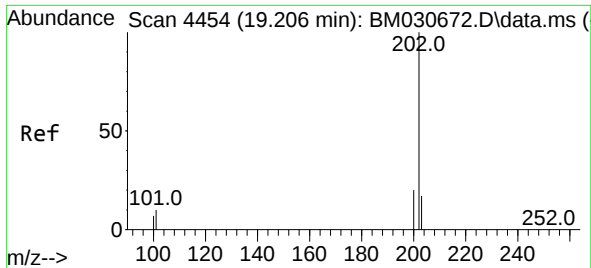

#19
Fluoranthene
Concen: 0.025 ng/ul
RT: 19.203 min Scan# 4453
Delta R.T. -0.008 min
Lab File: BM030683.D
Acq: 29 Jun 2021 10:02

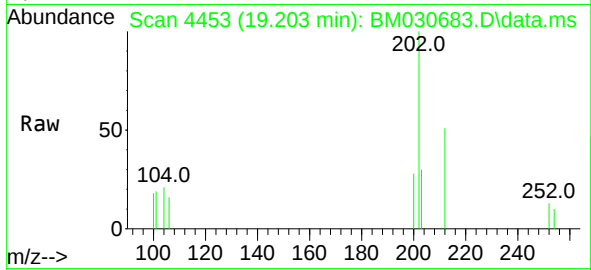

Tgt Ion:202 Resp: 1082
Ion Ratio Lower Upper
202 100
101 19.3 8.7 13.1#
100 17.9 6.6 9.8#

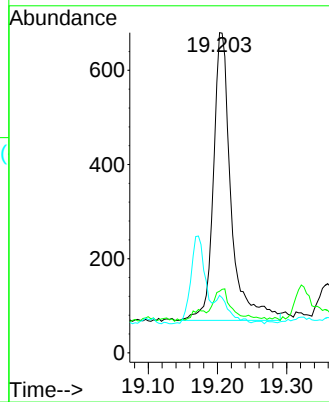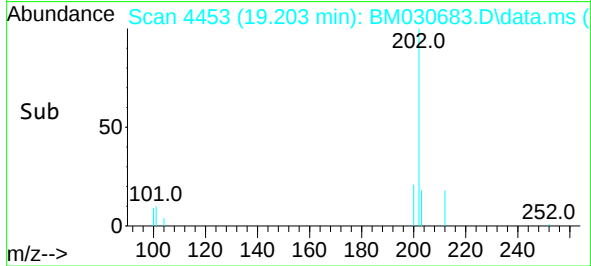

Instrument :
BNA_M
ClientSampleId :
JLX83

Manual Integrations
APPROVED

mohammad
6/30/2021 10:24:40 AM