

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035731.D
 Acq On : 28 Jun 2022 19:25
 Operator : CG/JU
 Sample : N3401-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 29 04:27:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 04:24:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	2142	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.578	136	6901	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.422	164	3713	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.18
17) Chrysene-d12	21.374	240	6514	0.400	ng/ul	# 0.00
23) Perylene-d12	23.689	264	8189	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	13041	4.486	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.211	152	3317	0.307	ng/ul	0.01
18) Fluoranthene-d10	19.205	212	7442	0.339	ng/ul	0.00
Target Compounds						
					Qvalue	
21) Benzo(a)anthracene	21.368	228	590	0.026	ng/ul#	31
22) Chrysene	21.418	228	924	0.032	ng/ul#	46
24) Benzo(b)fluoranthene	22.984	252	1368	0.039	ng/ul#	1
25) Benzo(k)fluoranthene	23.031	252	1192	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.517	252	2712	0.076	ng/ul#	29
27) Indeno(1,2,3-cd)pyrene	26.172	276	921	0.024	ng/ul#	45
28) Dibenzo(a,h)anthracene	26.165	278	743	0.024	ng/ul#	1
29) Benzo(g,h,i)perylene	26.879	276	895	0.025	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035731.D
Acq On : 28 Jun 2022 19:25
Operator : CG/JU
Sample : N3401-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 29 04:27:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 04:24:18 2022
Response via : Initial Calibration

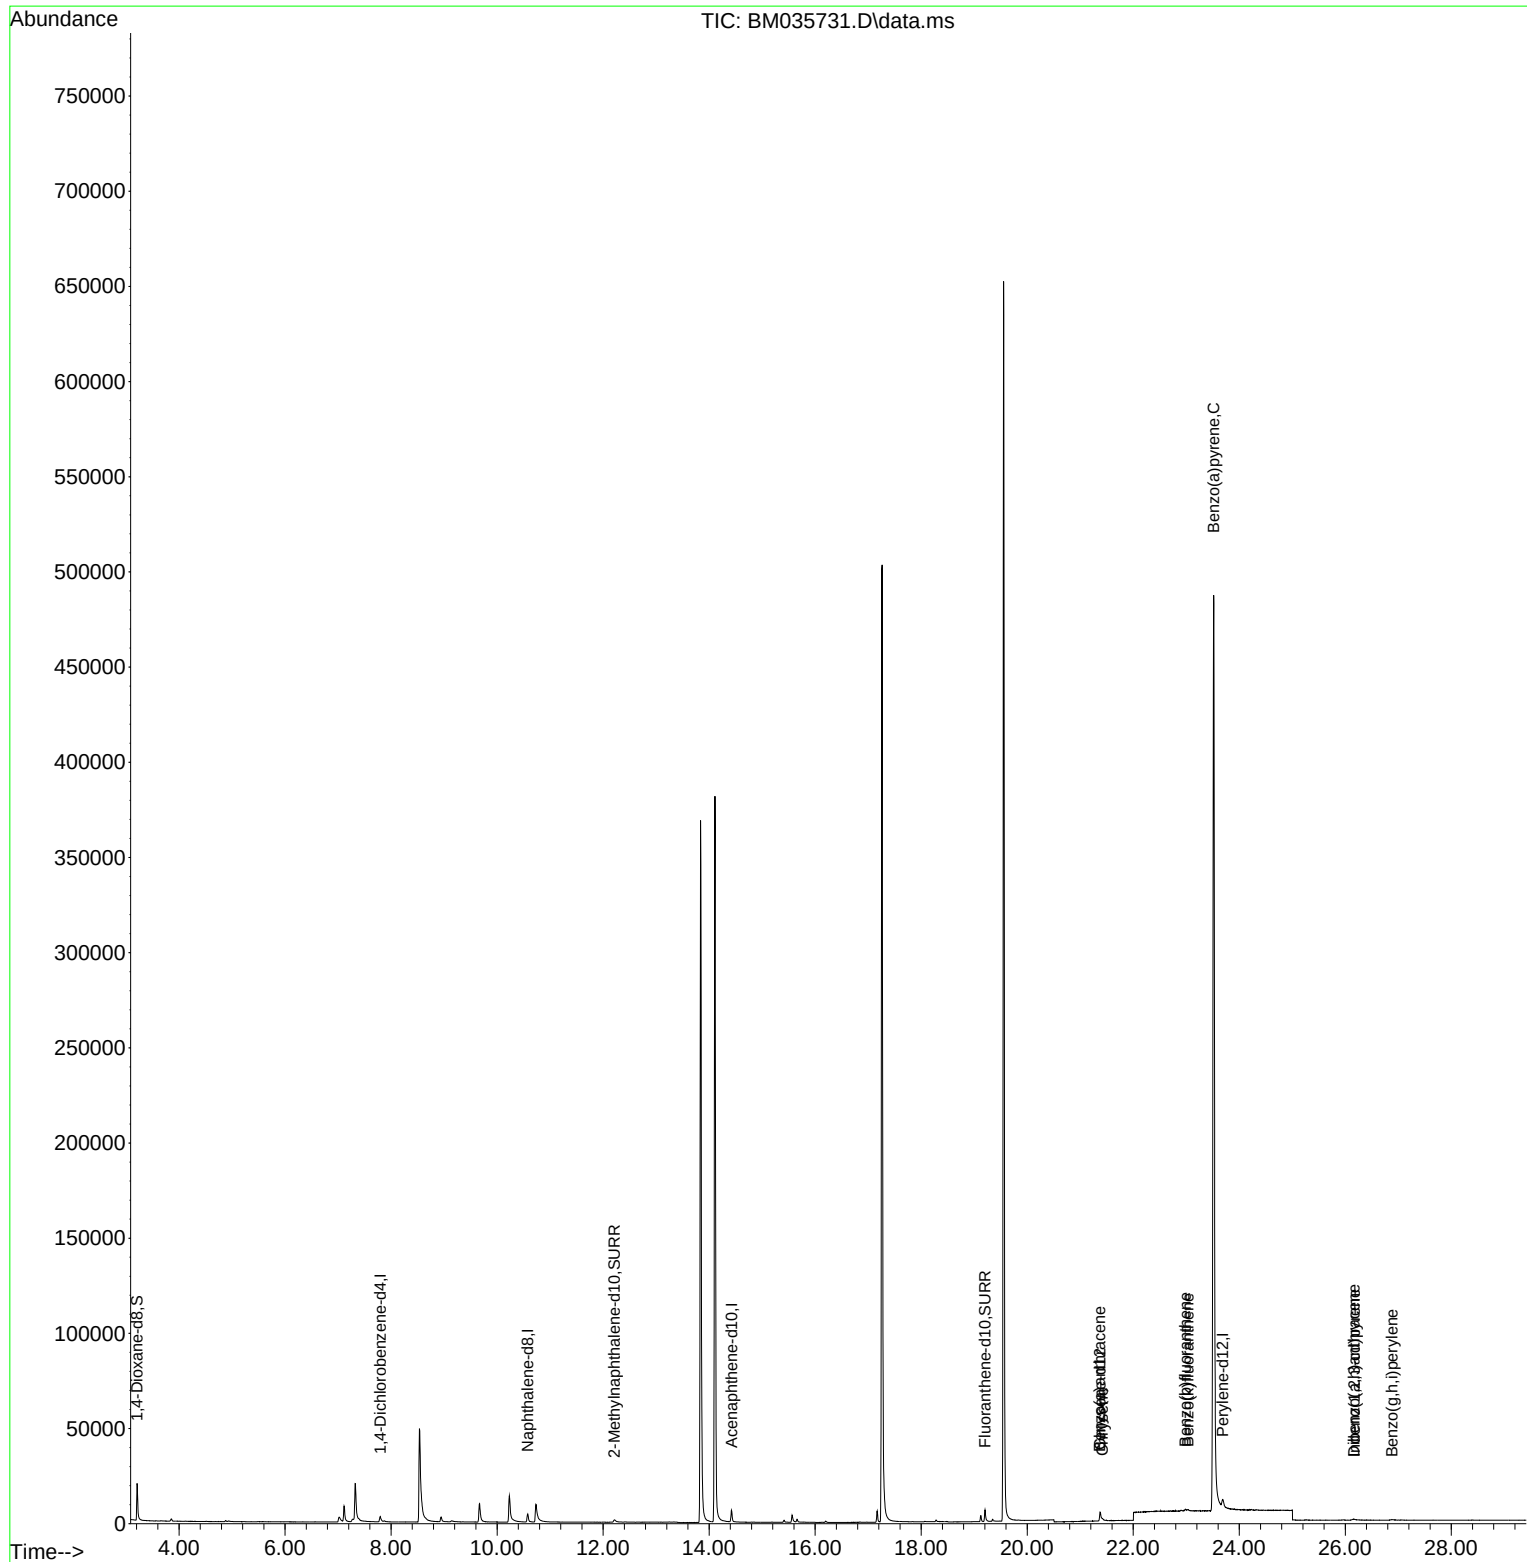

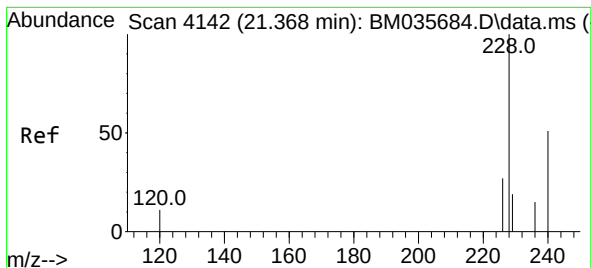

#21

Benzo(a)anthracene

Concen: 0.026 ng/u1

RT: 21.368 min Scan# 4142

Delta R.T. 0.009 min


Lab File: BM035731.D

Acq: 28 Jun 2022 19:25



Instrument :

BNA_M

ClientSampleId :

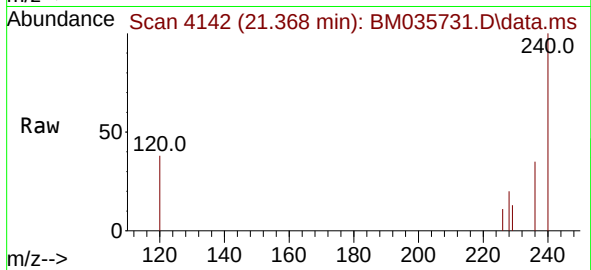

Tgt Ion:	228	Resp:	590
Ion	Ratio	Lower	Upper
228	100		
229	63.8	16.2	24.2#
226	54.7	22.5	33.7#

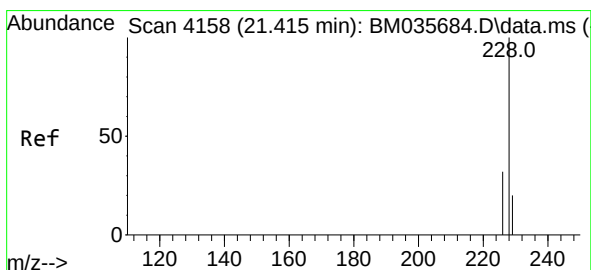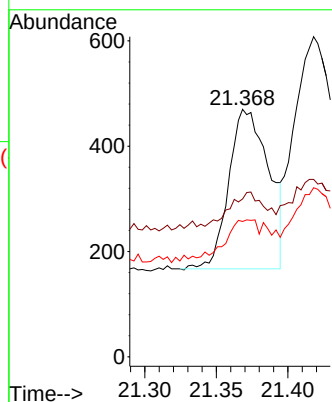

#22

Chrysene

Concen: 0.032 ng/u1




RT: 21.418 min Scan# 4159


Delta R.T. 0.006 min

Lab File: BM035731.D

Acq: 28 Jun 2022 19:25

Tgt Ion:	228	Resp:	924
Ion	Ratio	Lower	Upper
228	100		
226	52.8	24.6	37.0#
229	55.4	16.4	24.6#


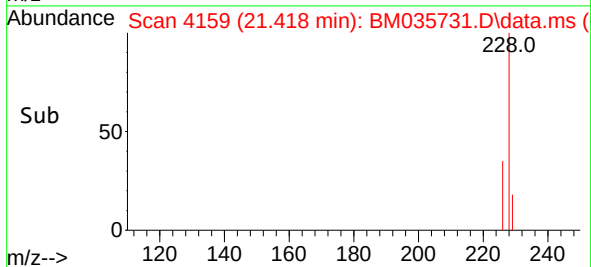
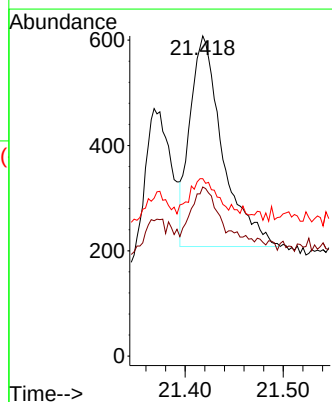
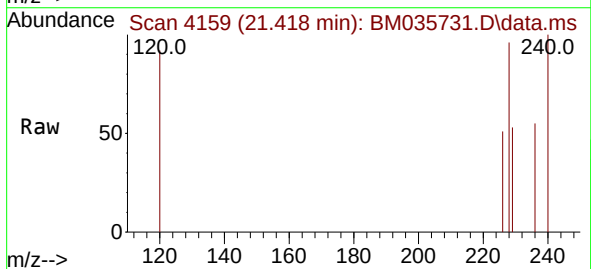


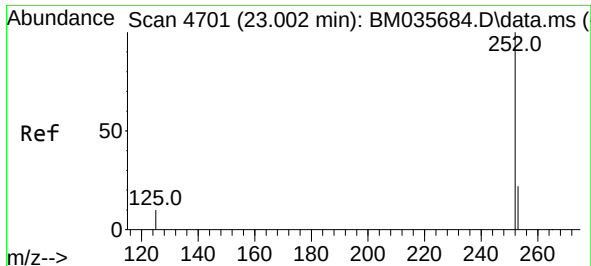

#24
Benzo(b)fluoranthene
Concen: 0.039 ng/ul
RT: 22.984 min Scan# 4701
Delta R.T. -0.012 min
Lab File: BM035731.D
Acq: 28 Jun 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:252 Resp: 1368
Ion Ratio Lower Upper
252 100
253 98.9 0.0 61.4#
125 82.9 0.0 42.6#

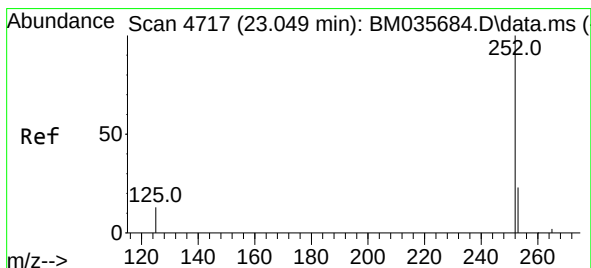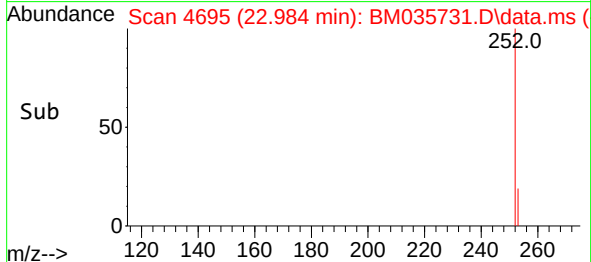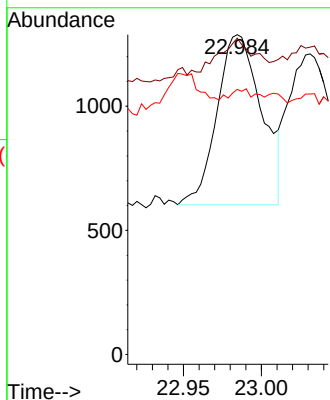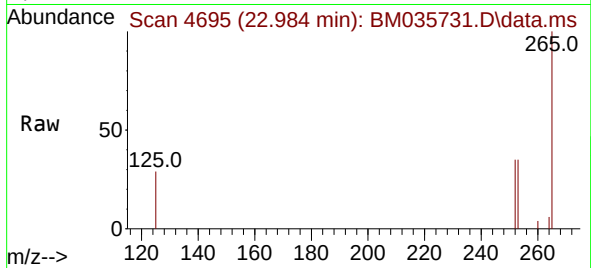

#25
Benzo(k)fluoranthene
Concen: 0.033 ng/ul
RT: 23.031 min Scan# 4711
Delta R.T. -0.012 min
Lab File: BM035731.D
Acq: 28 Jun 2022 19:25


Tgt Ion:252 Resp: 1192
Ion Ratio Lower Upper
252 100
253 102.2 25.2 37.8#
125 86.6 18.3 27.5#

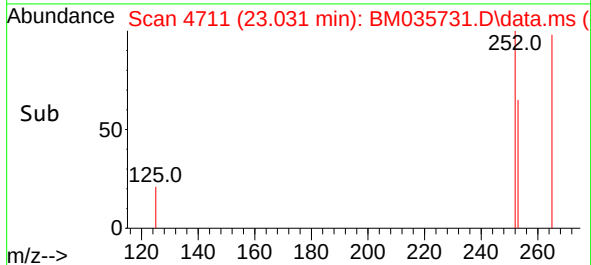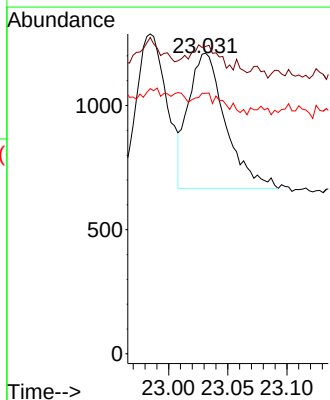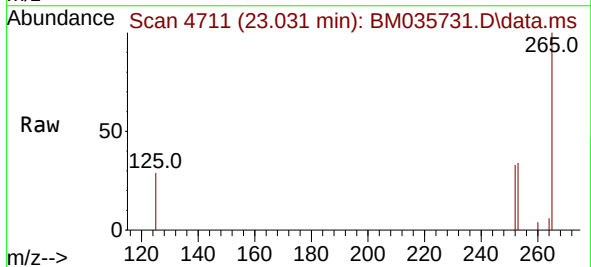



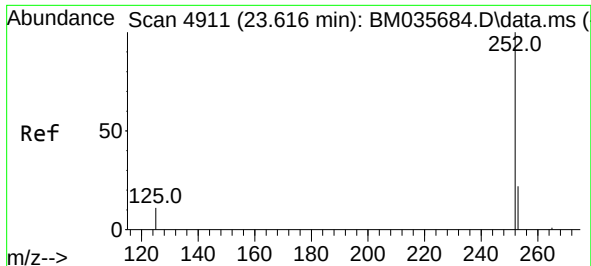


#26
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 23.517 min Scan# 4911
Delta R.T. -0.088 min
Lab File: BM035731.D
Acq: 28 Jun 2022 19:25

Instrument :
BNA_M
ClientSampleId :



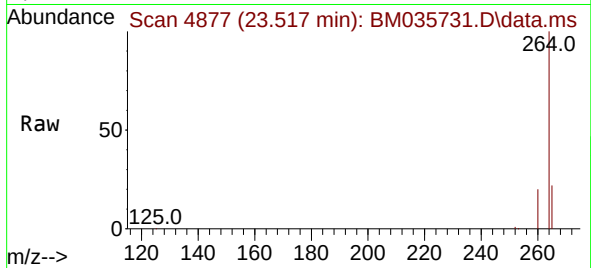



Tgt Ion:252 Resp: 2712
Ion Ratio Lower Upper
252 100
253 79.9 29.7 44.5#
125 66.8 23.6 35.4#

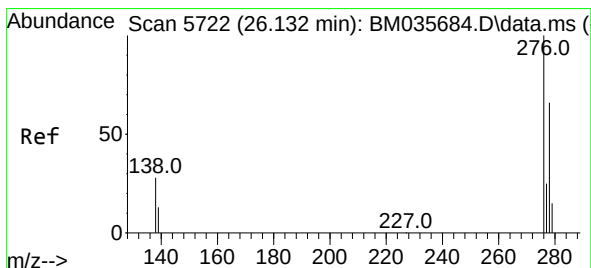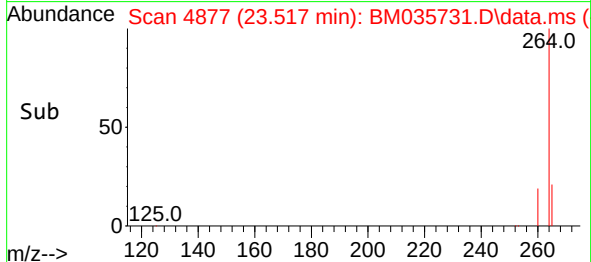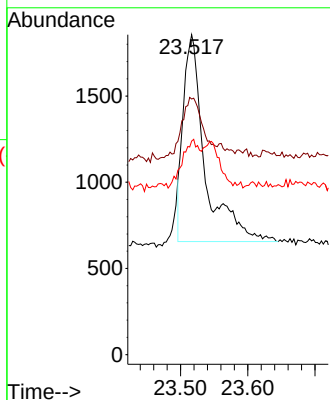

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.024 ng/ul
RT: 26.172 min Scan# 5734
Delta R.T. 0.060 min
Lab File: BM035731.D
Acq: 28 Jun 2022 19:25


Tgt Ion:276 Resp: 921
Ion Ratio Lower Upper
276 100
138 0.0 23.9 35.9#
227 1.5 0.1 0.1#

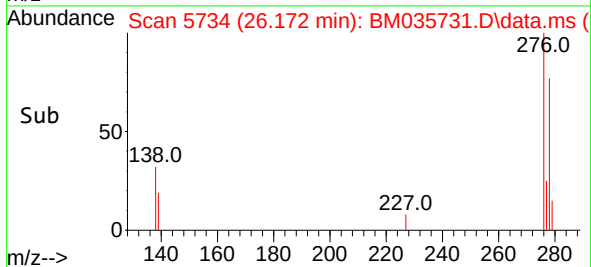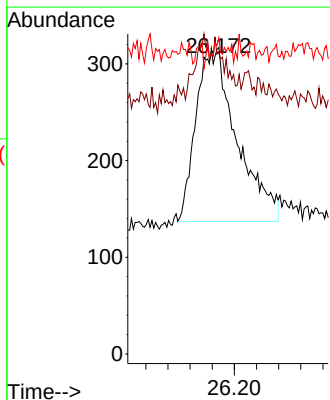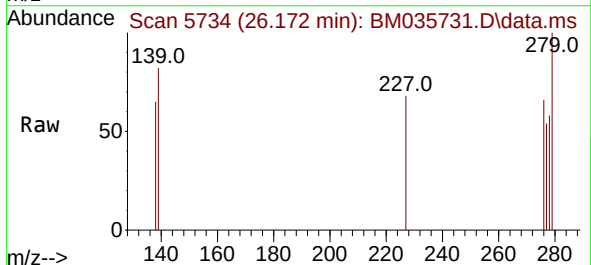



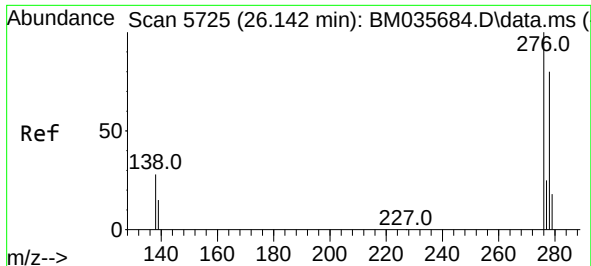


#28
 Dibenzo(a,h)anthracene
 Concen: 0.024 ng/ul
 RT: 26.165 min Scan# 51
 Delta R.T. 0.047 min
 Lab File: BM035731.D
 Acq: 28 Jun 2022 19:25

Instrument :
 BNA_M
 ClientSampleId :

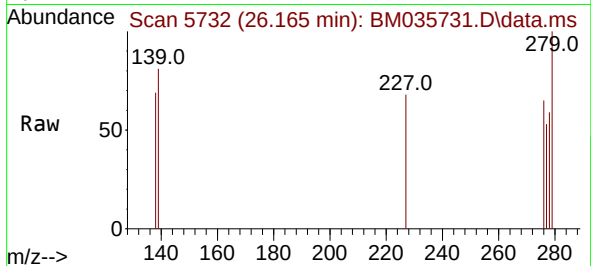

Tgt Ion:278 Resp: 743
 Ion Ratio Lower Upper
 278 100
 139 136.5 19.8 29.6#
 279 168.8 27.7 41.5#

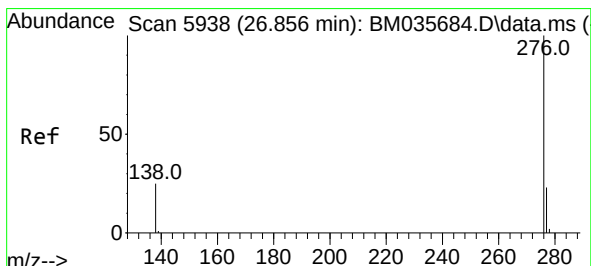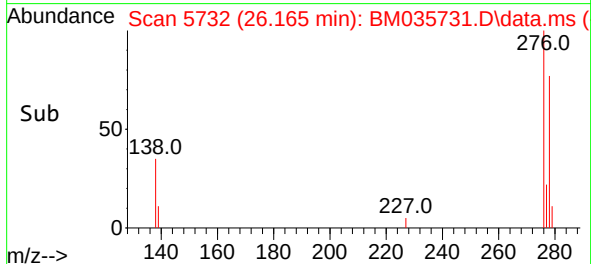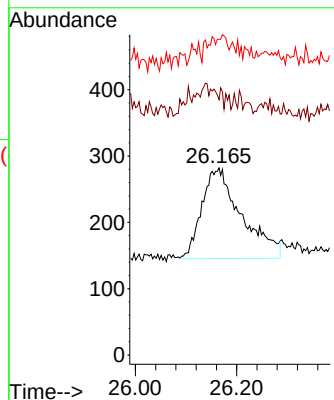

#29
 Benzo(g,h,i)perylene
 Concen: 0.025 ng/ul
 RT: 26.879 min Scan# 5945
 Delta R.T. 0.030 min
 Lab File: BM035731.D
 Acq: 28 Jun 2022 19:25

Tgt Ion:276 Resp: 895
 Ion Ratio Lower Upper
 276 100
 138 98.4 23.4 35.0#
 277 84.6 21.0 31.4#

