

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035740.D
 Acq On : 29 Jun 2022 01:36
 Operator : CG/JU
 Sample : PB145714BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 29 05:19:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 05:17:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	3893	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.572	136	13122	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.418	164	5182	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.389	240	11329	0.400	ng/ul	# 0.02
23) Perylene-d12	23.683	264	16673	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	34045	6.444	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	4925	0.240	ng/ul	0.00
18) Fluoranthene-d10	19.205	212	10087	0.264	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.554	202	1794	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.514	252	3516	0.048	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035740.D
Acq On : 29 Jun 2022 01:36
Operator : CG/JU
Sample : PB145714BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 29 05:19:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 05:17:22 2022
Response via : Initial Calibration




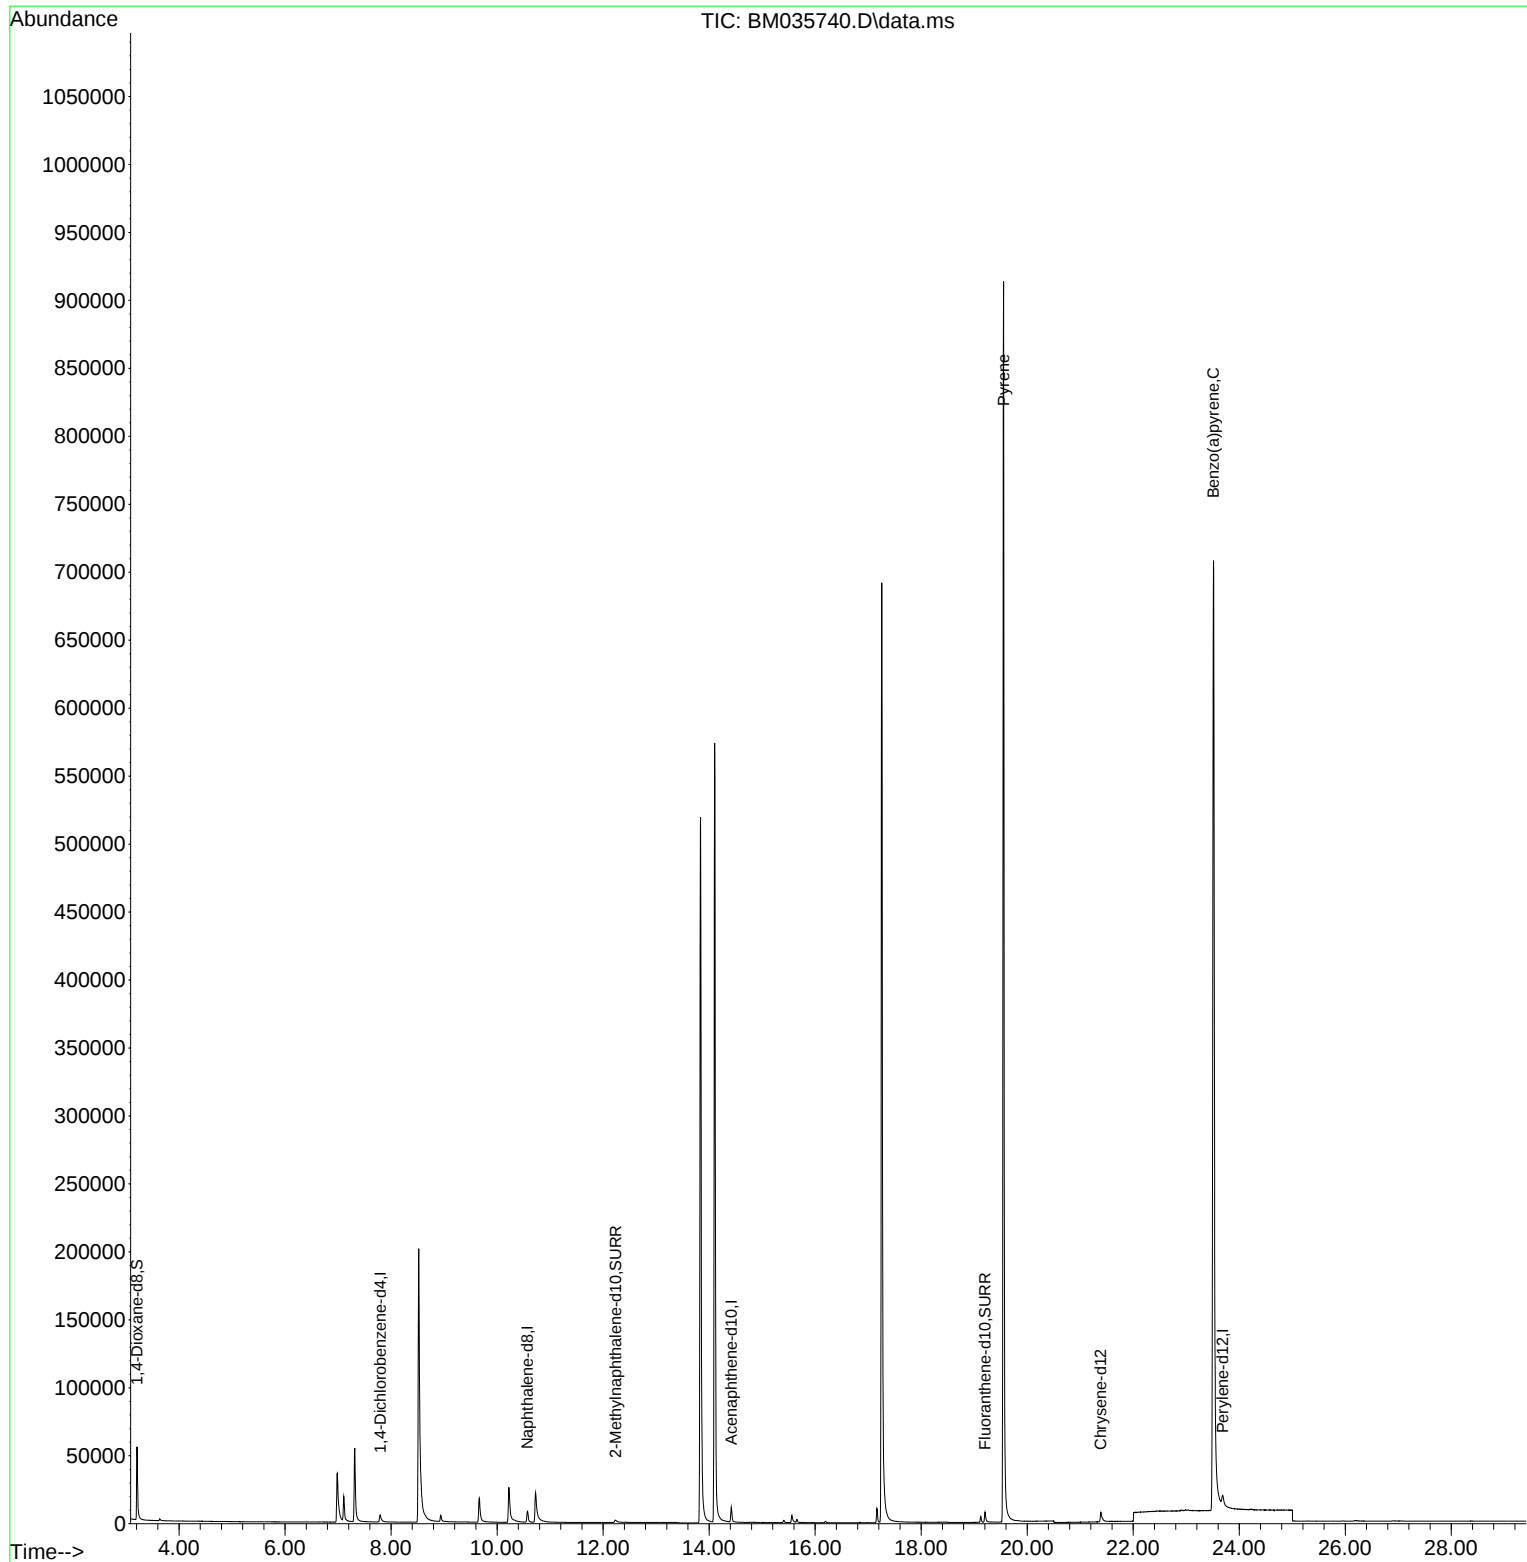


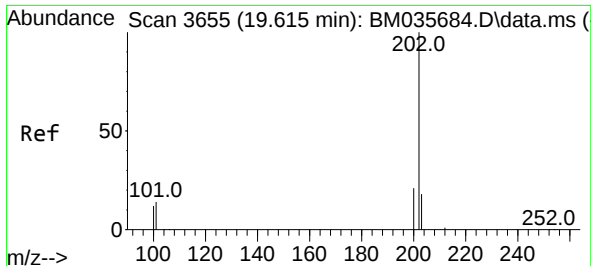

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.554 min Scan# 30
Delta R.T. -0.057 min
Lab File: BM035740.D
Acq: 29 Jun 2022 01:36

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1794
Ion Ratio Lower Upper
202 100
101 151.1 12.0 18.0#
100 1013.0 9.8 14.6#

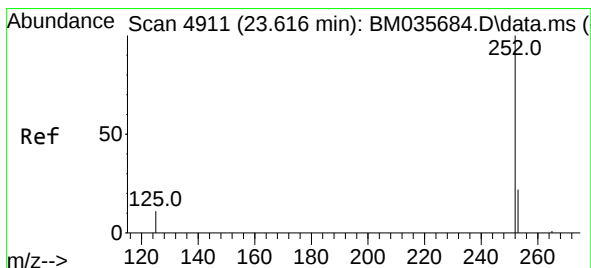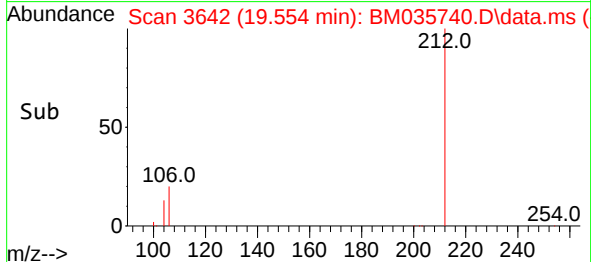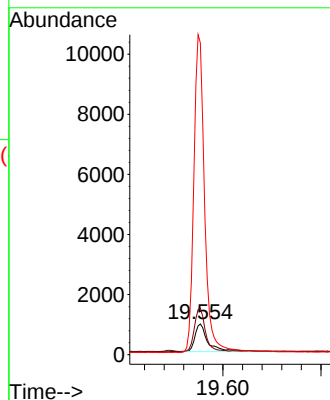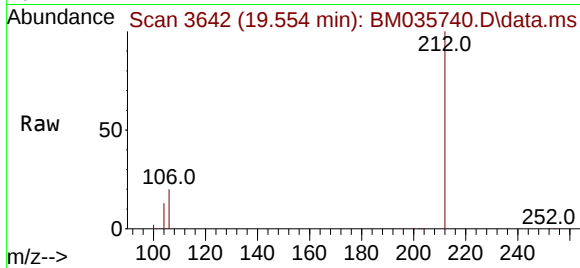

#26
Benzo(a)pyrene
Concen: 0.048 ng/ul
RT: 23.514 min Scan# 4876
Delta R.T. -0.087 min
Lab File: BM035740.D
Acq: 29 Jun 2022 01:36

Tgt Ion:252 Resp: 3516
Ion Ratio Lower Upper
252 100
253 75.9 29.7 44.5#
125 67.1 23.6 35.4#

