

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035742.D
 Acq On : 29 Jun 2022 02:50
 Operator : CG/JU
 Sample : PB145659BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 29 05:19:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 05:17:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.791	152	4813	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.573	136	17285	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.418	164	7554	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.389	240	12006	0.400	ng/ul	# 0.02
23) Perylene-d12	23.686	264	16408	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	41021	6.280	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	7090	0.262	ng/ul	0.00
18) Fluoranthene-d10	19.201	212	12918	0.319	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.554	202	2104	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.511	252	3442	0.048	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035742.D
Acq On : 29 Jun 2022 02:50
Operator : CG/JU
Sample : PB145659BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jun 29 05:19:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 05:17:22 2022
Response via : Initial Calibration

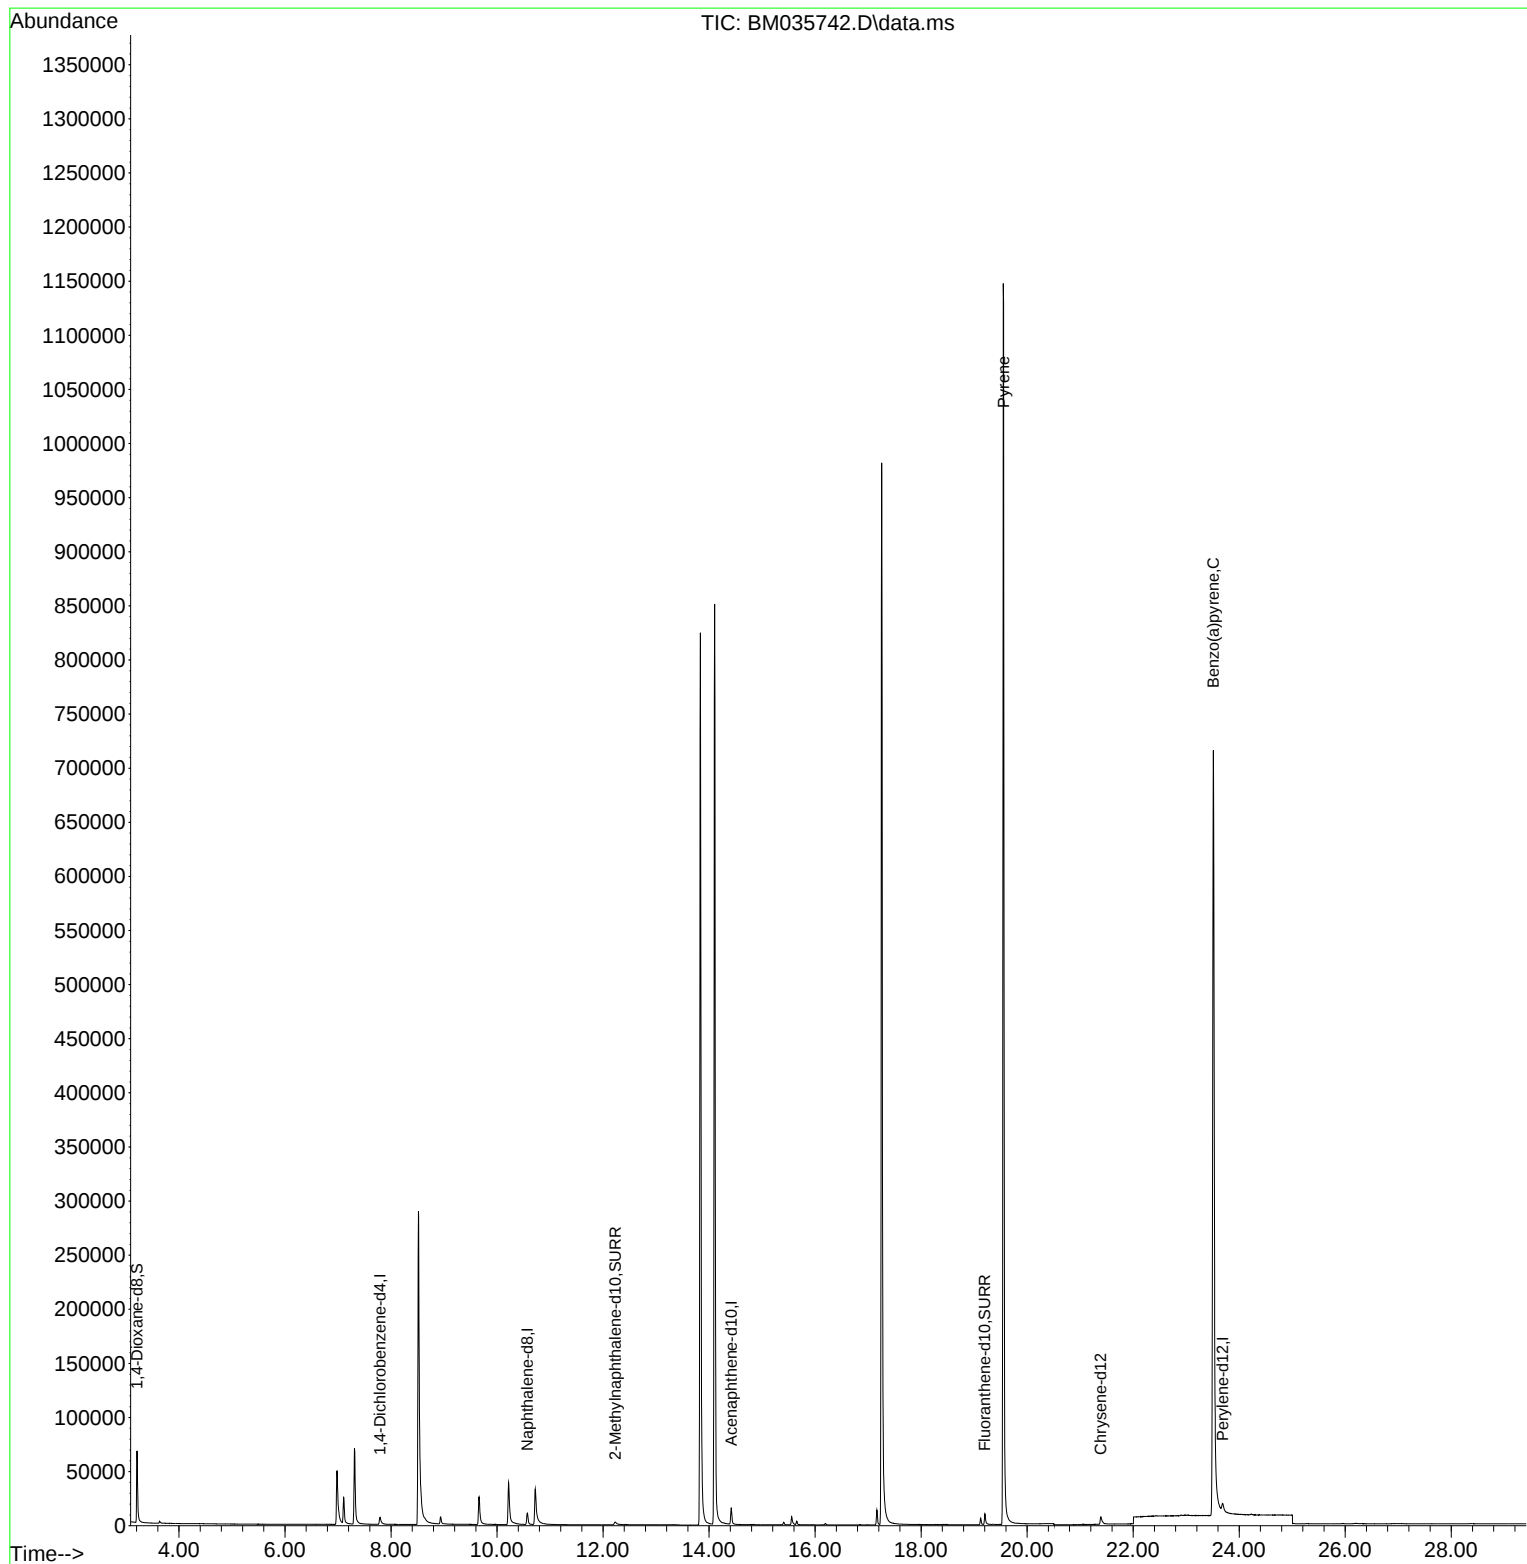



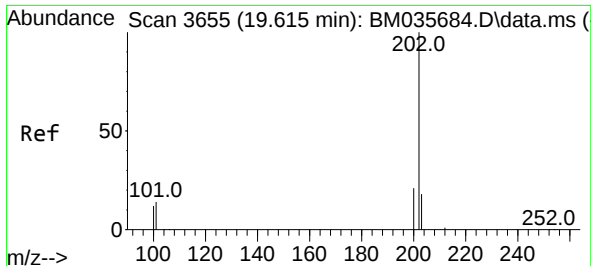


#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.554 min Scan# 30
Delta R.T. -0.056 min
Lab File: BM035742.D
Acq: 29 Jun 2022 02:50

Instrument :
BNA_M
ClientSampleId :

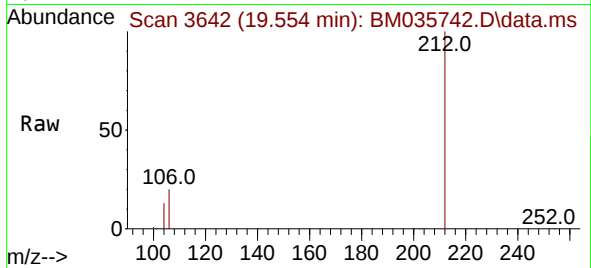

Tgt Ion:202 Resp: 2104
Ion Ratio Lower Upper
202 100
101 148.8 12.0 18.0#
100 976.2 9.8 14.6#

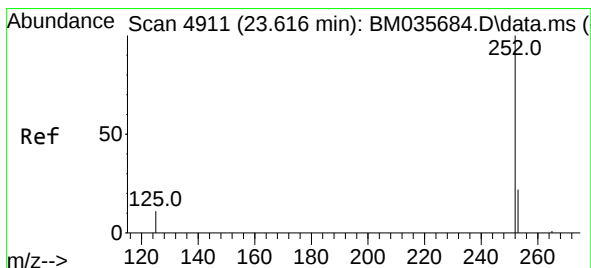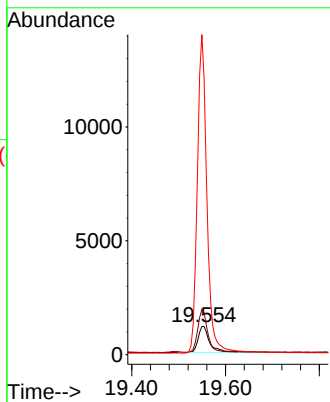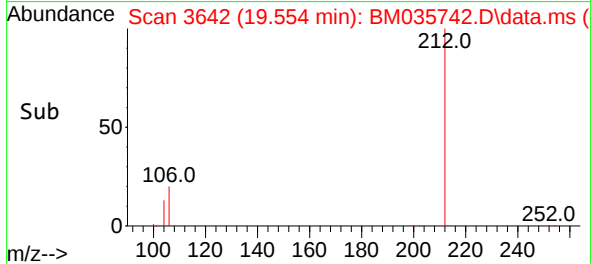

#26
Benzo(a)pyrene
Concen: 0.048 ng/ul
RT: 23.511 min Scan# 4875
Delta R.T. -0.090 min
Lab File: BM035742.D
Acq: 29 Jun 2022 02:50

Tgt Ion:252 Resp: 3442
Ion Ratio Lower Upper
252 100
253 74.6 29.7 44.5#
125 66.7 23.6 35.4#

