

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035743.D
 Acq On : 29 Jun 2022 03:27
 Operator : CG/JU
 Sample : PB145703BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 29 05:19:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 05:17:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	4038	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.572	136	13208	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.419	164	5471	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.391	240	10595	0.400	ng/ul	# 0.02
23) Perylene-d12	23.685	264	15580	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	36652	6.688	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	5429	0.262	ng/ul	0.00
18) Fluoranthene-d10	19.202	212	10531	0.295	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.550	202	1857	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.510	252	3200	0.047	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035743.D
Acq On : 29 Jun 2022 03:27
Operator : CG/JU
Sample : PB145703BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 29 05:19:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 05:17:22 2022
Response via : Initial Calibration




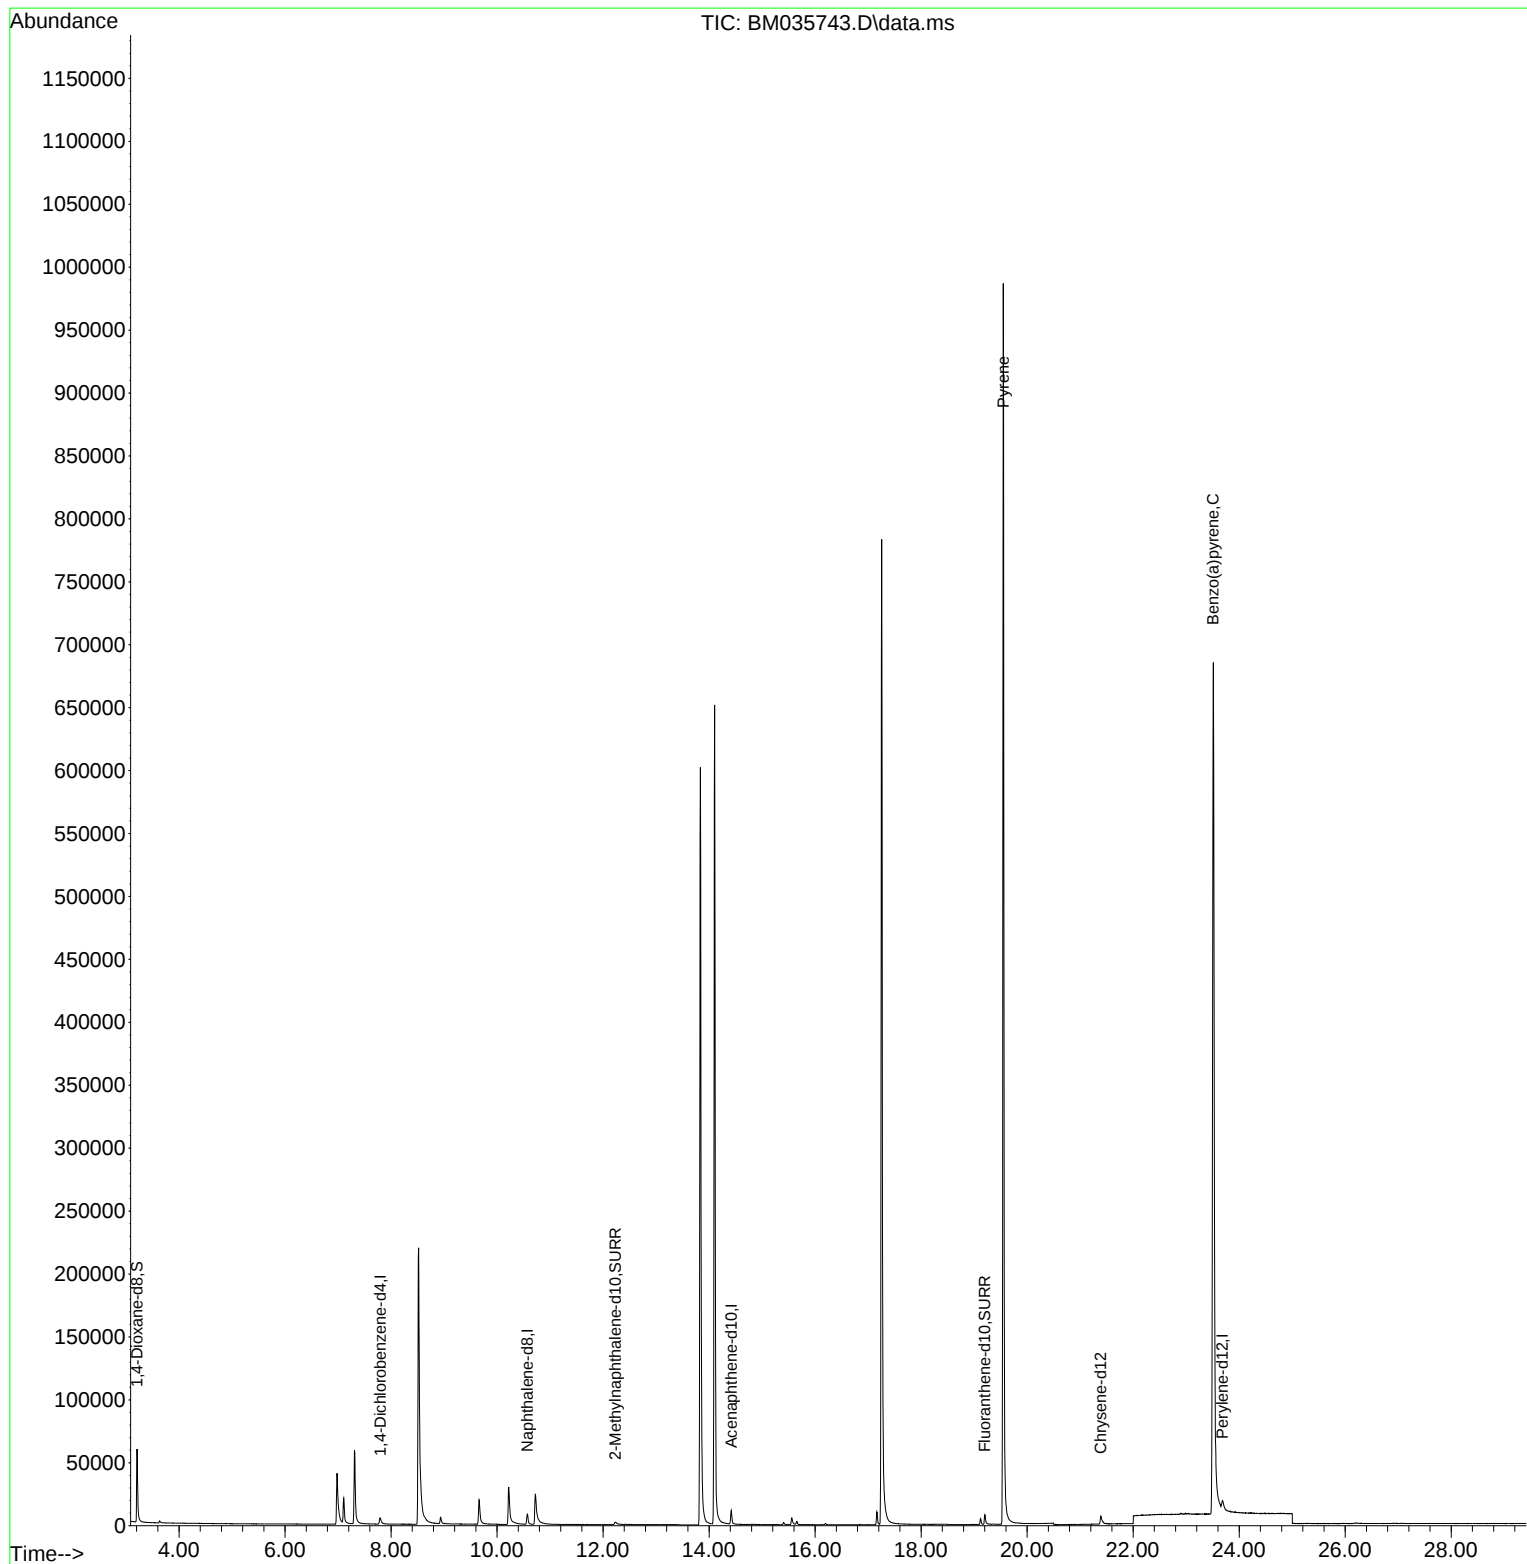


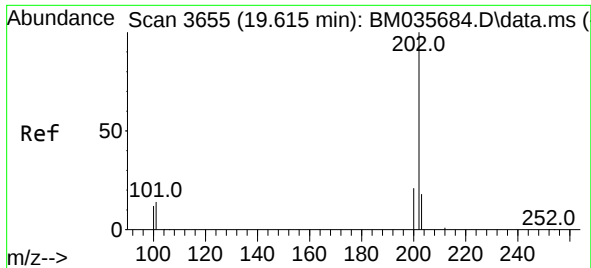

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.550 min Scan# 30
Delta R.T. -0.060 min
Lab File: BM035743.D
Acq: 29 Jun 2022 03:27

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1857
Ion Ratio Lower Upper
202 100
101 151.3 12.0 18.0#
100 1025.1 9.8 14.6#

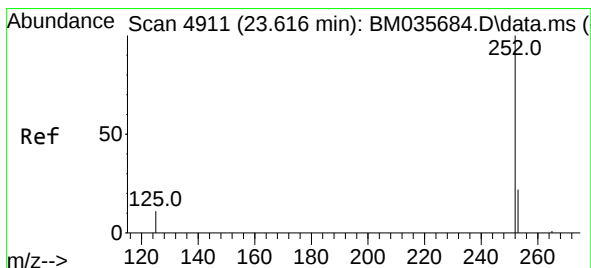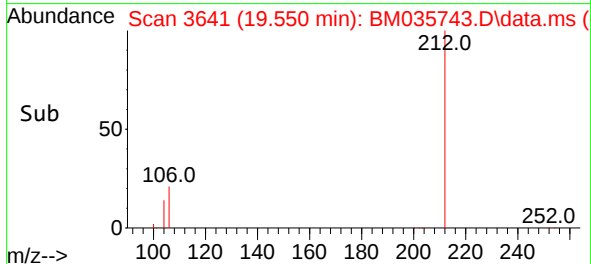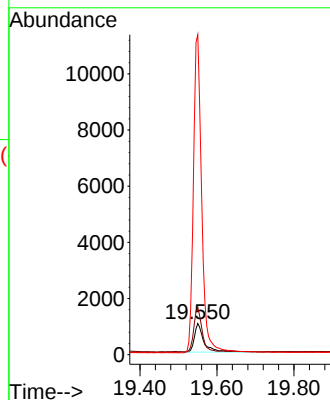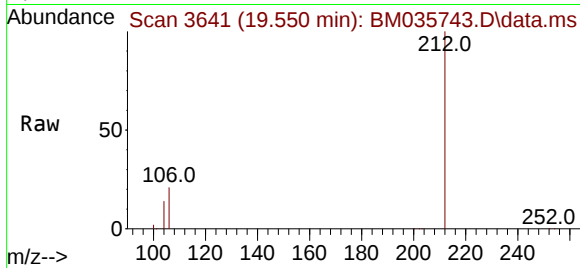

#26
Benzo(a)pyrene
Concen: 0.047 ng/ul
RT: 23.510 min Scan# 4875
Delta R.T. -0.091 min
Lab File: BM035743.D
Acq: 29 Jun 2022 03:27

Tgt Ion:252 Resp: 3200
Ion Ratio Lower Upper
252 100
253 74.9 29.7 44.5#
125 67.4 23.6 35.4#

