




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035767.D
 Acq On : 29 Jun 2022 18:53
 Operator : CG/JU
 Sample : N3374-03MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S6MSDA

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:00:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

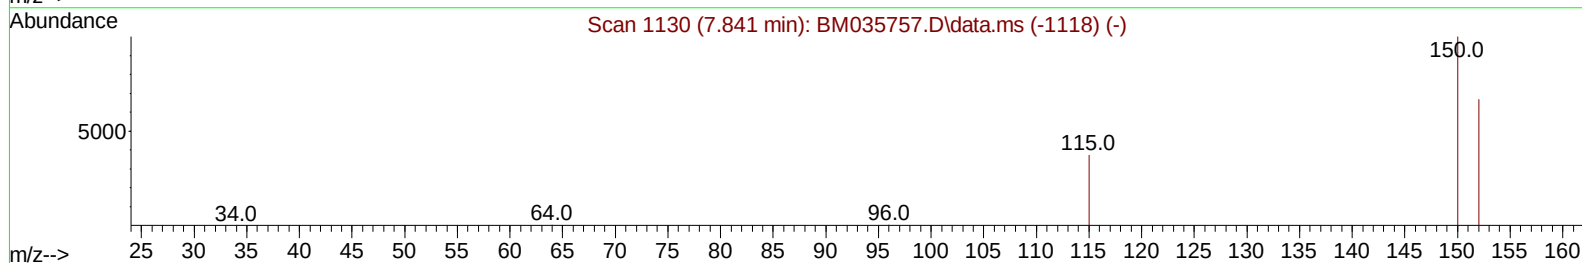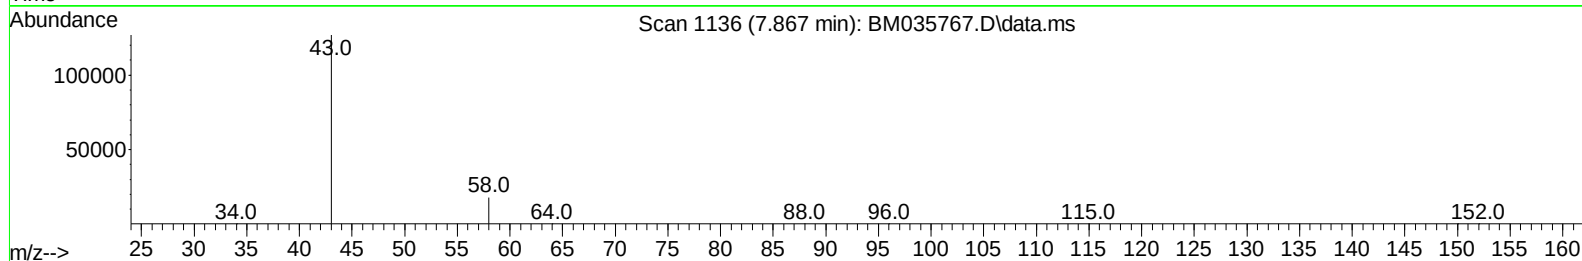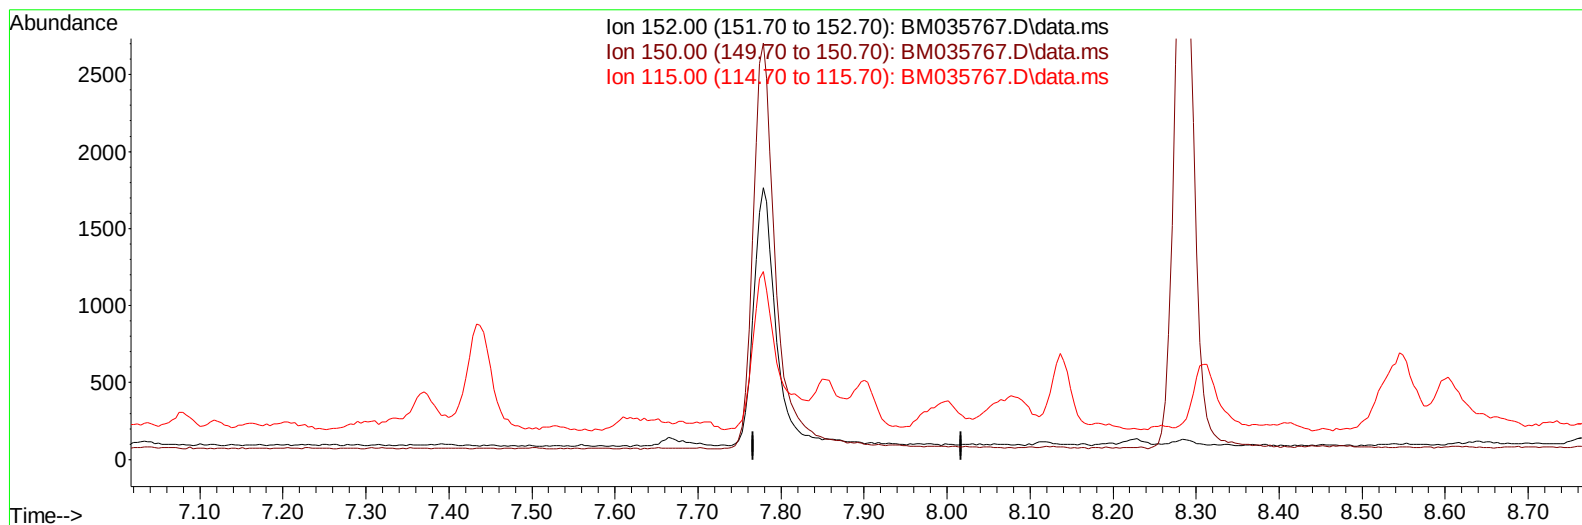

TIC: BM035767.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.867min (-7.867) 0.00 ng/ul

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	147.40	0.00#
115.00	74.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035767.D
Acq On : 29 Jun 2022 18:53
Operator : CG/JU
Sample : N3374-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S6MSDA

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:00:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

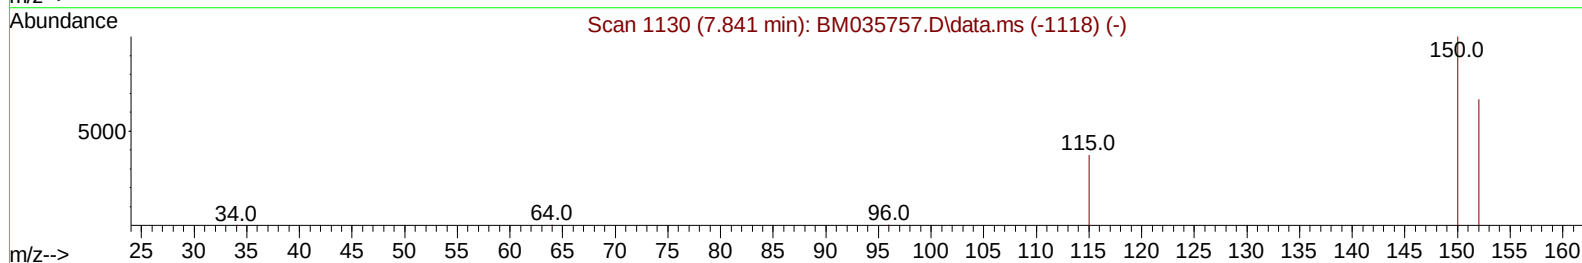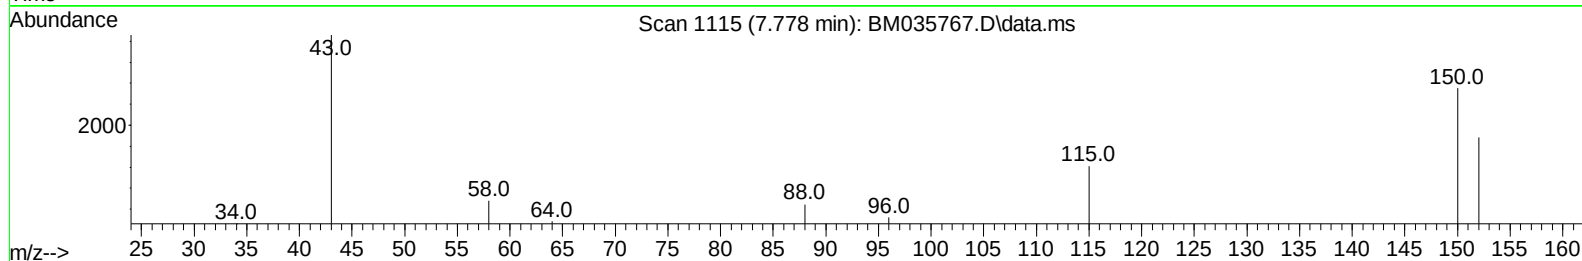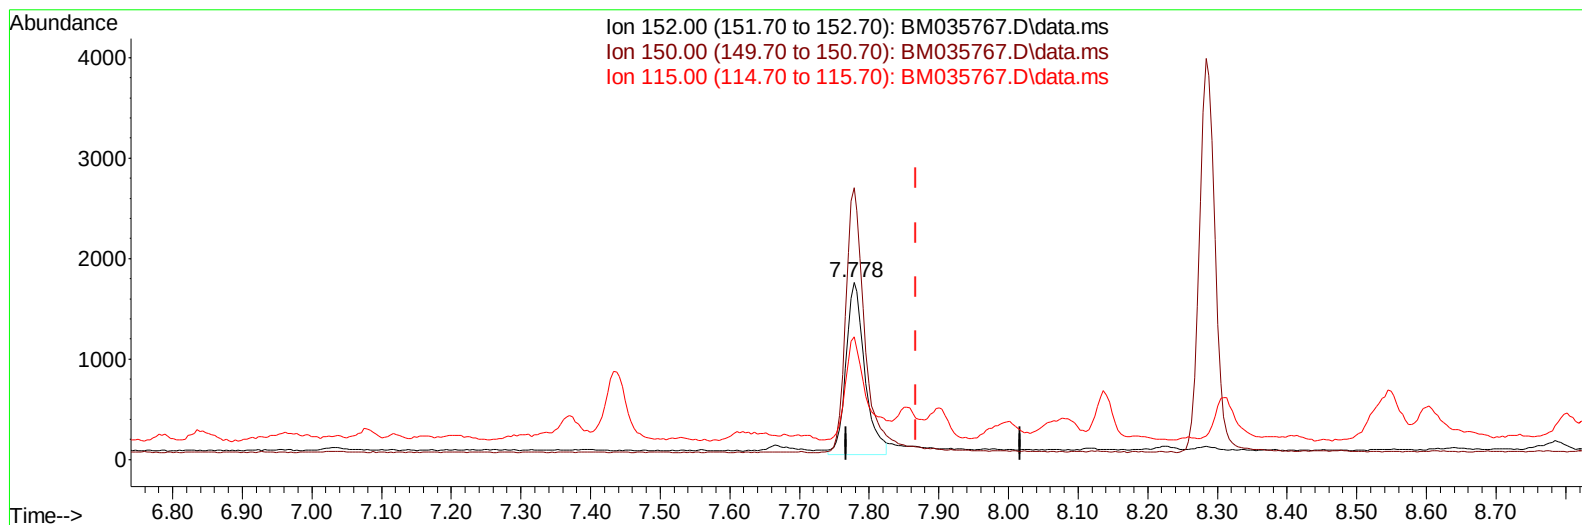

TIC: BM035767.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.778min (-0.089) 0.40 ng/ul m

response 3219

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	153.23
115.00	74.40	69.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035767.D
 Acq On : 29 Jun 2022 18:53
 Operator : CG/JU
 Sample : N3374-03MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S6MSDA

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:00:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

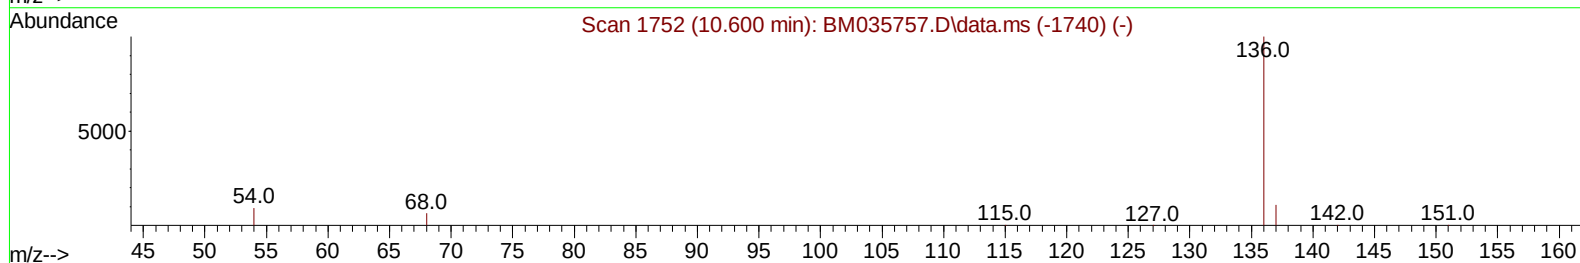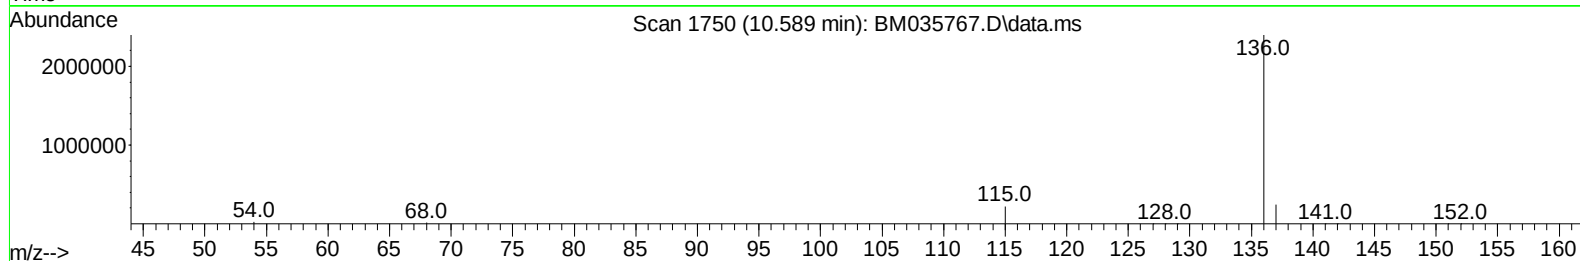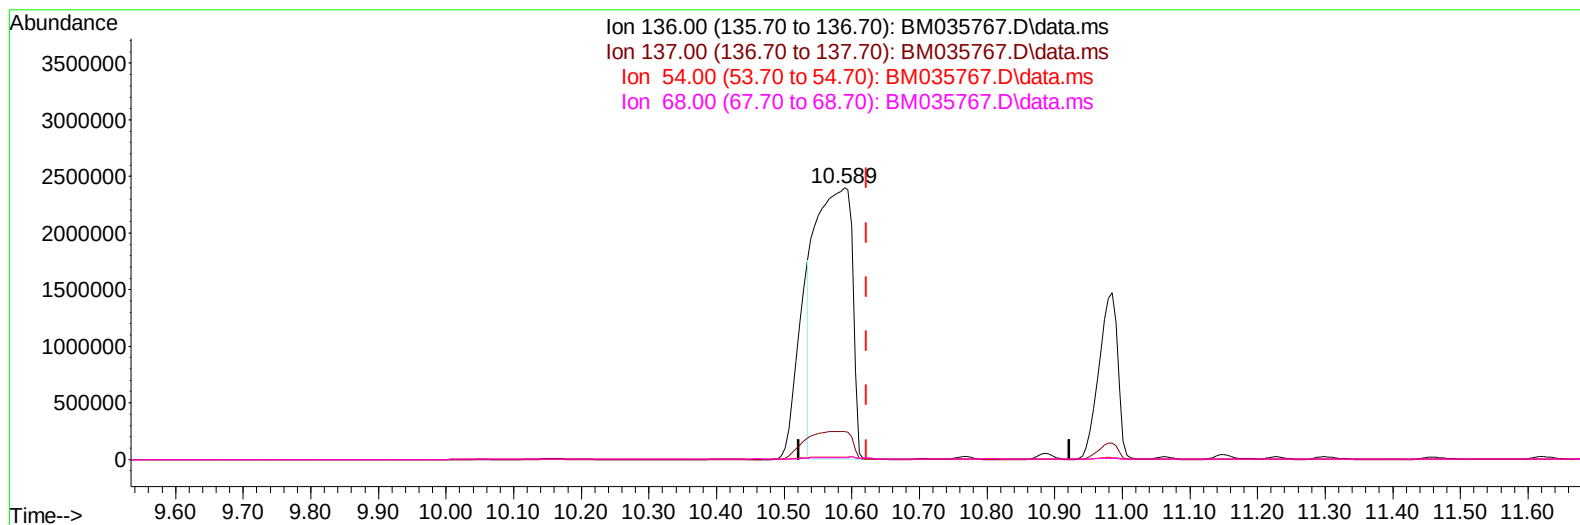

TIC: BM035767.D\data.ms

(4) Naphthalene-d8 (I)

10.589min (-0.033) 0.40 ng/u1

response 9125349

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	10.28
54.00	12.20	0.88#
68.00	8.00	0.57#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035767.D
Acq On : 29 Jun 2022 18:53
Operator : CG/JU
Sample : N3374-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S6MSDA

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:00:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

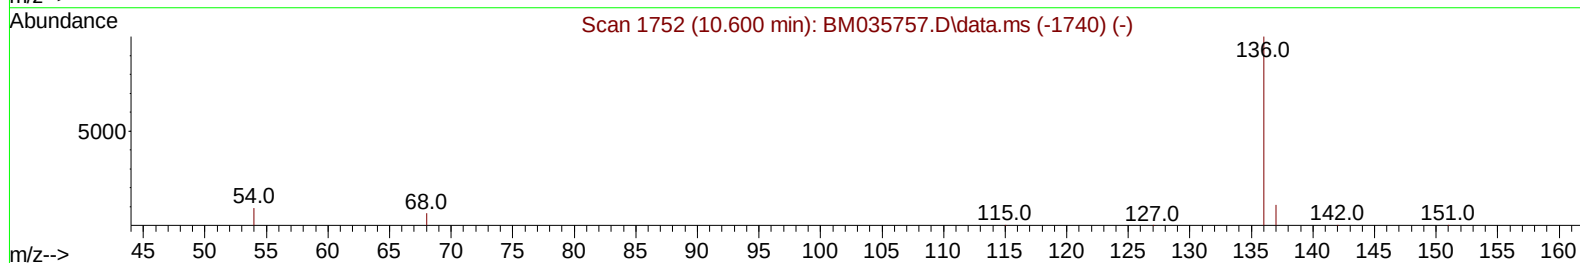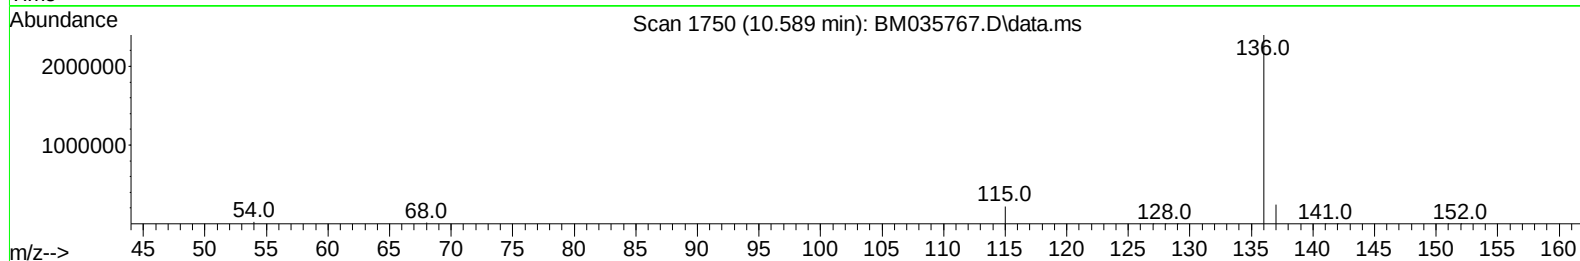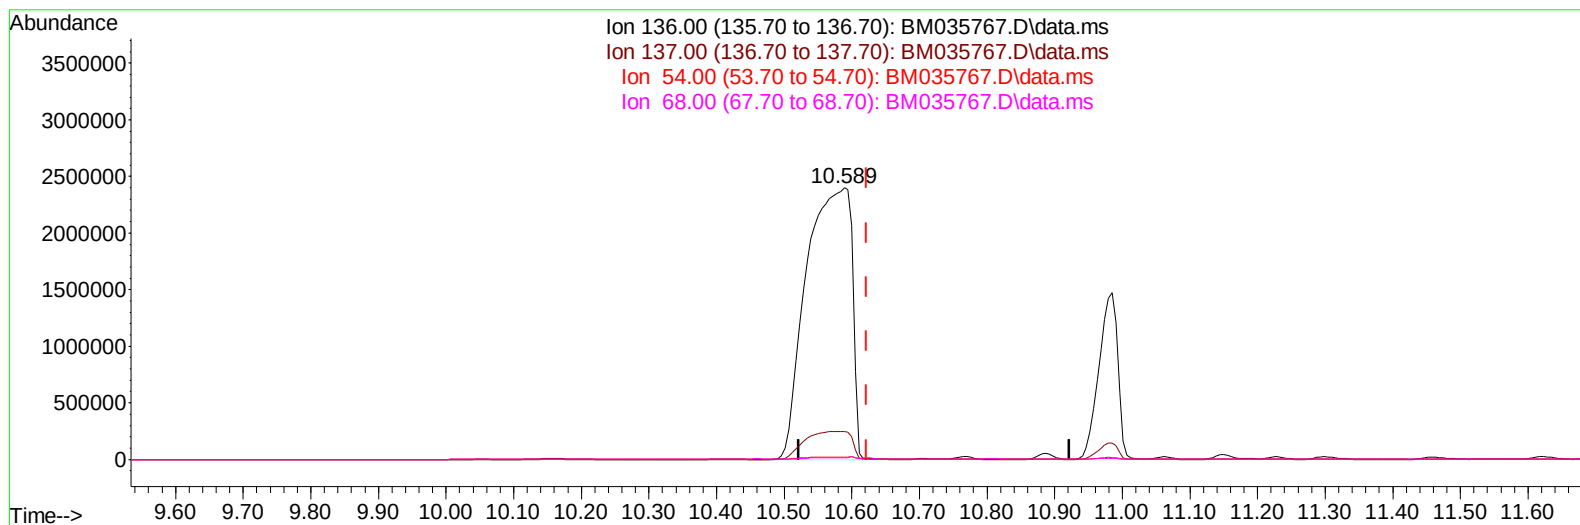

TIC: BM035767.D\data.ms

(4) Naphthalene-d8 (I)

10.589min (-0.033) 0.40 ng/ul m

response 11222354

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	10.28
54.00	12.20	0.88#
68.00	8.00	0.57#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035767.D
 Acq On : 29 Jun 2022 18:53
 Operator : CG/JU
 Sample : N3374-03MSD
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4S6MSDA

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 30 04:00:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.778	152		3219m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.589	136	11222354m		0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.418	164		7155	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.161	188		11655	0.400	ng/ul	#-0.03
17) Chrysene-d12	21.357	240		11709	0.400	ng/ul	#-0.02
23) Perylene-d12	23.677	264		12053	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.218	96		1282	0.293	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.167	152		11677	0.001	ng/ul	-0.06
18) Fluoranthene-d10	19.196	212		11575	0.293	ng/ul	-0.02
Target Compounds					Qvalue		
2) 1,4-Dioxane	3.247	88		19313	4.470	ng/ul#	1
11) Acenaphthene	14.478	153		32398	1.121	ng/ul	98
12) Fluorene	15.468	166		12711	0.382	ng/ul#	94
14) Pentachlorophenol	16.840	266		1034	0.562	ng/ul	97
15) Phenanthrene	17.204	178		23014	0.545	ng/ul#	90
16) Anthracene	17.296	178		25309	0.721	ng/ul#	90
19) Fluoranthene	19.224	202		21604	0.368	ng/ul#	88
20) Pyrene	19.587	202		20900	0.318	ng/ul#	89
21) Benzo(a)anthracene	21.339	228		15497	0.383	ng/ul#	80
22) Chrysene	21.392	228		16831	0.323	ng/ul#	81
24) Benzo(b)fluoranthene	22.973	252		17333	0.336	ng/ul	68
25) Benzo(k)fluoranthene	23.017	252		16775	0.318	ng/ul#	67
26) Benzo(a)pyrene	23.575	252		16601	0.314	ng/ul#	75
27) Indeno(1,2,3-cd)pyrene	26.084	276		19885	0.346	ng/ul#	97
28) Dibenzo(a,h)anthracene	26.088	278		16165	0.355	ng/ul#	70
29) Benzo(g,h,i)perylene	26.825	276		17387	0.328	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035767.D
Acq On : 29 Jun 2022 18:53
Operator : CG/JU
Sample : N3374-03MSD
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4S6MSDA

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:00:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

