




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

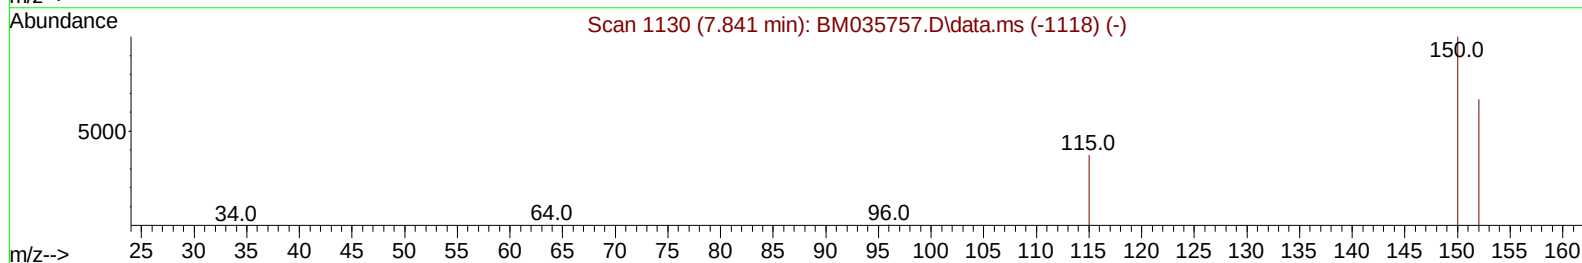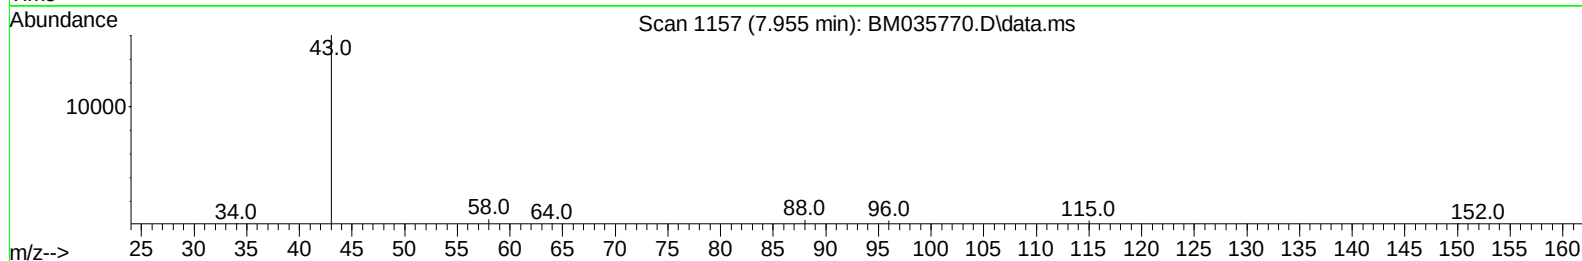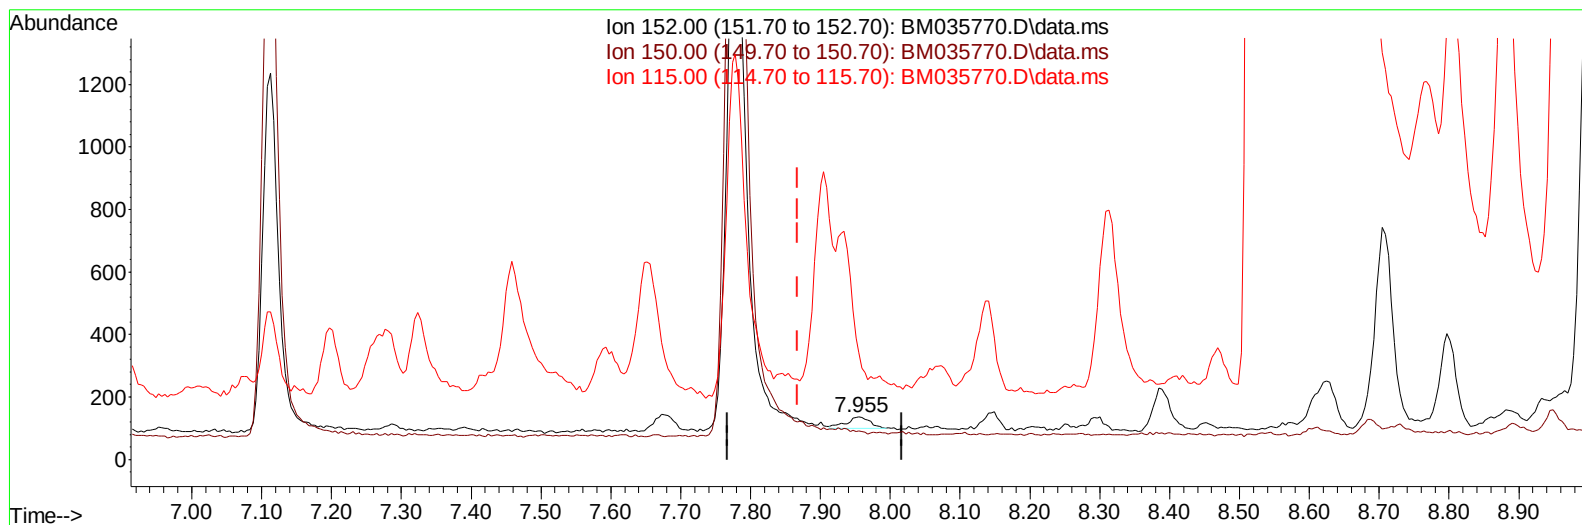

TIC: BM035770.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.955min (+ 0.088) 0.40 ng/ul

response 88

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	67.15#
115.00	74.40	250.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

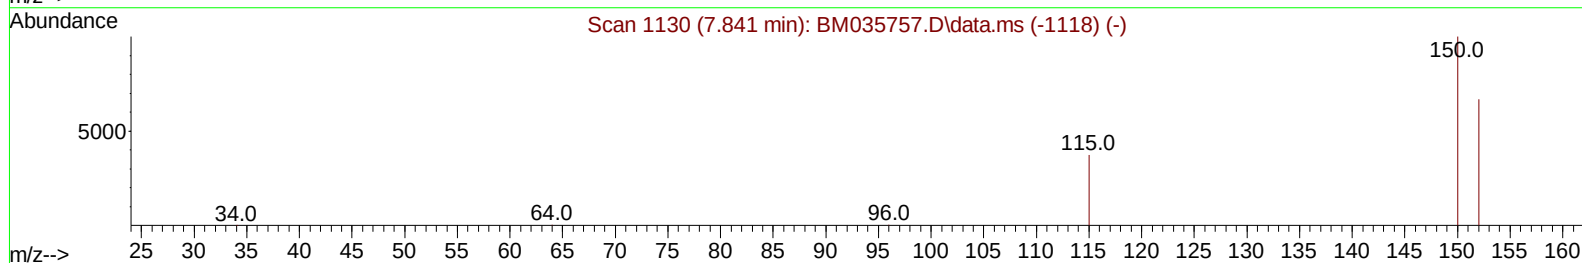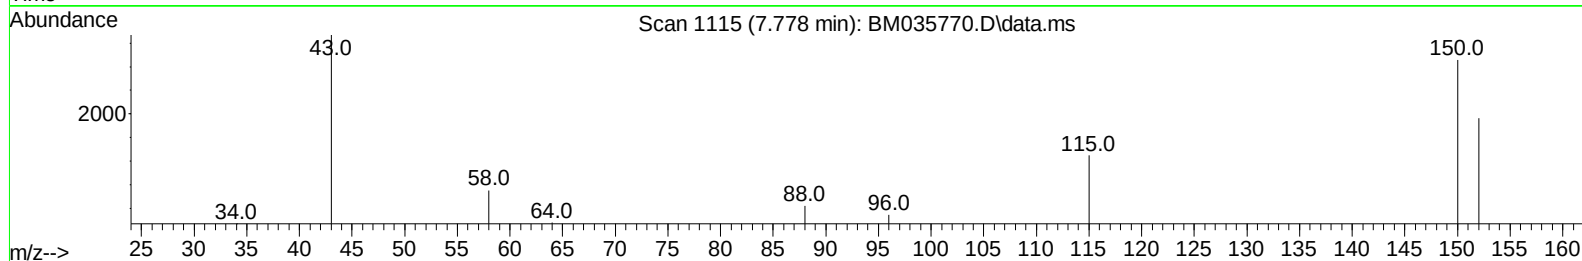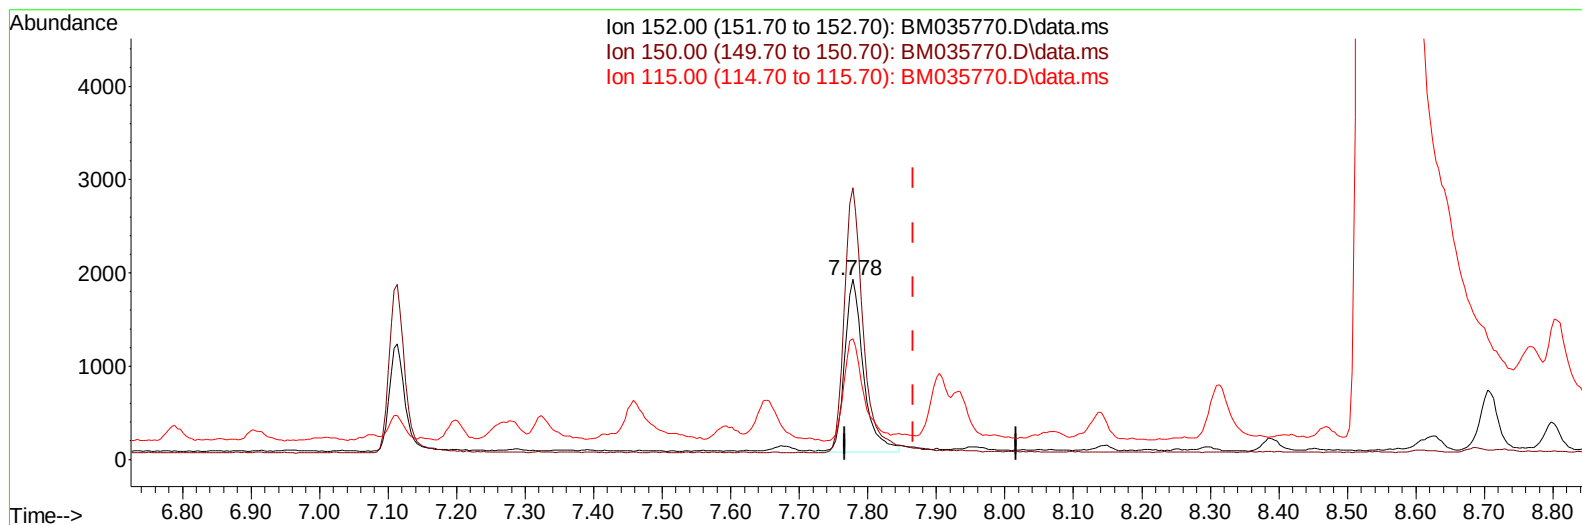

TIC: BM035770.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.778min (-0.089) 0.40 ng/ul m

response 3540

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	150.86
115.00	74.40	67.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

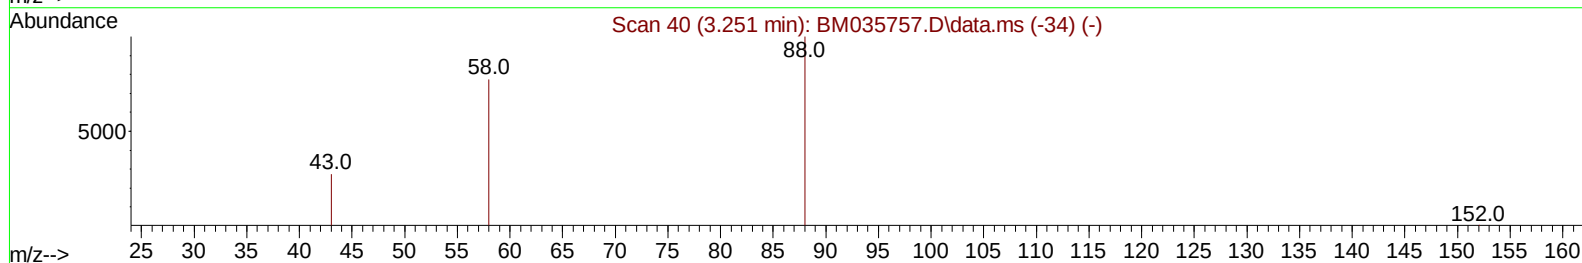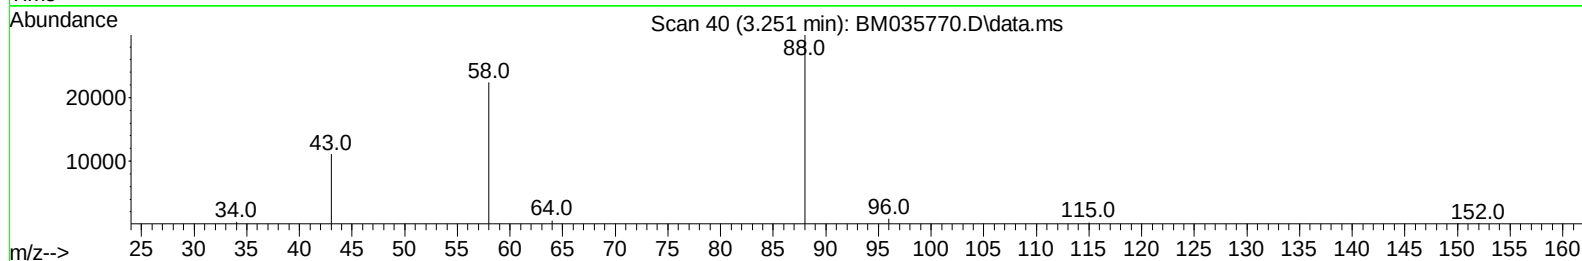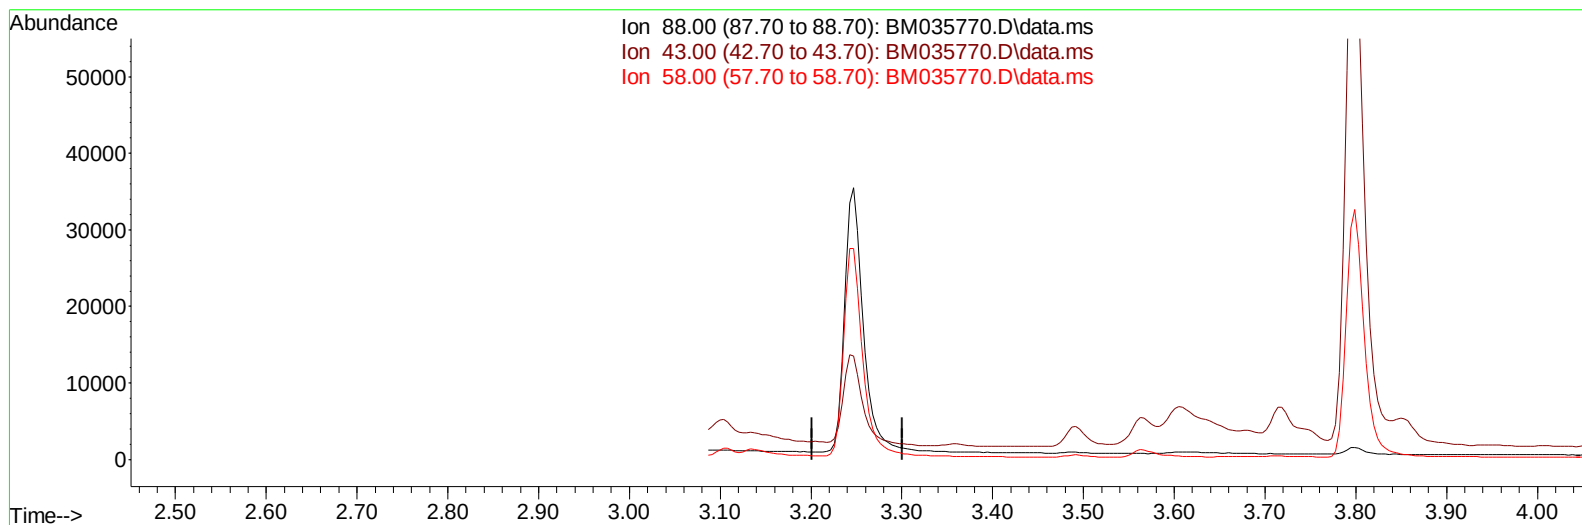

TIC: BM035770.D\data.ms

(2) 1,4-Dioxane

3.251min (-3.251) 0.00 ng/ul

response 0

Ion	Exp%	Act%
88.00	100.00	0.00
43.00	47.20	0.00#
58.00	53.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

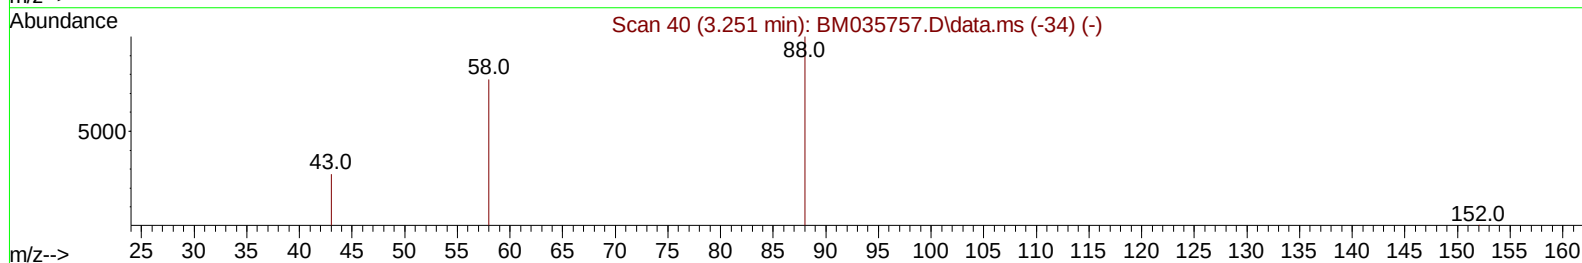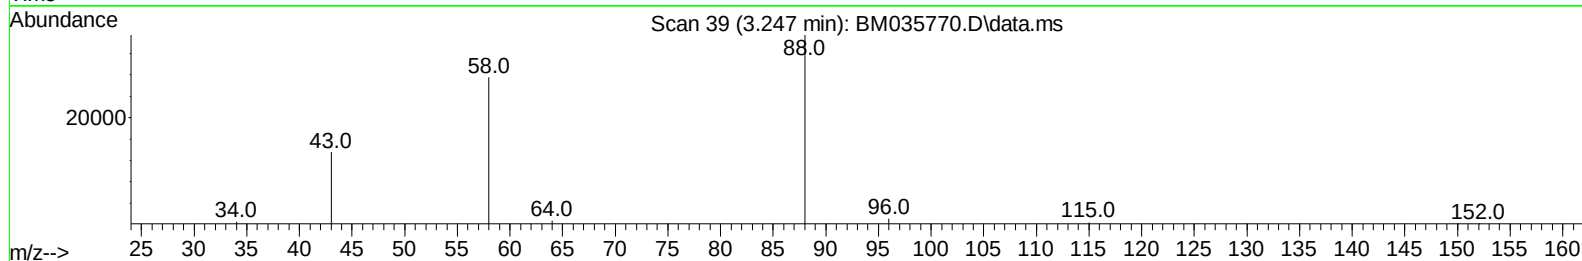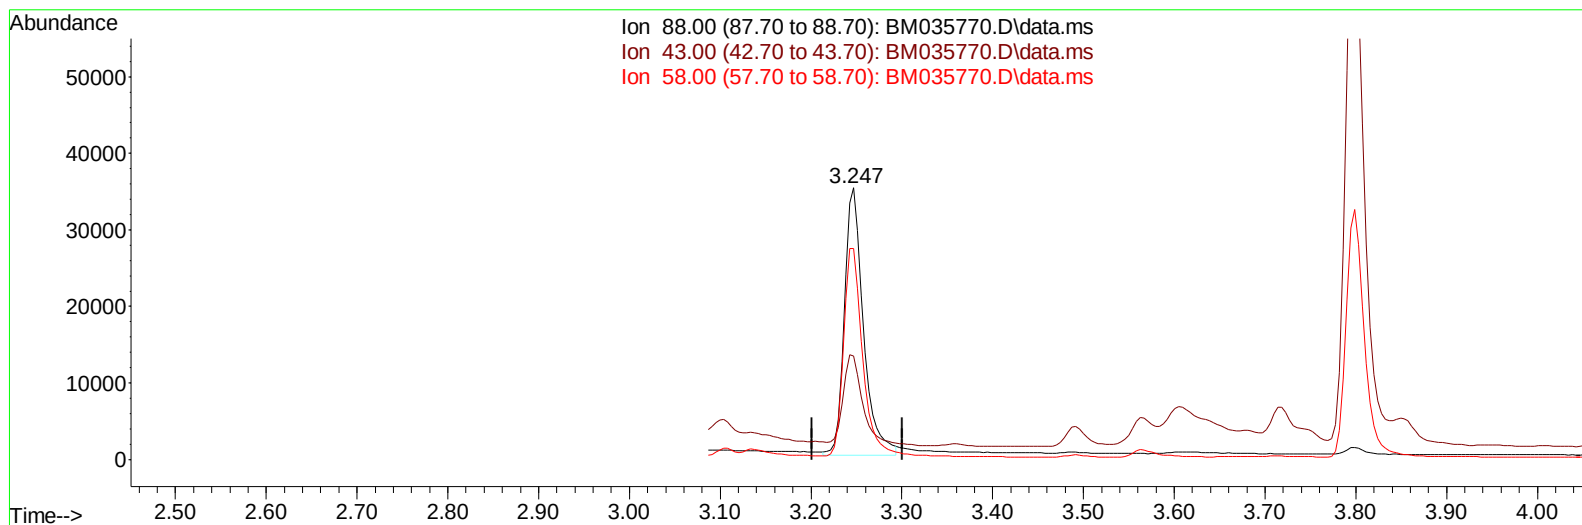

TIC: BM035770.D\data.ms

(2) 1,4-Dioxane

3.247min (-0.004) 10.63 ng/ul m

response 50510

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	38.05
58.00	53.20	77.59#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

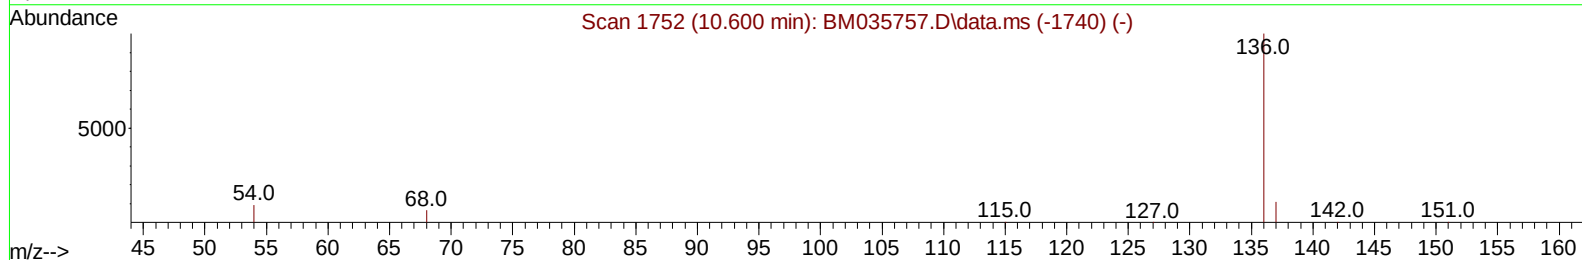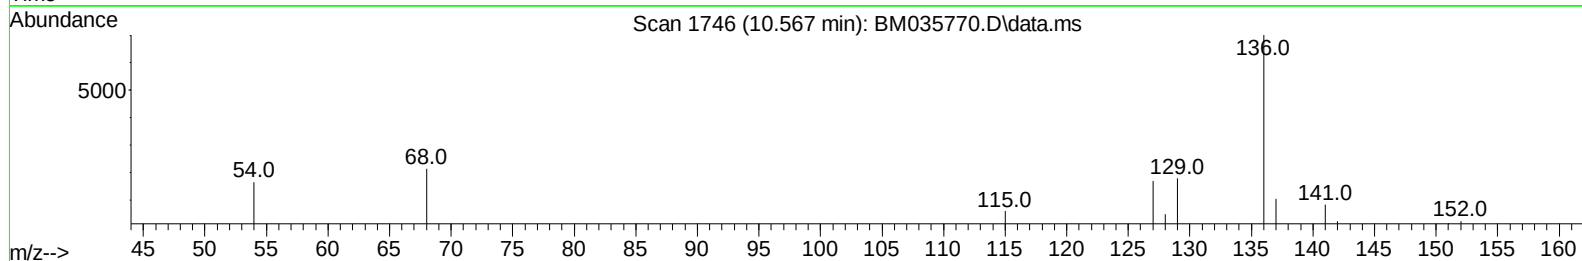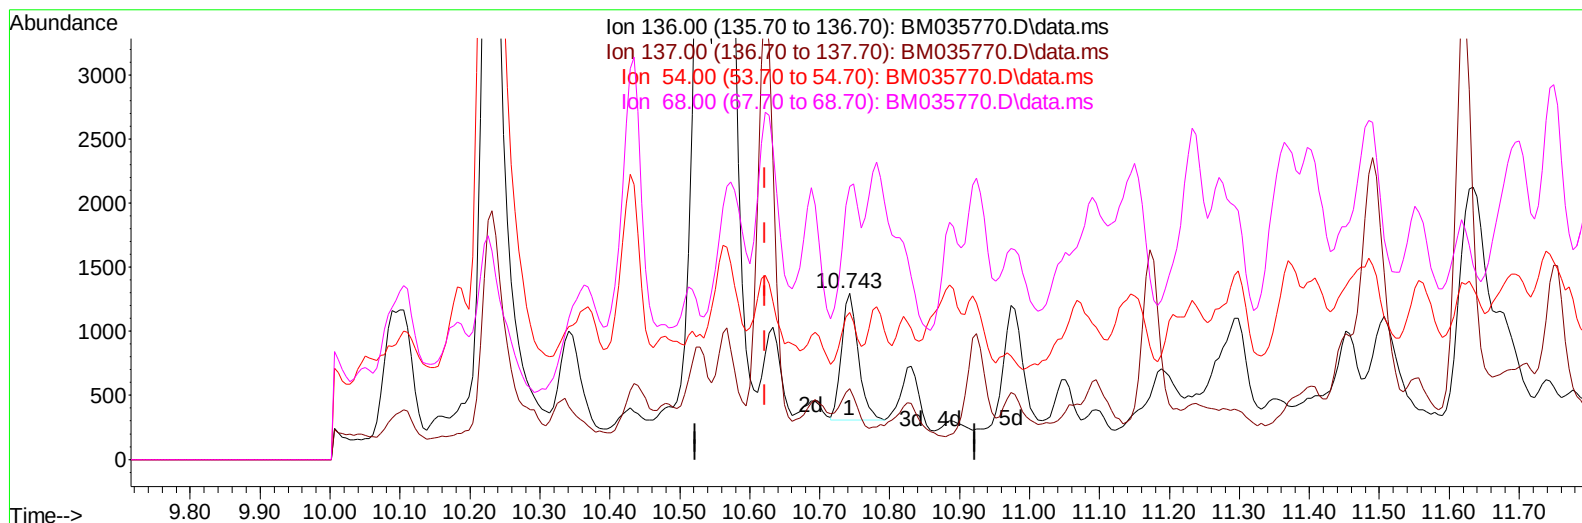

TIC: BM035770.D\data.ms

(4) Naphthalene-d8 (I)

10.743min (+ 0.121) 0.40 ng/u1

response 1632

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	42.53#
54.00	12.20	88.44#
68.00	8.00	164.10#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

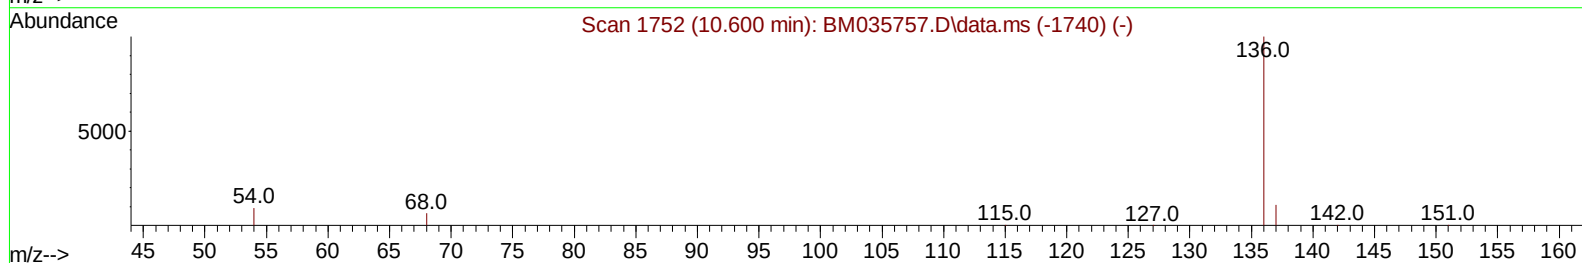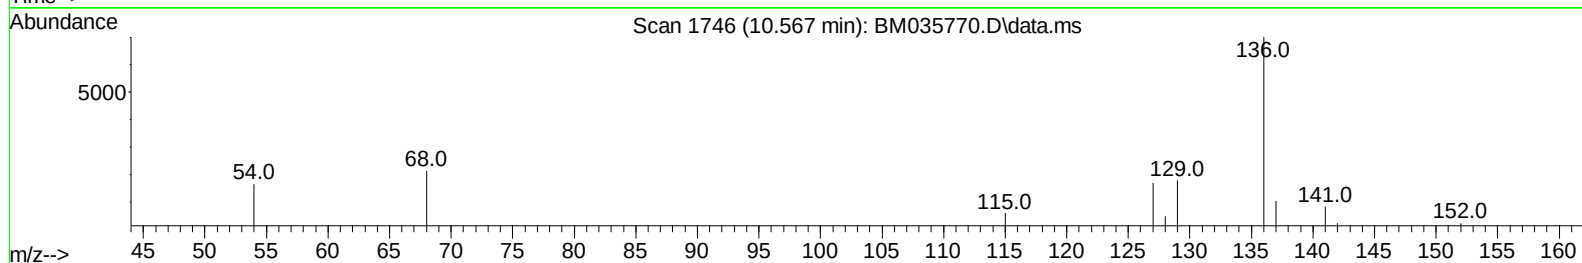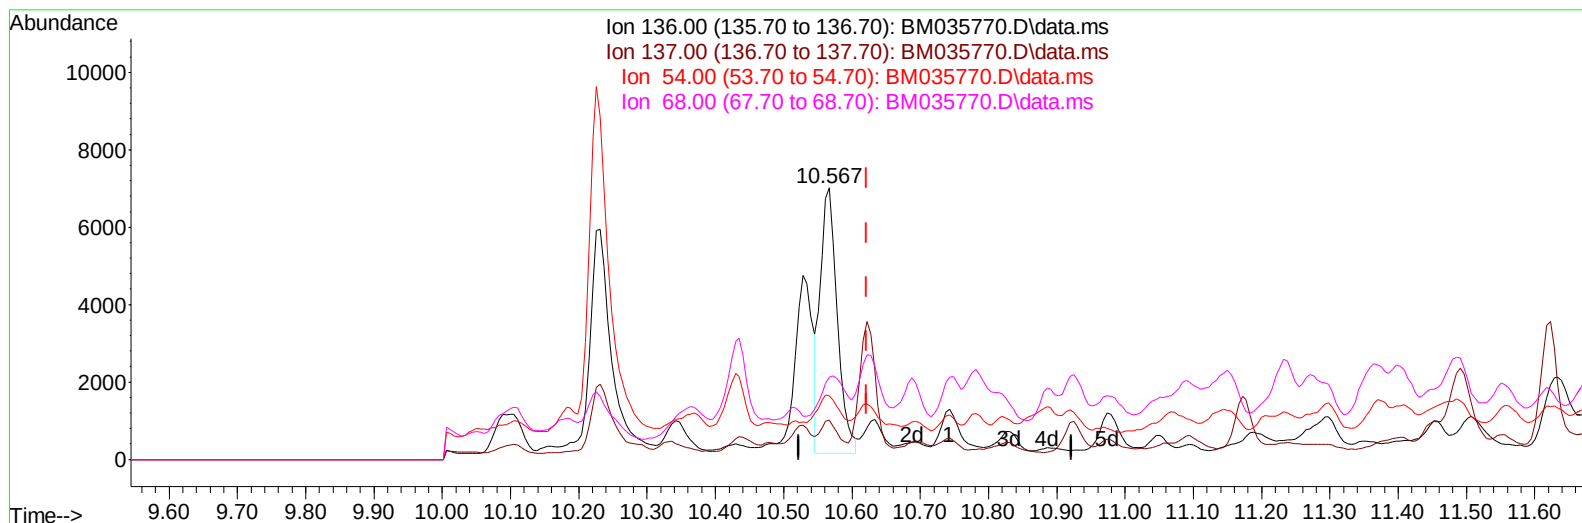

TIC: BM035770.D\data.ms

(4) Naphthalene-d8 (I)

10.567min (-0.055) 0.40 ng/ul m

response 11948

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	14.63
54.00	12.20	23.60#
68.00	8.00	30.37#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

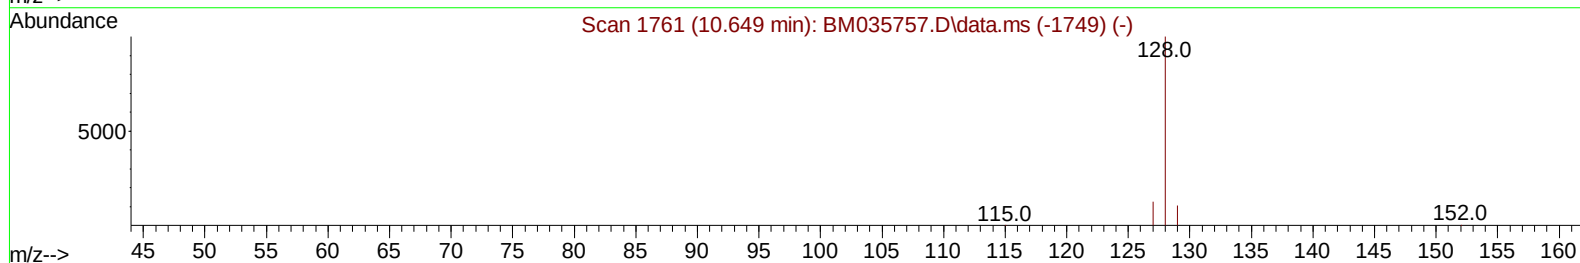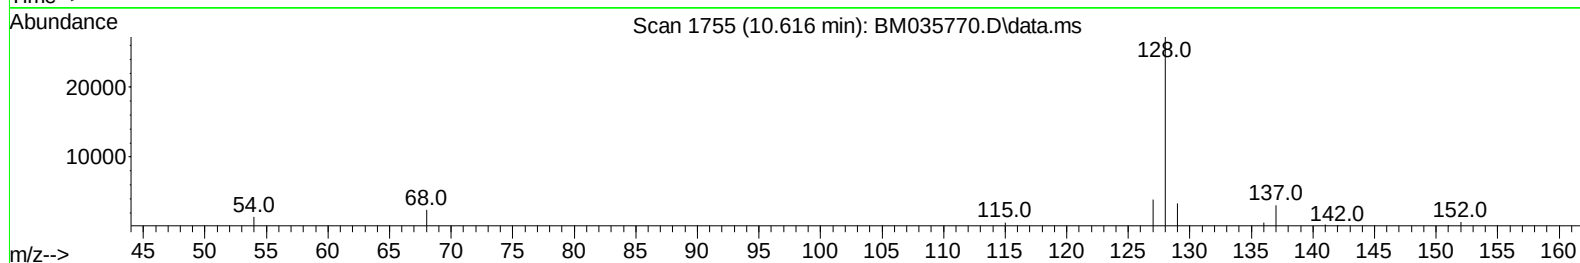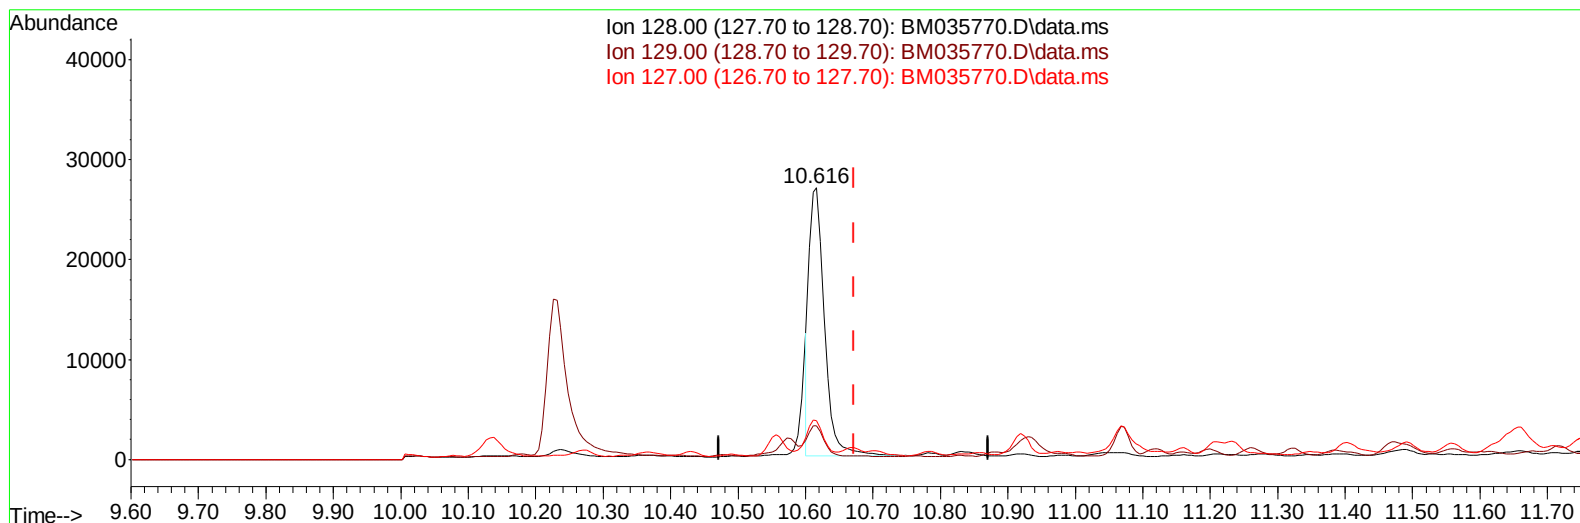

TIC: BM035770.D\data.ms

(5) Naphthalene

10.616min (-0.055) 1.17 ng/u1

response 42811

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	12.45
127.00	14.60	14.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

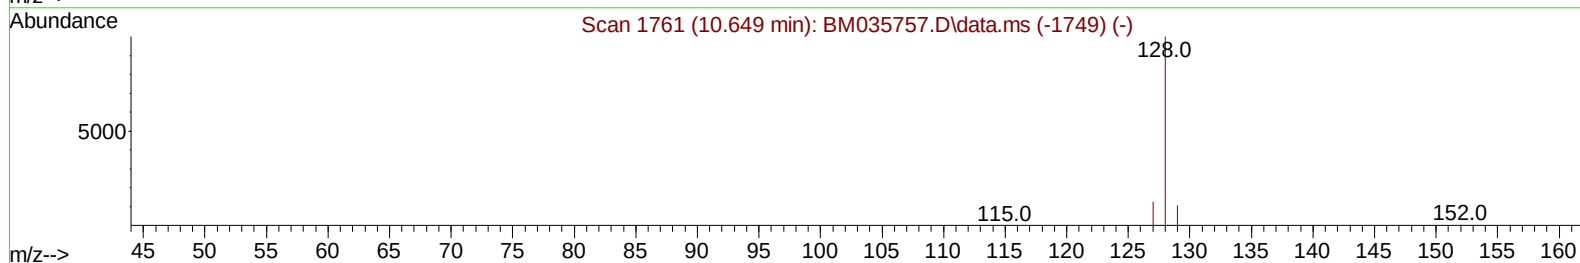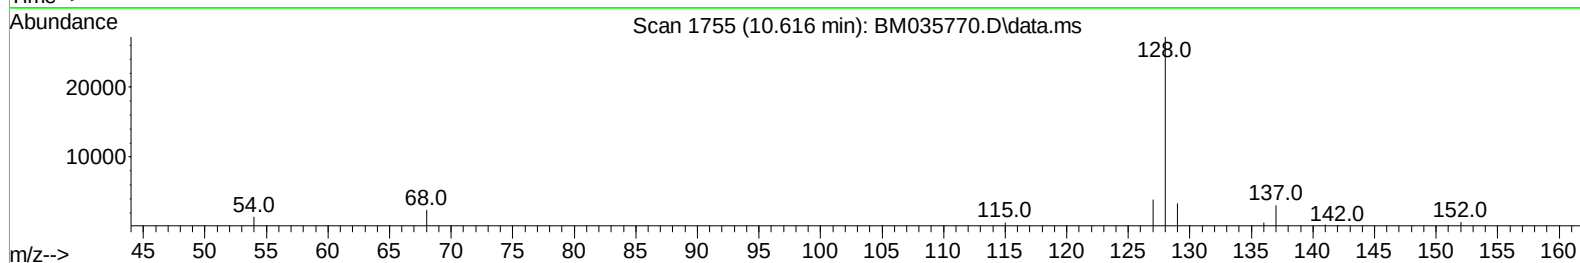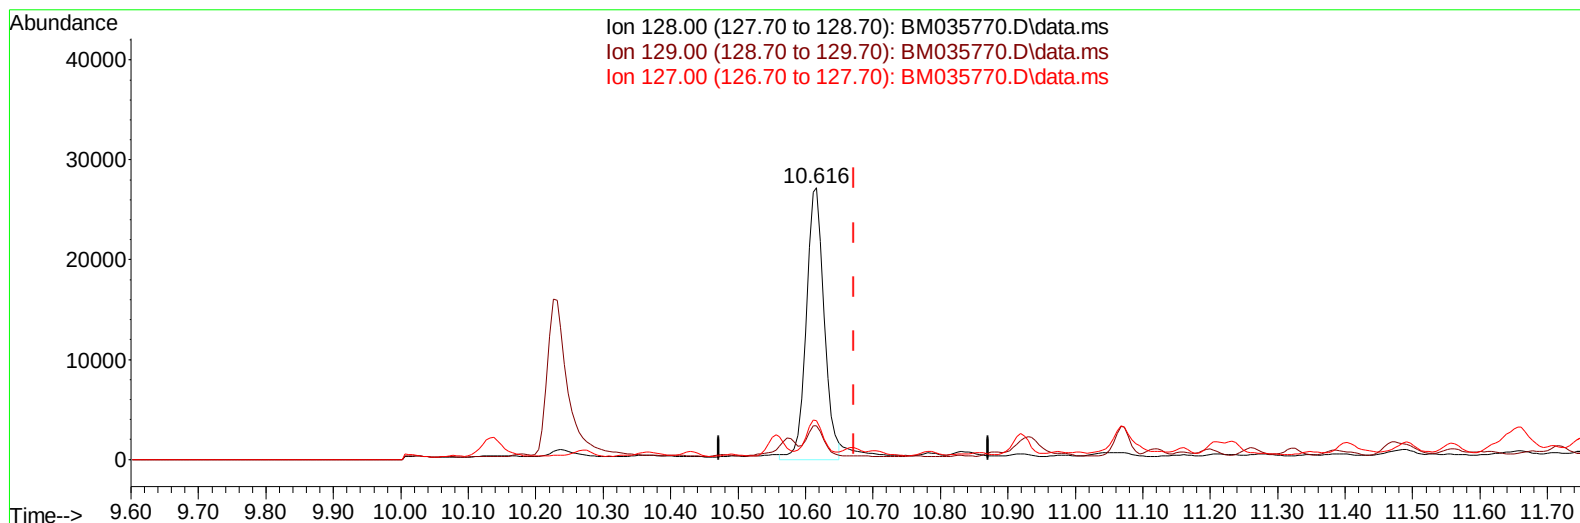

TIC: BM035770.D\data.ms

(5) Naphthalene

10.616min (-0.055) 1.37 ng/ul m

response 50059

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	12.45
127.00	14.60	14.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

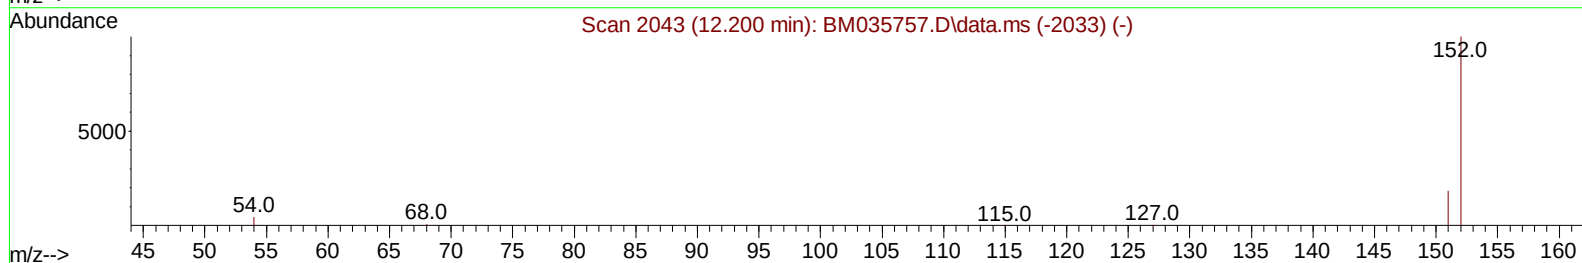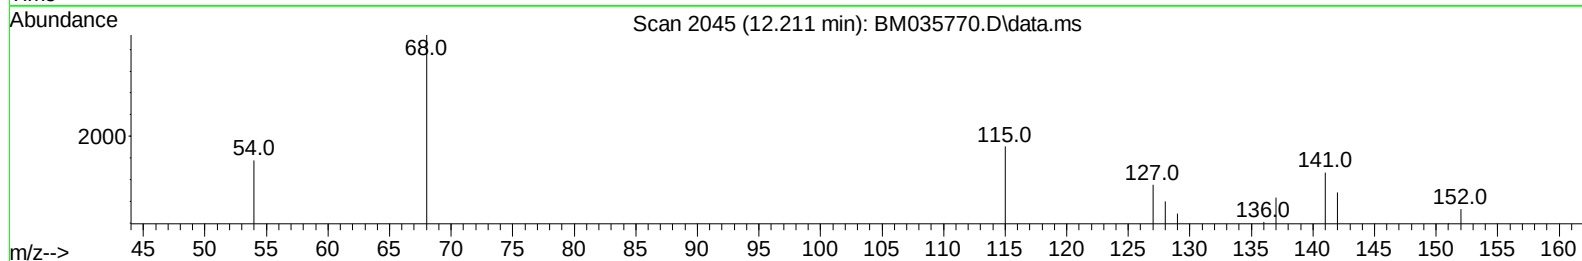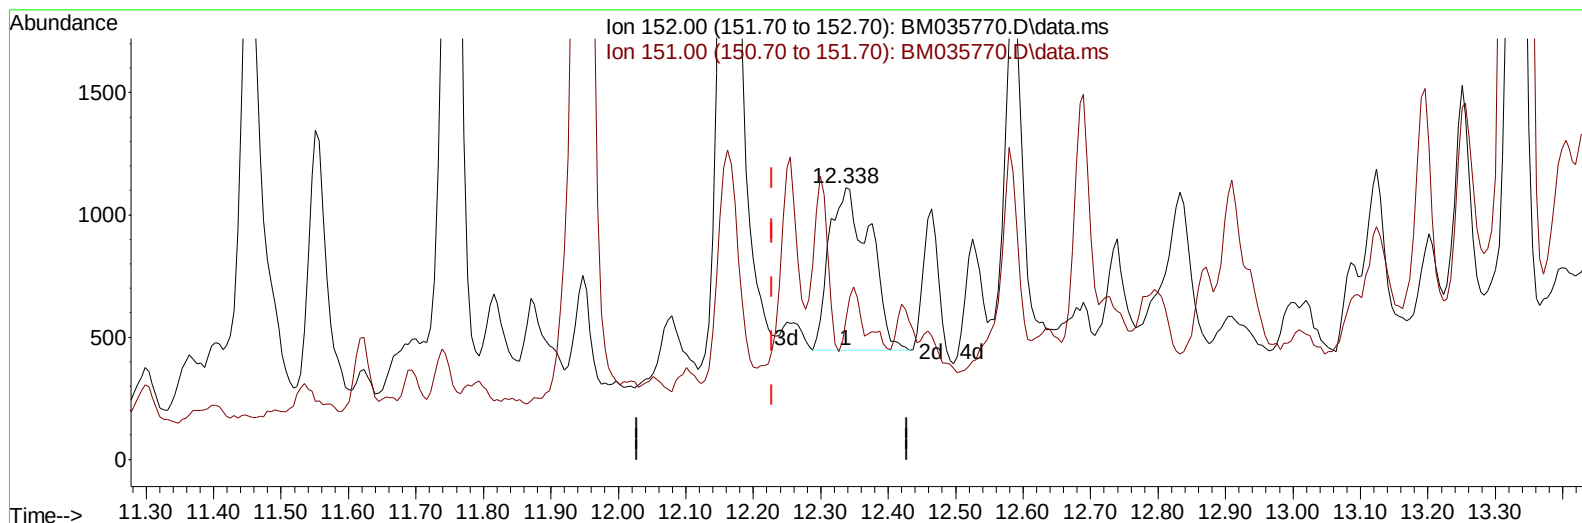

TIC: BM035770.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.338min (+ 0.110) 0.15 ng/u1

response 2795

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	30.09#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

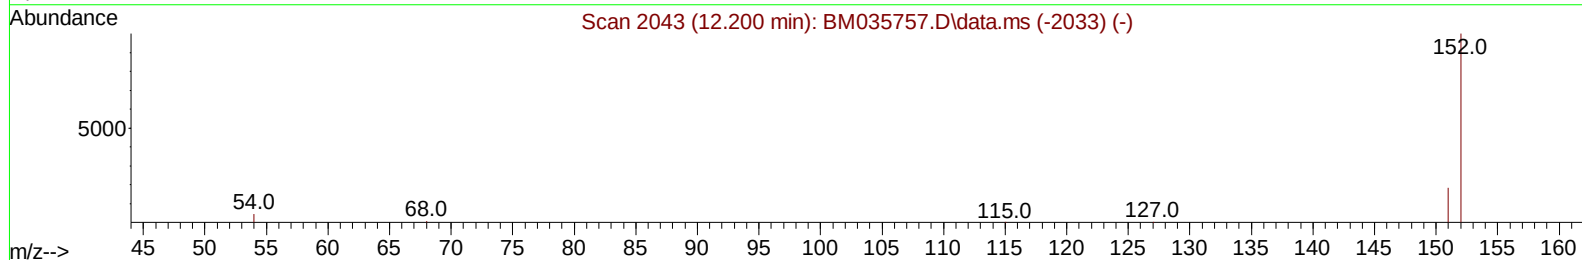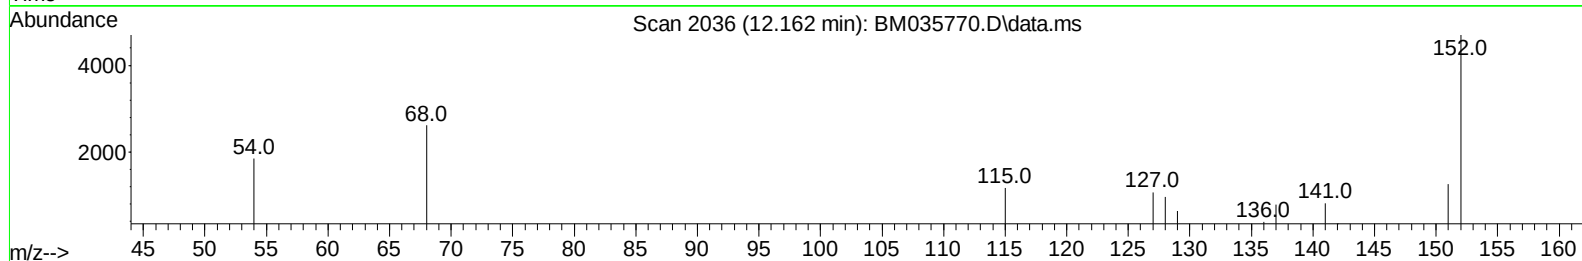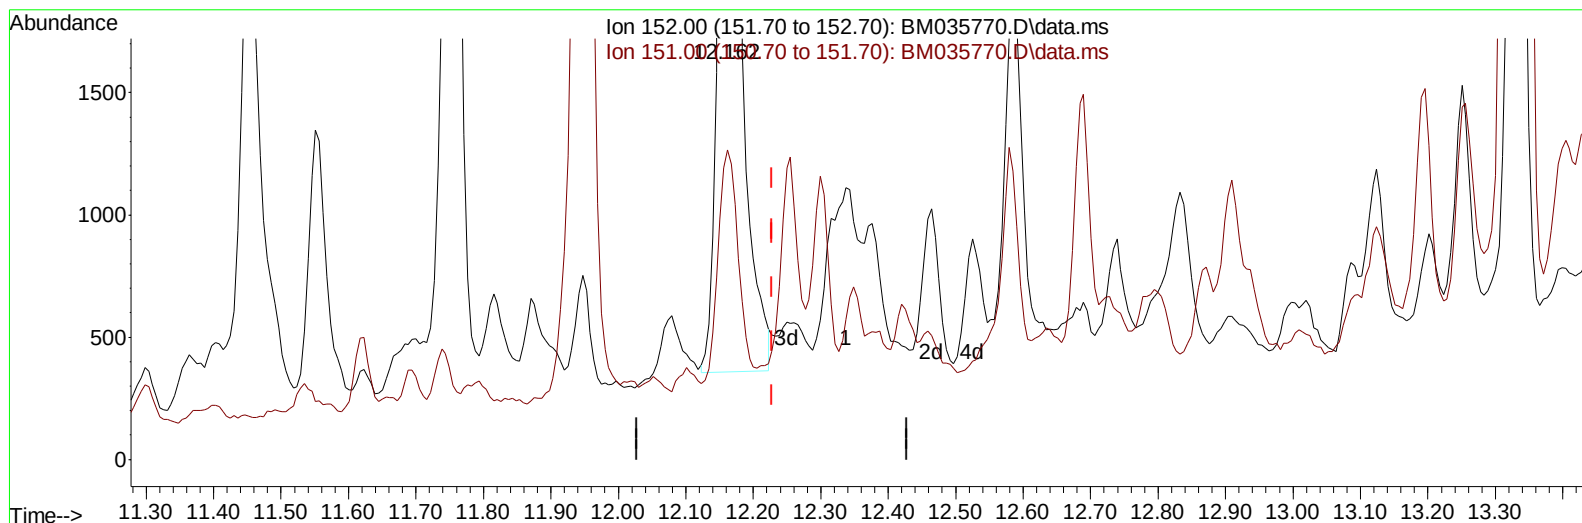

TIC: BM035770.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.162min (-0.066) 0.46 ng/ul m

response 8605

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	9.77#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

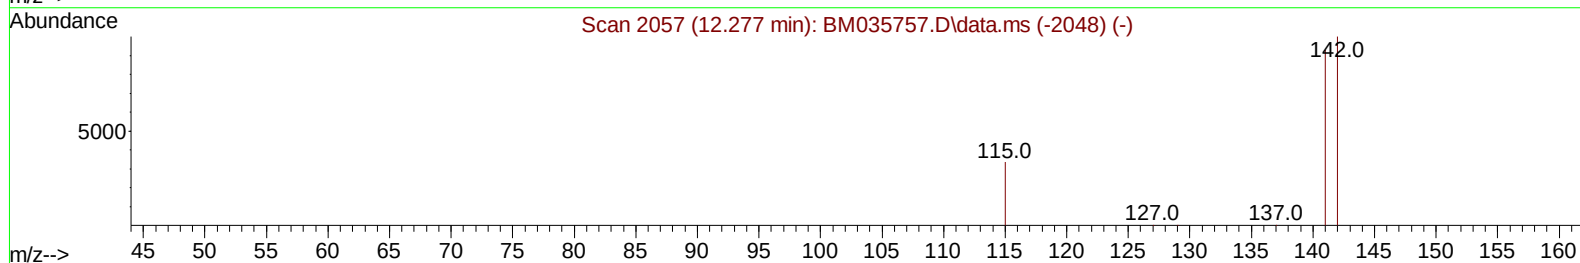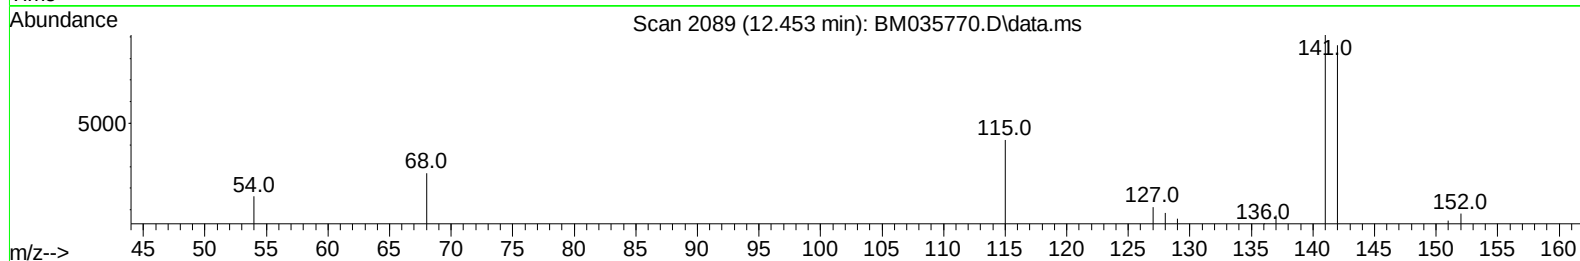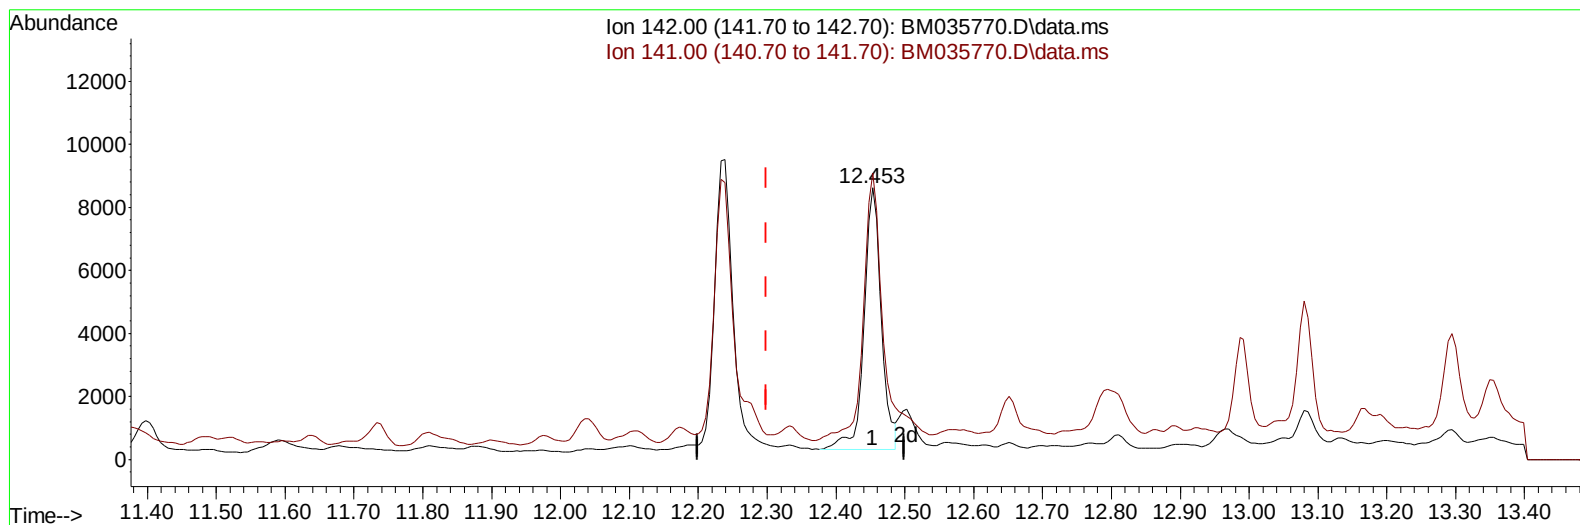

TIC: BM035770.D\data.ms

(7) 2-Methylnaphthalene

12.453min (+ 0.154) 0.64 ng/u1

response 14582

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	96.70	119.85#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

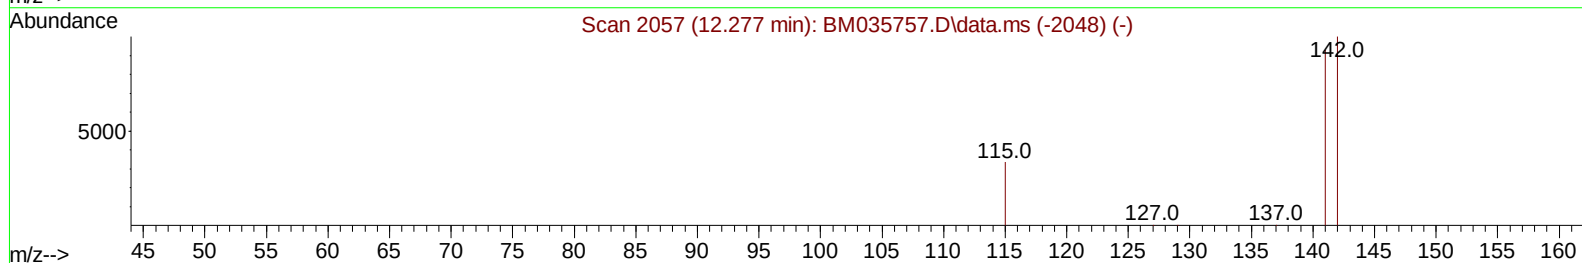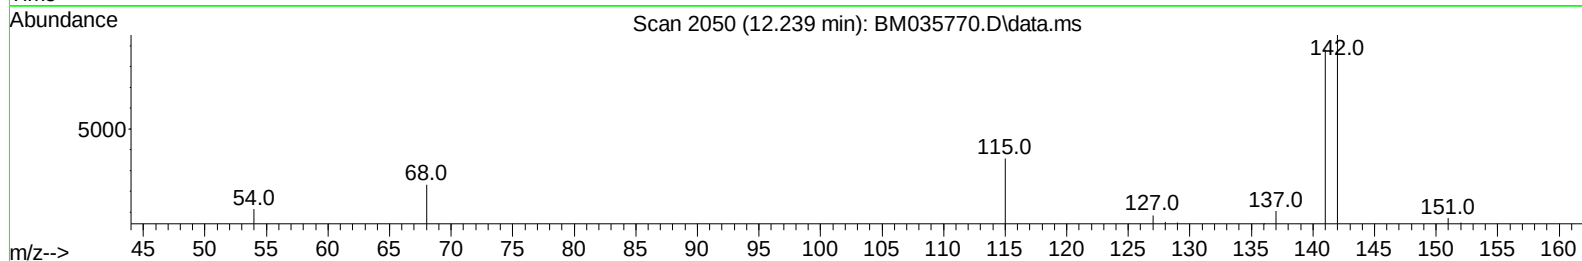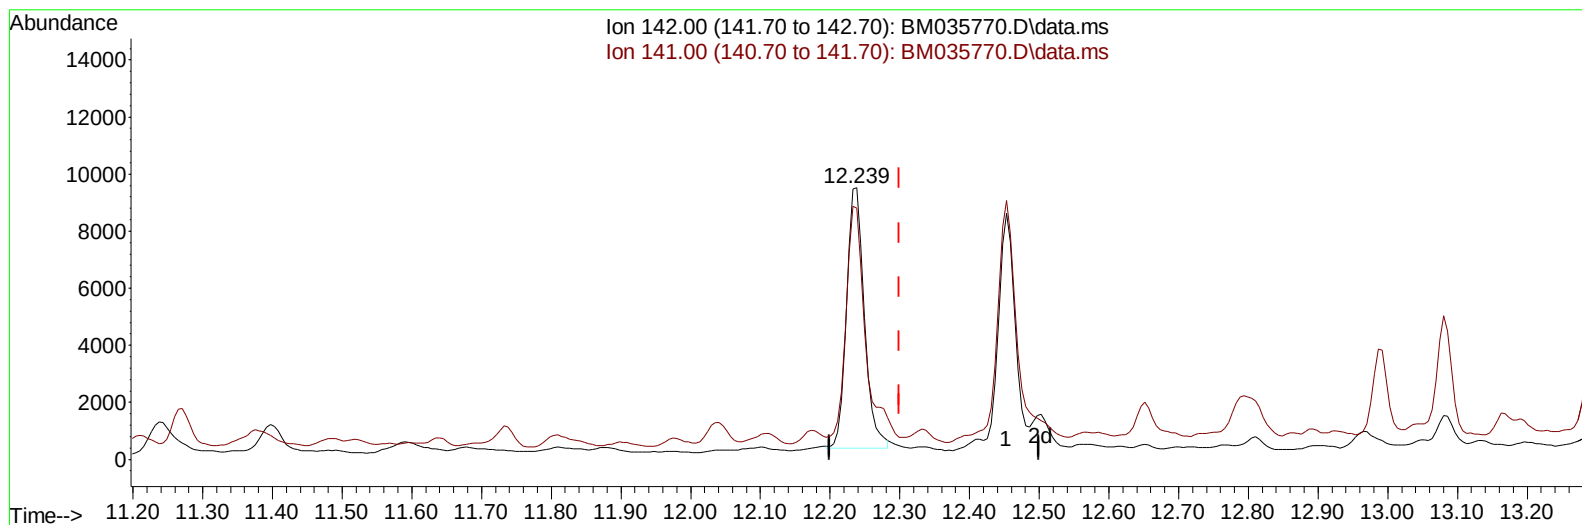

TIC: BM035770.D\data.ms

(7) 2-Methylnaphthalene

12.239min (-0.060) 0.71 ng/ul m

response 16169

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	96.70	108.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

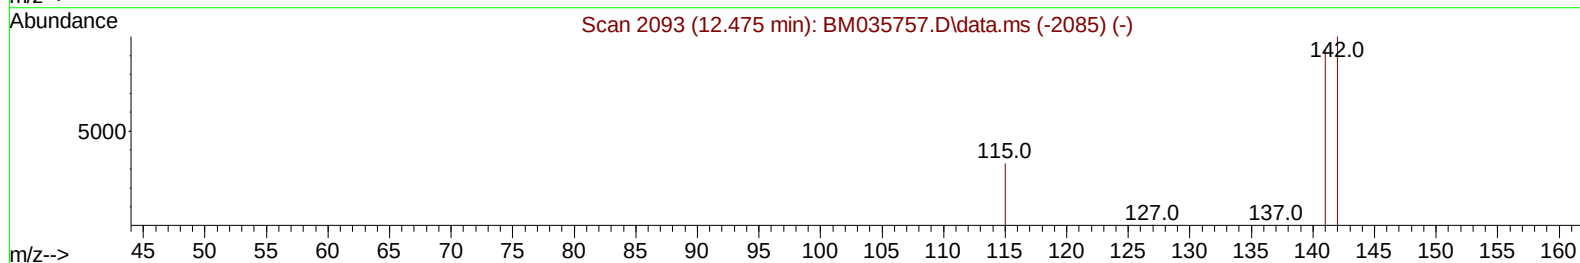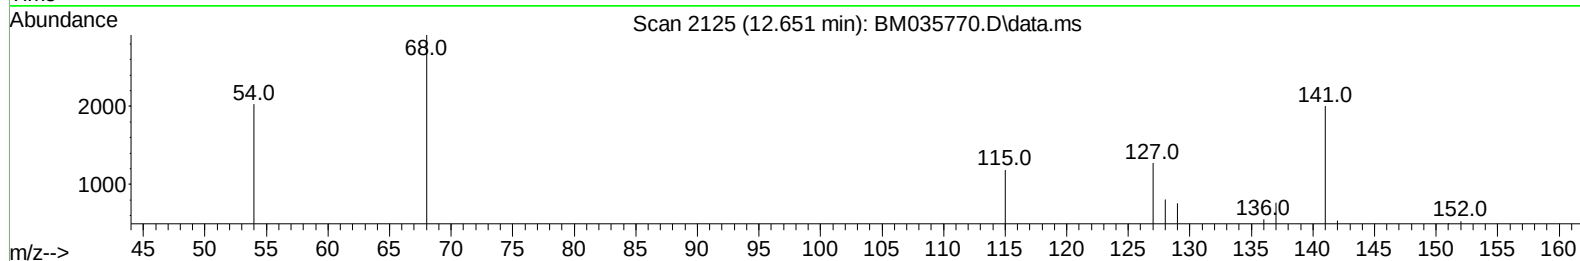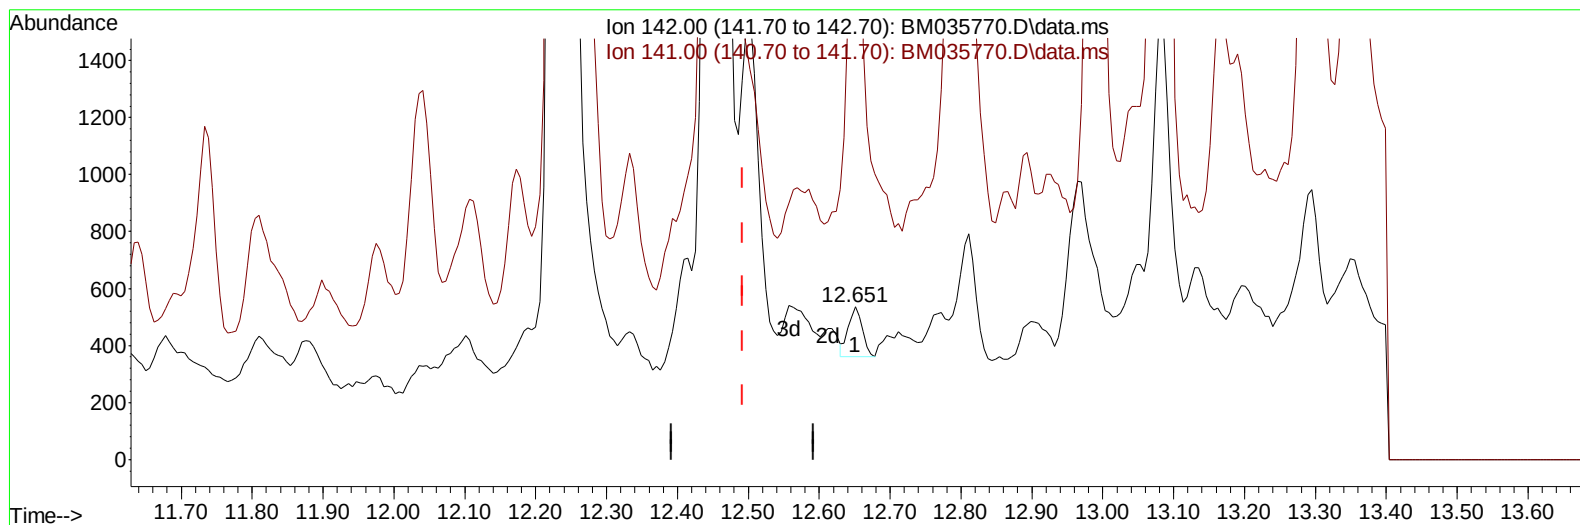

TIC: BM035770.D\data.ms

(8) 1-Methylnaphthalene

12.651min (+ 0.160) 0.01 ng/ul

response 242

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	895.04#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

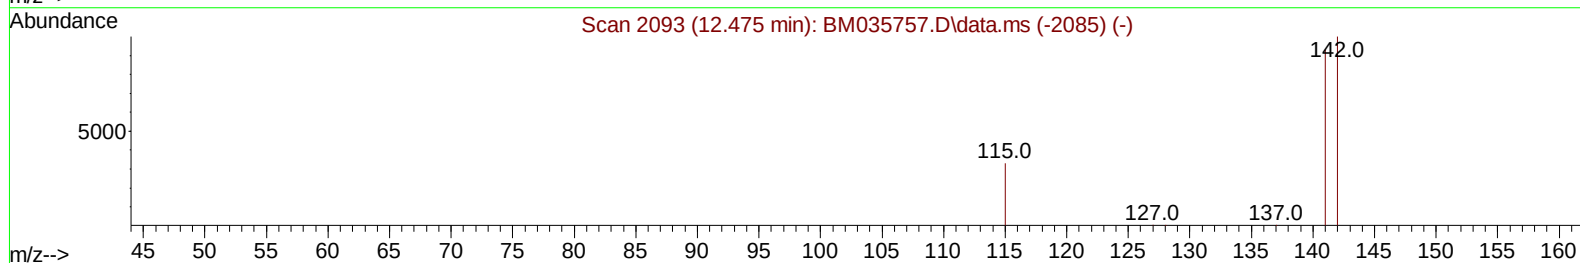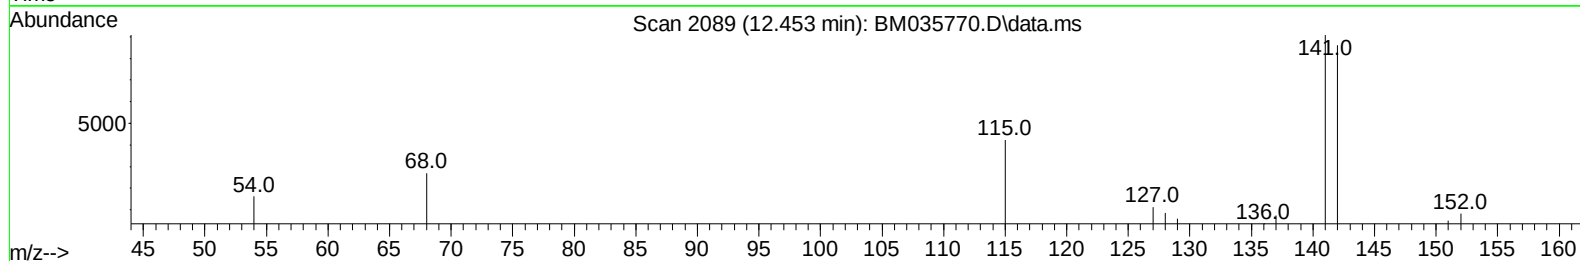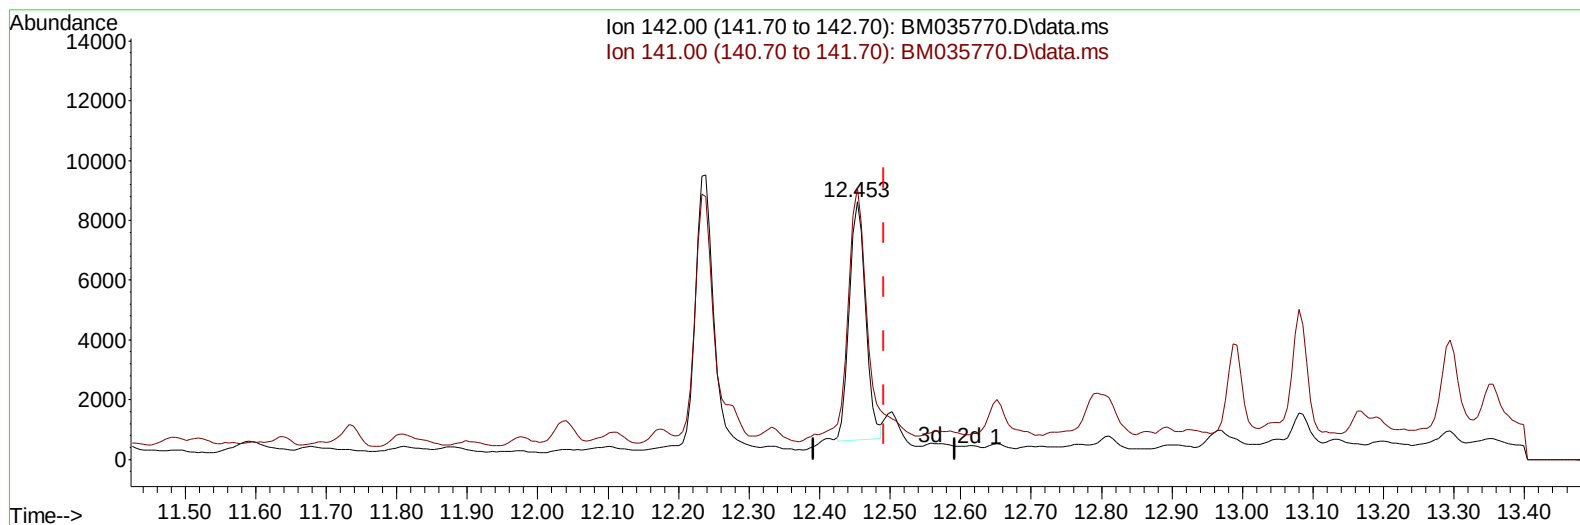

TIC: BM035770.D\data.ms

(8) 1-Methylnaphthalene

12.453min (-0.038) 0.58 ng/ul m

response 12575

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	17.22#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

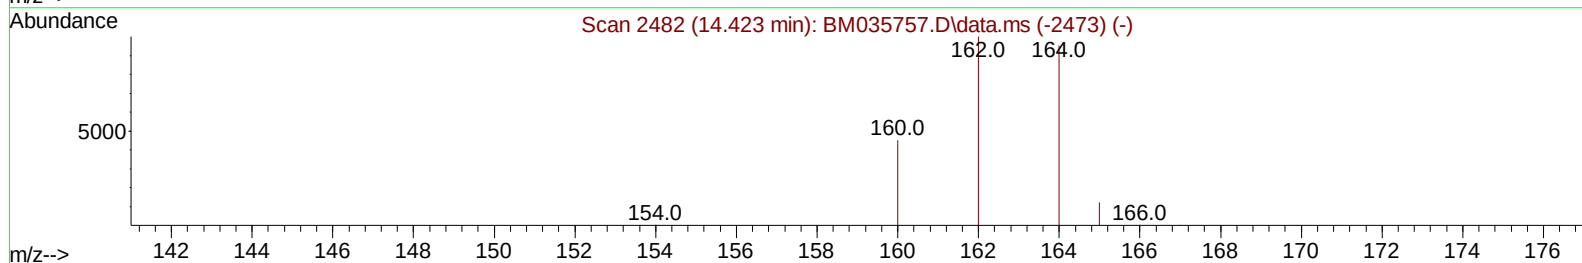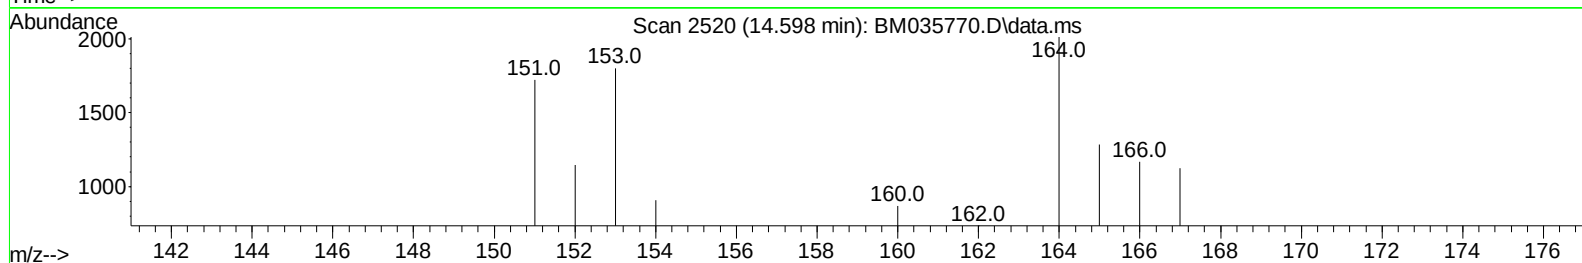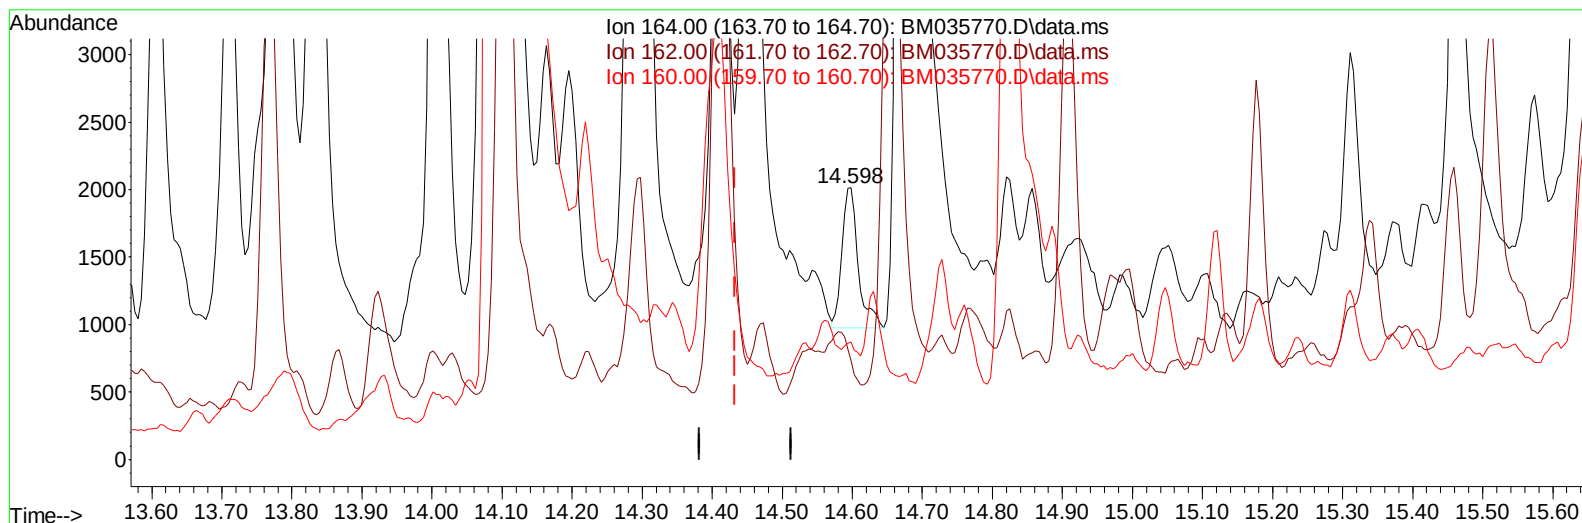

TIC: BM035770.D\data.ms

(9) Acenaphthene-d10 (I)

14.598min (+ 0.166) 0.40 ng/ul

response 1696

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	36.48#
160.00	48.90	43.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

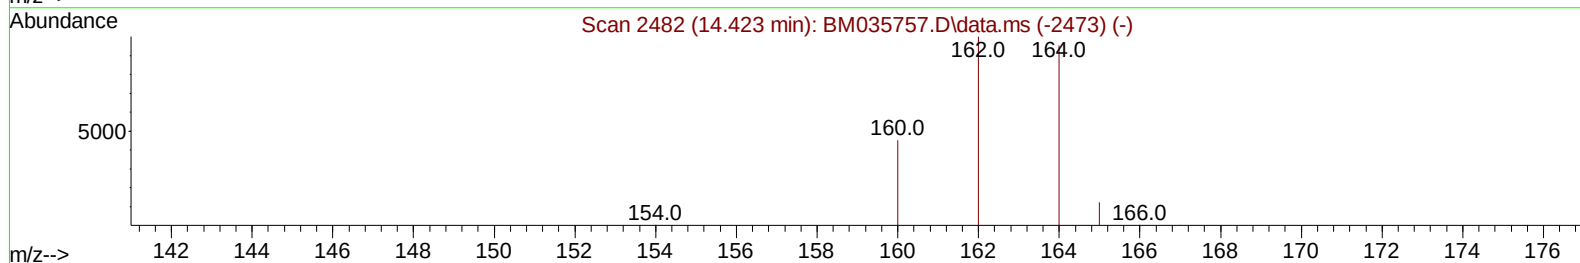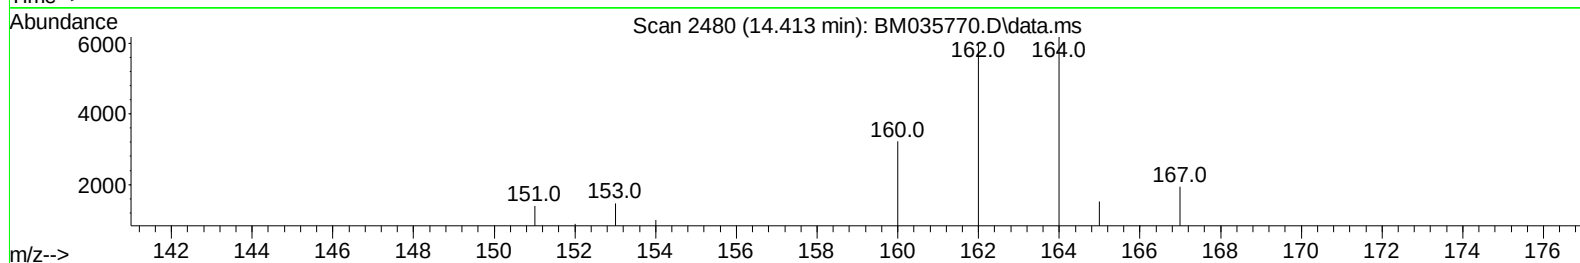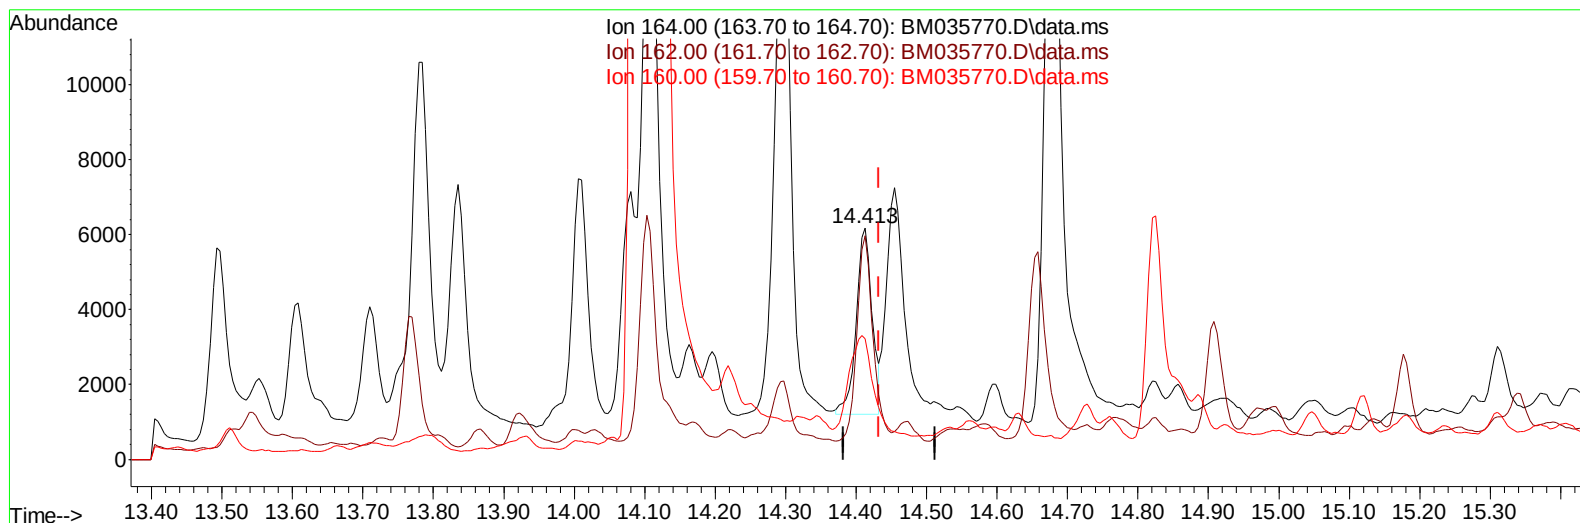

TIC: BM035770.D\data.ms

(9) Acenaphthene-d10 (I)

14.413min (-0.019) 0.40 ng/ul m

response 7829

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	96.55
160.00	48.90	52.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

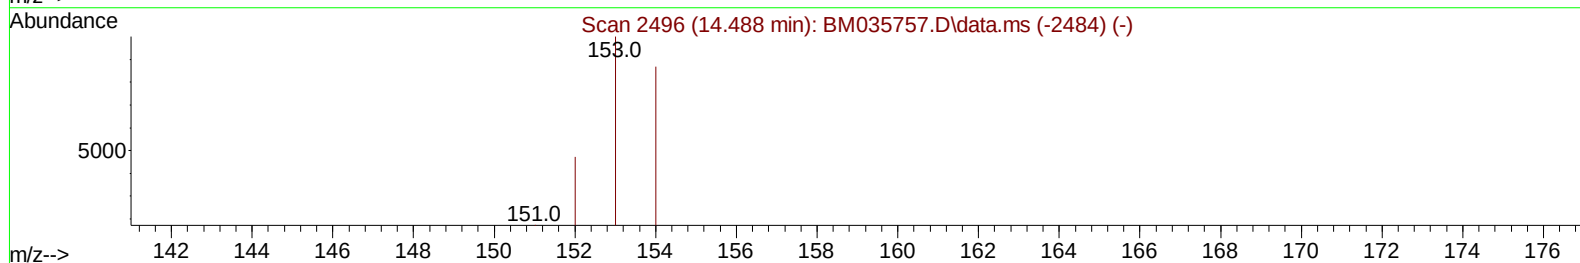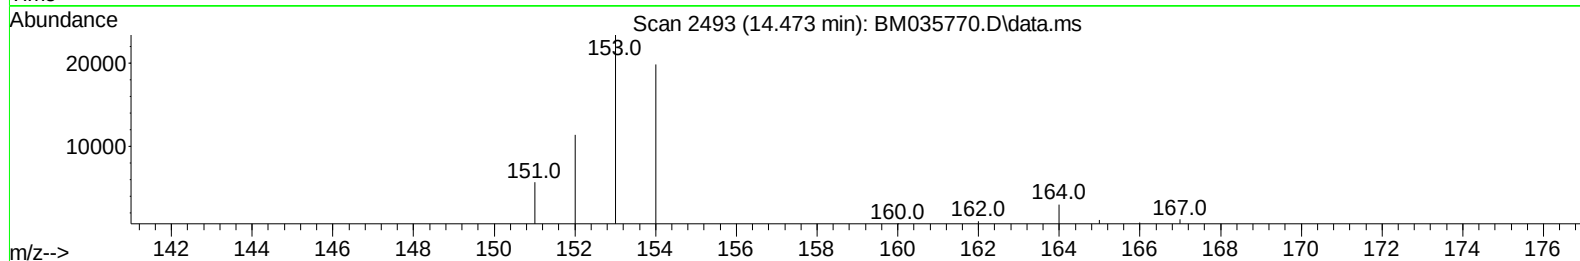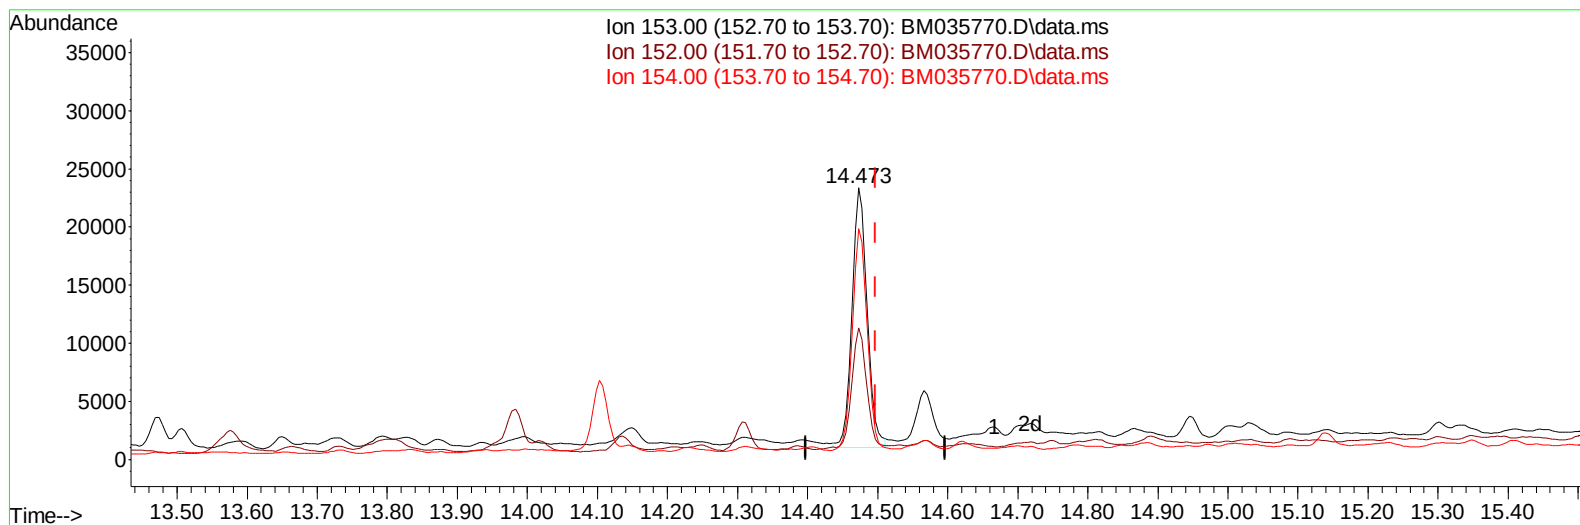

TIC: BM035770.D\data.ms

(11) Acenaphthene (C)

14.473min (-0.024) 1.05 ng/ul m

response 33313

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.30	48.47
154.00	87.10	85.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

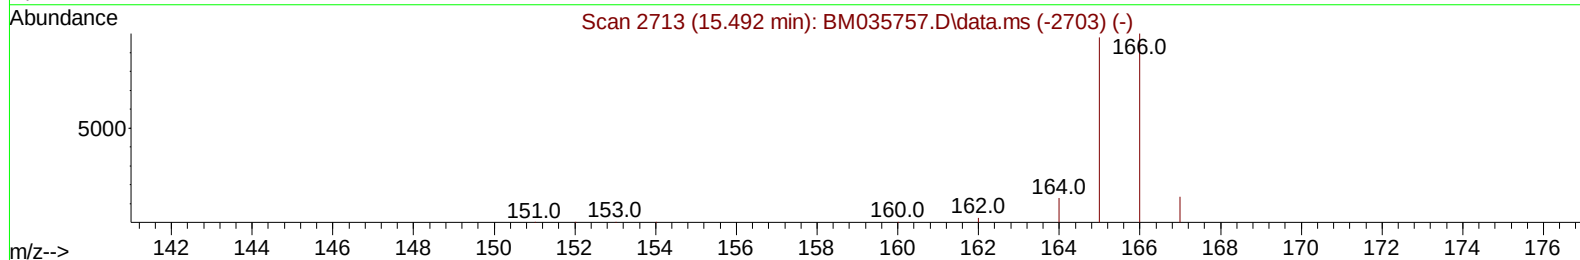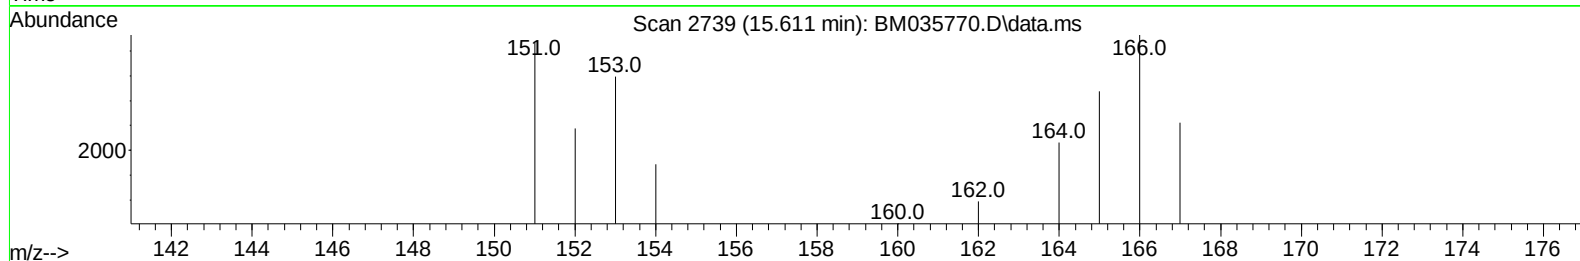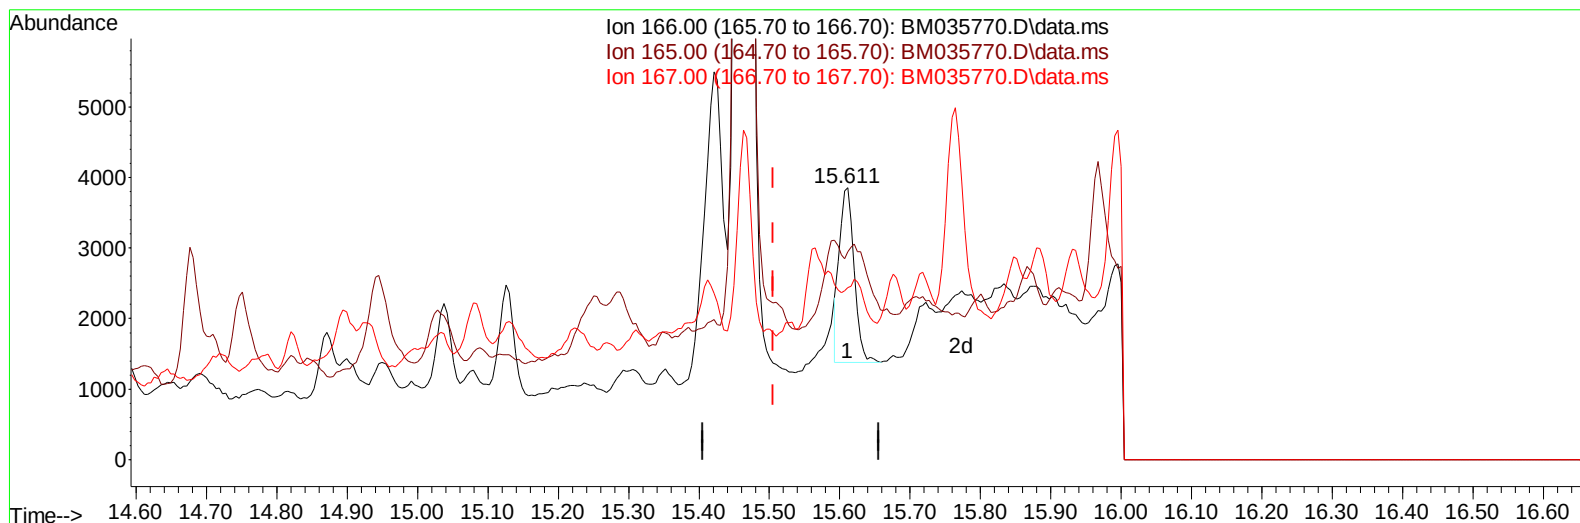

TIC: BM035770.D\data.ms

(12) Fluorene

15.611min (+ 0.106) 0.10 ng/u1

response 3625

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.60	76.57#
167.00	14.10	63.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

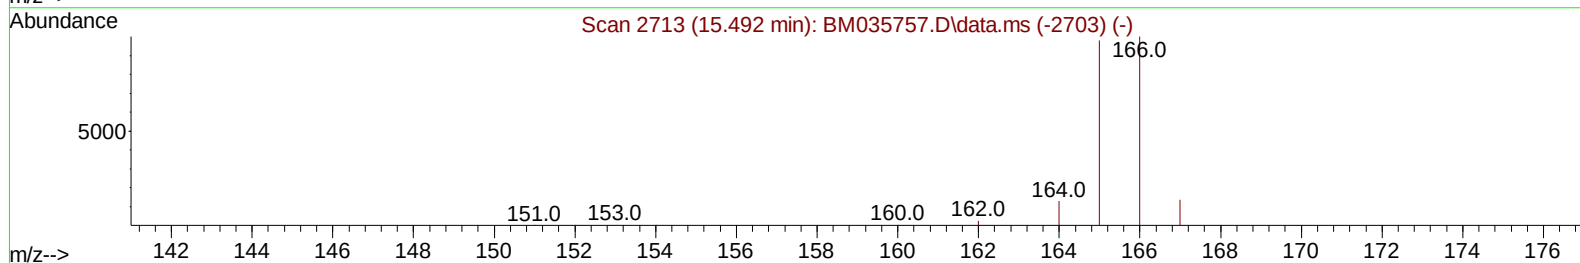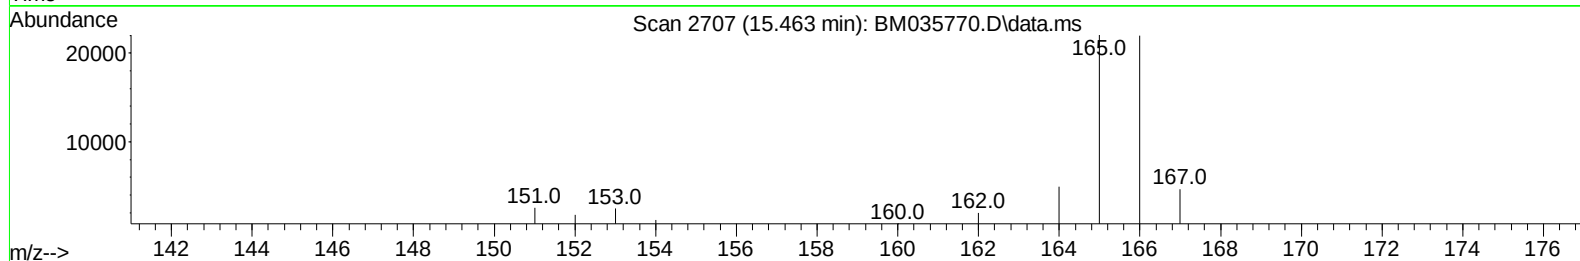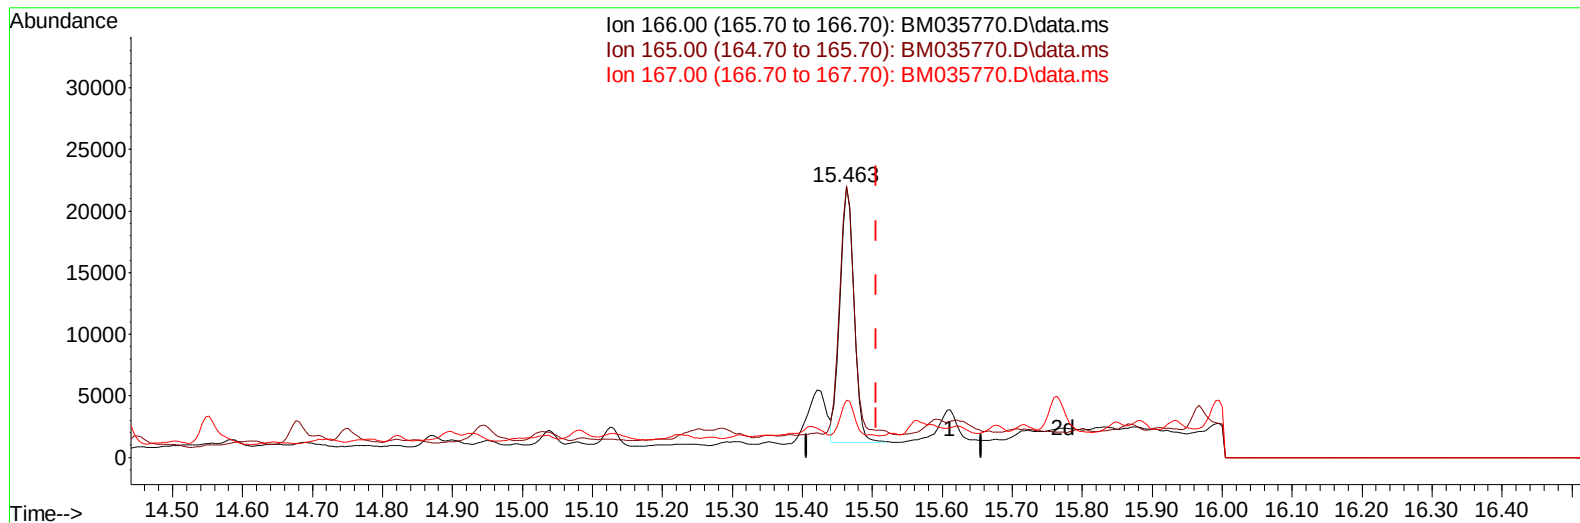

TIC: BM035770.D\data.ms

(12) Fluorene

15.463min (-0.042) 0.80 ng/ul m

response 29282

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.60	100.29
167.00	14.10	21.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

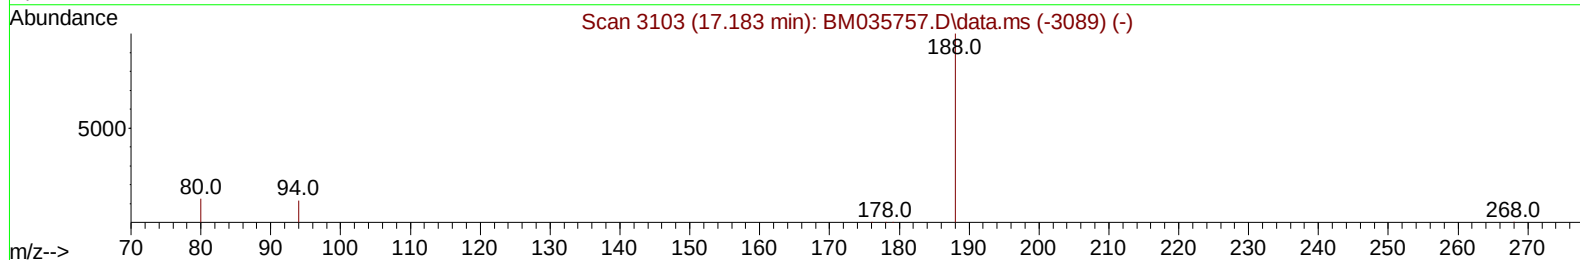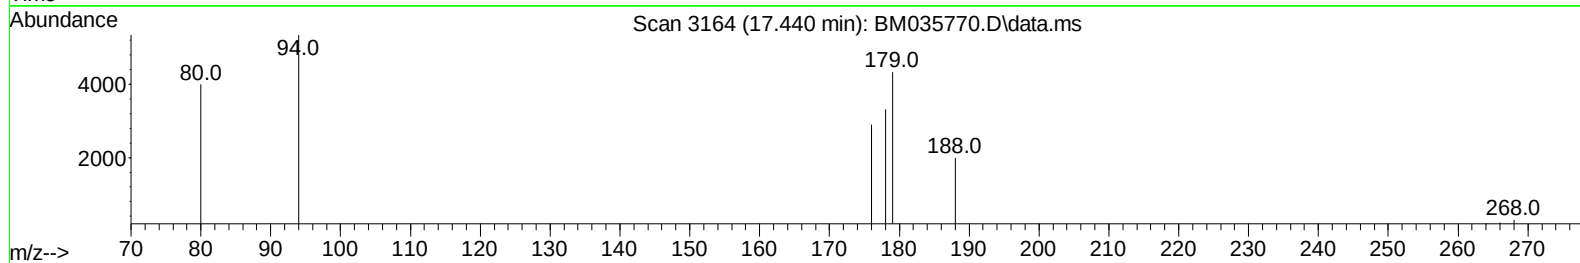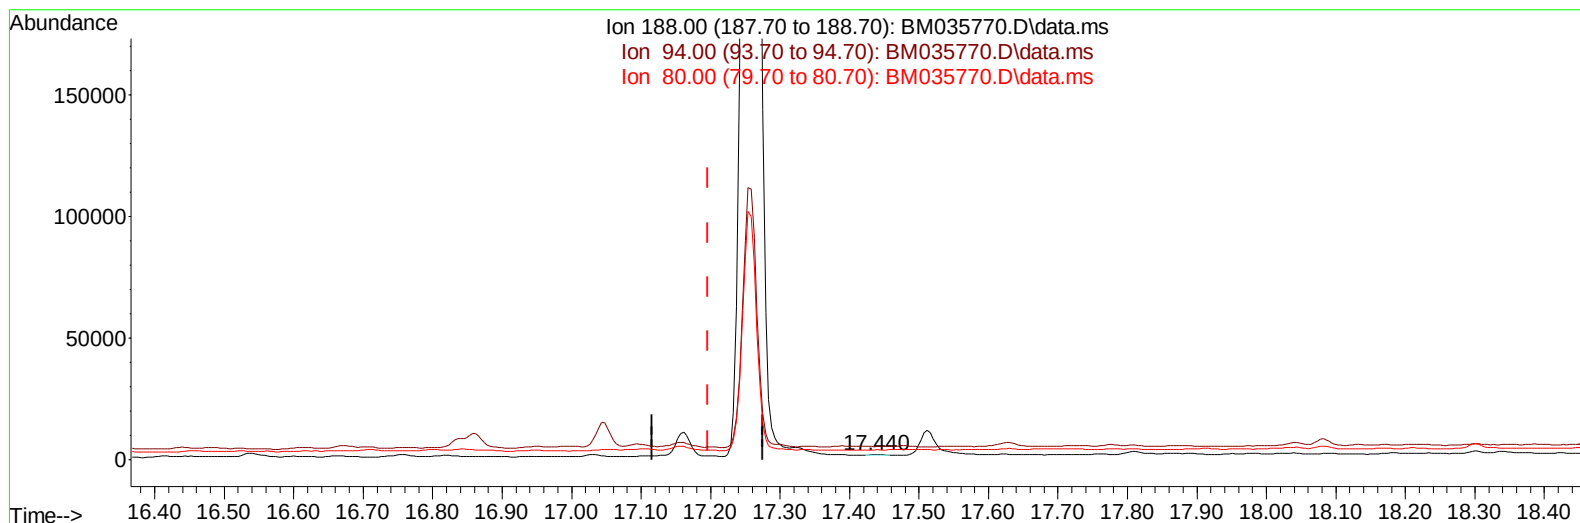

TIC: BM035770.D\data.ms

(13) Phenanthrene-d10 (I)

17.440min (+ 0.244) 0.40 ng/u1

response 268

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	268.98#
80.00	12.70	200.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

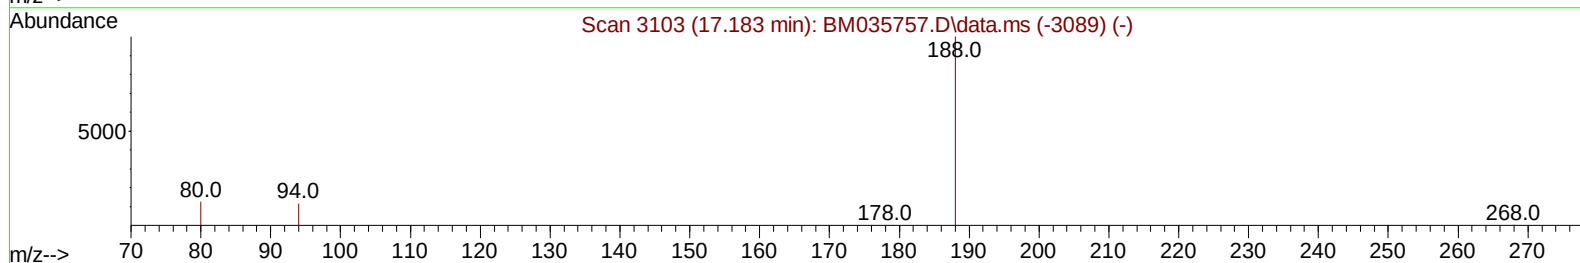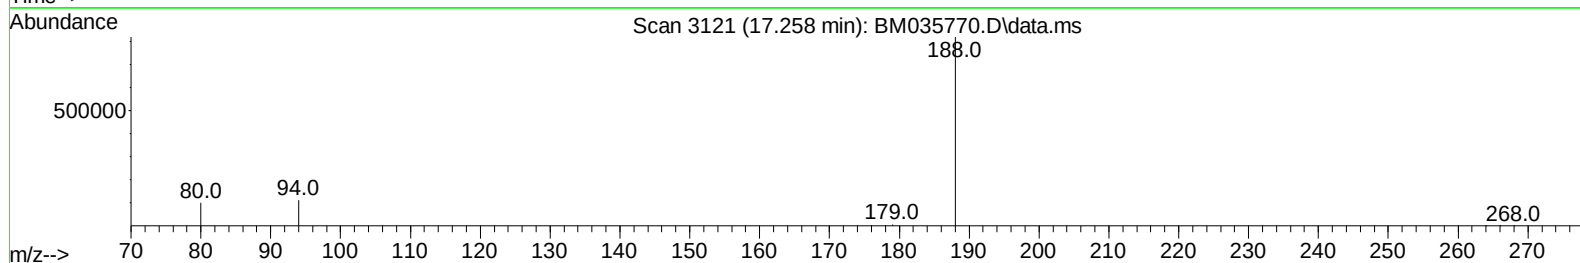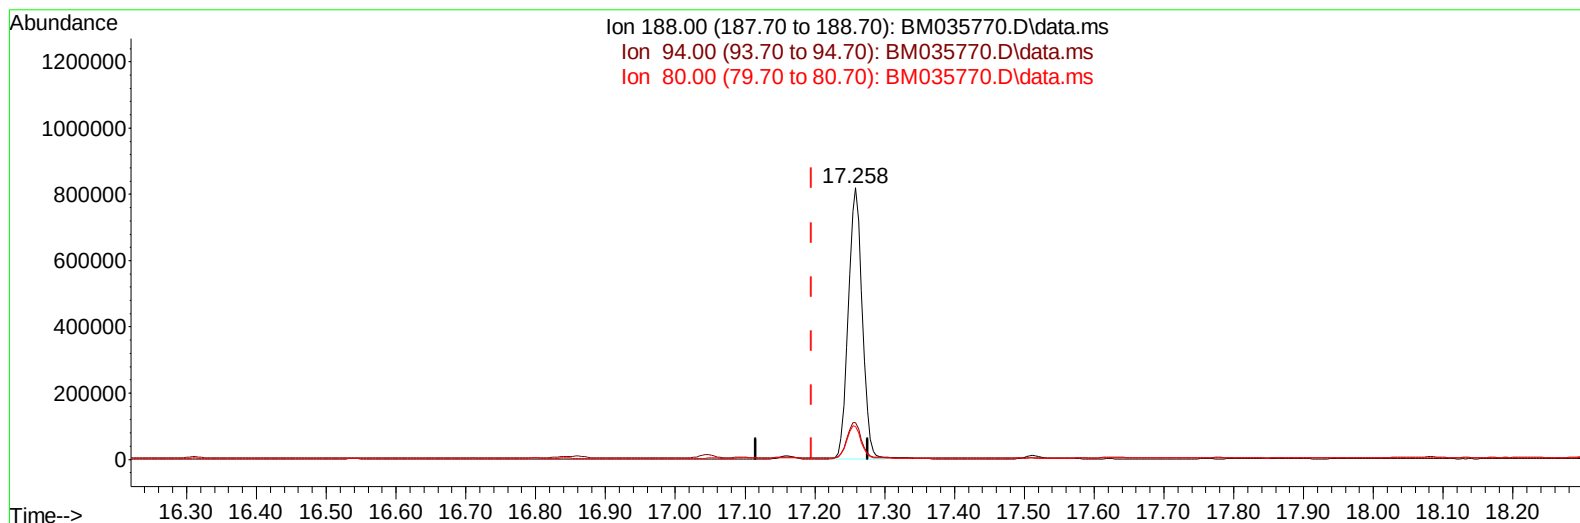

TIC: BM035770.D\data.ms

(13) Phenanthrene-d10 (I)

17.258min (+ 0.063) 0.40 ng/ul m

response 1137942

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	13.59
80.00	12.70	12.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

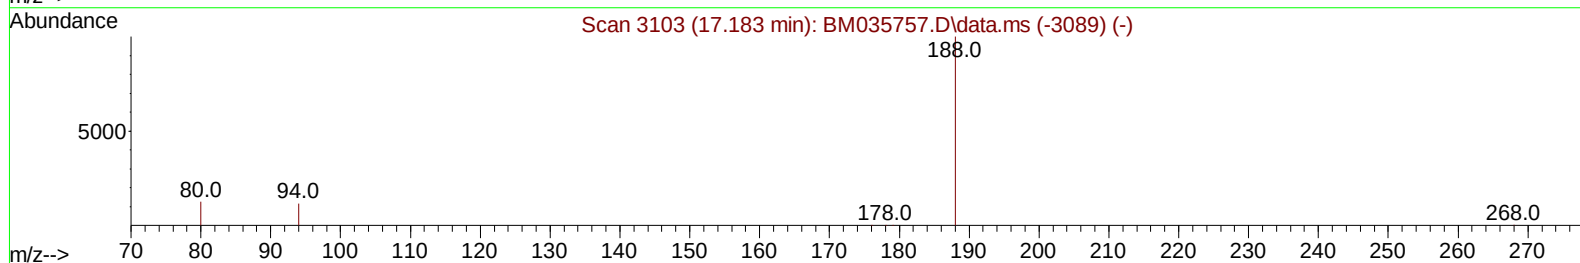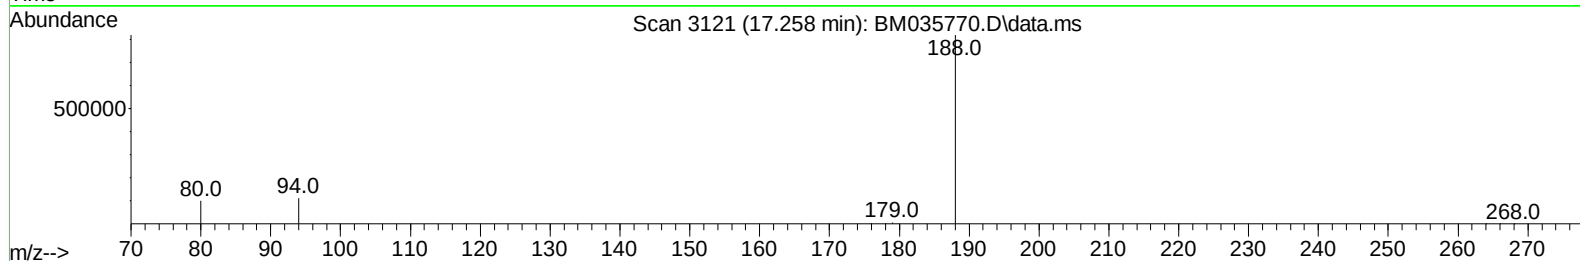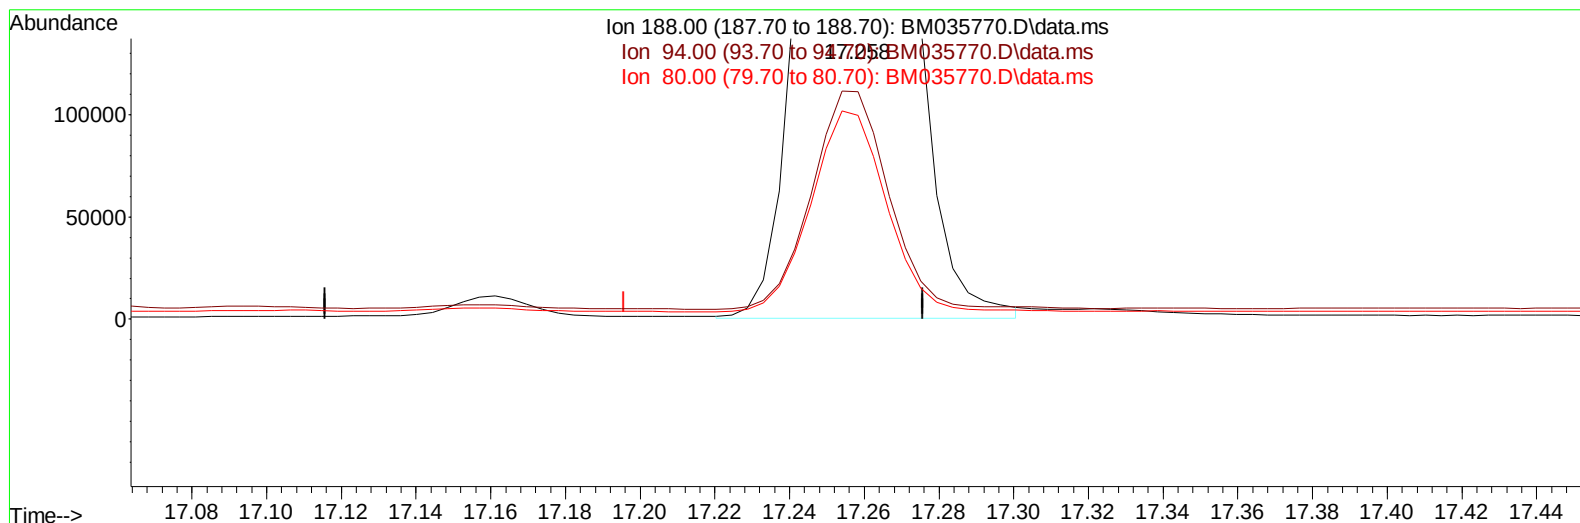

TIC: BM035770.D\data.ms

(13) Phenanthrene-d10 (I)

17.258min (+ 0.063) 0.40 ng/ul m

response 1137942

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	13.59
80.00	12.70	12.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

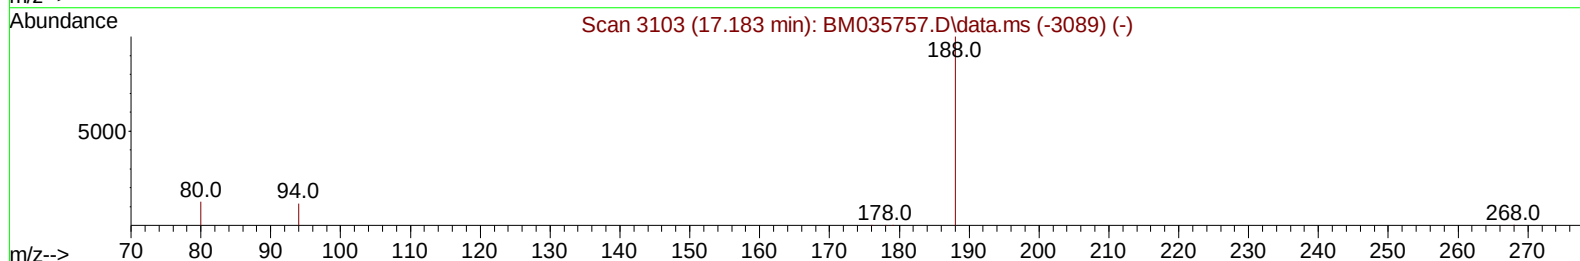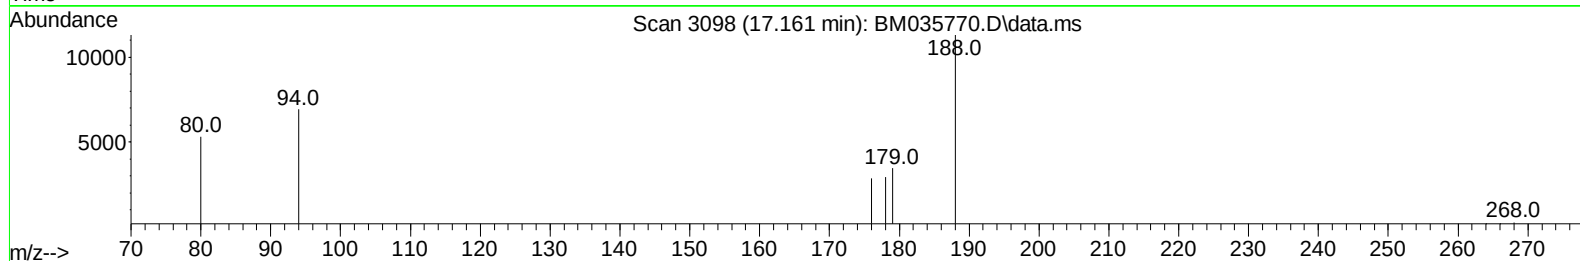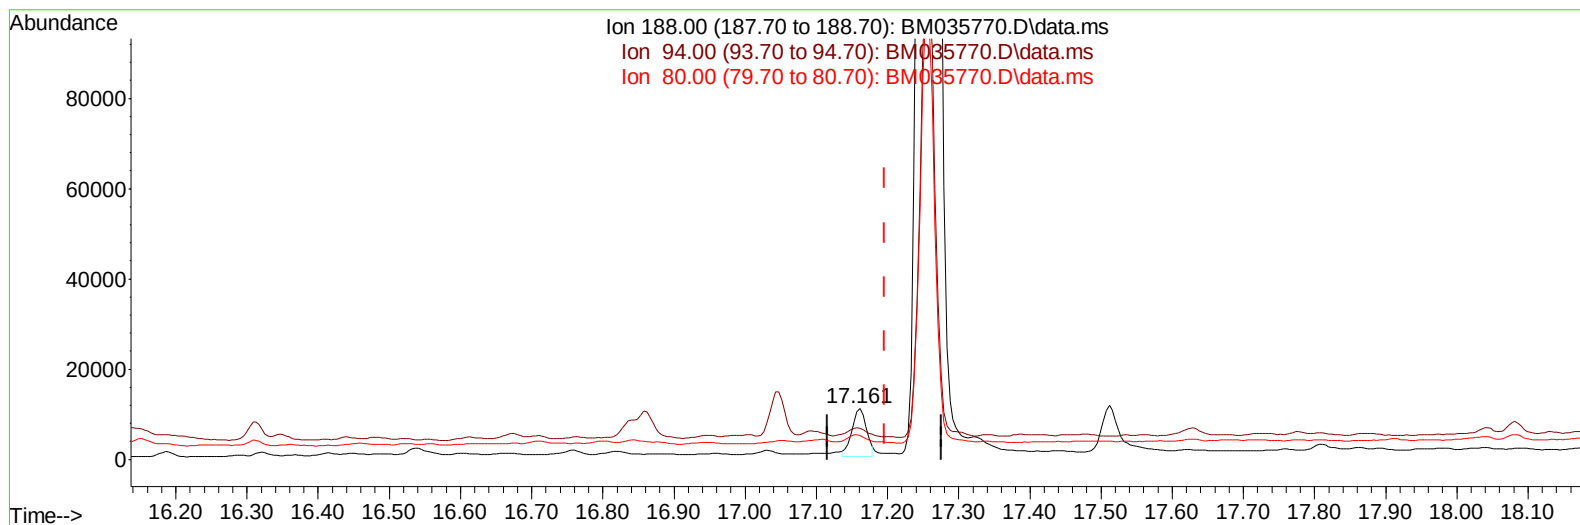

TIC: BM035770.D\data.ms

(13) Phenanthrene-d10 (I)

17.161min (-0.035) 0.40 ng/ul m

response 15320

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	61.30#
80.00	12.70	47.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

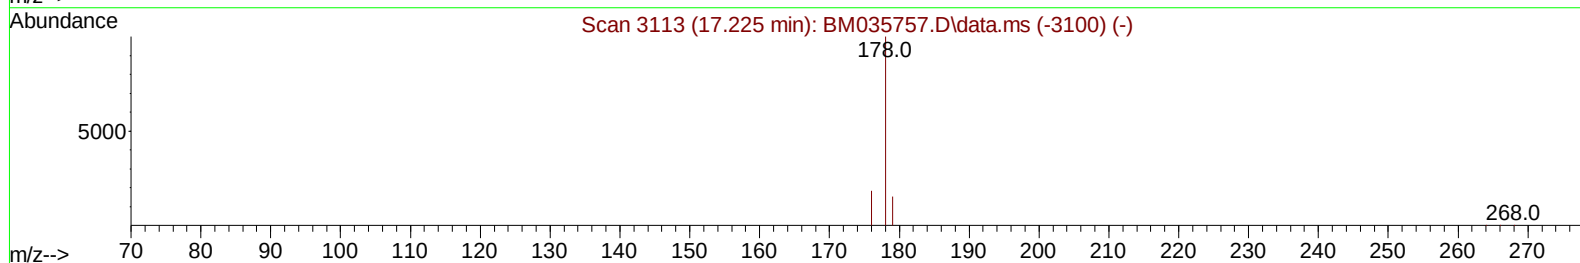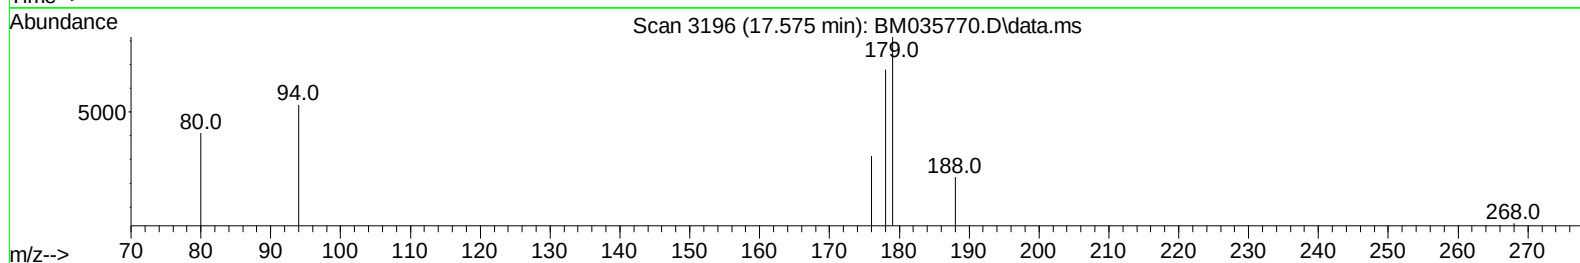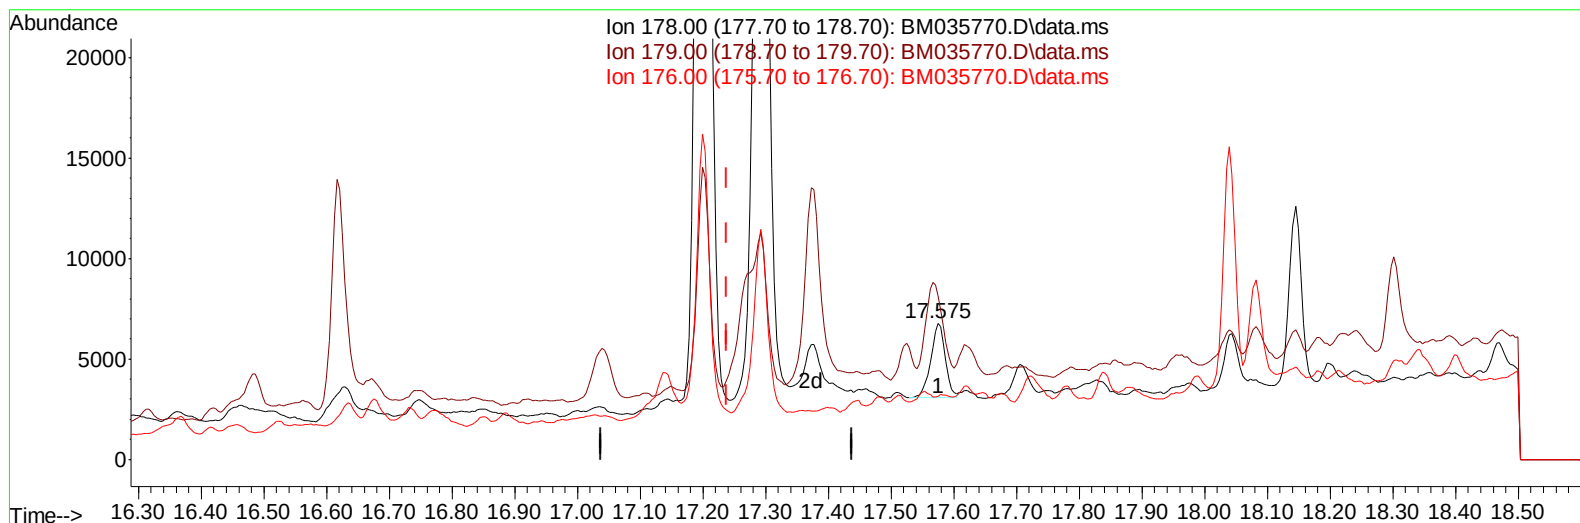

TIC: BM035770.D\data.ms

(15) Phenanthrene

17.575min (+ 0.337) 0.11 ng/ul

response 6015

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	120.23#
176.00	19.50	46.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

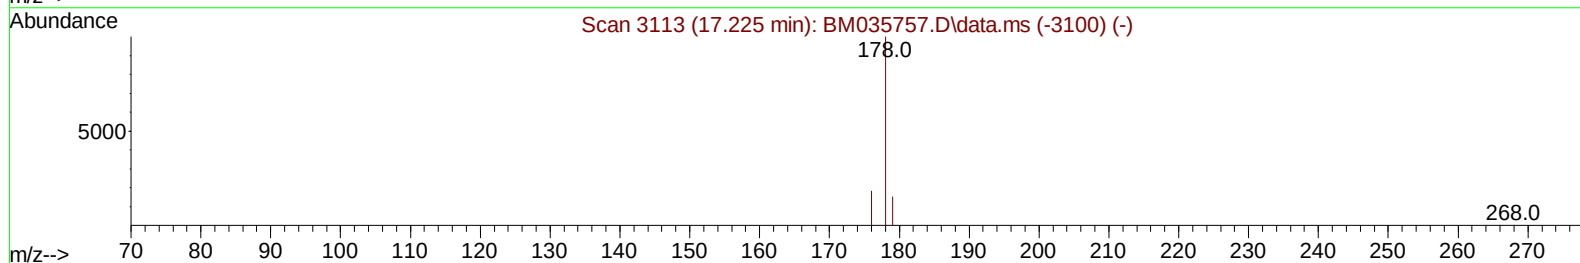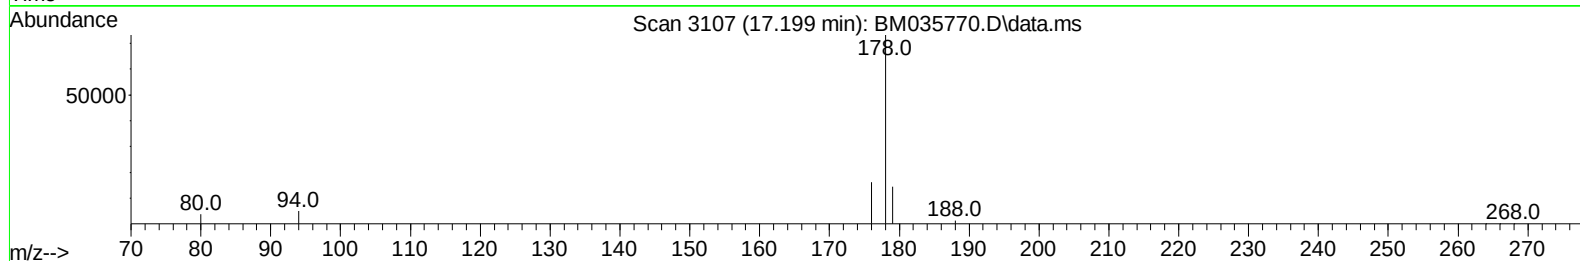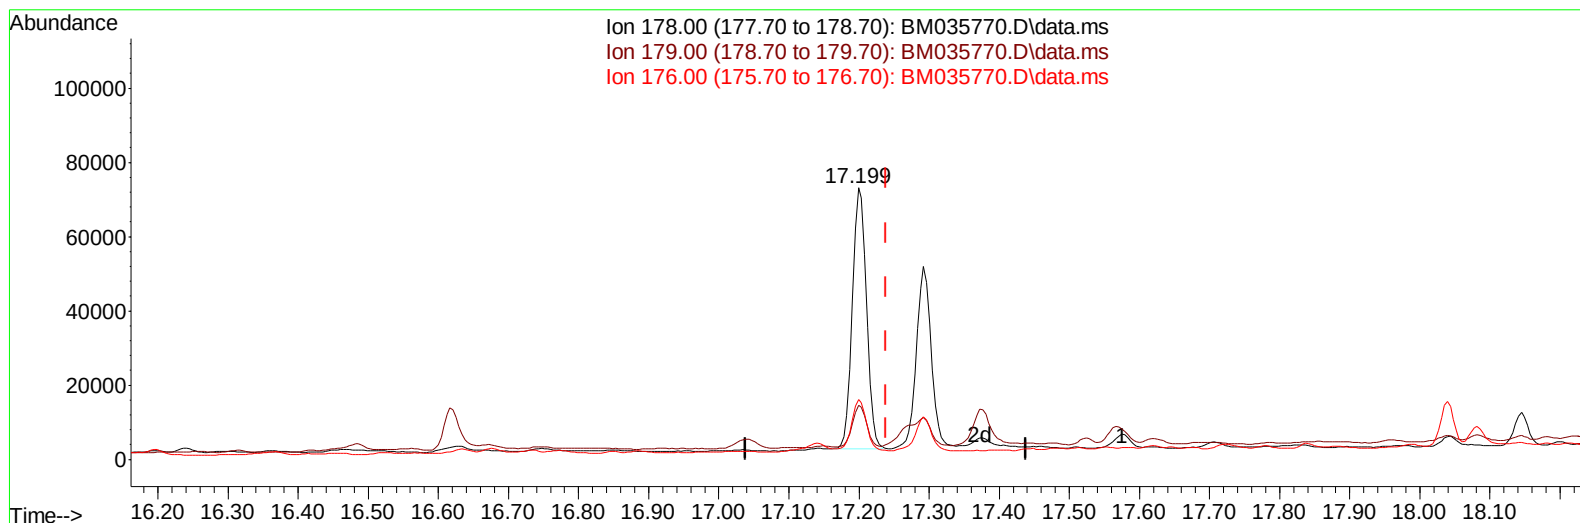

TIC: BM035770.D\data.ms

(15) Phenanthrene

17.199min (-0.039) 1.77 ng/ul m

response 98337

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	19.87#
176.00	19.50	22.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

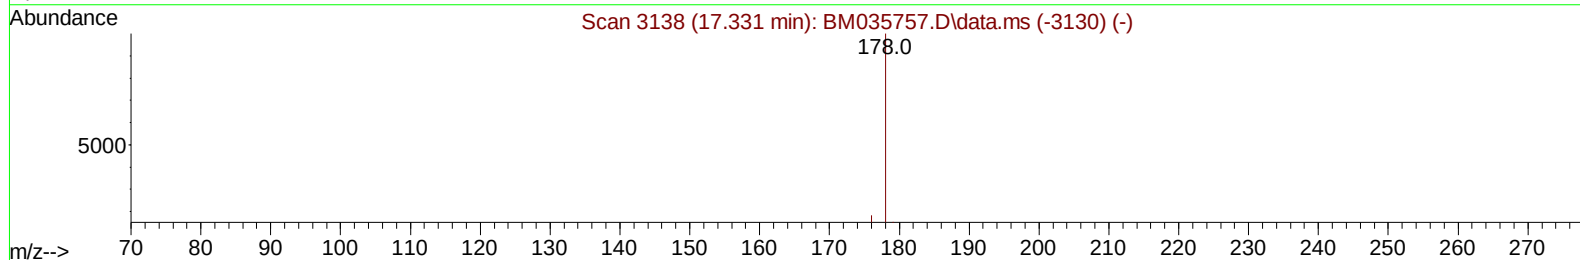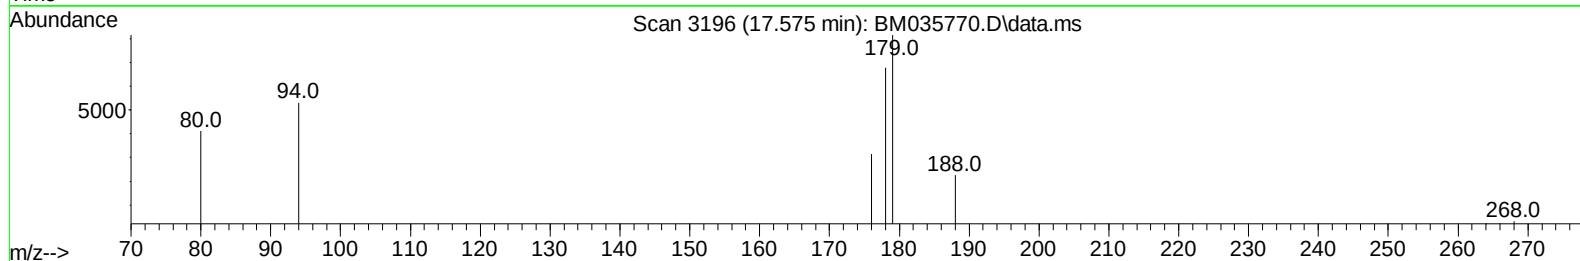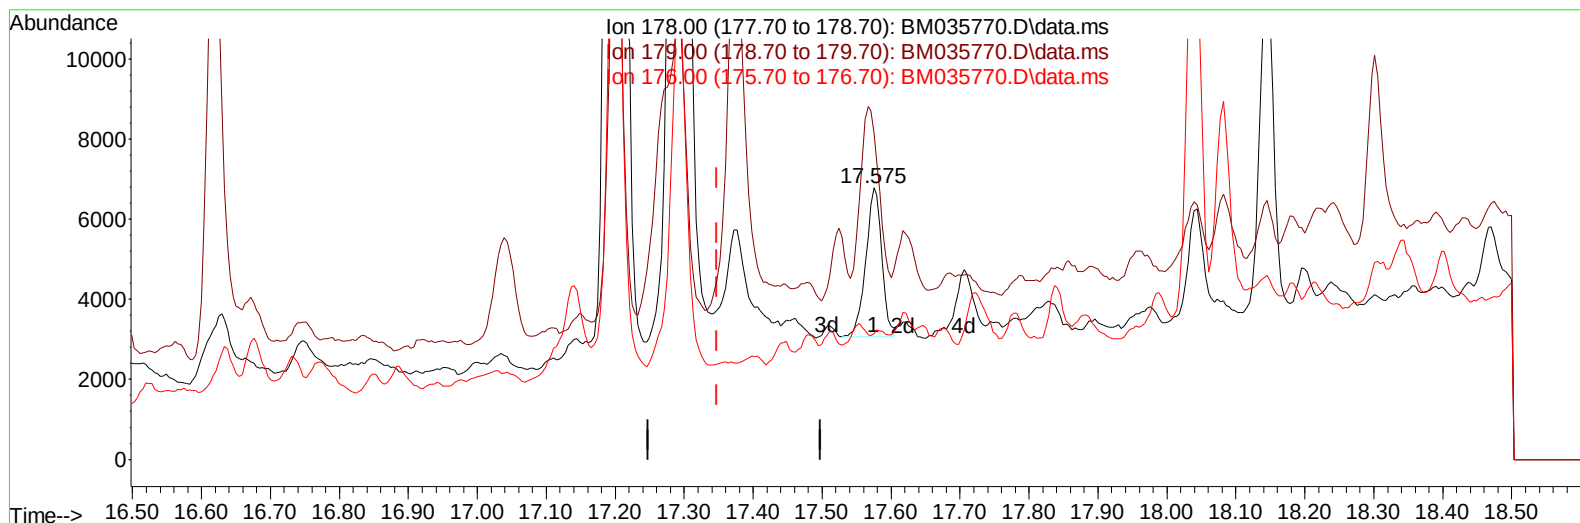

TIC: BM035770.D\data.ms

(16) Anthracene

17.575min (+ 0.227) 0.13 ng/u1

response 6015

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.00	120.23#
176.00	19.50	46.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

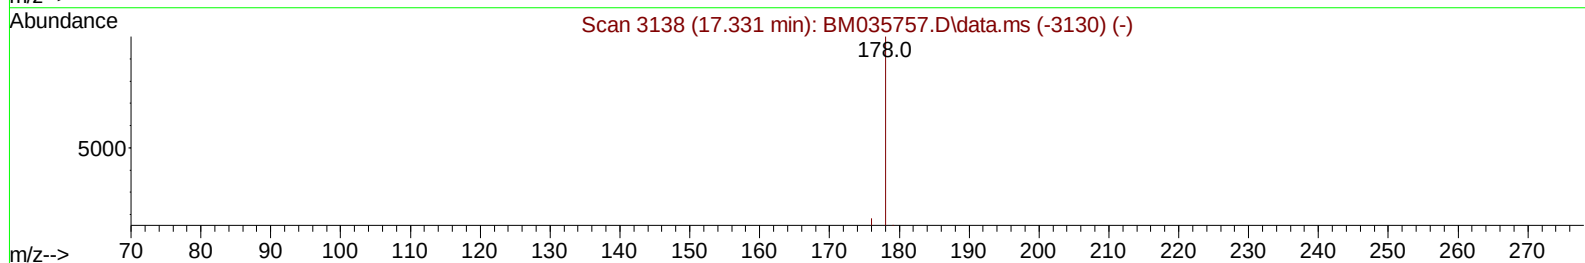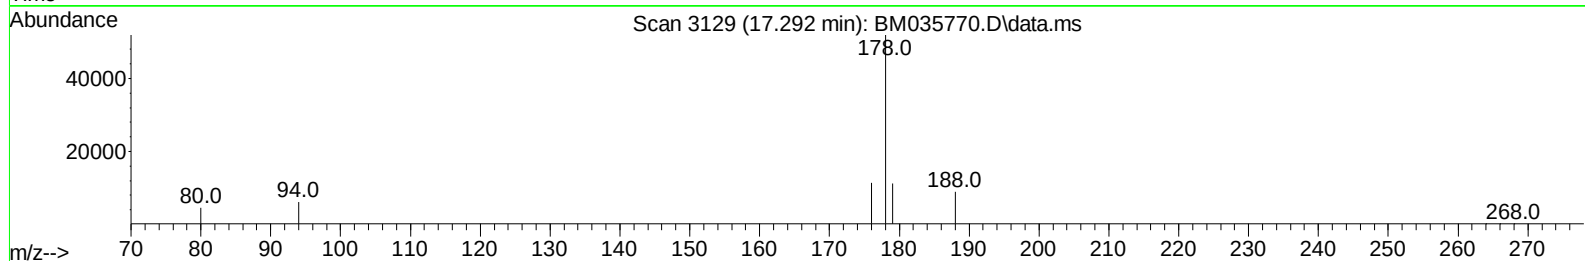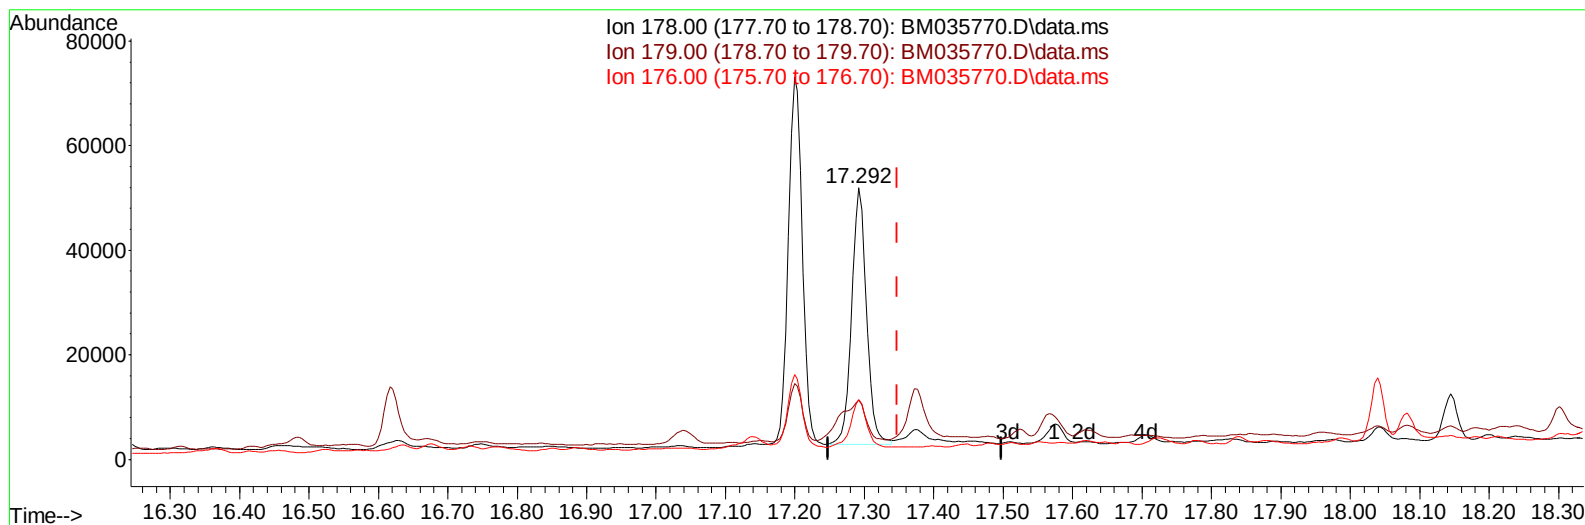

TIC: BM035770.D\data.ms

(16) Anthracene

17.292min (-0.056) 1.59 ng/ul m

response 73332

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.00	21.78#
176.00	19.50	22.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

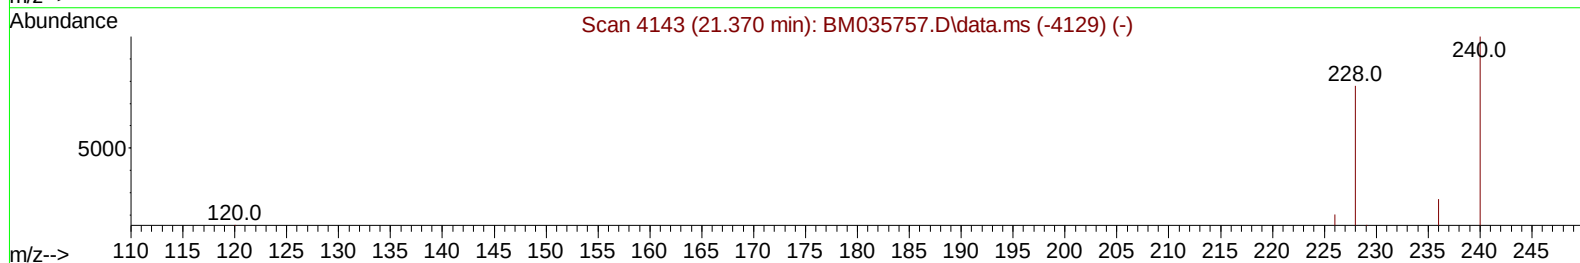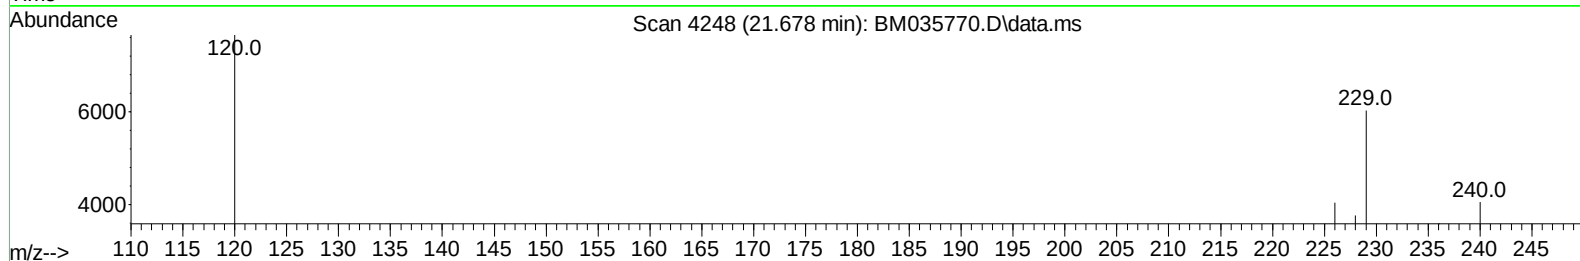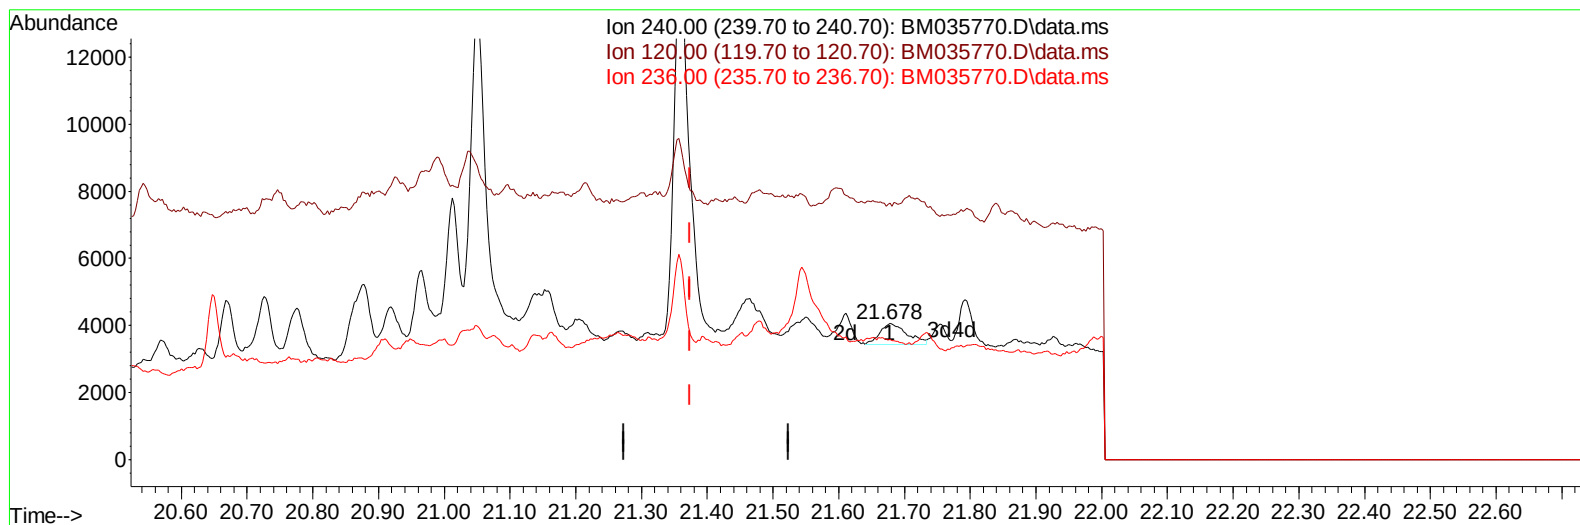

TIC: BM035770.D\data.ms

(17) Chrysene-d12

21.678min (+ 0.305) 0.40 ng/u1

response 1846

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.90	188.63#
236.00	29.40	88.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

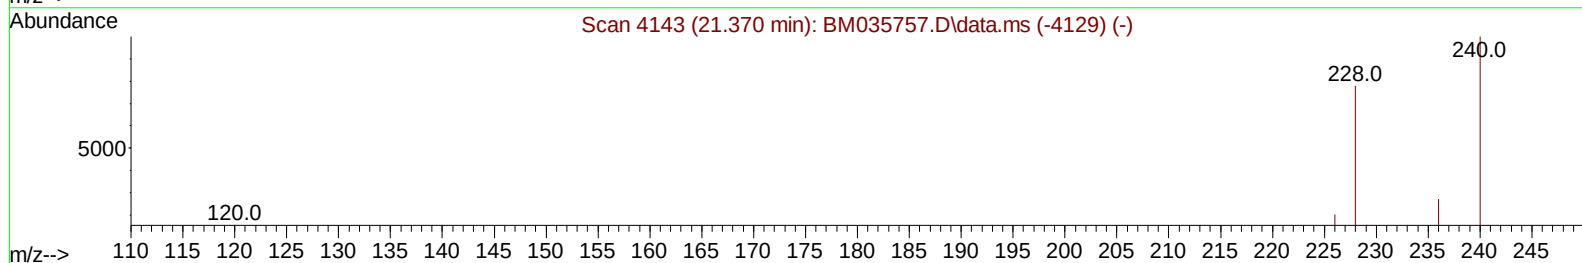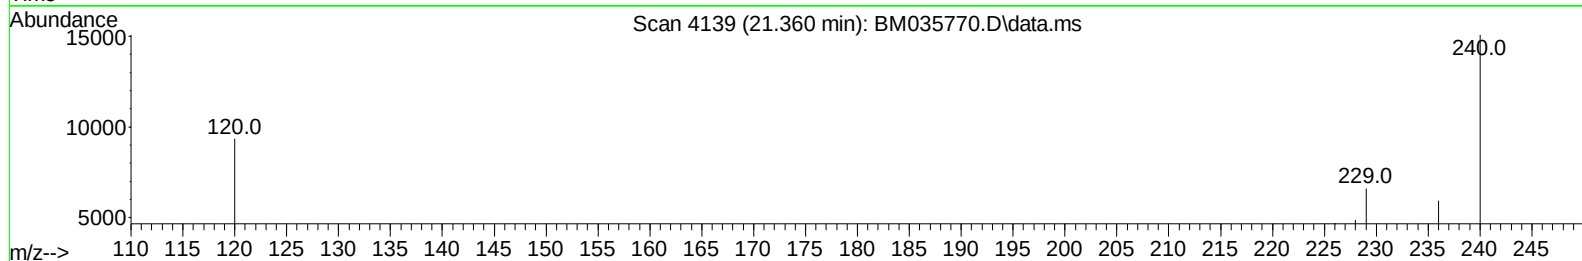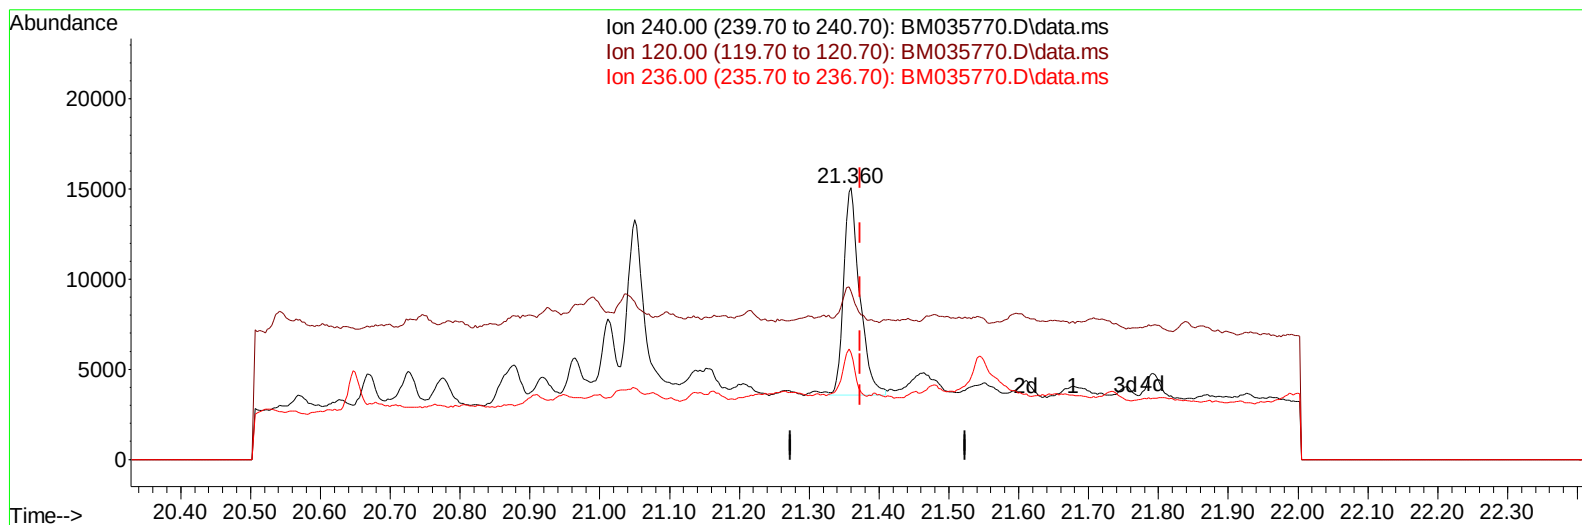

TIC: BM035770.D\data.ms

(17) Chrysene-d12

21.360min (-0.014) 0.40 ng/ul m

response 18399

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.90	61.99#
236.00	29.40	39.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

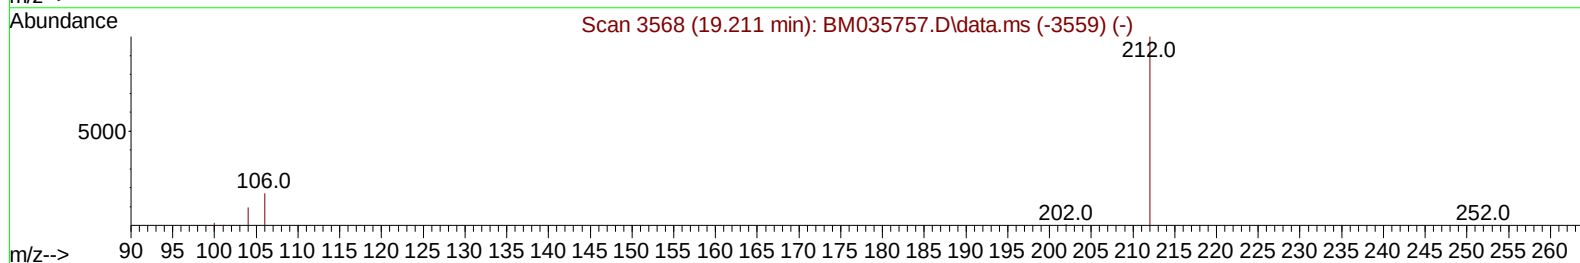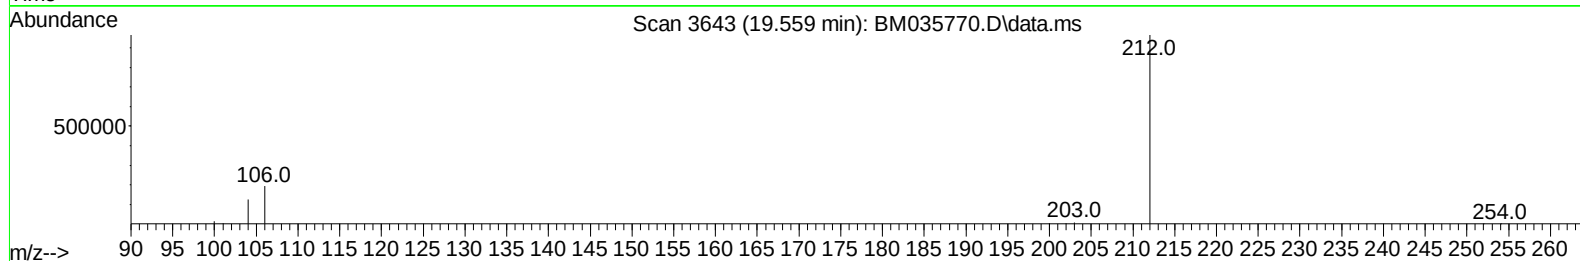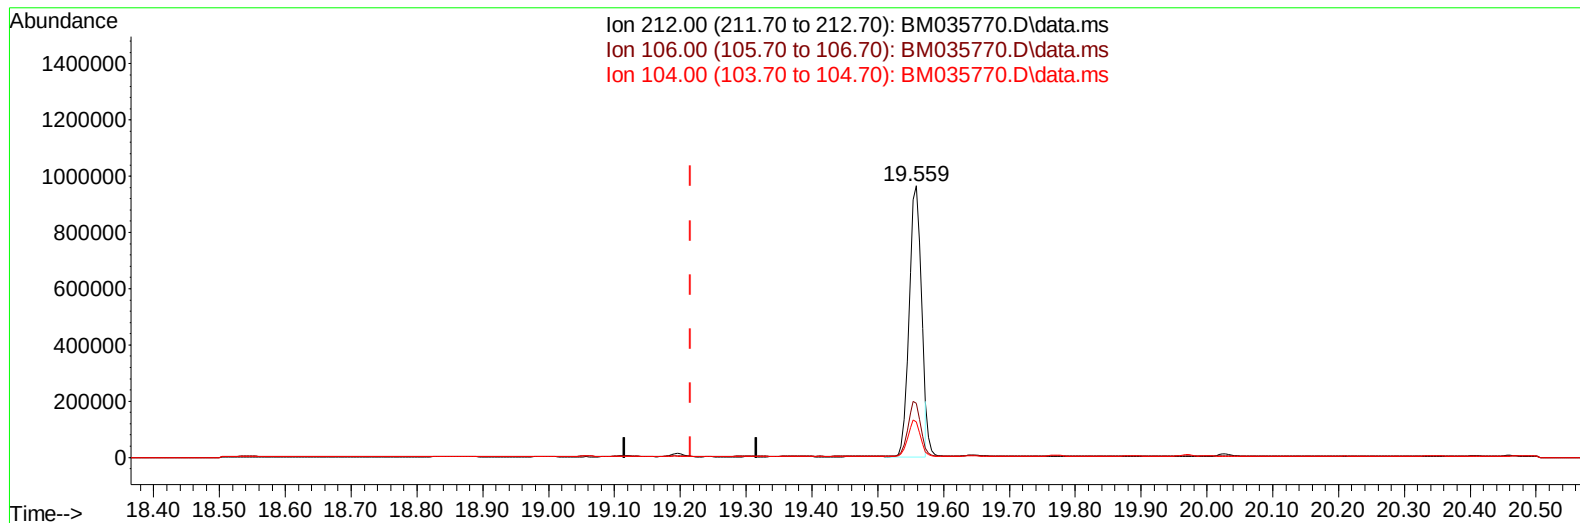

TIC: BM035770.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.559min (+ 0.343) 20.08 ng/u1

response 1245476

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.20	20.38#
104.00	9.70	13.42#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

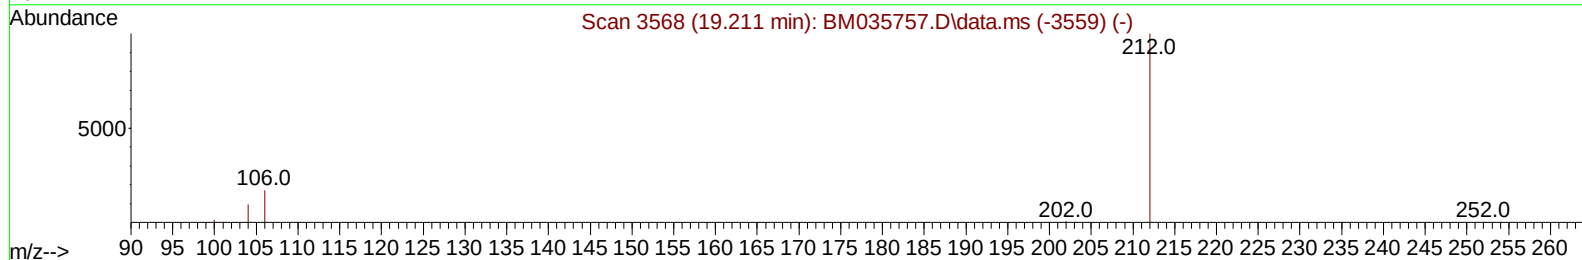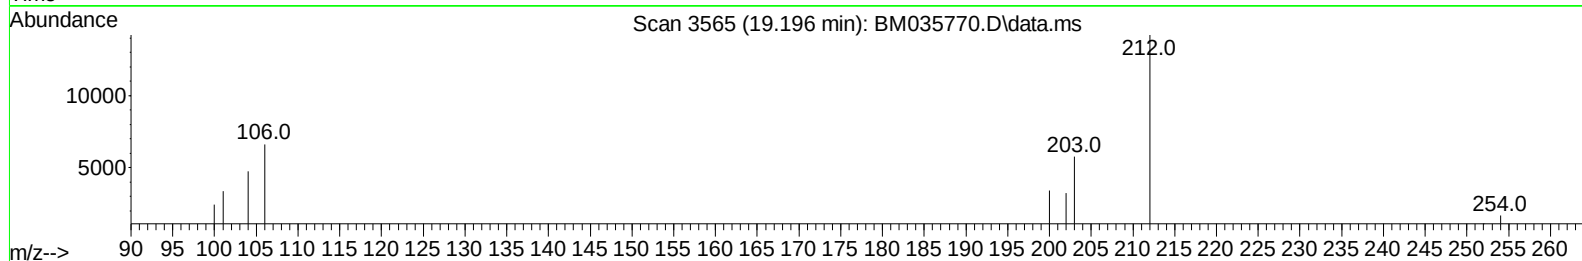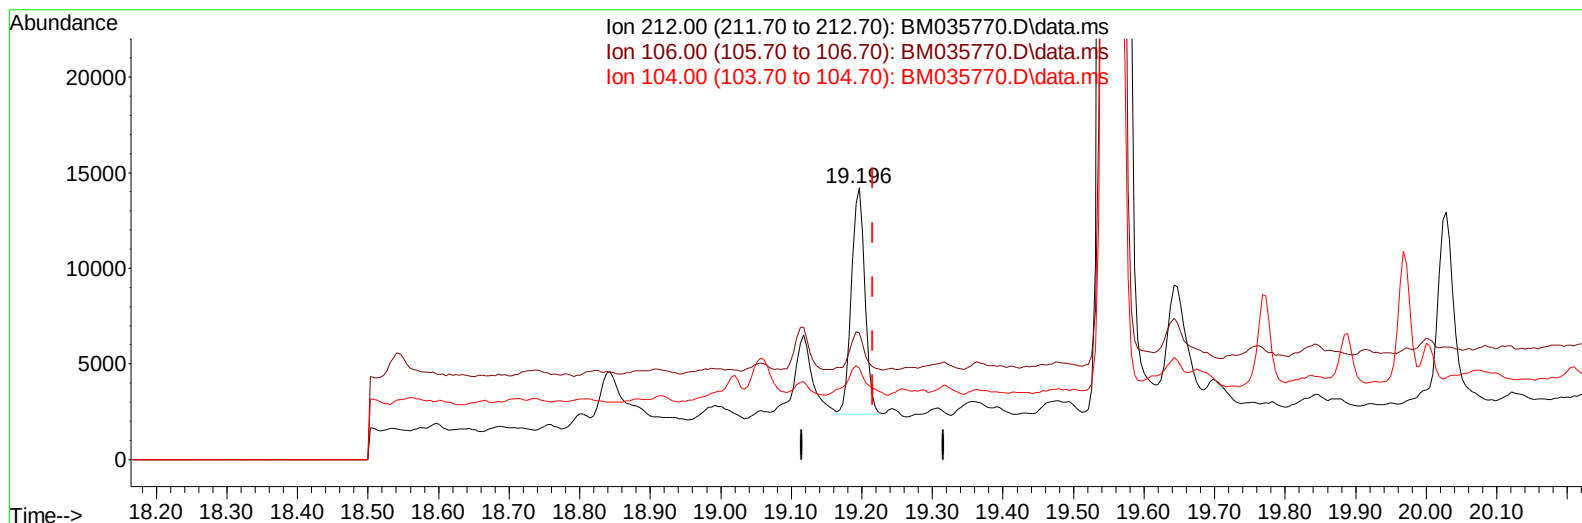

TIC: BM035770.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.196min (-0.019) 0.25 ng/ul m

response 15667

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.20	1619.92#
104.00	9.70	1067.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

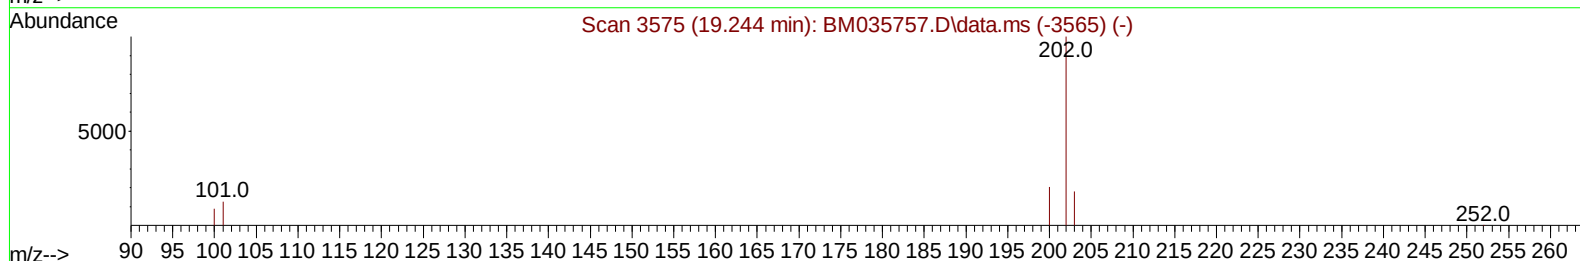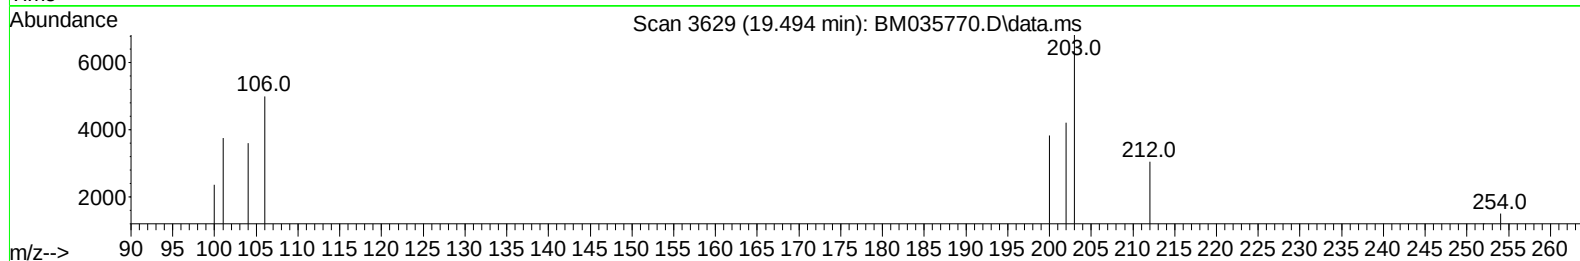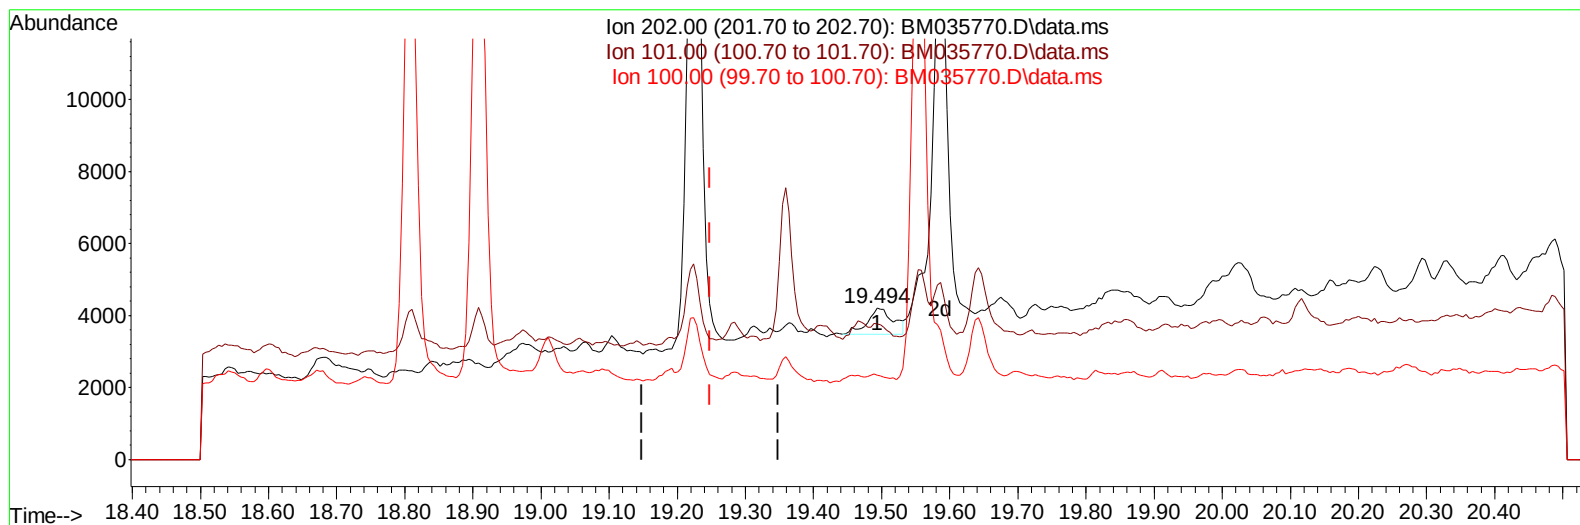

TIC: BM035770.D\data.ms

(19) Fluoranthene (C)

19.494min (+ 0.245) 0.02 ng/u1

response 1950

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.60	89.36#
100.00	9.90	55.77#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

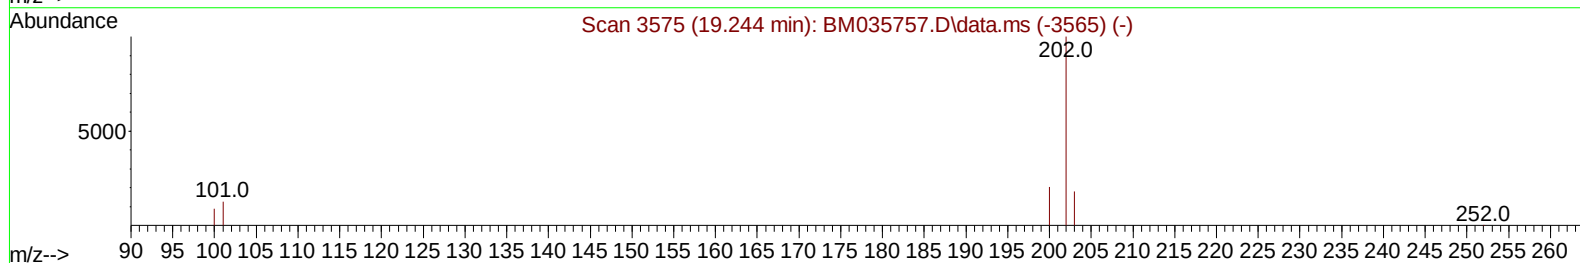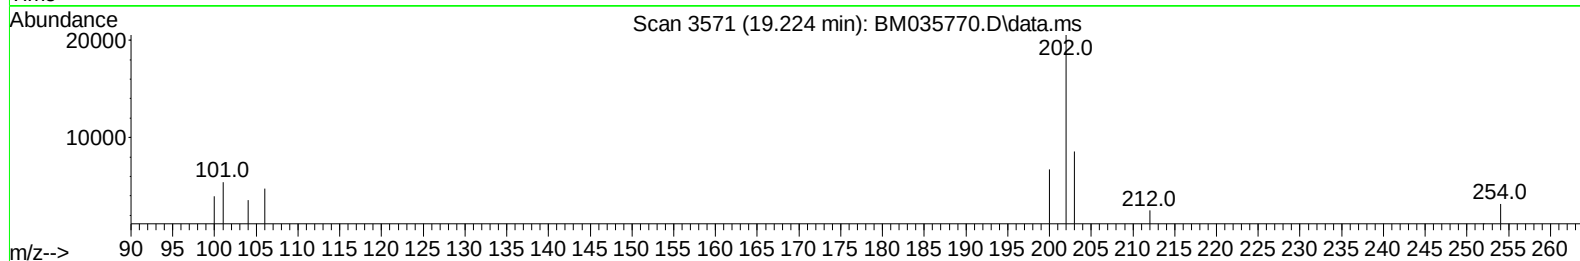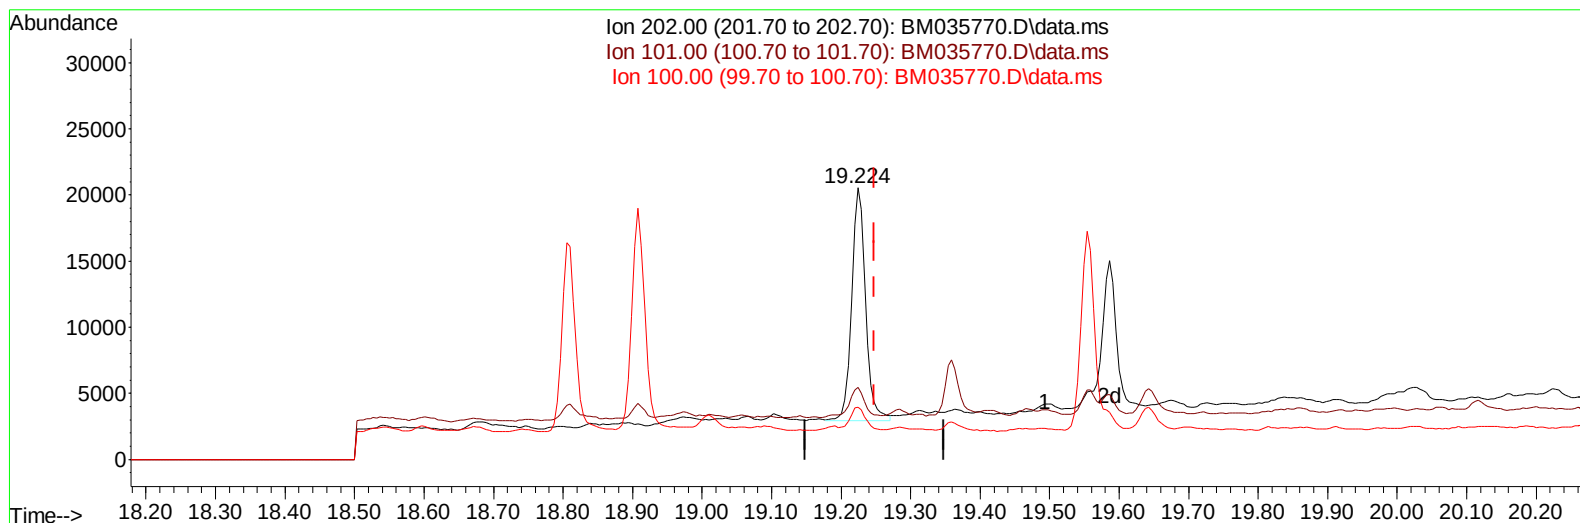

TIC: BM035770.D\data.ms

(19) Fluoranthene (C)

19.224min (-0.024) 0.27 ng/ul m

response 24522

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.60	26.45#
100.00	9.90	19.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

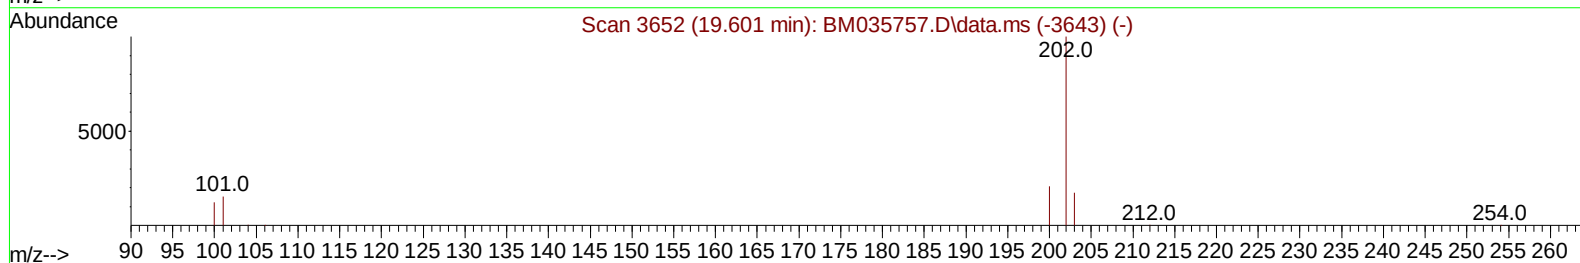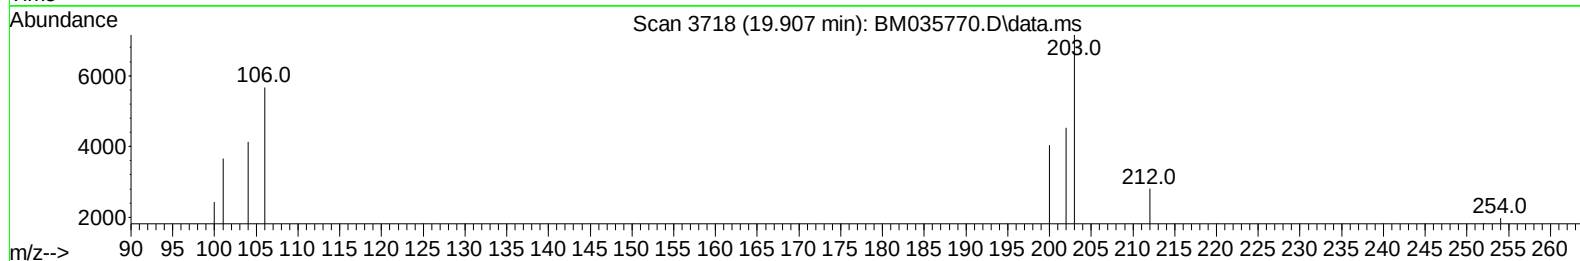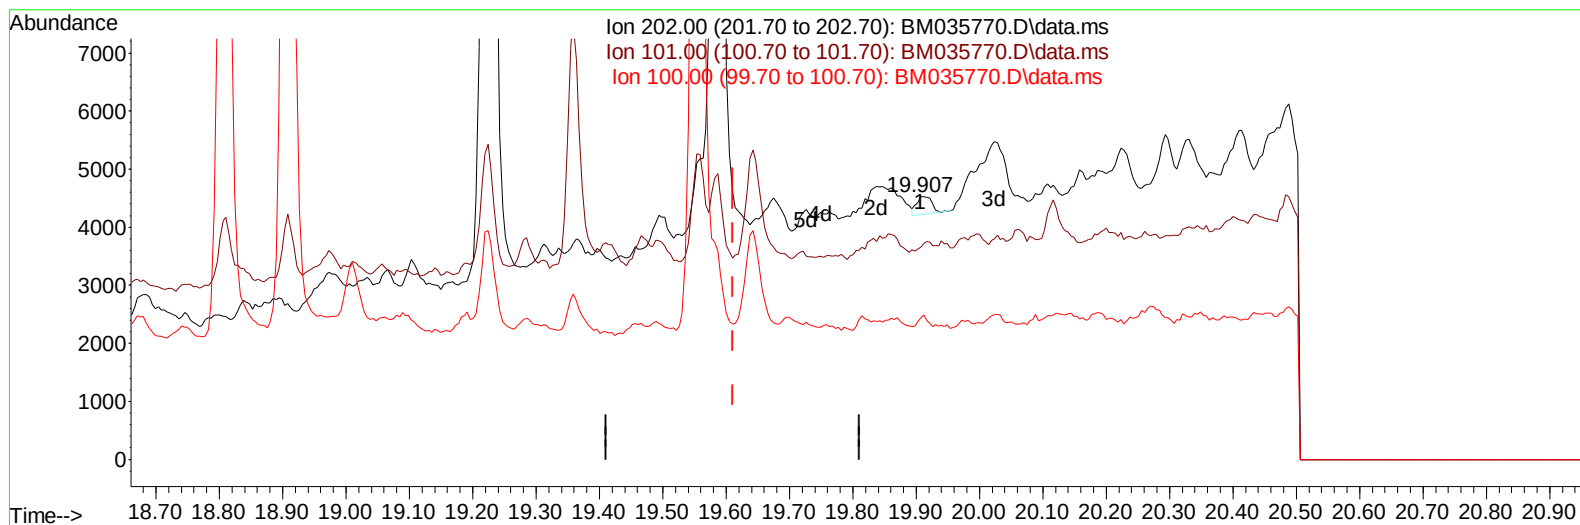

TIC: BM035770.D\data.ms

(20) Pyrene

19.907min (+ 0.297) 0.00 ng/u1

response 516

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	80.62#
100.00	12.20	53.82#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

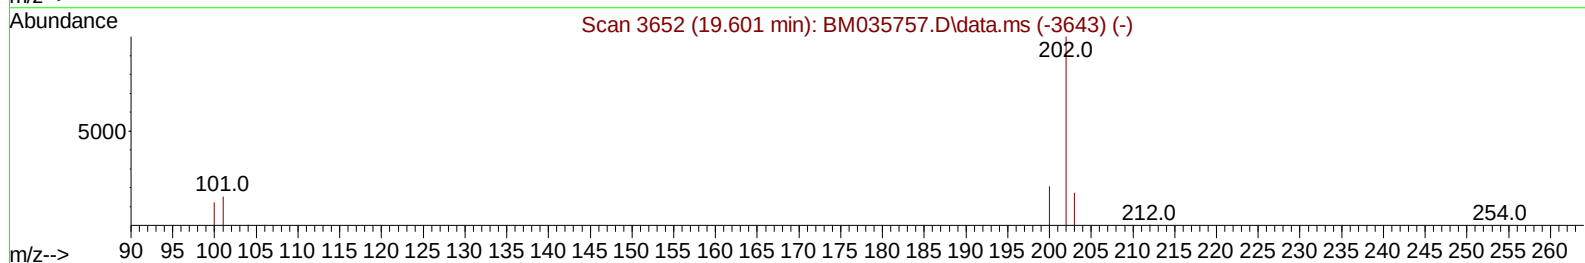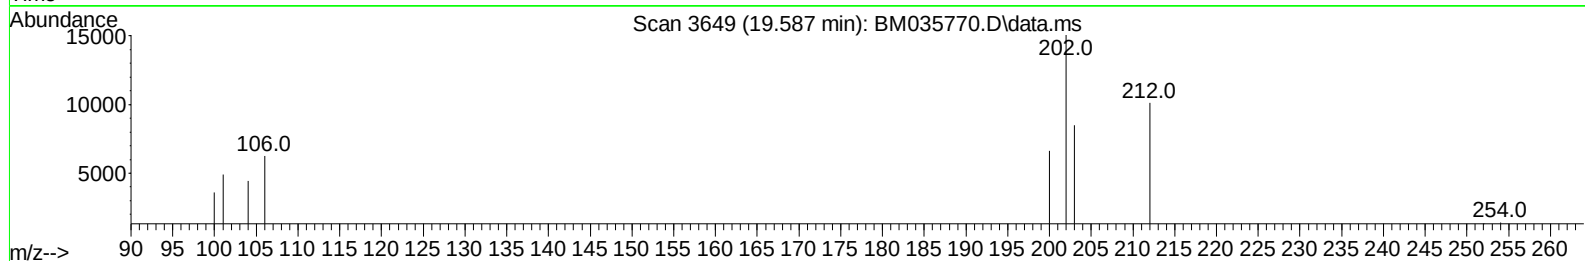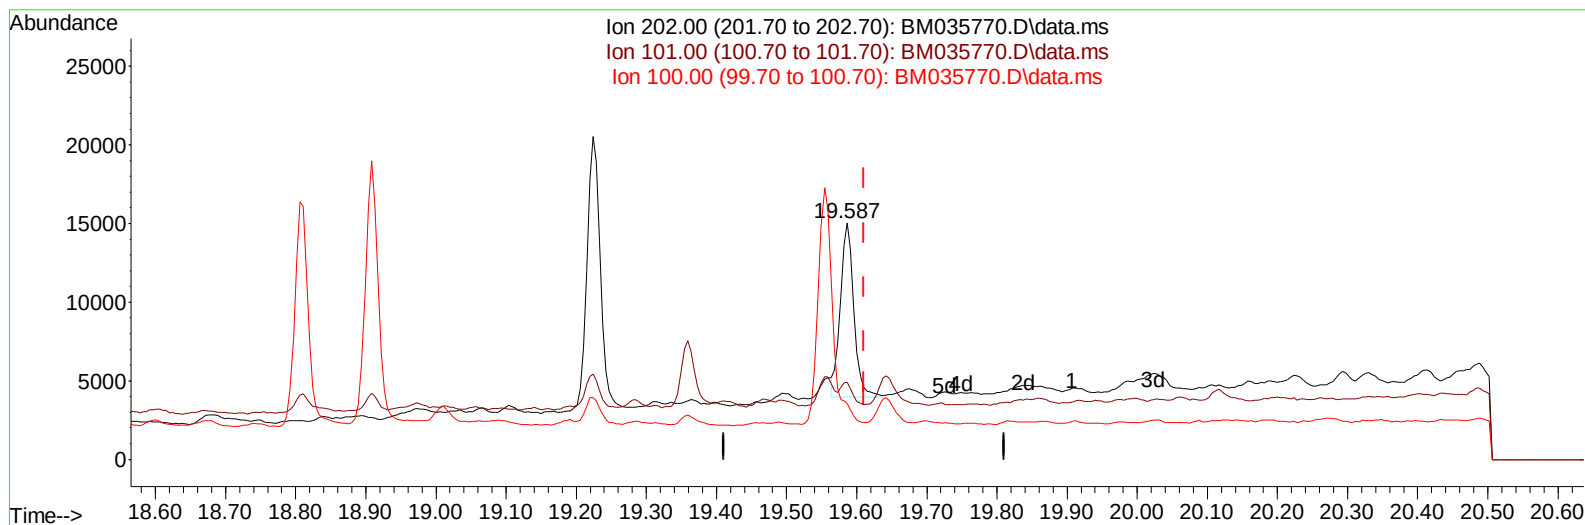

TIC: BM035770.D\data.ms

(20) Pyrene

19.587min (-0.024) 0.14 ng/ul m

response 14854

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	32.69#
100.00	12.20	23.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

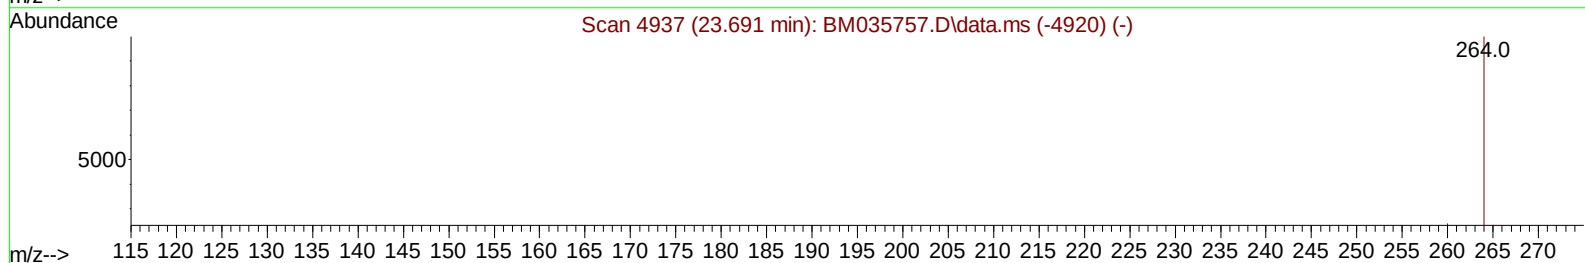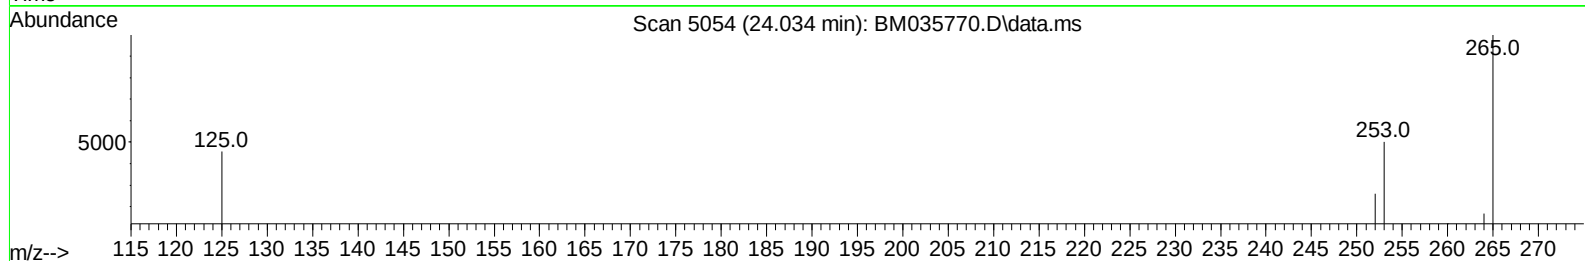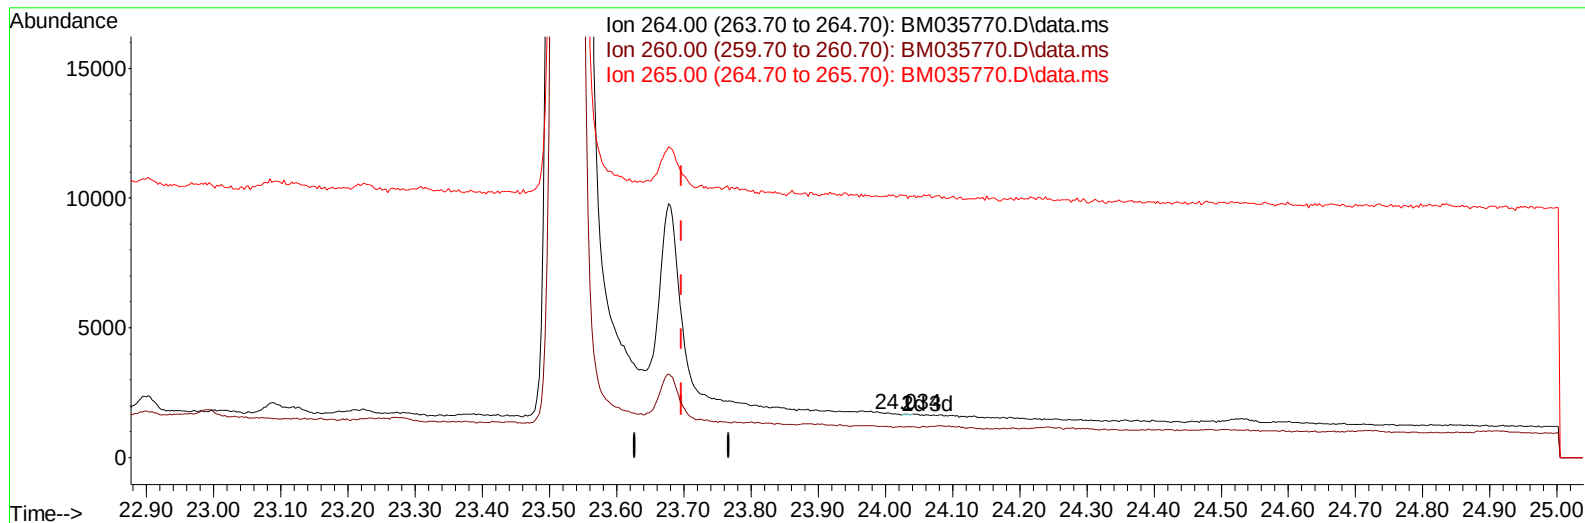

TIC: BM035770.D\data.ms

(23) Perylene-d12 (I)

24.034min (+ 0.337) 0.40 ng/ul

response 17

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	71.39#
265.00	119.70	595.17#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

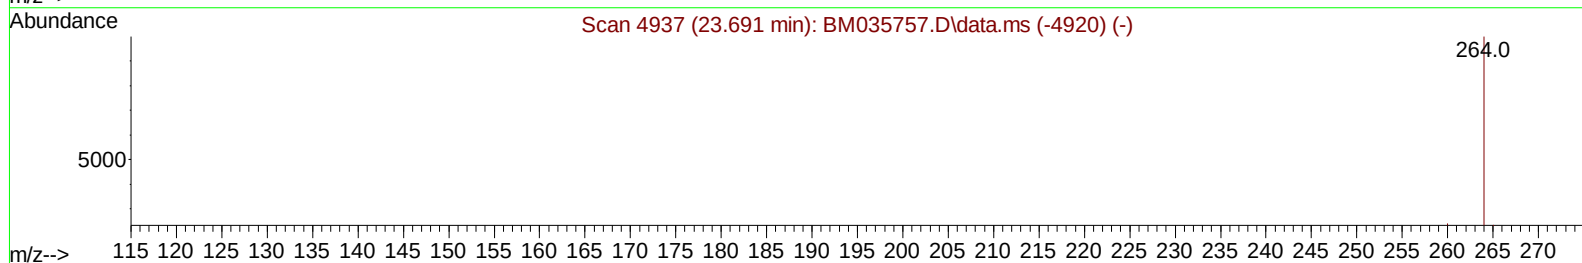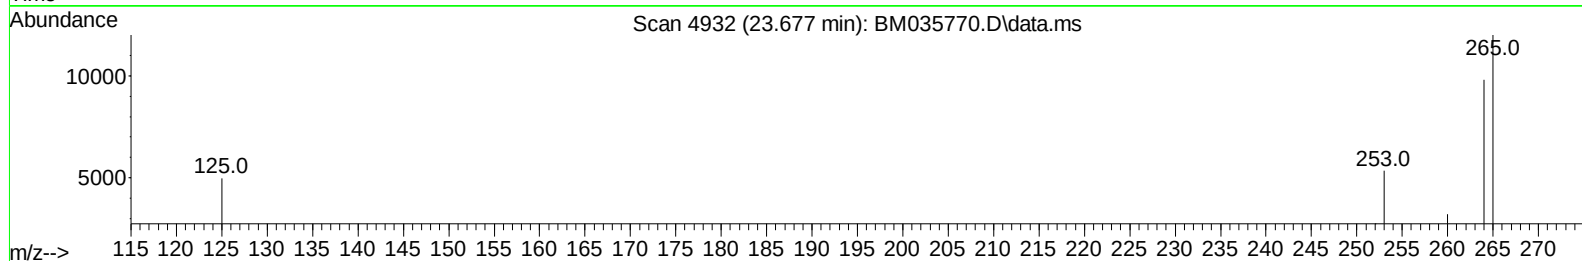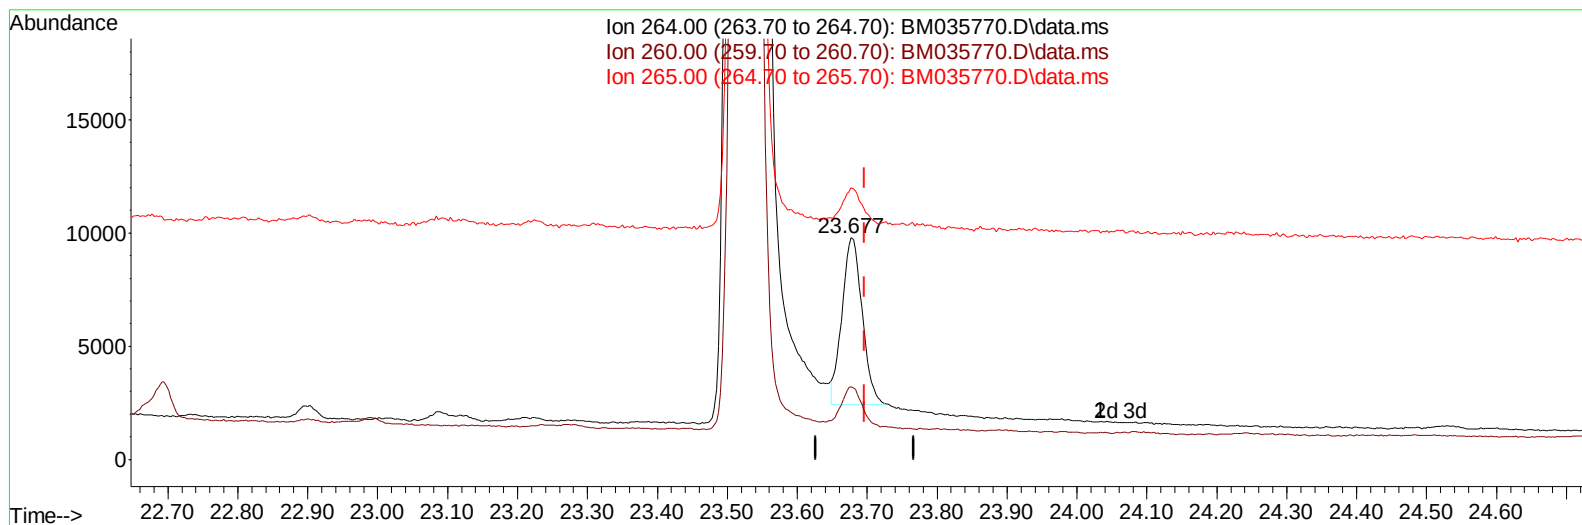

TIC: BM035770.D\data.ms

(23) Perylene-d12 (I)

23.677min (-0.020) 0.40 ng/ul m

response 14821

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	32.83#
265.00	119.70	122.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035770.D
 Acq On : 29 Jun 2022 20:46
 Operator : CG/JU
 Sample : N3374-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/30/2022
 Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 30 04:10:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.778	152		3540m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.567	136		11948m	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.413	164		7829m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.161	188		15320m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.360	240		18399m	0.400	ng/ul	-0.01
23) Perylene-d12	23.677	264		14821m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.213	96		24800	5.162	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.162	152		8605m	0.460	ng/ul	-0.07
18) Fluoranthene-d10	19.196	212		15667m	0.253	ng/ul	-0.02
Target Compounds					Qvalue		
2) 1,4-Dioxane	3.247	88		50510m	10.630	ng/ul	
5) Naphthalene	10.616	128		50059m	1.371	ng/ul	
7) 2-Methylnaphthalene	12.239	142		16169m	0.707	ng/ul	
8) 1-Methylnaphthalene	12.453	142		12575m	0.581	ng/ul	
11) Acenaphthene	14.473	153		33313m	1.054	ng/ul	
12) Fluorene	15.463	166		29282m	0.804	ng/ul	
15) Phenanthrene	17.199	178		98337m	1.771	ng/ul	
16) Anthracene	17.292	178		73332m	1.590	ng/ul	
19) Fluoranthene	19.224	202		24522m	0.266	ng/ul	
20) Pyrene	19.587	202		14854m	0.144	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035770.D
Acq On : 29 Jun 2022 20:46
Operator : CG/JU
Sample : N3374-09
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jun 30 04:10:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/30/2022
Supervised By :mohammad ahmed 07/01/2022

