

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035728.D
 Acq On : 28 Jun 2022 17:32
 Operator : CG/JU
 Sample : N3401-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
 Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 29 04:27:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 04:24:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.791	152	2425	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.578	136	7515	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.423	164	4618	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.171	188	9532m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.371	240	9151	0.400	ng/ul	# 0.00
23) Perylene-d12	23.685	264	11009	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	14687	4.463	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	4060	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.202	212	9666	0.313	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.628	128	1243	0.054	ng/ul#	73
7) 2-Methylnaphthalene	12.277	142	293	0.020	ng/ul	91
21) Benzo(a)anthracene	21.365	228	750	0.024	ng/ul#	32
22) Chrysene	21.411	228	1097	0.027	ng/ul#	51
24) Benzo(b)fluoranthene	22.990	252	1533	0.032	ng/ul#	1
25) Benzo(k)fluoranthene	23.033	252	1425	0.030	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035728.D
Acq On : 28 Jun 2022 17:32
Operator : CG/JU
Sample : N3401-05
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AF9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022


Quant Time: Jun 29 04:27:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 04:24:18 2022
Response via : Initial Calibration

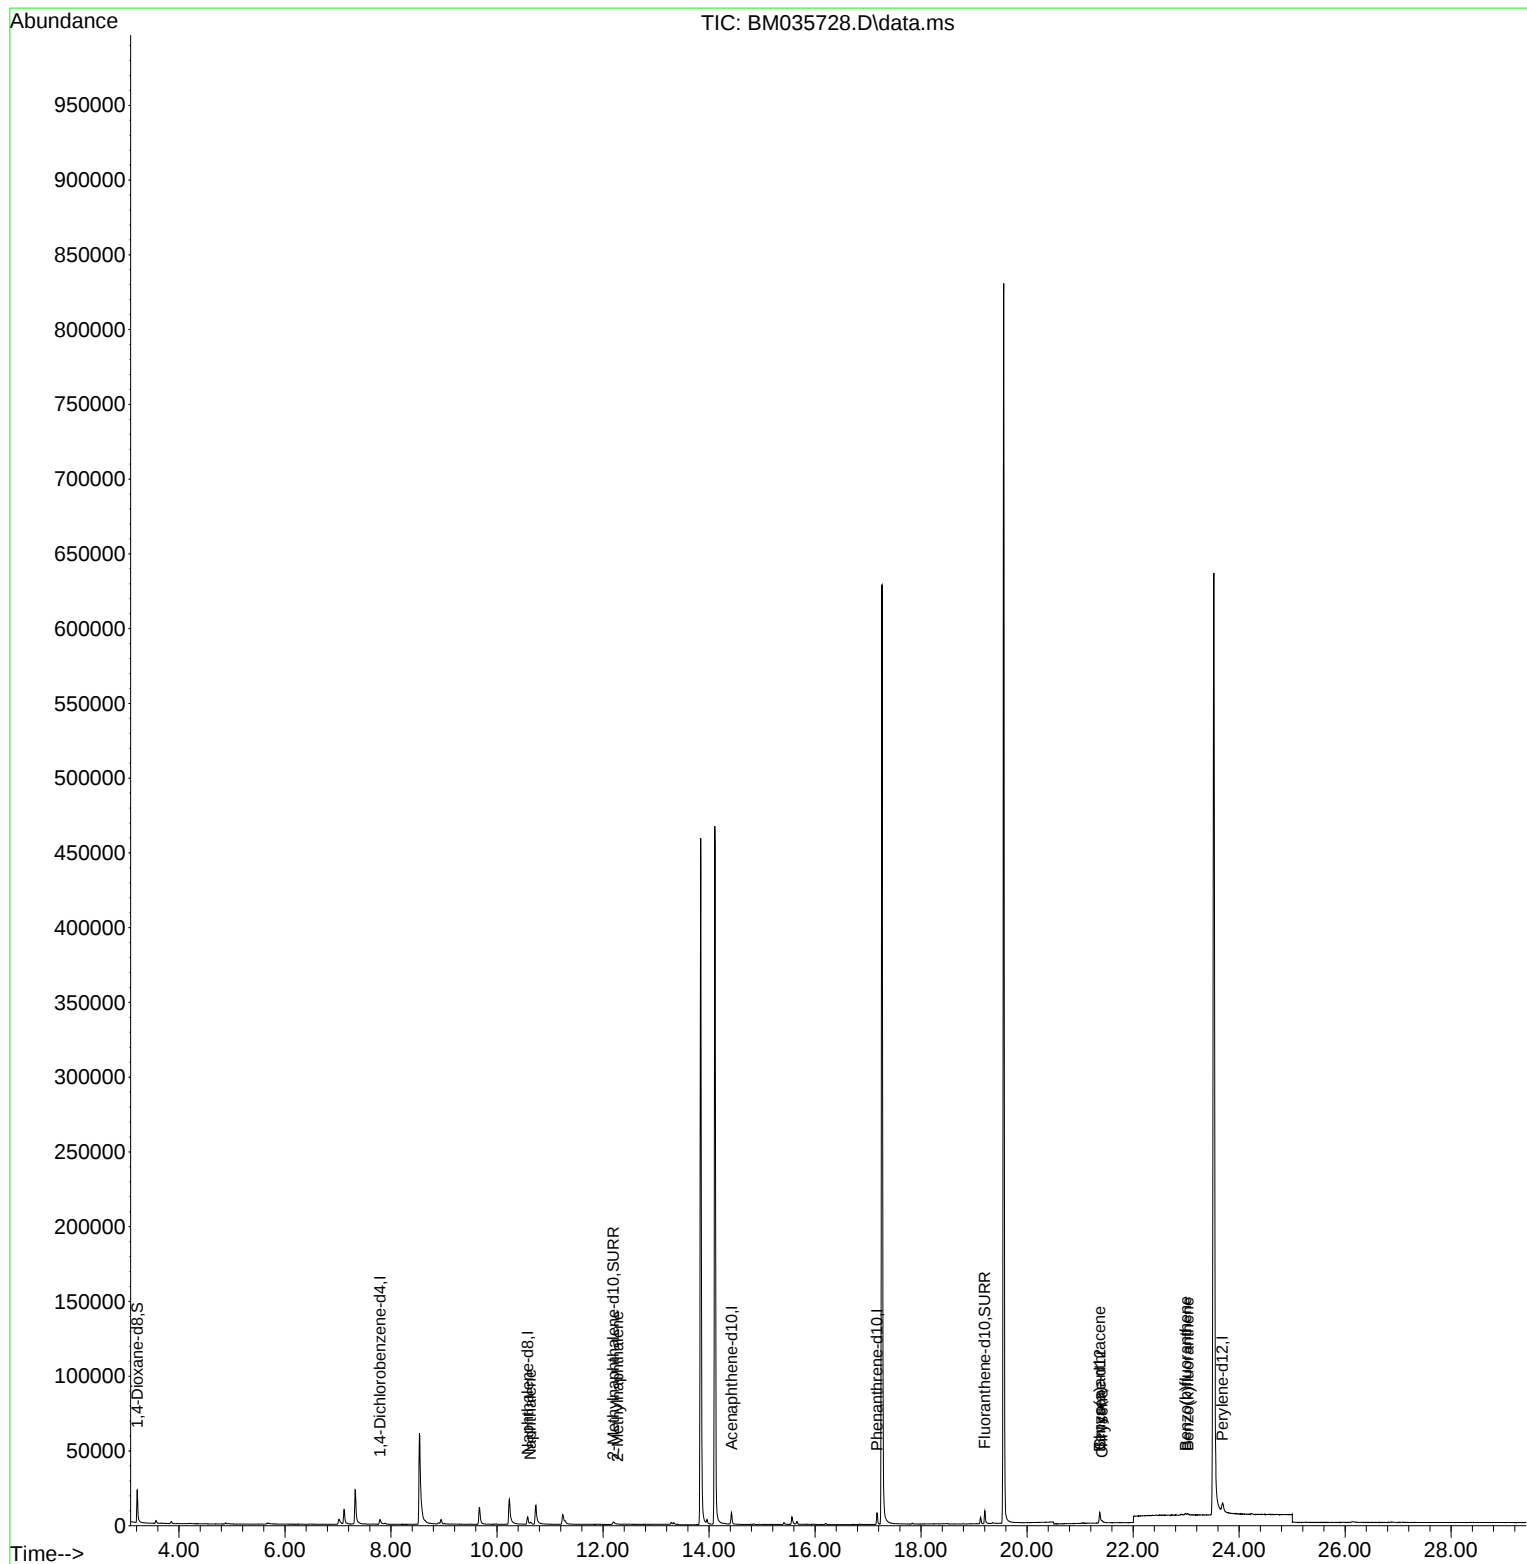

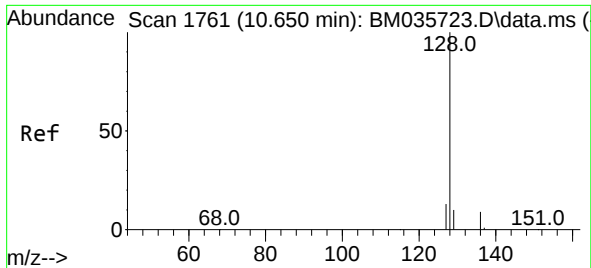

#5
Naphthalene
Concen: 0.054 ng/ul
RT: 10.628 min Scan# 1761
Delta R.T. -0.022 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32




Instrument :
BNA_M
ClientSampleId :
C0AF9

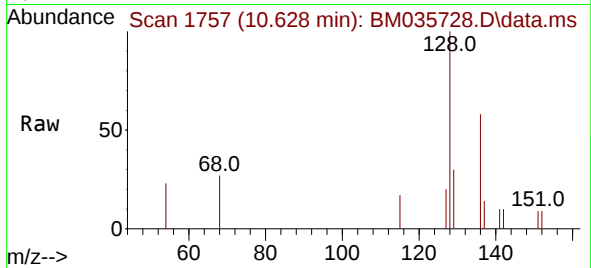

Tgt Ion:128 Resp: 124
Ion Ratio Lower Upper
128 100
129 29.8 10.2 15.2
127 20.1 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022

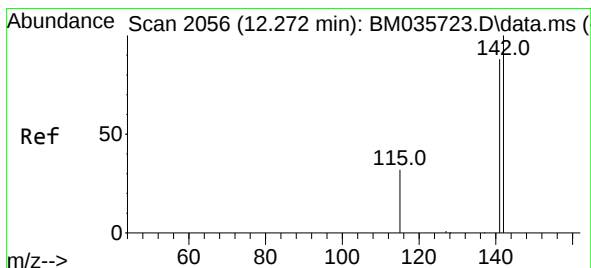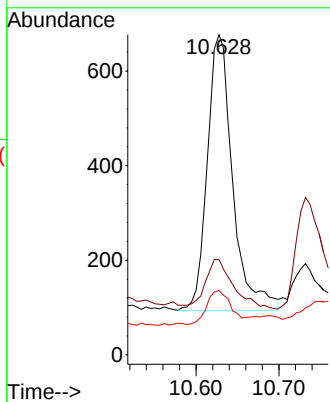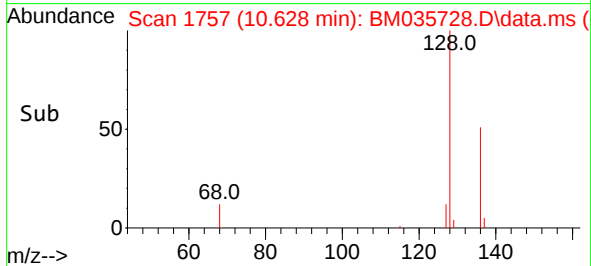

#7
2-Methylnaphthalene
Concen: 0.020 ng/ul
RT: 12.277 min Scan# 2057
Delta R.T. 0.006 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32


Tgt Ion:142 Resp: 293
Ion Ratio Lower Upper
142 100
141 87.7 77.4 116.0

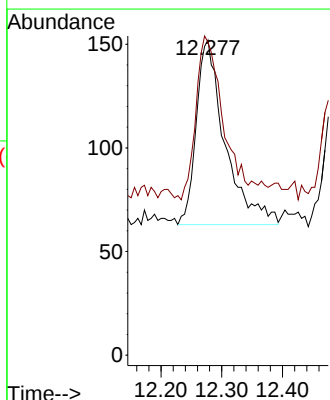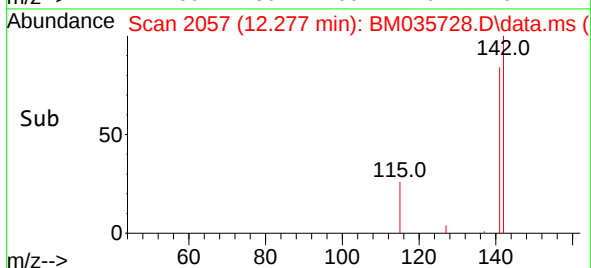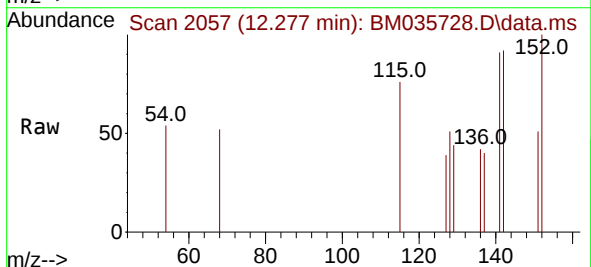

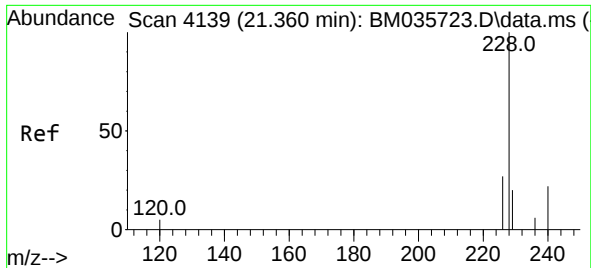

#21
Benzo(a)anthracene
Concen: 0.024 ng/u1
RT: 21.365 min Scan# 4139
Delta R.T. 0.005 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32




Instrument :
BNA_M
ClientSampleId :
C0AF9

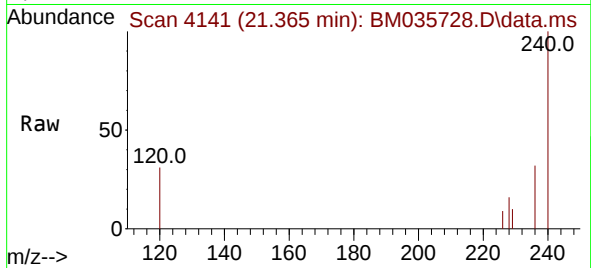

Tgt Ion:228 Resp: 750
Ion Ratio Lower Upper
228 100
229 64.1 16.2 24.2#
226 53.9 22.5 33.7#




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022

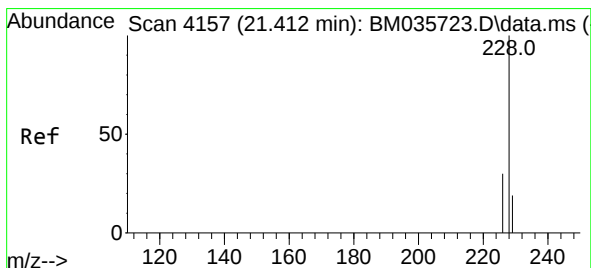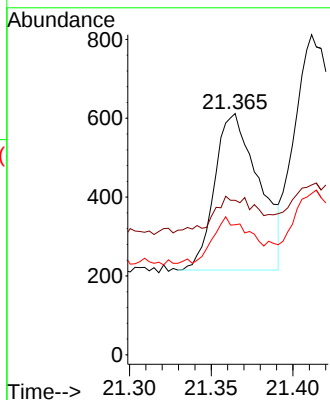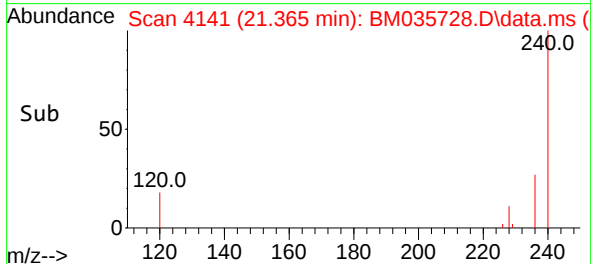

#22
Chrysene
Concen: 0.027 ng/u1
RT: 21.411 min Scan# 4157
Delta R.T. -0.001 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32


Tgt Ion:228 Resp: 1097
Ion Ratio Lower Upper
228 100
226 50.4 24.6 37.0#
229 53.1 16.4 24.6#

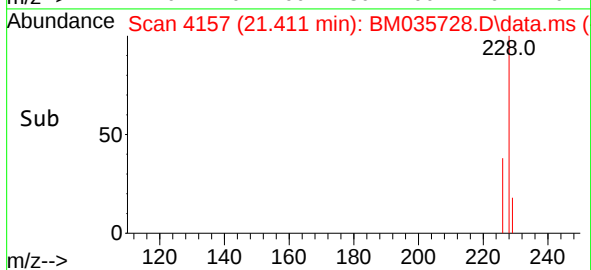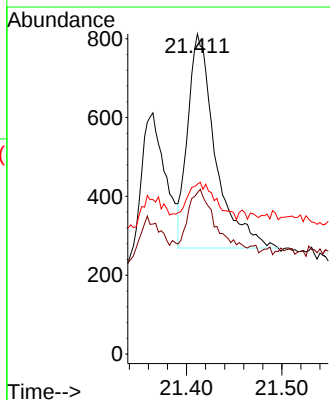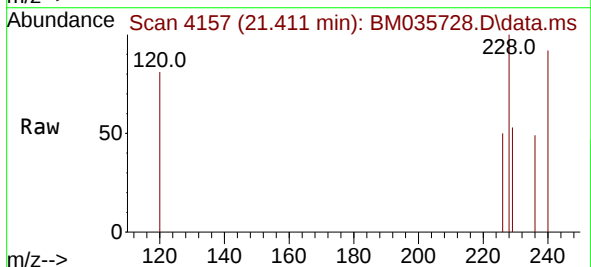

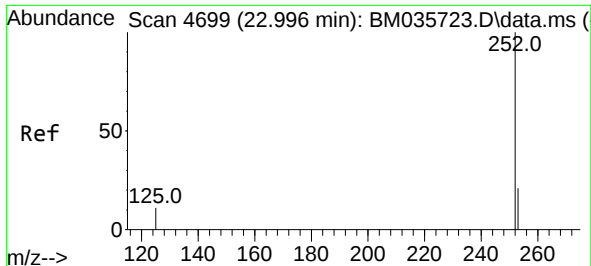

#24
Benzo(b)fluoranthene
Concen: 0.032 ng/ul
RT: 22.990 min Scan# 4699
Delta R.T. -0.007 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32




Instrument :
BNA_M
ClientSampleId :
C0AF9

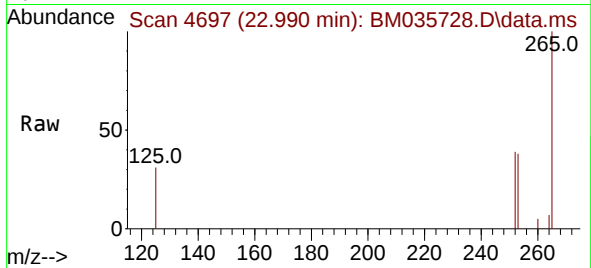


Tgt Ion:252 Resp: 153
Ion Ratio Lower Upper
252 100
253 97.6 0.0 61.4
125 80.4 0.0 42.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022

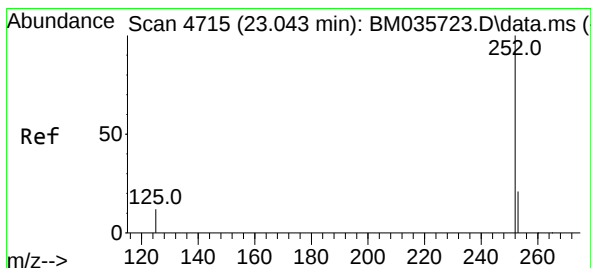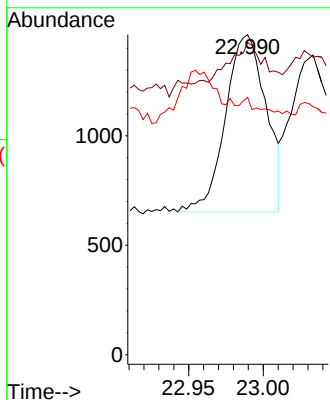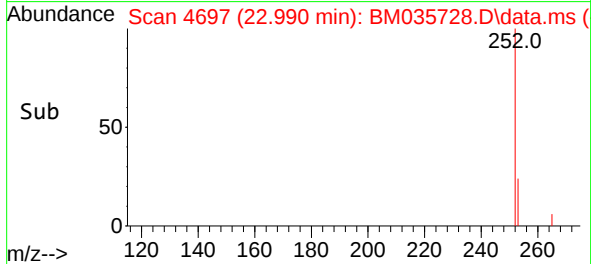

#25
Benzo(k)fluoranthene
Concen: 0.030 ng/ul
RT: 23.033 min Scan# 4712
Delta R.T. -0.010 min
Lab File: BM035728.D
Acq: 28 Jun 2022 17:32

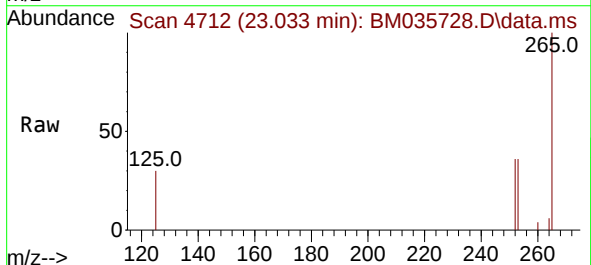

Tgt Ion:252 Resp: 1425
Ion Ratio Lower Upper
252 100
253 99.3 25.2 37.8#
125 82.8 18.3 27.5#

