

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035733.D
 Acq On : 28 Jun 2022 20:39
 Operator : CG/JU
 Sample : N3400-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
 Supervised By :mohammad ahmed 07/01/2022

Quant Time: Jun 29 04:27:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 04:24:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	2097	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.578	136	6936	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.422	164	3842	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.170	188	7404m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.380	240	6548	0.400	ng/ul	# 0.00
23) Perylene-d12	23.686	264	8410	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	14282	5.019	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.211	152	3828	0.352	ng/ul	0.01
18) Fluoranthene-d10	19.206	212	8180	0.371	ng/ul	0.00
Target Compounds						Qvalue
21) Benzo(a)anthracene	21.377	228	528	0.023	ng/ul#	25
22) Chrysene	21.418	228	786	0.027	ng/ul#	44
24) Benzo(b)fluoranthene	22.987	252	1307	0.036	ng/ul#	1
25) Benzo(k)fluoranthene	23.031	252	1034	0.028	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035733.D
Acq On : 28 Jun 2022 20:39
Operator : CG/JU
Sample : N3400-21
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AF6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022


Quant Time: Jun 29 04:27:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 04:24:18 2022
Response via : Initial Calibration

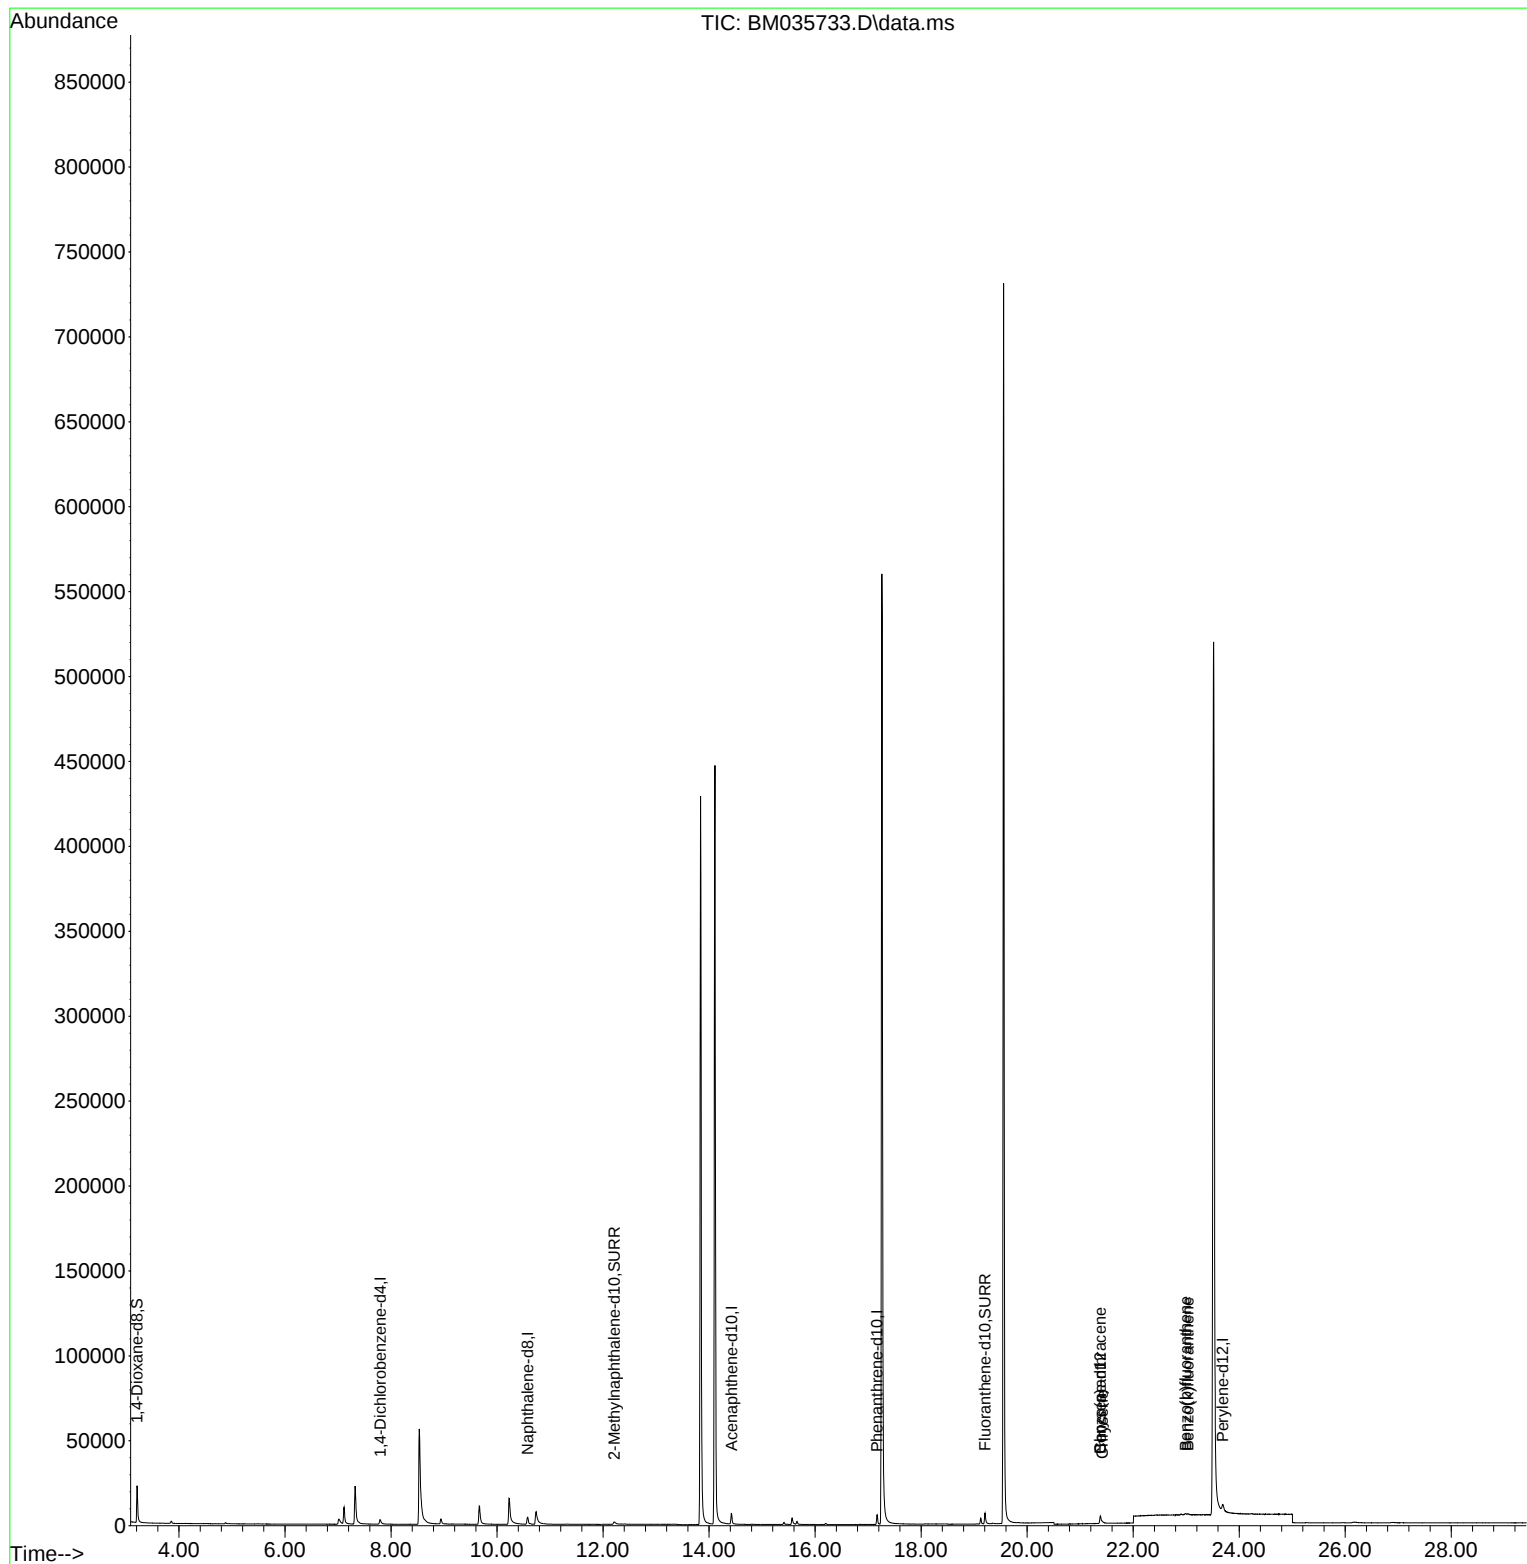

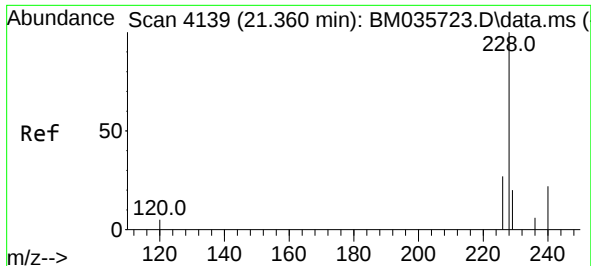

#21
Benzo(a)anthracene
Concen: 0.023 ng/u1
RT: 21.377 min Scan# 4139
Delta R.T. 0.018 min
Lab File: BM035733.D
Acq: 28 Jun 2022 20:39




Instrument :
BNA_M
ClientSampleId :
C0AF6

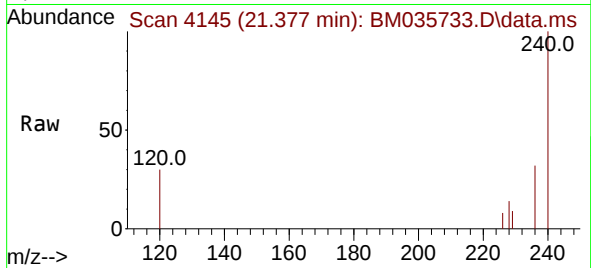


Tgt Ion:228 Resp: 528
Ion Ratio Lower Upper
228 100
229 64.4 16.2 24.2#
226 59.7 22.5 33.7#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022

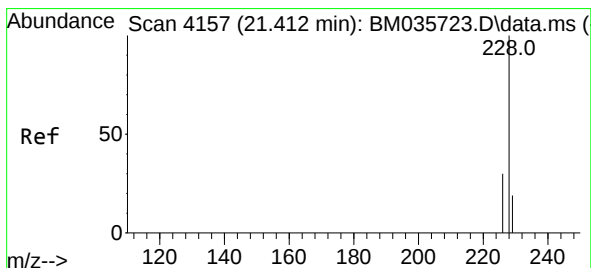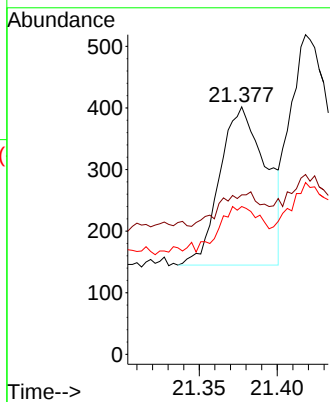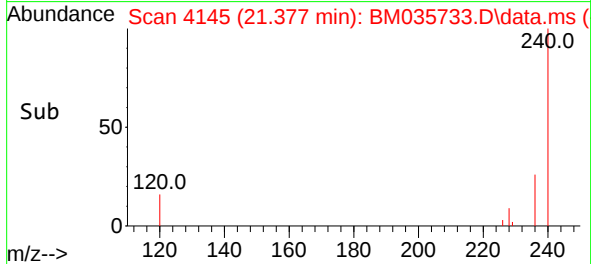


#22
Chrysene
Concen: 0.027 ng/u1
RT: 21.418 min Scan# 4159
Delta R.T. 0.006 min
Lab File: BM035733.D
Acq: 28 Jun 2022 20:39

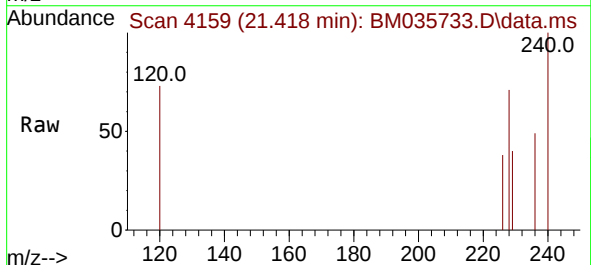


Tgt Ion:228 Resp: 786
Ion Ratio Lower Upper
228 100
226 53.8 24.6 37.0#
229 56.3 16.4 24.6#

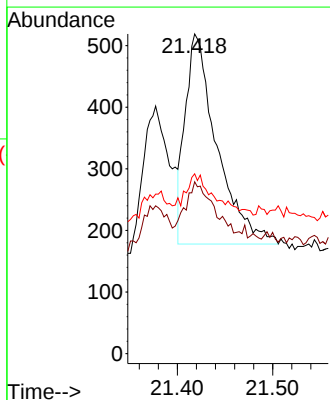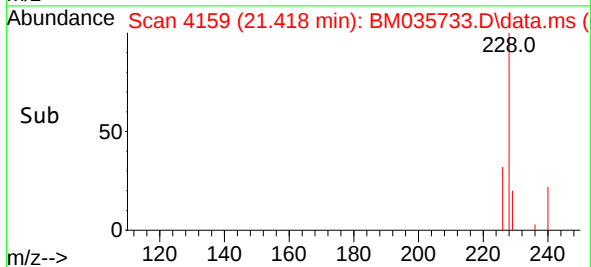

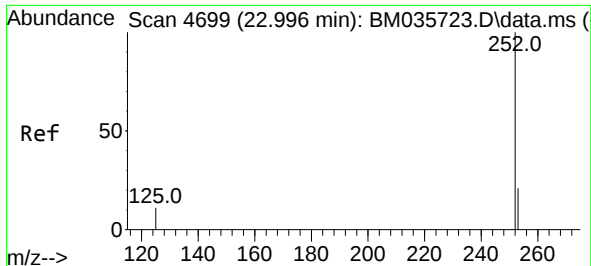

#24
Benzo(b)fluoranthene
Concen: 0.036 ng/ul
RT: 22.987 min Scan# 4696
Delta R.T. -0.009 min
Lab File: BM035733.D
Acq: 28 Jun 2022 20:39




Instrument :
BNA_M
ClientSampleId :
C0AF6

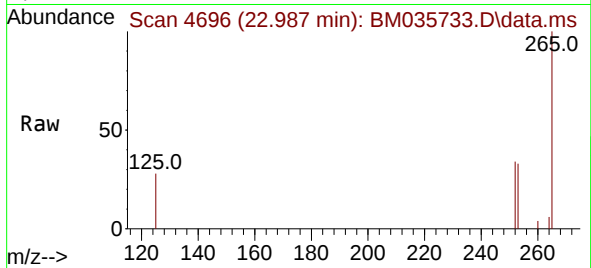


Tgt Ion:252 Resp: 1307
Ion Ratio Lower Upper
252 100
253 95.6 0.0 61.4#
125 80.6 0.0 42.6#

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/29/2022
Supervised By :mohammad ahmed 07/01/2022

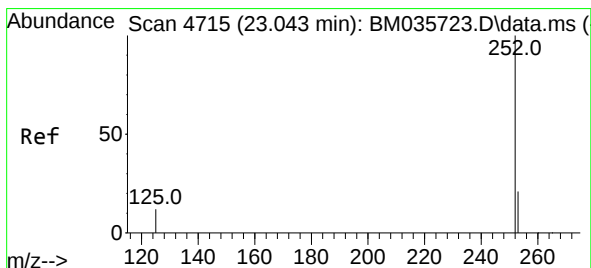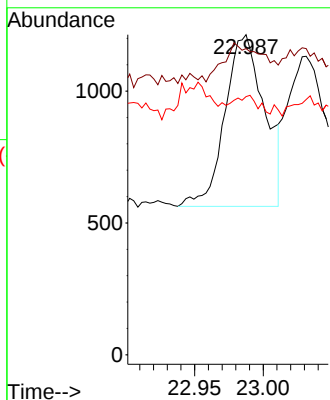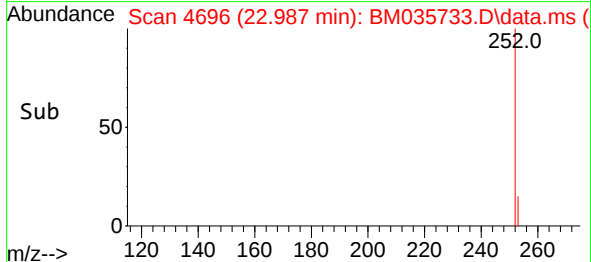

#25
Benzo(k)fluoranthene
Concen: 0.028 ng/ul
RT: 23.031 min Scan# 4711
Delta R.T. -0.012 min
Lab File: BM035733.D
Acq: 28 Jun 2022 20:39

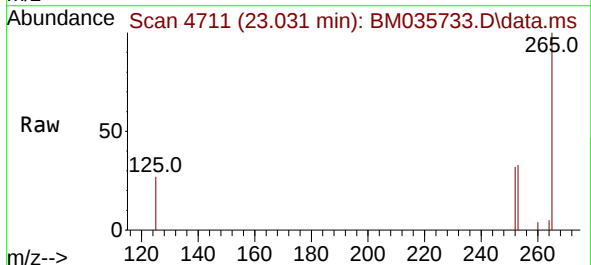

Tgt Ion:252 Resp: 1034
Ion Ratio Lower Upper
252 100
253 102.6 25.2 37.8#
125 85.5 18.3 27.5#

