

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062916\
 Data File : BM006133.D
 Acq On : 29 Jun 2016 19:51
 Operator : UM/SJ
 Sample : H3779-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YE1

Quant Time: Jun 30 03:30:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 29 00:57:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	185882	20.00	ng/ul	0.00
7) Naphthalene-d8	10.43	136	917989	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.30	164	562865	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.05	188	1347917	20.00	ng/ul	0.00
29) Chrysene-d12	21.24	240	1470402	20.00	ng/ul	0.00
34) Perylene-d12	23.46	264	1285695	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.16	96	5768	1.44	ng/uL	0.00
3) Phenol-d5	6.82	99	320210	21.09	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.99	67	200850	22.43	ng/ul	0.00
5) 2-Chlorophenol-d4	7.18	132	245468	21.06	ng/ul	0.00
6) 4-Methylphenol-d8	8.35	113	271494	22.21	ng/ul	-0.01
8) Nitrobenzene-d5	8.80	128	127150	20.56	ng/ul	0.00
9) 2-Nitrophenol-d4	9.52	143	142676	20.16	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.05	165	261267	20.23	ng/ul	0.00
12) 4-Chloroaniline-d4	10.57	131	326083	31.95	ng/ul	0.00
16) Dimethylphthalate-d6	13.71	166	848401	21.03	ng/ul	0.00
17) Acenaphthylene-d8	13.99	160	1065979	21.77	ng/ul	0.00
20) 4-Nitrophenol-d4	14.50	143	136869	17.88	ng/ul	0.00
21) Fluorene-d10	15.30	176	752842	21.87	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.42	200	115112	24.11	ng/ul	0.00
26) Anthracene-d10	17.14	188	1167594	21.59	ng/ul	0.00
30) Pyrene-d10	19.45	212	1334926	22.55	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.32	264	1097140	21.44	ng/ul	0.00

Target Compounds


						Qvalue
25) Phenanthrene	17.09	178	420484	6.59	ng/ul	100
27) Anthracene	17.18	178	75745	1.16	ng/ul	99
28) Fluoranthene	19.11	202	1271131	16.27	ng/ul	99
31) Pyrene	19.48	202	1007166	12.99	ng/ul	96
32) Benzo(a)anthracene	21.23	228	579150	7.57	ng/ul	97
33) Chrysene	21.28	228	612767	8.70	ng/ul	97
35) Benzo(b)fluoranthene	22.80	252	825179	12.37	ng/ul	98
36) Benzo(k)fluoranthene	22.80	252	825179	13.18	ng/ul	99
38) Benzo(a)pyrene	23.36	252	476287	7.56	ng/ul	98
41) Benzo(g,h,i)perylene	26.35	276	254546	4.64	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062916\
Data File : BM006133.D
Acq On : 29 Jun 2016 19:51
Operator : UM/SJ
Sample : H3779-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9YE1

Quant Time: Jun 30 03:30:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 29 00:57:09 2016
Response via : Initial Calibration

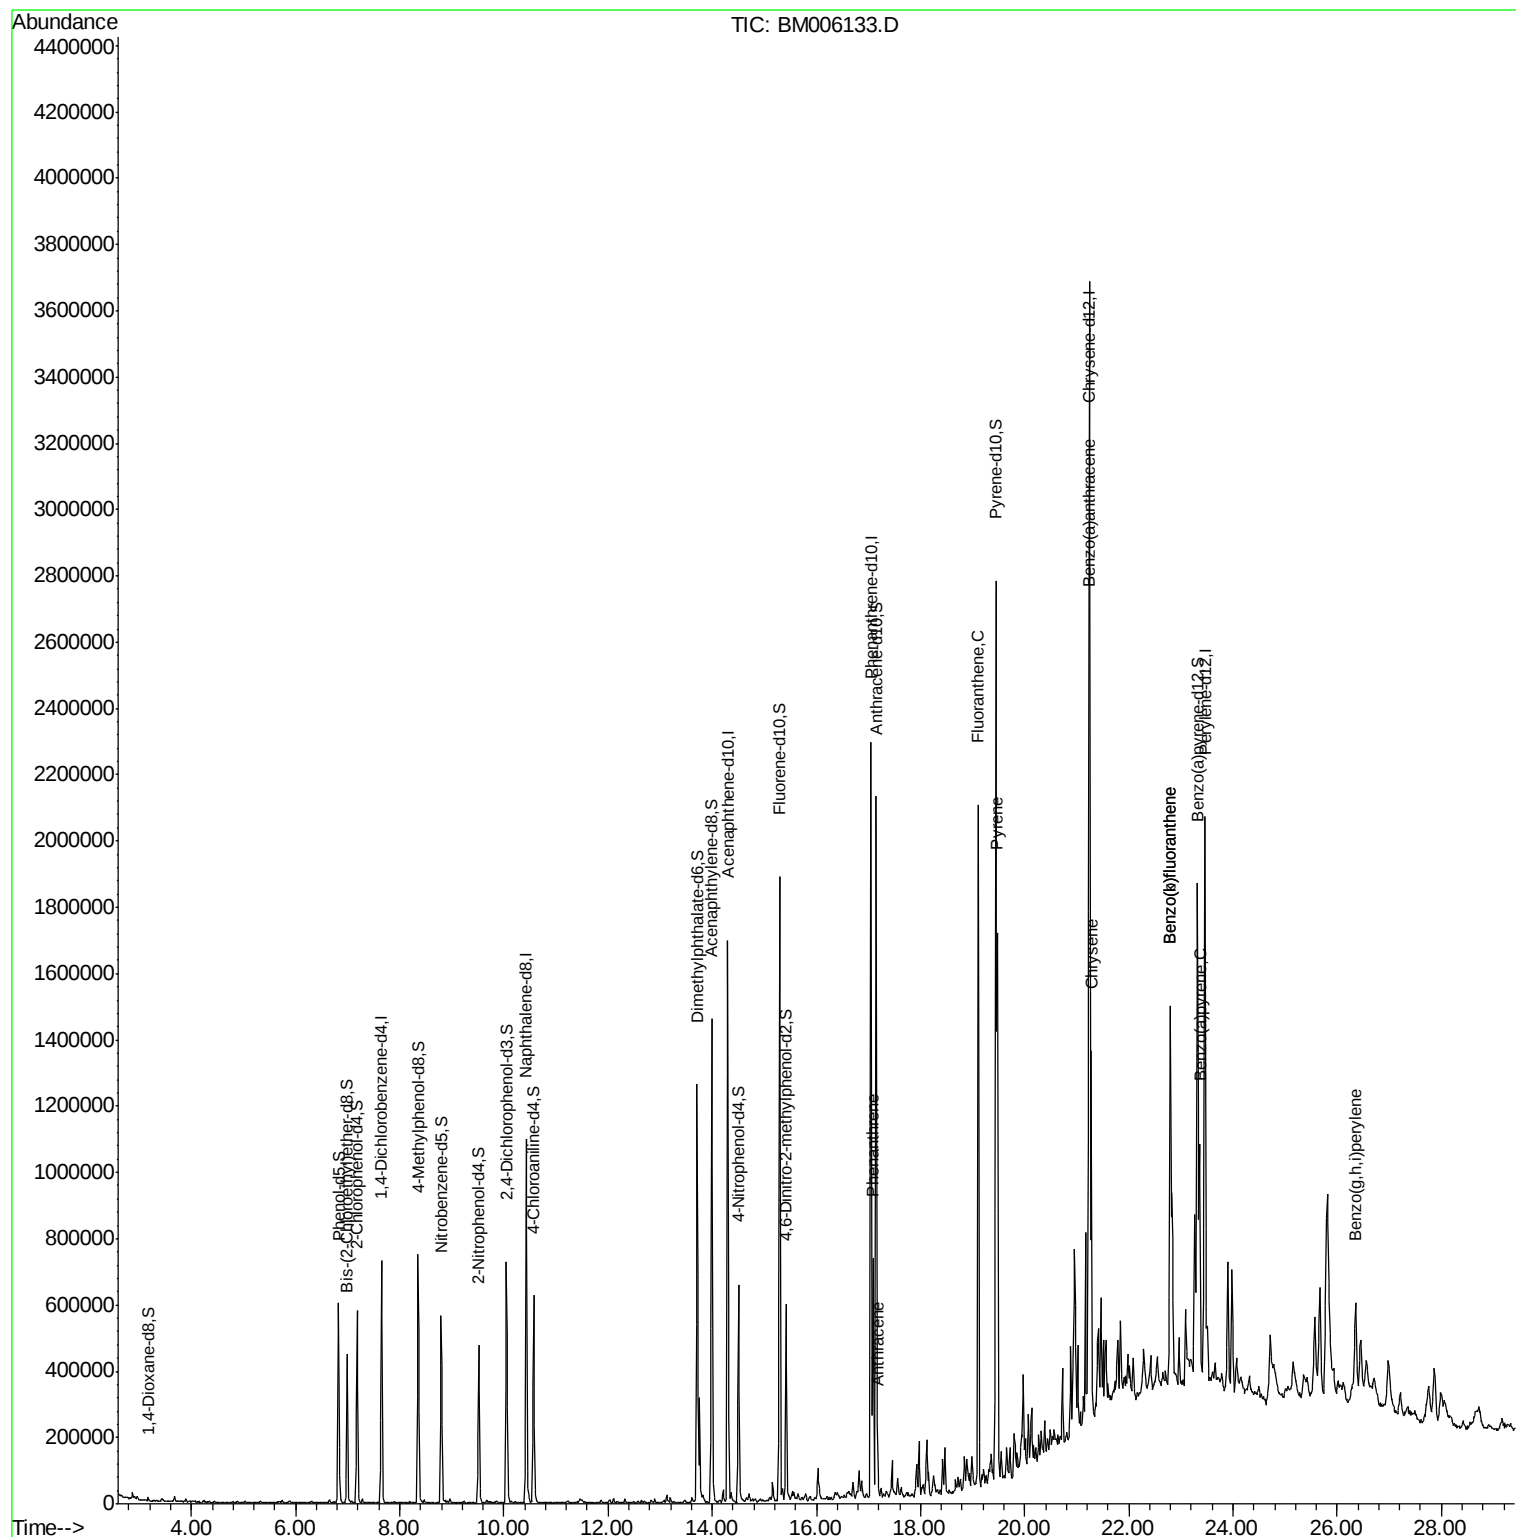

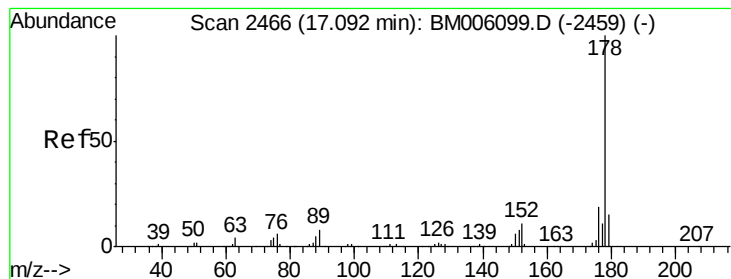

#25

Phenanthrene

Concen: 6.59 ng/ul

RT: 17.09 min Scan# 2466

Delta R.T. -0.00 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51

Instrument :

BNA_M

ClientSampleId :

D9YE1


Tgt Ion:178 Resp: 420484

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2




176 18.7 15.3 22.9

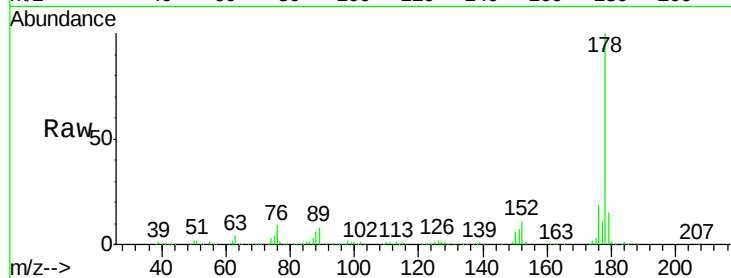

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

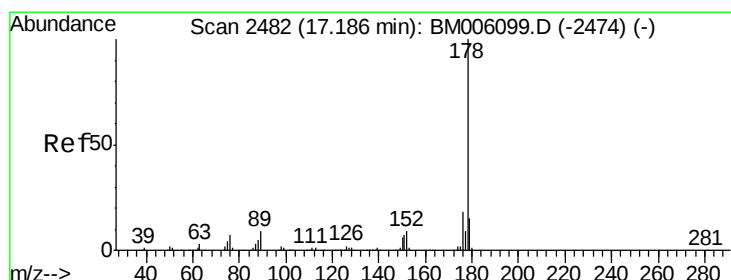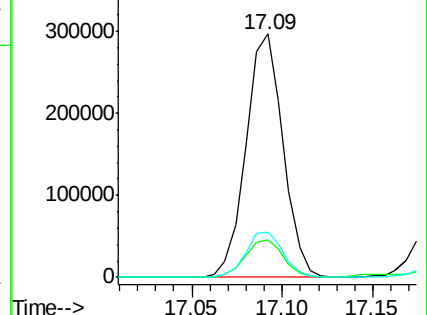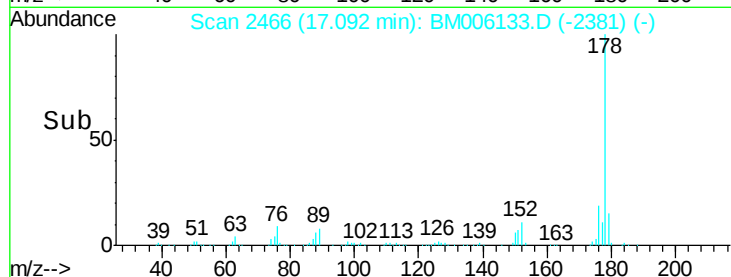

#27

Anthracene

Concen: 1.16 ng/ul

RT: 17.18 min Scan# 2481

Delta R.T. -0.01 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51


Tgt Ion:178 Resp: 75745

Ion Ratio Lower Upper

178 100

179 15.1 12.3 18.5



176 18.5 14.6 22.0

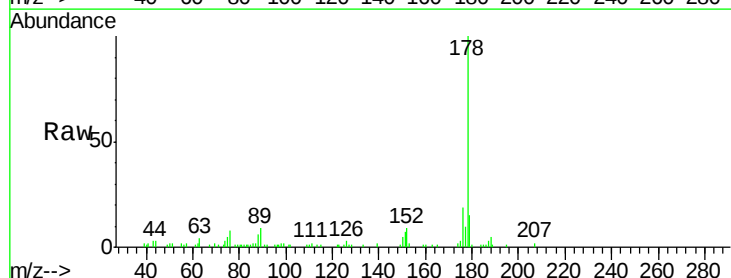


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

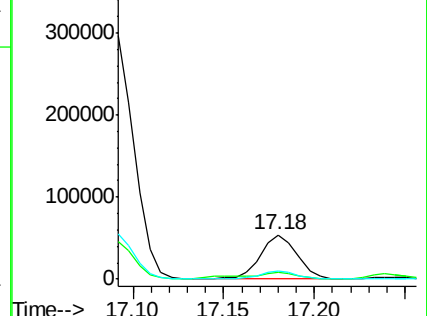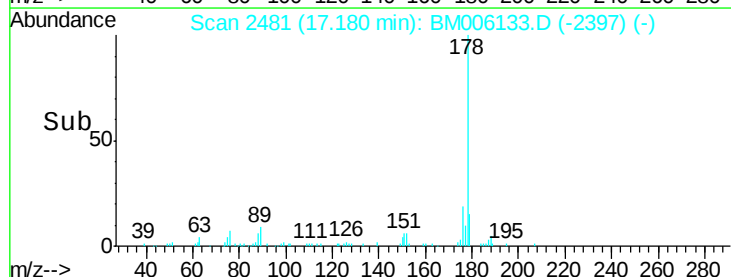

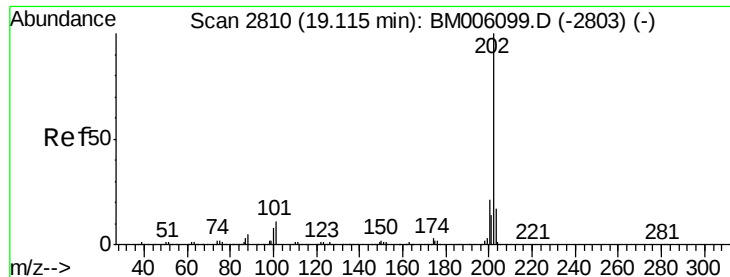

#28

Fluoranthene

Concen: 16.27 ng/ul

RT: 19.11 min Scan# 2809

Delta R.T. -0.01 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51

Instrument :

BNA_M

ClientSampleId :

D9YE1


Tgt Ion:202 Resp: 1271131

Ion Ratio Lower Upper

202 100

101 10.6 8.5 12.7




100 8.6 6.5 9.7

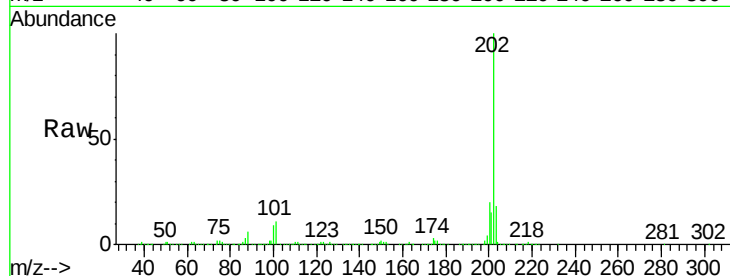

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

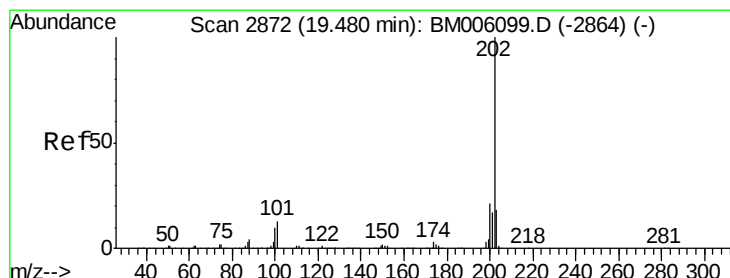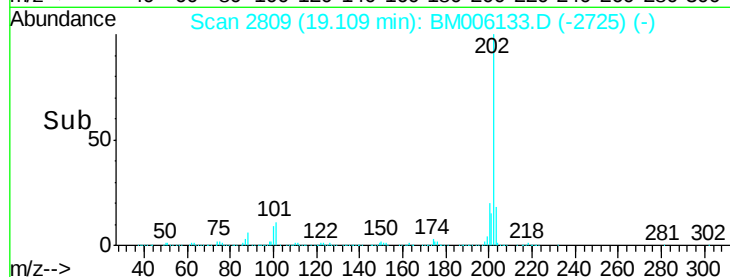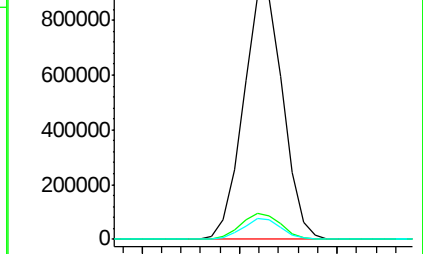

#31

Pyrene

Concen: 12.99 ng/ul

RT: 19.48 min Scan# 2872

Delta R.T. -0.00 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51


Tgt Ion:202 Resp: 1007166

Ion Ratio Lower Upper

202 100

101 12.0 11.0 16.4



100 9.3 8.9 13.3

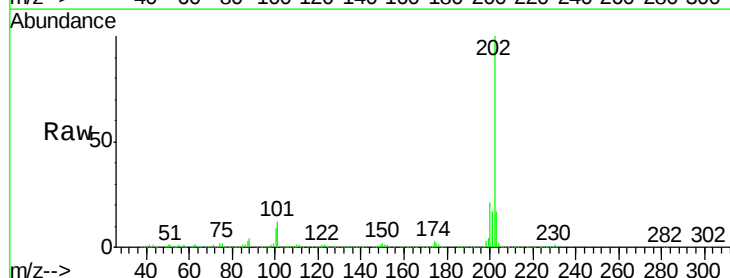


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

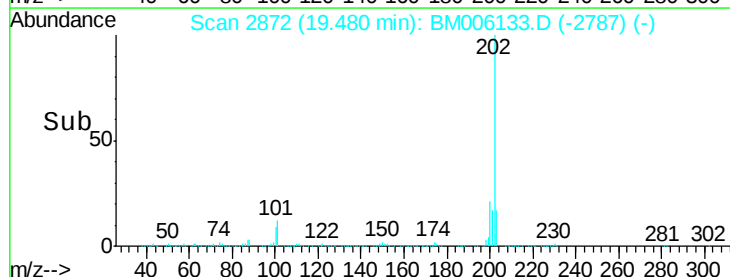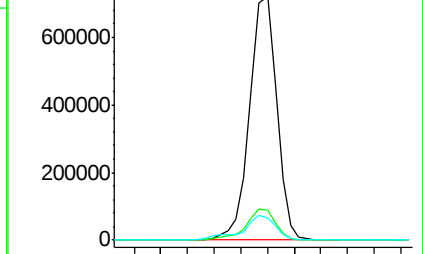

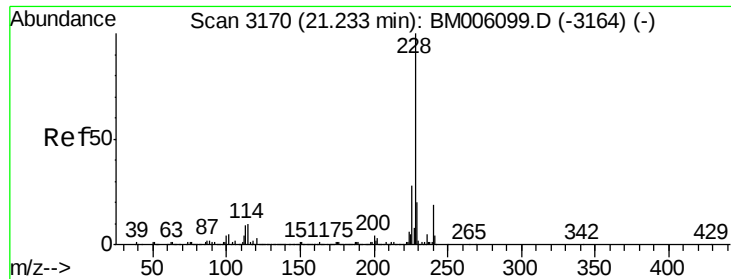

#32

Benzo(a)anthracene

Concen: 7.57 ng/ul

RT: 21.23 min Scan# 3169

Delta R.T. -0.01 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51

Instrument :

BNA_M

ClientSampleId :

D9YE1


Tgt Ion:228 Resp: 579150

Ion Ratio Lower Upper

228 100

229 21.5 15.6 23.4




226 27.7 21.6 32.4

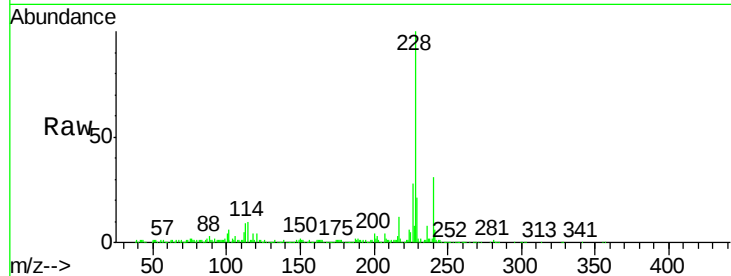

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

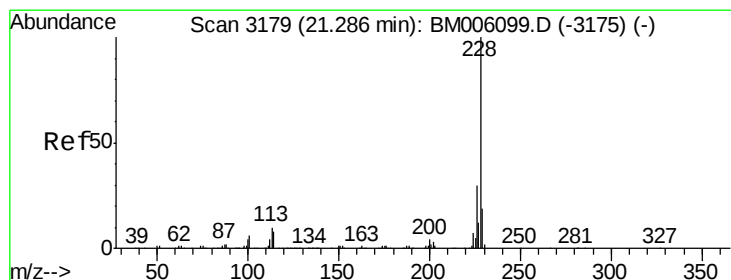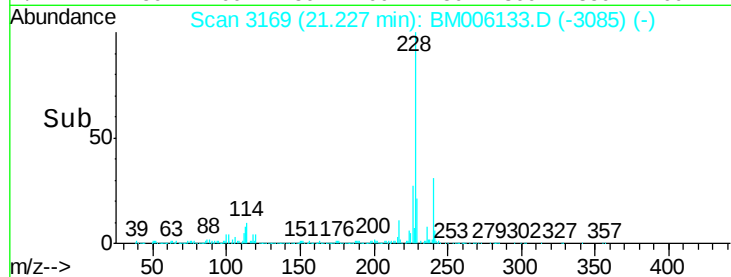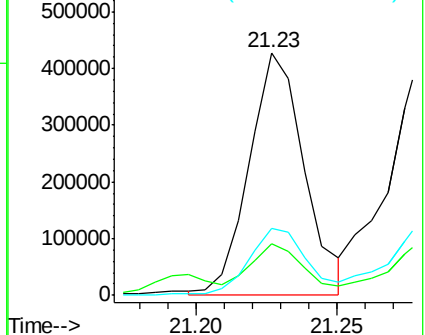

#33

Chrysene

Concen: 8.70 ng/ul

RT: 21.28 min Scan# 3178

Delta R.T. -0.01 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51


Tgt Ion:228 Resp: 612767

Ion Ratio Lower Upper

228 100

226 30.9 23.8 35.6



229 22.0 15.8 23.6

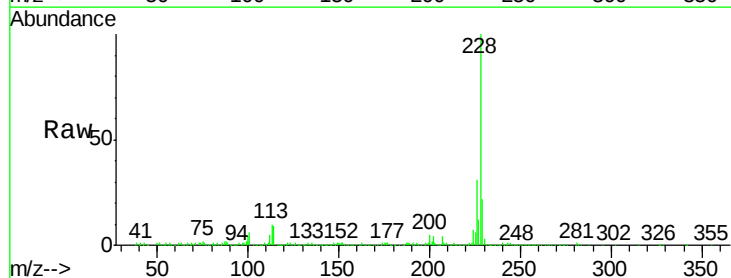


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

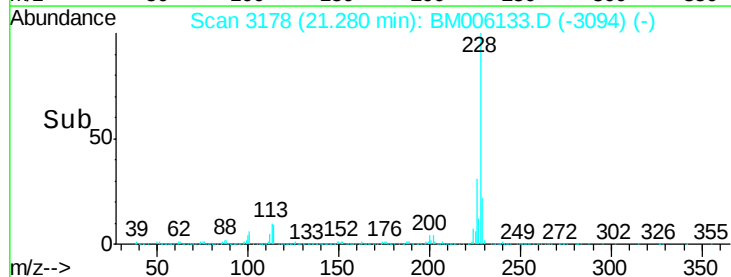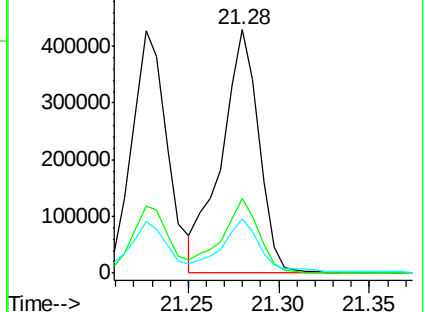

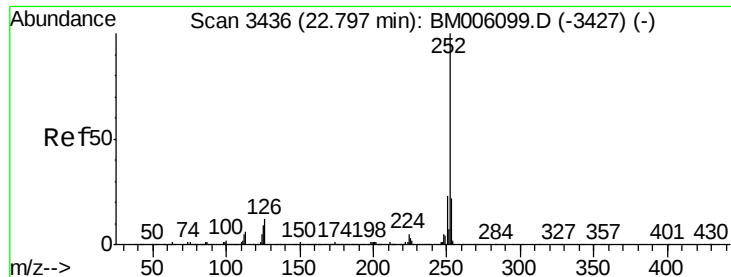

#35

Benzo(b)fluoranthene

Concen: 12.37 ng/ul

RT: 22.80 min Scan# 3436

Delta R.T. -0.00 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51

Instrument :

BNA_M

ClientSampleId :

D9YE1


Tgt Ion:252 Resp: 825179

Ion Ratio Lower Upper

252 100

253 22.5 17.2 25.8




125 10.0 7.8 11.6

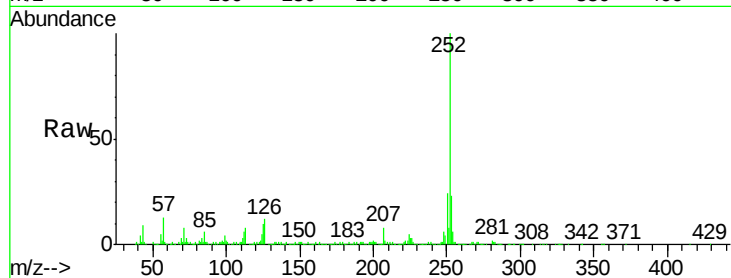

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

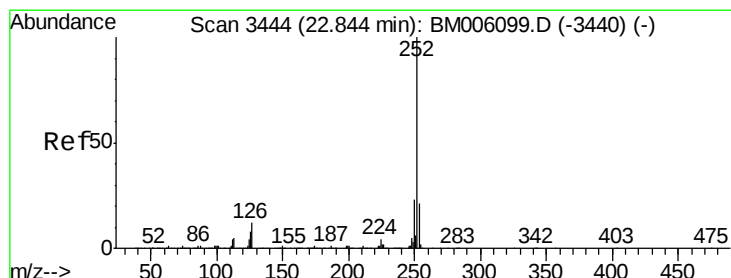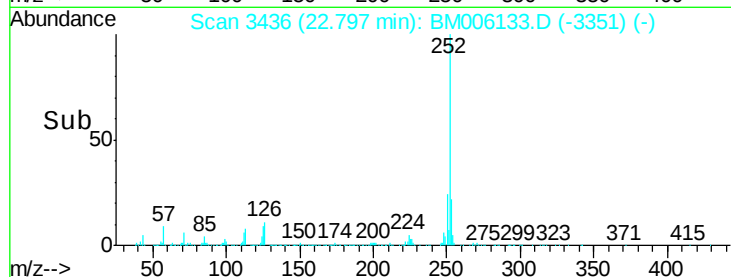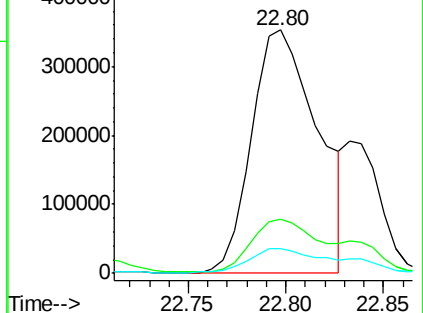

#36

Benzo(k)fluoranthene

Concen: 13.18 ng/ul

RT: 22.80 min Scan# 3436

Delta R.T. -0.05 min

Lab File: BM006133.D

Acq: 29 Jun 2016 19:51


Tgt Ion:252 Resp: 825179

Ion Ratio Lower Upper

252 100

253 22.5 17.6 26.4



125 10.0 8.1 12.1

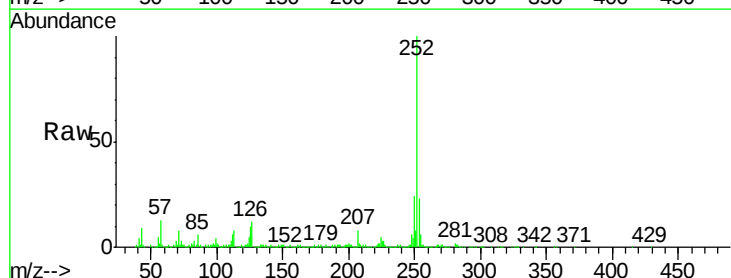


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



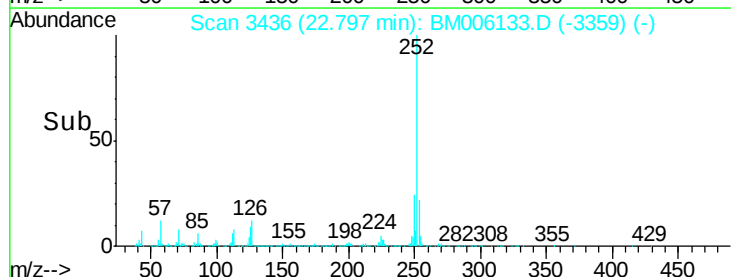
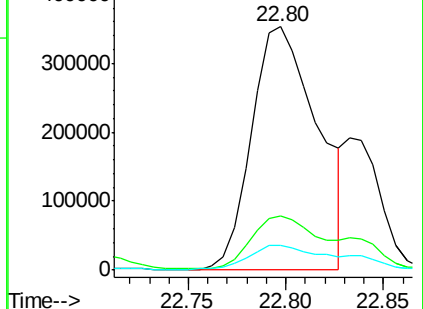


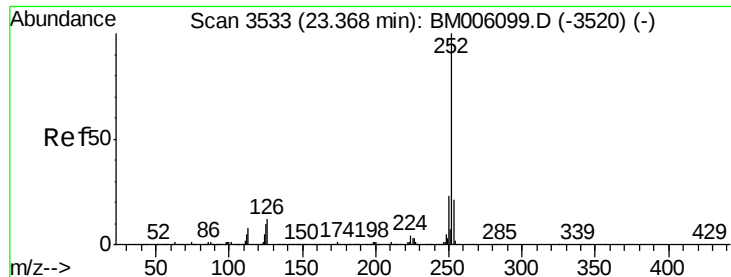

#38
Benzo(a)pyrene
Concen: 7.56 ng/ul
RT: 23.36 min Scan# 3532
Delta R.T. -0.01 min
Lab File: BM006133.D
Acq: 29 Jun 2016 19:51

Instrument :
BNA_M
ClientSampleId :
D9YE1

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.8	26.6
125	10.4	8.7	13.1

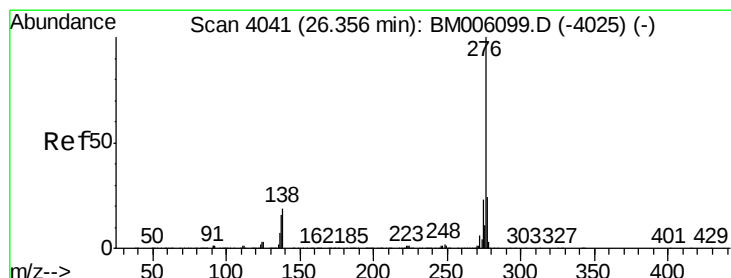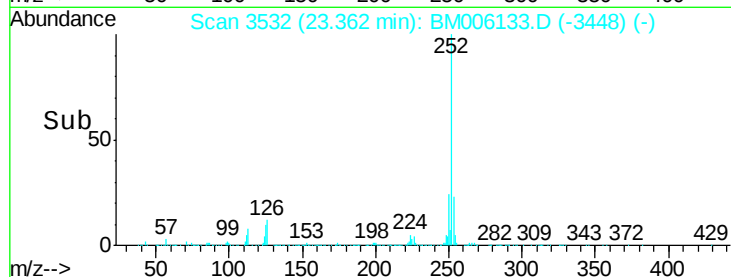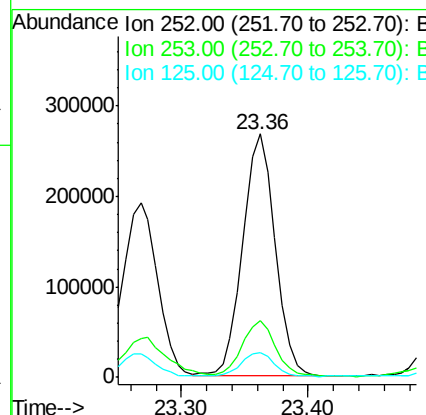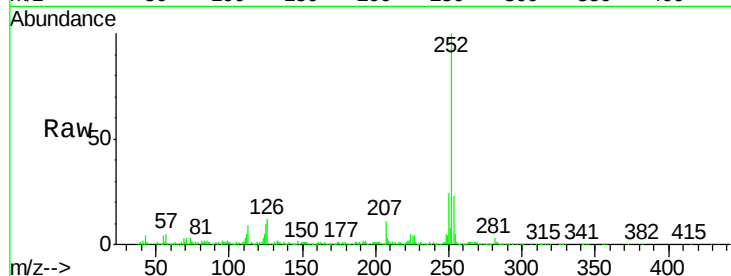

#41
Benzo(g,h,i)perylene
Concen: 4.64 ng/ul
RT: 26.35 min Scan# 4040
Delta R.T. -0.01 min
Lab File: BM006133.D
Acq: 29 Jun 2016 19:51

Tgt Ion	Ratio	Lower	Upper
276	100		
138	17.7	16.6	25.0
277	26.2	18.9	28.3

