

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062919\
 Data File : BM021290.D
 Acq On : 30 Jun 2019 08:08
 Operator : HP/JU
 Sample : PB121025BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	12	rVB	121633	146882	2.10%	0.192%
2	3.281	47	50	61	rVB	56913	94300	1.35%	0.123%
3	6.934	664	671	683	rVB	1164102	1873505	26.77%	2.450%
4	7.098	693	699	715	rVB	927984	1435414	20.51%	1.877%
5	7.292	725	732	741	rVB	1252679	1981736	28.31%	2.592%
6	7.757	804	811	819	rVB	946451	1492618	21.33%	1.952%
7	8.463	924	931	943	rBV	1571777	2538757	36.27%	3.320%
8	8.922	1001	1009	1020	rBV	1217748	2018300	28.84%	2.640%
9	9.633	1123	1130	1139	rBV	1078319	1796212	25.66%	2.349%
10	10.169	1213	1221	1232	rBV	1724284	2933468	41.91%	3.837%
11	10.545	1278	1285	1293	rVB	1431237	2380225	34.01%	3.113%
12	10.692	1302	1310	1325	rBV	1635813	2777466	39.68%	3.633%
13	12.133	1547	1555	1563	rBV	31998	55029	0.79%	0.072%
14	13.363	1756	1764	1770	rBV6	3978	7583	0.11%	0.010%
15	13.816	1831	1841	1851	rBV	3267858	4493251	64.20%	5.877%
16	14.092	1881	1888	1900	rBV	3754590	5506819	78.68%	7.202%
17	14.398	1933	1940	1949	rBV2	2285079	3562060	50.89%	4.659%
18	14.615	1971	1977	2000	rBV	930756	1721613	24.60%	2.252%
19	15.398	2103	2110	2119	rBV	4818306	6810002	97.30%	8.907%
20	15.527	2125	2132	2144	rBV	1004509	1421497	20.31%	1.859%
21	15.633	2146	2150	2155	rVB	57470	81939	1.17%	0.107%
22	16.180	2239	2243	2249	rBV4	9426	16298	0.23%	0.021%
23	16.933	2368	2371	2378	rVB2	10626	15515	0.22%	0.020%
24	17.151	2401	2408	2415	rBV2	2965824	4117365	58.83%	5.385%
25	17.251	2418	2425	2437	rVV	5181260	6999179	100.00%	9.154%
26	17.439	2452	2457	2459	rBV5	6774	10388	0.15%	0.014%
27	19.180	2748	2753	2758	rBV	60006	88901	1.27%	0.116%
28	19.433	2792	2796	2799	rBV	41604	57000	0.81%	0.075%
29	19.545	2809	2815	2823	rBV	4960958	6753921	96.50%	8.833%
30	21.339	3115	3120	3125	rBV	2515781	3275581	46.80%	4.284%
31	23.462	3475	3481	3498	rVV	3490179	6522627	93.19%	8.531%
32	23.609	3500	3506	3515	rVB	1889506	3472784	49.62%	4.542%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062919\
Data File : BM021290.D
Acq On : 30 Jun 2019 08:08
Operator : HP/JU
Sample : PB121025BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 76458235

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062919\
Data File : BM021290.D
Acq On : 30 Jun 2019 08:08
Operator : HP/JU
Sample : PB121025BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

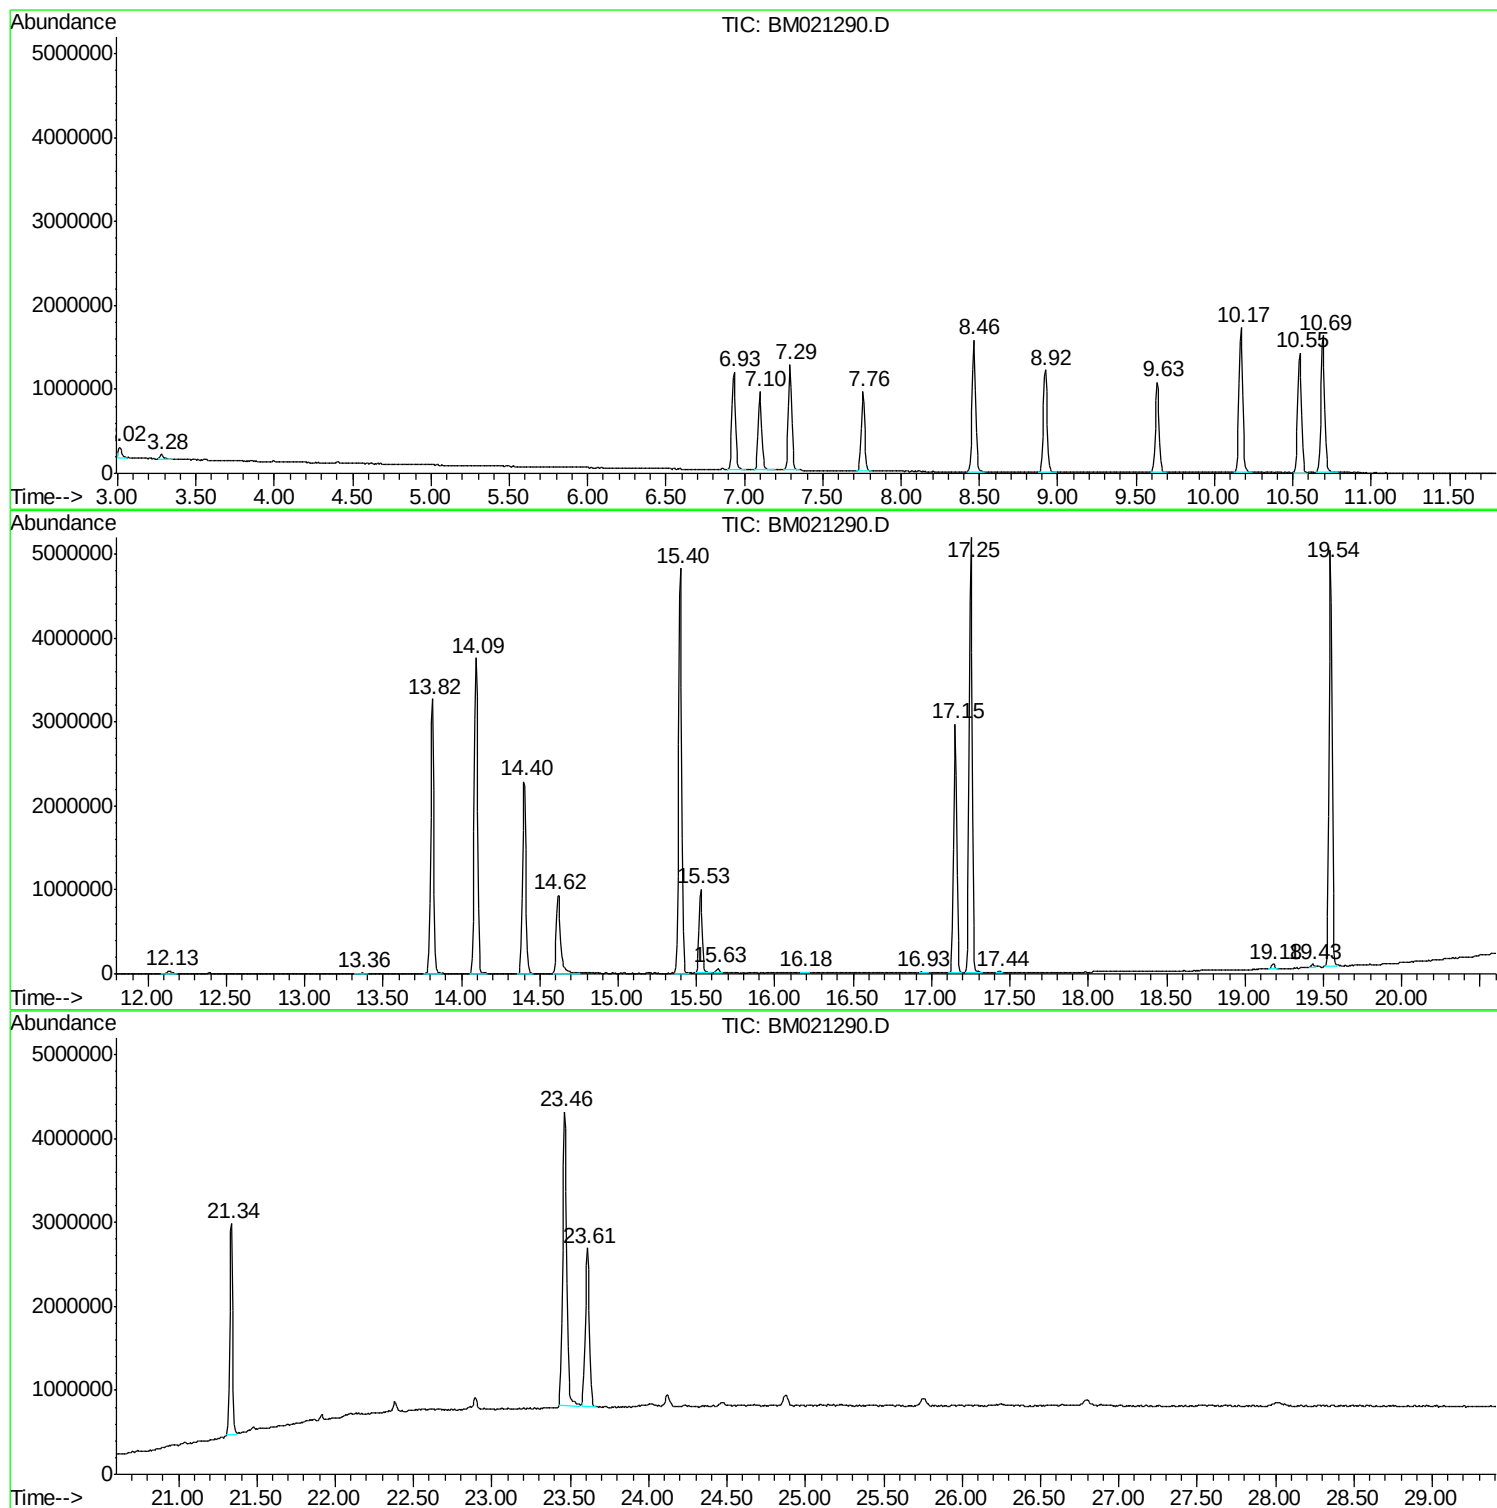

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062919\
Data File : BM021290.D
Acq On : 30 Jun 2019 08:08
Operator : HP/JU
Sample : PB121025BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062919\
Data File : BM021290.D
Acq On : 30 Jun 2019 08:08
Operator : HP/JU
Sample : PB121025BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc