

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM063016\
 Data File : BM006166.D
 Acq On : 30 Jun 2016 20:24
 Operator : UM/SJ
 Sample : H3780-04MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YF4MS

Quant Time: Jul 01 00:59:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 29 00:57:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	226023	20.00	ng/ul	0.00
7) Naphthalene-d8	10.44	136	901305	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.30	164	460862	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.06	188	964703	20.00	ng/ul	0.00
29) Chrysene-d12	21.26	240	1023930	20.00	ng/ul	0.00
34) Perylene-d12	23.48	264	1145407	20.00	ng/ul	0.02

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.18	96	8656	1.78	ng/uL	0.00
3) Phenol-d5	6.83	99	343181	18.59	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.99	67	211223	19.40	ng/ul	0.00
5) 2-Chlorophenol-d4	7.19	132	269385	19.01	ng/ul	0.00
6) 4-Methylphenol-d8	8.36	113	258697	17.41	ng/ul	0.00
8) Nitrobenzene-d5	8.81	128	126728	20.88	ng/ul	0.00
9) 2-Nitrophenol-d4	9.53	143	139424	20.07	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.06	165	239689	18.91	ng/ul	0.00
12) 4-Chloroaniline-d4	10.58	131	205459	20.50	ng/ul	0.00
16) Dimethylphthalate-d6	13.72	166	664175	20.10	ng/ul	0.00
17) Acenaphthylene-d8	14.00	160	855039	21.33	ng/ul	0.00
20) 4-Nitrophenol-d4	14.52	143	126280	20.15	ng/ul	0.01
21) Fluorene-d10	15.30	176	575461	20.41	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.44	200	82707	24.21	ng/ul	0.01
26) Anthracene-d10	17.16	188	874021	22.58	ng/ul	0.00
30) Pyrene-d10	19.46	212	947783	22.99	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.34	264	1031365	22.63	ng/ul	0.02

Target Compounds


						Qvalue
18) Acenaphthylene	14.03	152	60678	1.45	ng/ul	97
19) Acenaphthene	14.37	153	520667	19.44	ng/ul	99
25) Phenanthrene	17.10	178	579867	12.70	ng/ul	99
27) Anthracene	17.19	178	144144	3.07	ng/ul	99
28) Fluoranthene	19.12	202	1590009	28.44	ng/ul	99
31) Pyrene	19.49	202	2230731	41.30	ng/ul	96
32) Benzo(a)anthracene	21.24	228	766090	14.39	ng/ul	97
33) Chrysene	21.29	228	796900	16.26	ng/ul	97
35) Benzo(b)fluoranthene	22.81	252	1278098	21.50	ng/ul	97
36) Benzo(k)fluoranthene	22.81	252	1278098	22.92	ng/ul	98
38) Benzo(a)pyrene	23.38	252	788891	14.05	ng/ul	97
39) Indeno(1,2,3-cd)pyrene	25.70	276	639389	10.95	ng/ul#	93
40) Dibenzo(a,h)anthracene	25.71	278	165885	3.43	ng/ul#	82
41) Benzo(g,h,i)perylene	26.39	276	597048	12.22	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM063016\
Data File : BM006166.D
Acq On : 30 Jun 2016 20:24
Operator : UM/SJ
Sample : H3780-04MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9YF4MS

Quant Time: Jul 01 00:59:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 29 00:57:09 2016
Response via : Initial Calibration

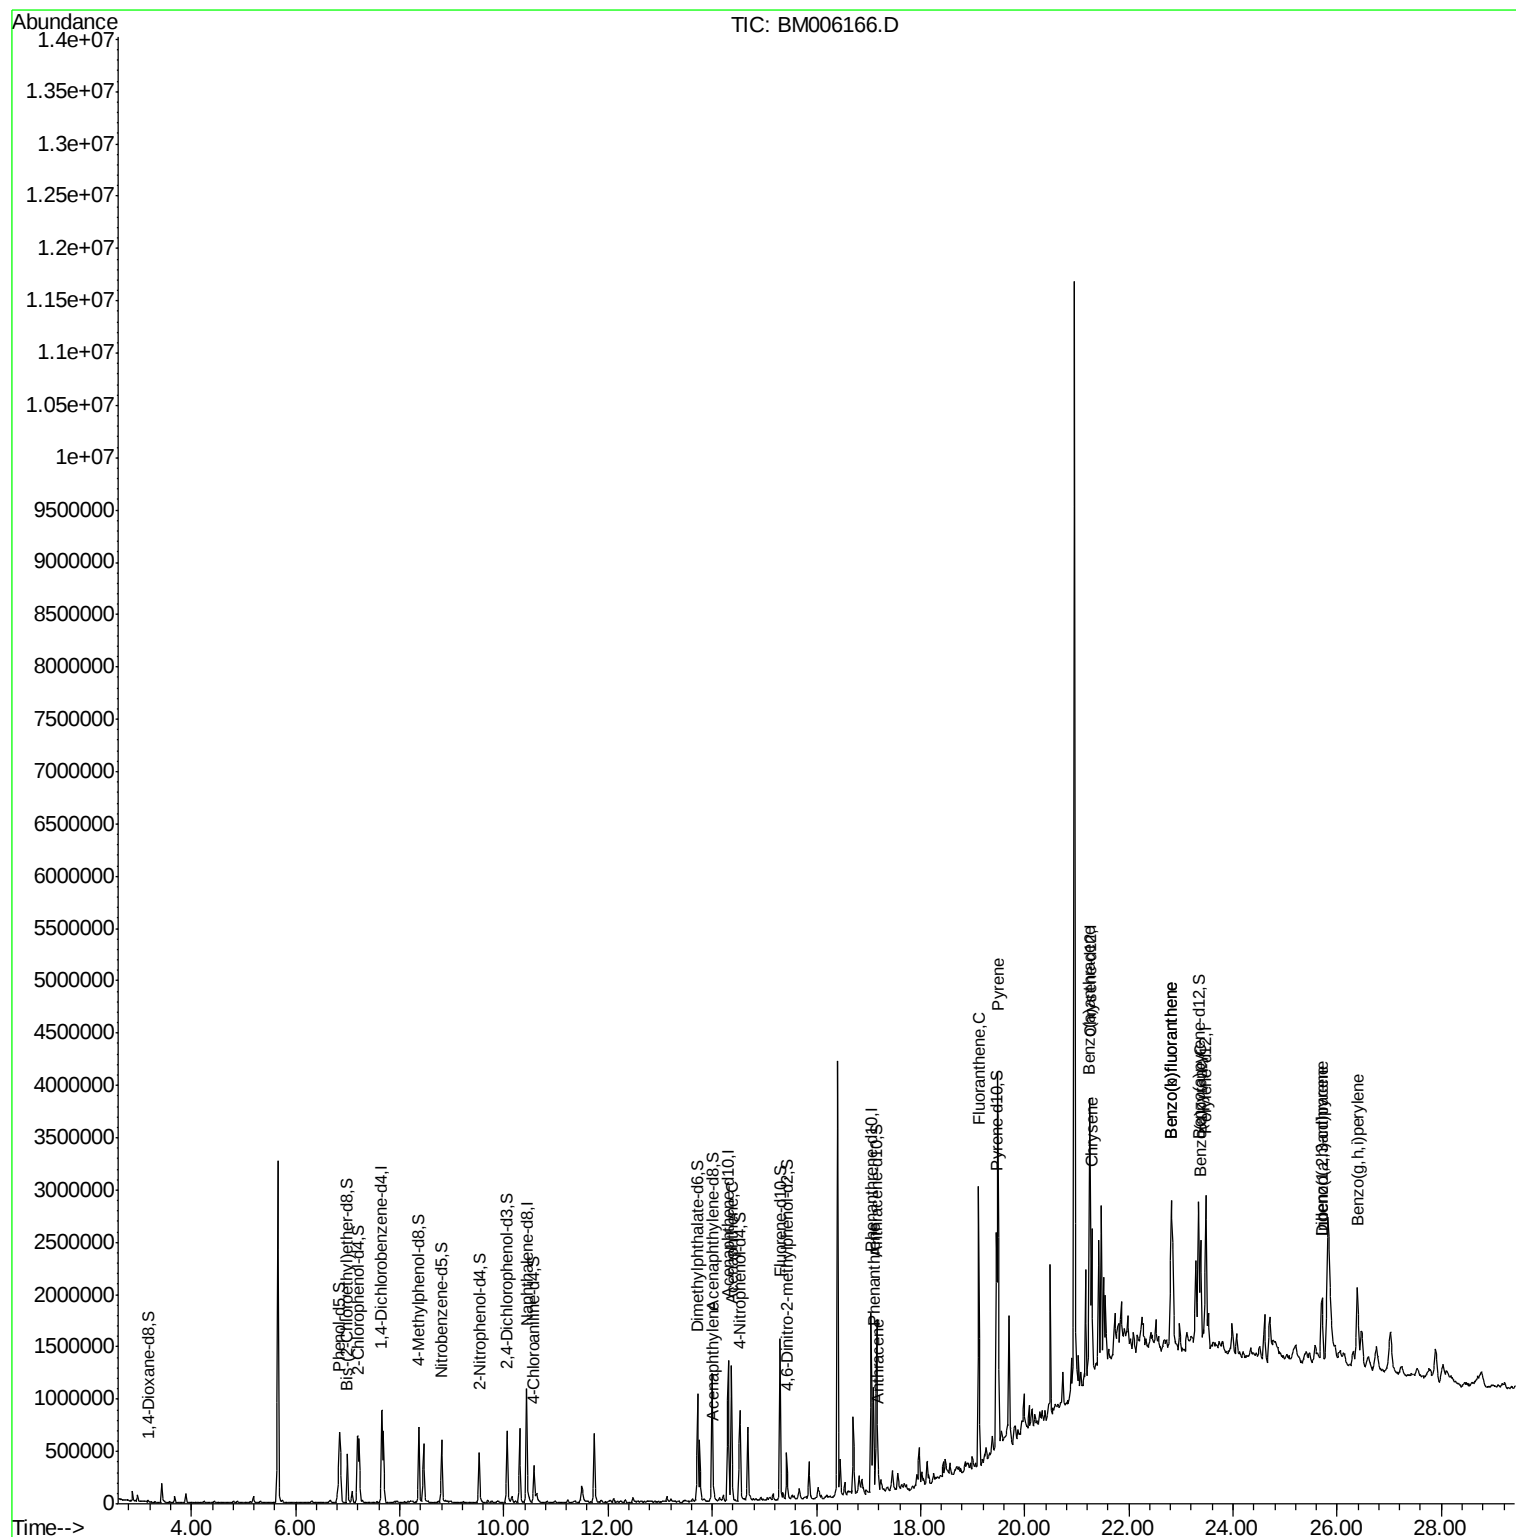



#18

Acenaphthylene

Concen: 1.45 ng/ul

RT: 14.03 min Scan# 1945

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:152 Resp: 60678

Ion Ratio Lower Upper

152 100

151 18.3 15.8 23.6




153 14.5 10.3 15.5

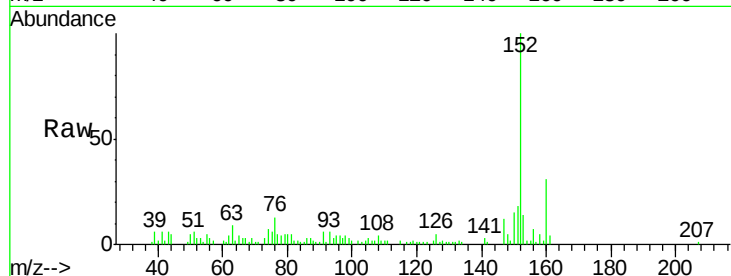

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

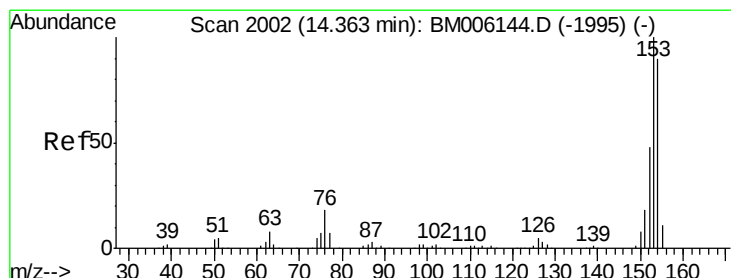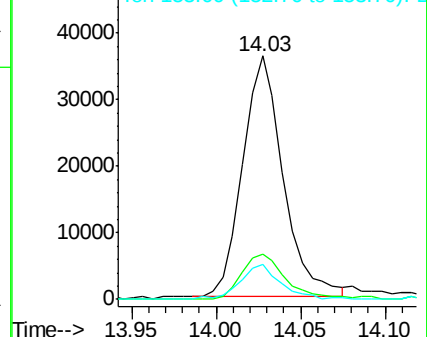

#19

Acenaphthene

Concen: 19.44 ng/ul

RT: 14.37 min Scan# 2003

Delta R.T. 0.00 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:153 Resp: 520667

Ion Ratio Lower Upper

153 100

152 48.0 38.1 57.1



154 87.9 71.6 107.4

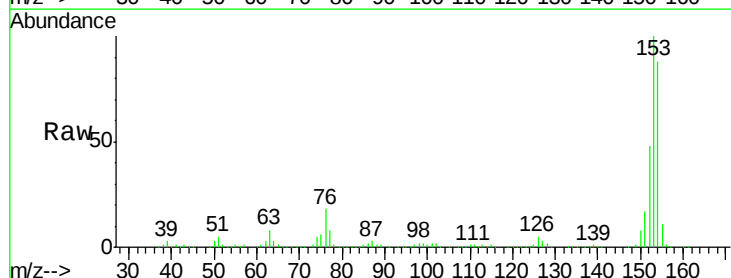


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



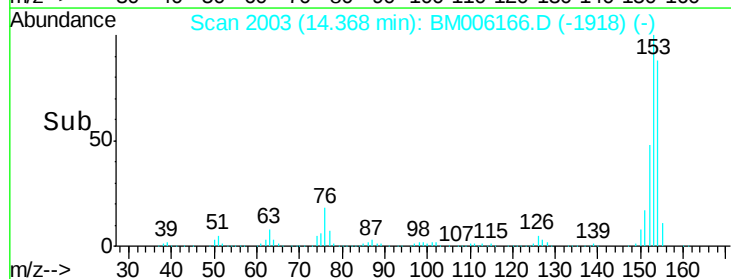
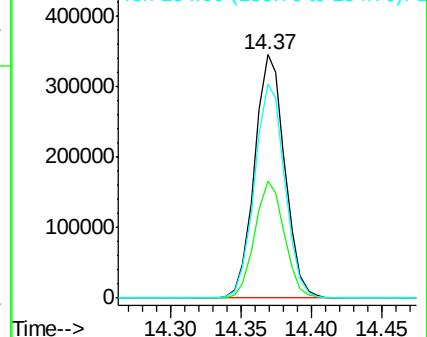




#25
Phenanthrene
Concen: 12.70 ng/ul
RT: 17.10 min Scan# 2467
Delta R.T. 0.01 min
Lab File: BM006166.D
Acq: 30 Jun 2016 20:24




Instrument :
BNA_M
ClientSampleId :
D9YF4MS


Tgt Ion:178 Resp: 579867
Ion Ratio Lower Upper
178 100
179 15.6 12.2 18.2
176 18.9 15.3 22.9

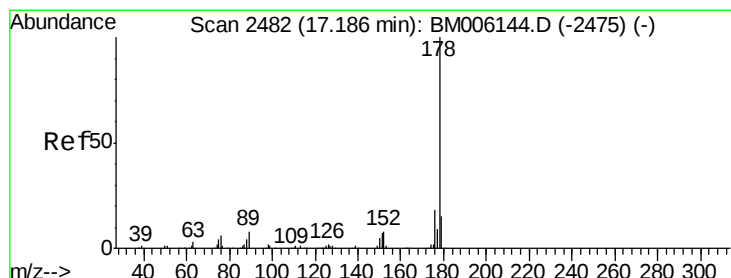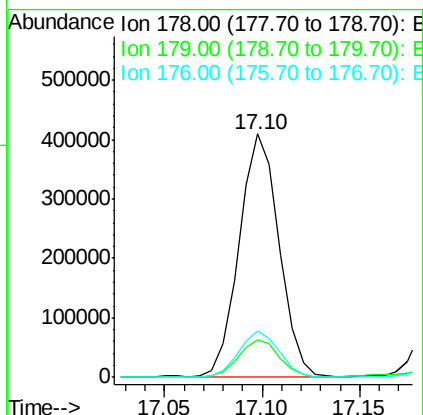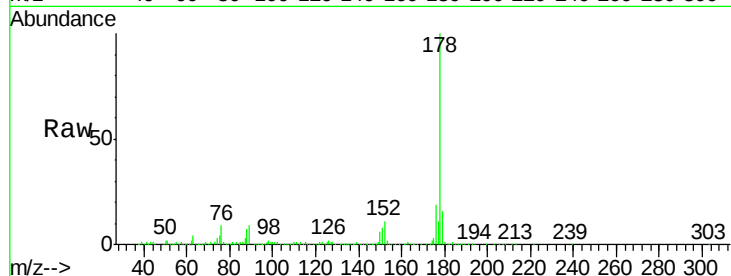

#27
Anthracene
Concen: 3.07 ng/ul
RT: 17.19 min Scan# 2483
Delta R.T. 0.01 min
Lab File: BM006166.D
Acq: 30 Jun 2016 20:24

Tgt Ion:178 Resp: 144144
Ion Ratio Lower Upper
178 100
179 16.4 12.3 18.5
176 18.3 14.6 22.0

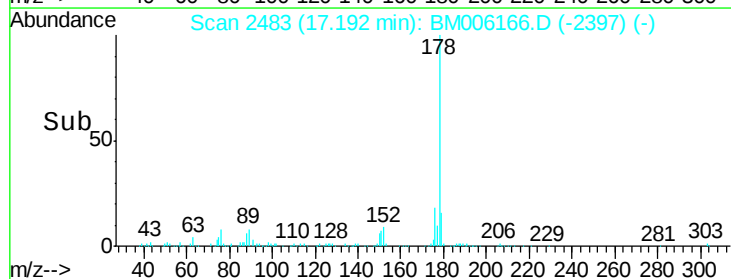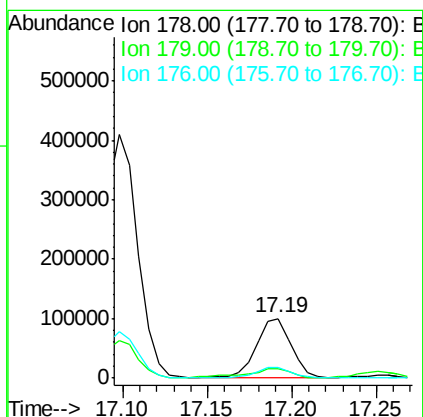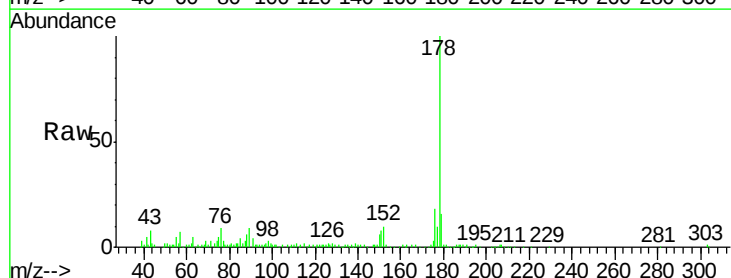



#28

Fluoranthene

Concen: 28.44 ng/ul

RT: 19.12 min Scan# 2811

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:202 Resp: 1590009

Ion Ratio Lower Upper

202 100

101 10.4 8.5 12.7


100 7.7 6.5 9.7

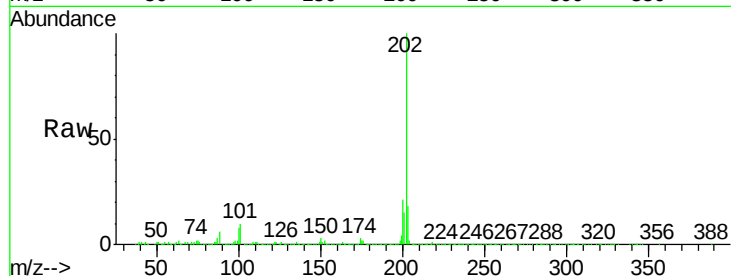



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

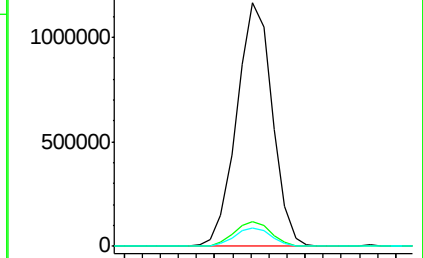

Time--> 19.05 19.10 19.15

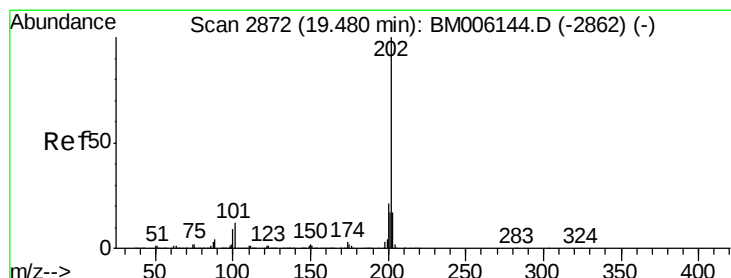

#31

Pyrene

Concen: 41.30 ng/ul

RT: 19.49 min Scan# 2873

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:202 Resp: 2230731

Ion Ratio Lower Upper

202 100

101 12.2 11.0 16.4


100 9.9 8.9 13.3

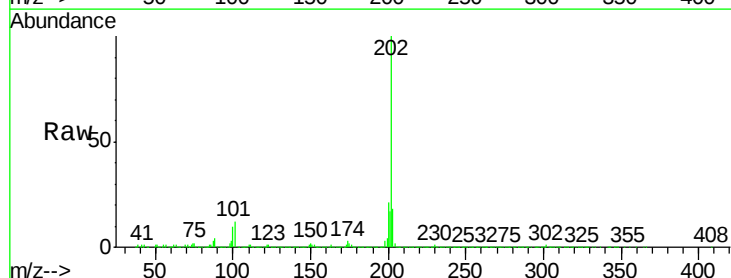


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

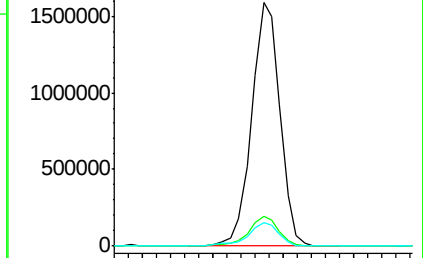

Time--> 19.40 19.45 19.50 19.55



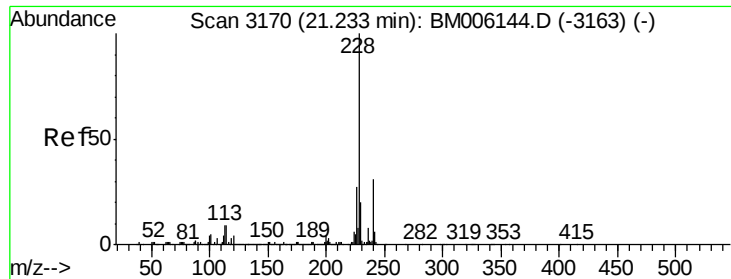

#32

Benzo(a)anthracene

Concen: 14.39 ng/ul

RT: 21.24 min Scan# 3171

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:228 Resp: 766090

Ion Ratio Lower Upper

228 100

229 20.7 15.6 23.4




226 28.9 21.6 32.4

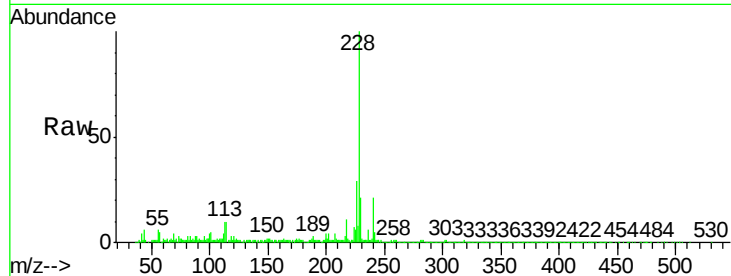

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

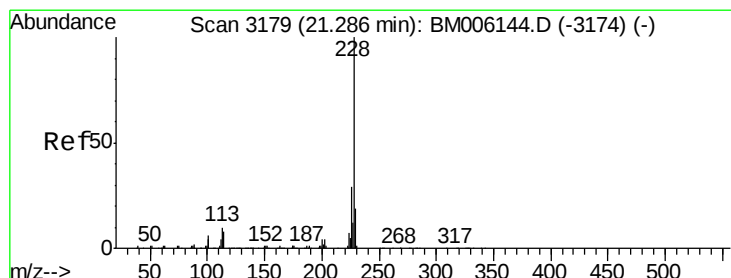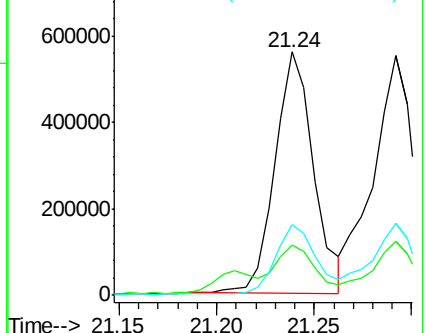

#33

Chrysene

Concen: 16.26 ng/ul

RT: 21.29 min Scan# 3180

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:228 Resp: 796900

Ion Ratio Lower Upper

228 100

226 29.9 23.8 35.6



229 22.4 15.8 23.6

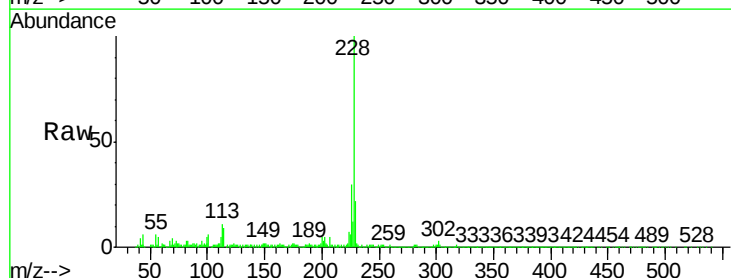


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

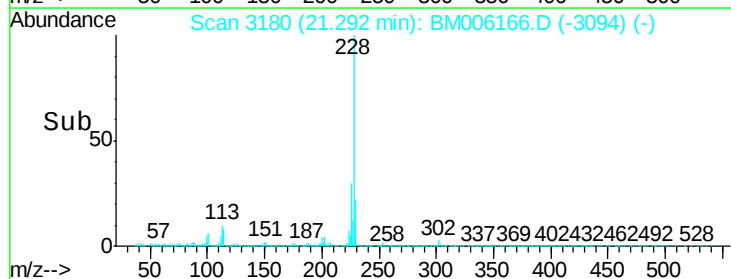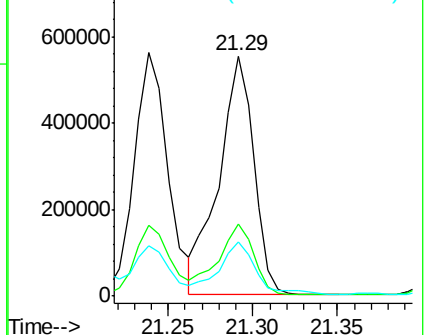

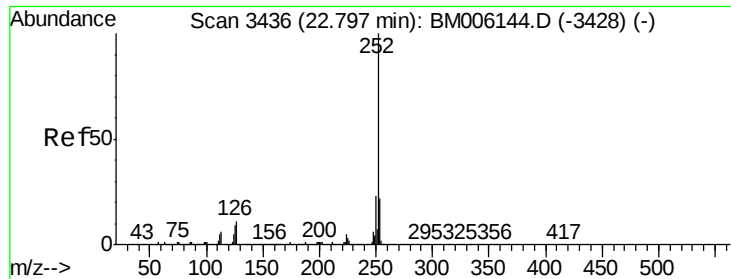

#35

Benzo(b)fluoranthene

Concen: 21.50 ng/ul

RT: 22.81 min Scan# 3439

Delta R.T. 0.02 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:252 Resp: 1278098

Ion Ratio Lower Upper

252 100

253 23.1 17.2 25.8




125 10.1 7.8 11.6

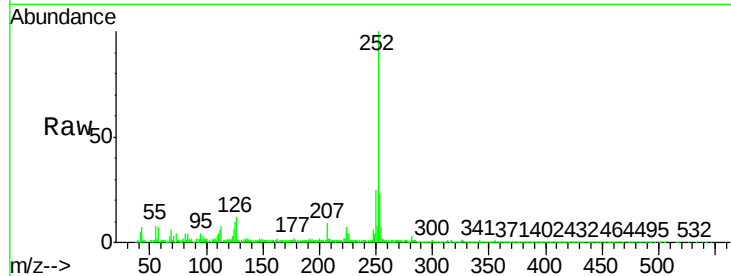

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

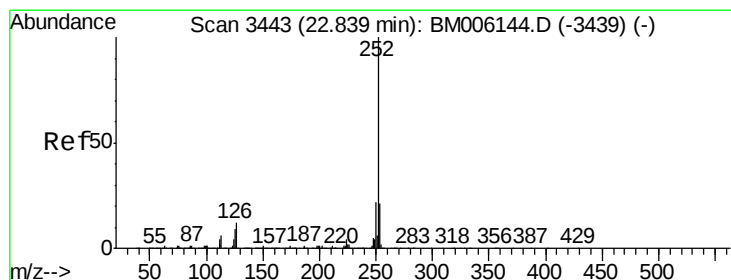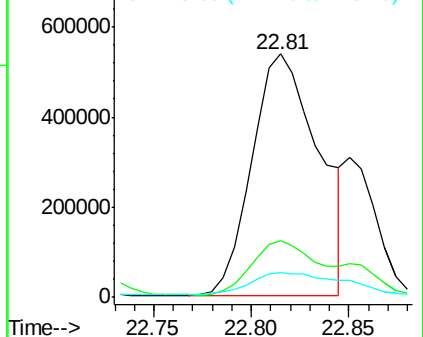

#36

Benzo(k)fluoranthene

Concen: 22.92 ng/ul

RT: 22.81 min Scan# 3439

Delta R.T. -0.03 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:252 Resp: 1278098

Ion Ratio Lower Upper

252 100

253 23.1 17.6 26.4



125 10.1 8.1 12.1

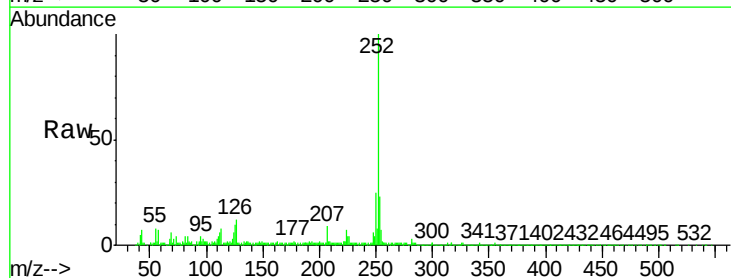


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

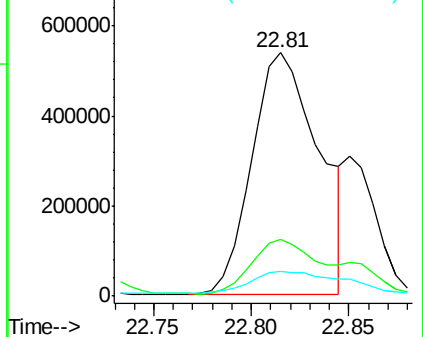

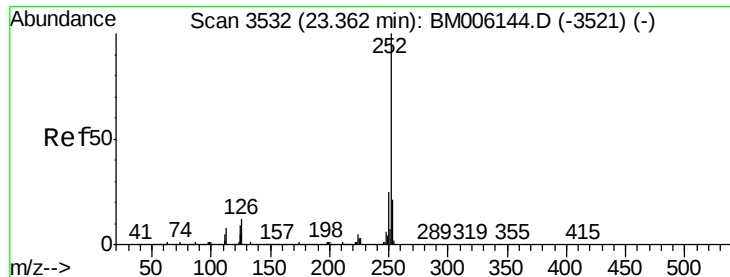

#38

Benzo(a)pyrene

Concen: 14.05 ng/ul

RT: 23.38 min Scan# 3535

Delta R.T. 0.01 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:252 Resp: 788891

Ion Ratio Lower Upper

252 100

253 23.8 17.8 26.6




125 10.4 8.7 13.1

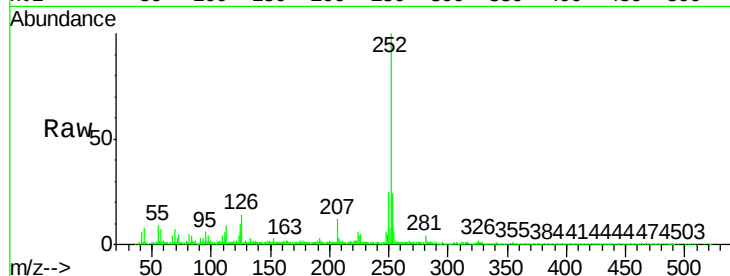

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

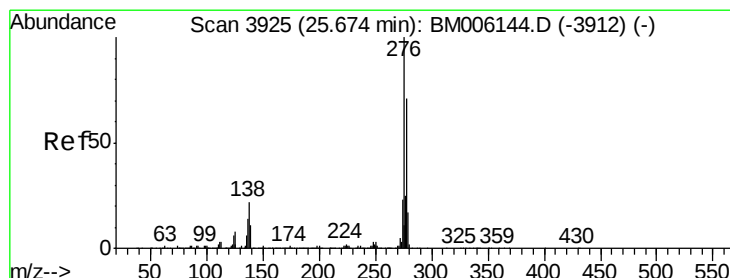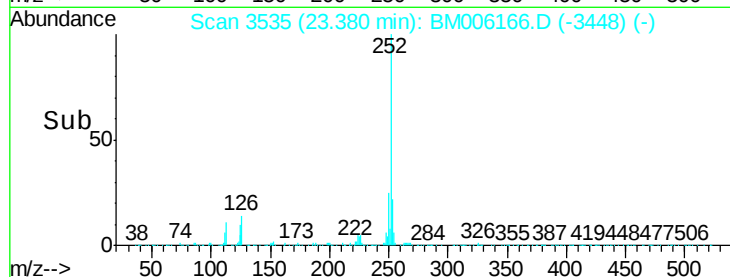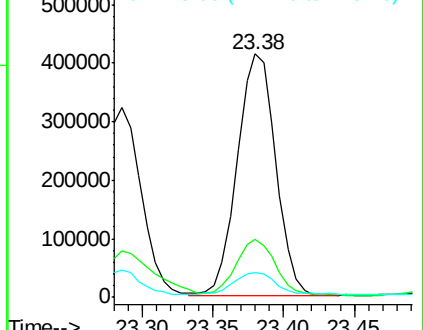

#39

Indeno(1,2,3-cd)pyrene

Concen: 10.95 ng/ul

RT: 25.70 min Scan# 3930

Delta R.T. 0.02 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:276 Resp: 639389

Ion Ratio Lower Upper

276 100

138 19.6 20.4 30.6#



277 26.5 20.6 30.8

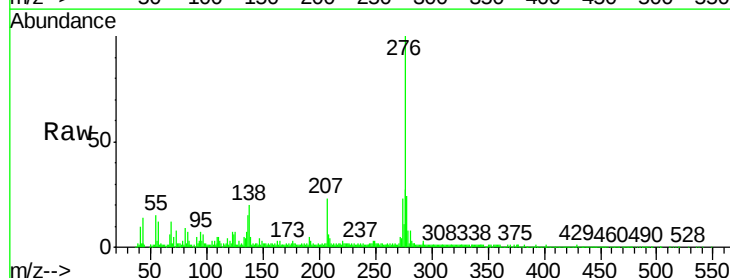


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

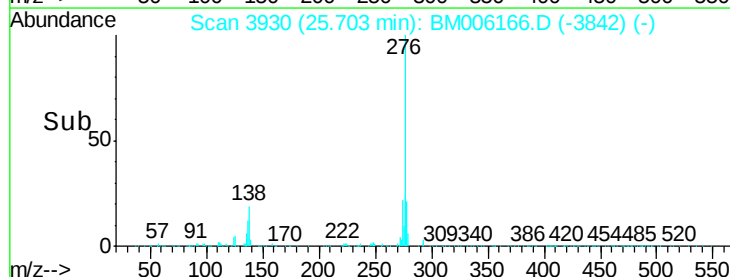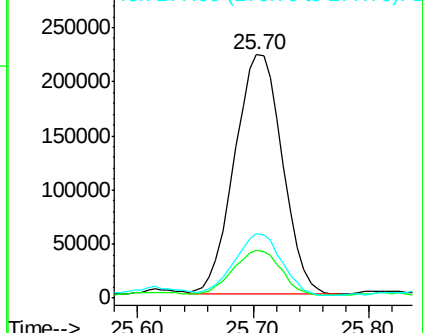

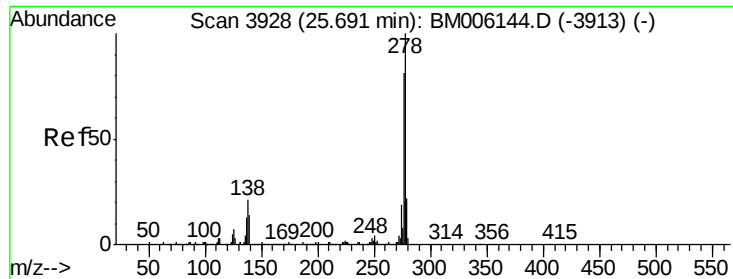

#40

Dibenzo(a,h)anthracene

Concen: 3.43 ng/ul

RT: 25.71 min Scan# 3931

Delta R.T. 0.02 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24

Instrument :

BNA_M

ClientSampleId :

D9YF4MS


Tgt Ion:278 Resp: 165885

Ion Ratio Lower Upper

278 100

139 22.8 13.0 19.4#




279 33.0 18.8 28.2#

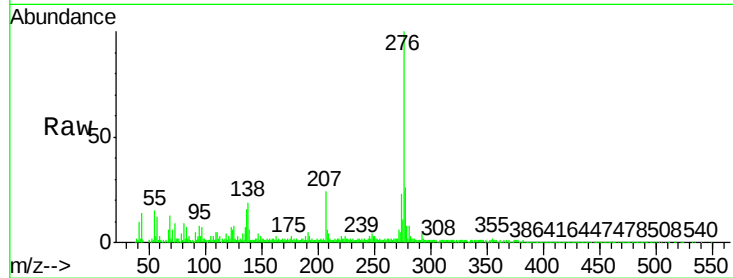

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

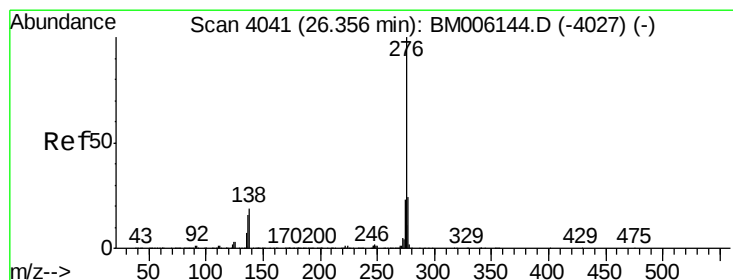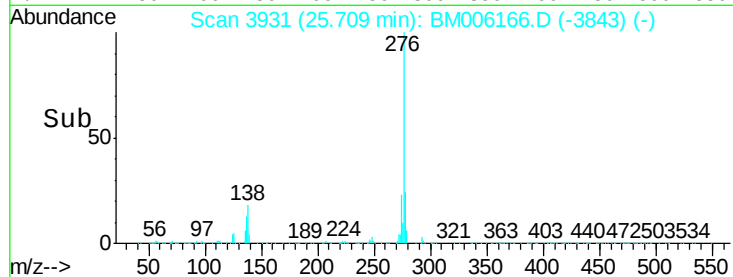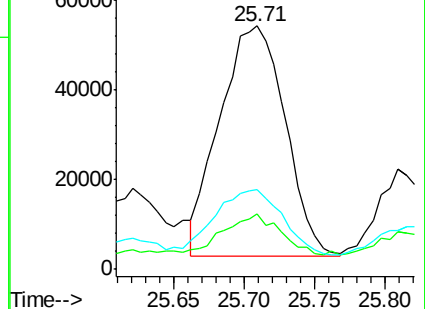

#41

Benzo(g,h,i)perylene

Concen: 12.22 ng/ul

RT: 26.39 min Scan# 4047

Delta R.T. 0.04 min

Lab File: BM006166.D

Acq: 30 Jun 2016 20:24


Tgt Ion:276 Resp: 597048

Ion Ratio Lower Upper

276 100

138 19.7 16.6 25.0

277 25.3 18.9 28.3

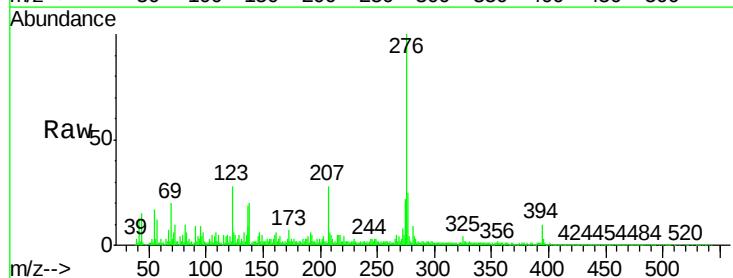

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

