

Data Path : Z:\HPCHEM1\BNA M\DATA\BM063016\
 Data File : BM006164.D
 Acq On : 30 Jun 2016 19:12
 Operator : UM/SJ
 Sample : H3779-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:15:27 PM

Quant Time: Jul 01 01:03:13 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 29 00:57:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	205788	20.00	ng/ul	0.00
7) Naphthalene-d8	10.43	136	812478	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.30	164	421403	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.05	188	910525	20.00	ng/ul	0.00
29) Chrysene-d12	21.25	240	965543	20.00	ng/ul	0.00
34) Perylene-d12	23.47	264	1035562	20.00	ng/ul	0.01

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	6025	1.36	ng/uL	0.00
3) Phenol-d5	6.83	99	251942	14.99	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.99	67	154462	15.58	ng/ul	0.00
5) 2-Chlorophenol-d4	7.19	132	195750	15.17	ng/ul	0.00
6) 4-Methylphenol-d8	8.36	113	192053	14.19	ng/ul	0.00
8) Nitrobenzene-d5	8.80	128	93680	17.12	ng/ul	0.00
9) 2-Nitrophenol-d4	9.52	143	99032	15.81	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.06	165	179836	15.74	ng/ul	0.00
12) 4-Chloroaniline-d4	10.57	131	93258	10.32	ng/ul	0.00
16) Dimethylphthalate-d6	13.72	166	491986	16.29	ng/ul	0.00
17) Acenaphthylene-d8	13.99	160	647804	17.67	ng/ul	0.00
20) 4-Nitrophenol-d4	14.52	143	86395	15.07	ng/ul	0.00
21) Fluorene-d10	15.30	176	444037	17.23	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.43	200	47803	14.82	ng/ul	0.00
26) Anthracene-d10	17.15	188	668165	18.29	ng/ul	0.00
30) Pyrene-d10	19.45	212	708204	18.21	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.33	264	744103	18.06	ng/ul	0.01

Target Compounds

						Ovalue
18) Acenaphthylene	14.02	152	58166	1.52	ng/ul	98
25) Phenanthrene	17.10	178	488827	11.34	ng/ul	99
27) Anthracene	17.19	178	156713	3.54	ng/ul	99
28) Fluoranthene	19.12	202	1365805	25.88	ng/ul	100
31) Pyrene	19.49	202	1101139	21.62	ng/ul	96
32) Benzo(a)anthracene	21.24	228	756124	15.06	ng/ul	97
33) Chrysene	21.29	228	732972	15.86	ng/ul	98
35) Benzo(b)fluoranthene	22.81	252	1122037	20.88	ng/ul	97
36) Benzo(k)fluoranthene	22.85	252	386632m	7.67	ng/ul	
38) Benzo(a)pyrene	23.38	252	743079	14.63	ng/ul	99
39) Indeno(1,2,3-cd)pyrene	25.71	276	590212	11.18	ng/ul#	93
40) Dibenzo(a,h)anthracene	25.70	278	158099	3.62	ng/ul#	72
41) Benzo(g,h,i)perylene	26.39	276	540088	12.23	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM063016\
Data File : BM006164.D
Acq On : 30 Jun 2016 19:12
Operator : UM/SJ
Sample : H3779-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9YD5

Quant Time: Jul 01 01:03:13 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 29 00:57:09 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
7/1/2016 7:15:27 PM

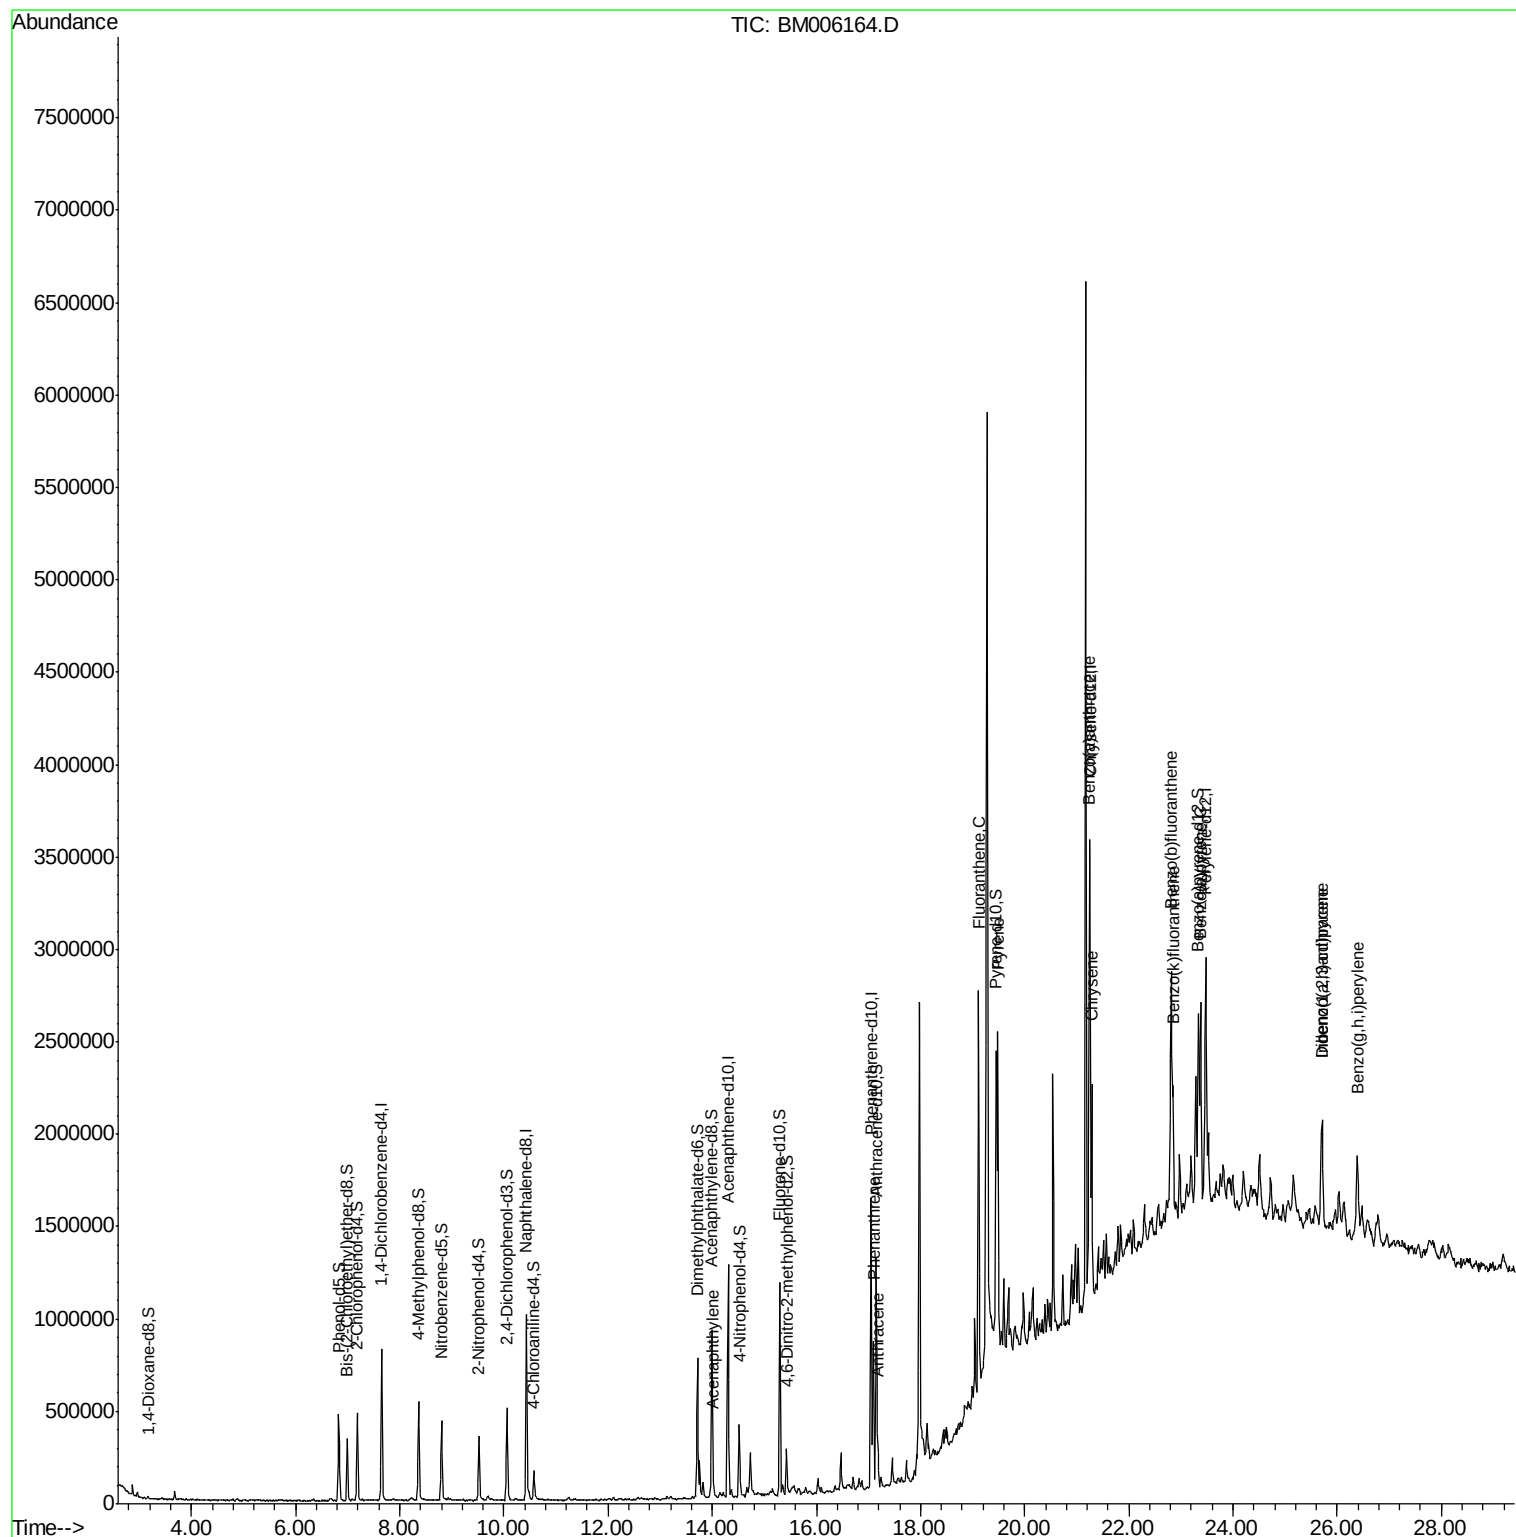



#18

Acenaphthylene

Concen: 1.52 ng/ul

RT: 14.02 min Scan# 1944

Delta R.T. 0.00 min

Lab File: BM006164.D

Acq: 30 Jun 2016 19:12

Instrument :

BNA_M





ClientSampleId :

D9YD5

Tot Ion:	152	Resp:	58166
Ion Ratio	Lower	Upper	
152	100		
151	20.8	15.8	23.6
153	13.0	10.3	15.5

Manual Integrations
APPROVED

sohil
7/1/2016 7:15:27 PM

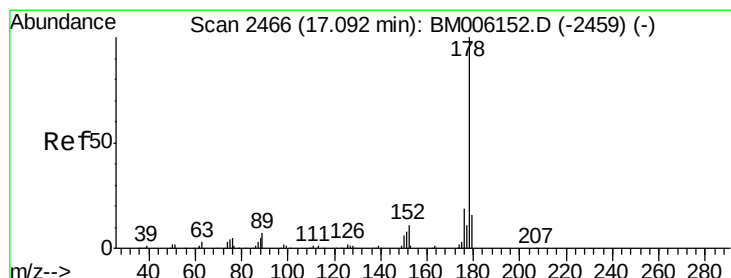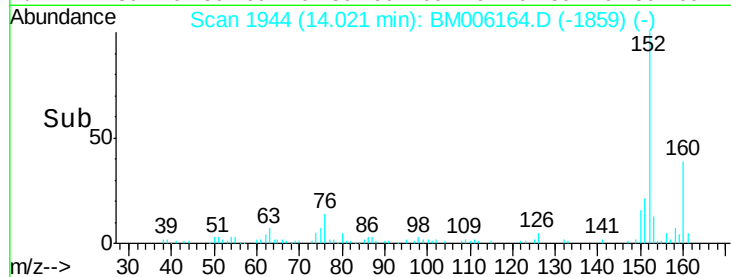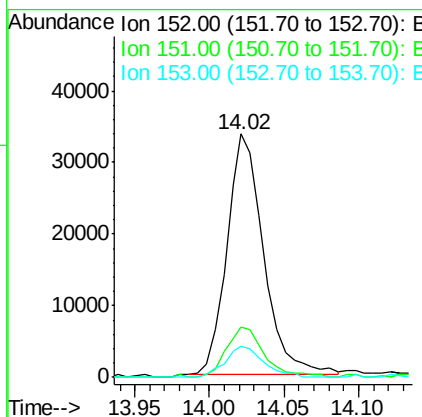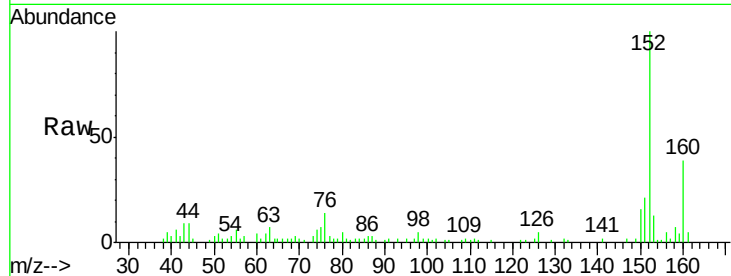

#25

Phenanthrene

Concen: 11.34 ng/ul




RT: 17.10 min Scan# 2467


Delta R.T. 0.01 min

Lab File: BM006164.D

Acq: 30 Jun 2016 19:12

Tgt Ion:	178	Resp:	488827
Ion Ratio	Lower	Upper	
178	100		
179	15.1	12.2	18.2
176	19.5	15.3	22.9

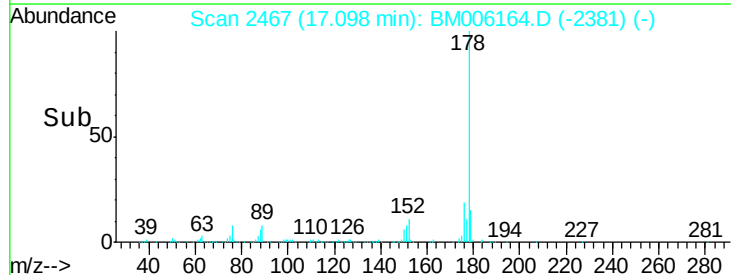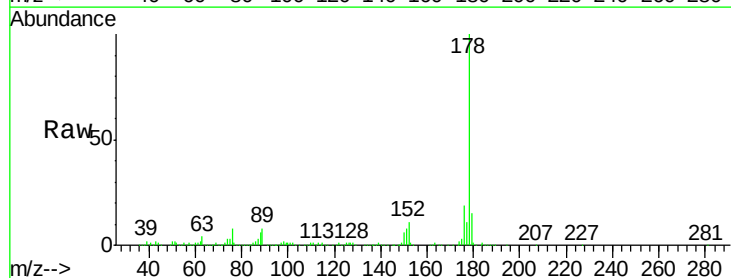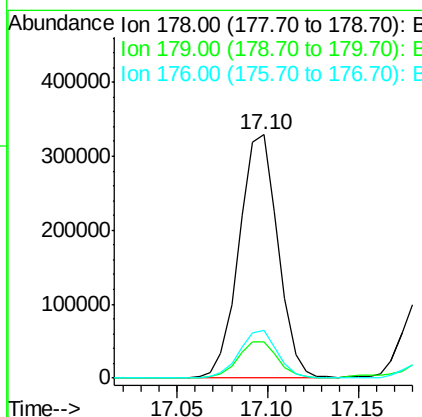

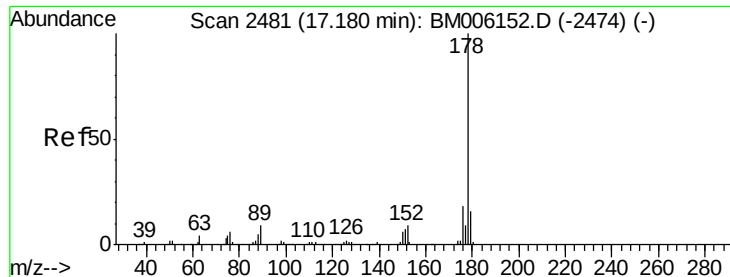


#27
 Anthracene
 Concen: 3.54 ng/ul
 RT: 17.19 min Scan# 2482
 Delta R.T. 0.00 min
 Lab File: BM006164.D
 Acq: 30 Jun 2016 19:12

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5




Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.3	18.5
176	19.3	14.6	22.0

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:15:27 PM

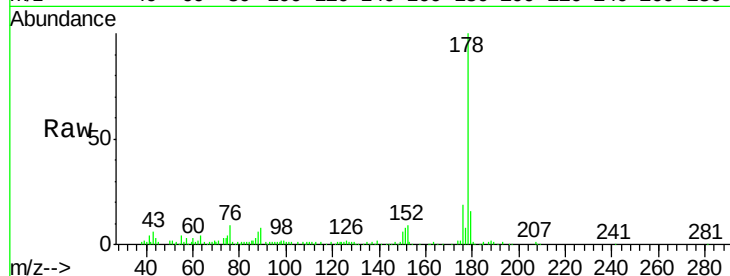


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

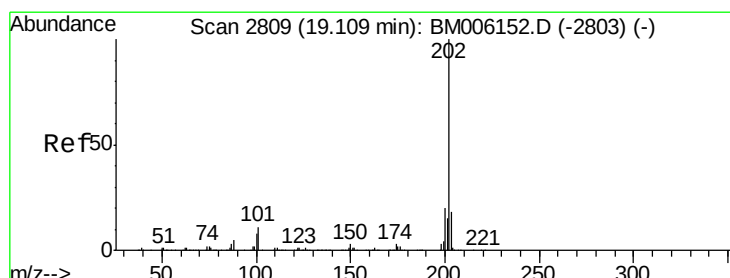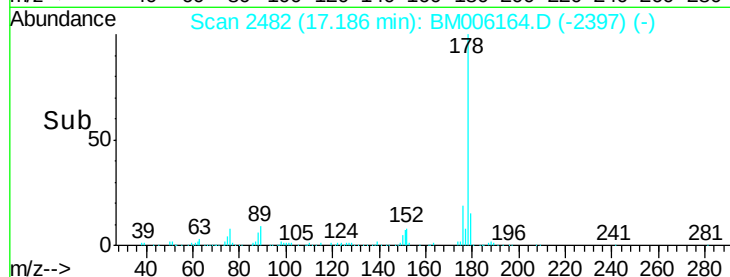
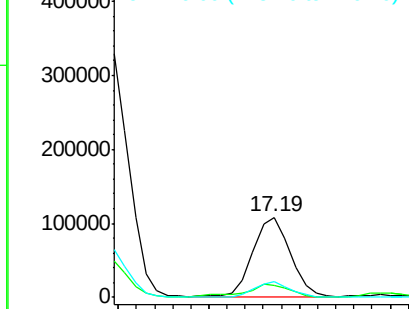



#28
 Fluoranthene
 Concen: 25.88 ng/ul
 RT: 19.12 min Scan# 2810
 Delta R.T. 0.00 min
 Lab File: BM006164.D
 Acq: 30 Jun 2016 19:12

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.6	8.5	12.7
100	8.0	6.5	9.7

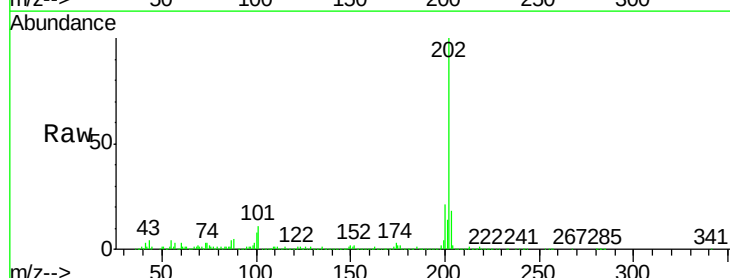

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

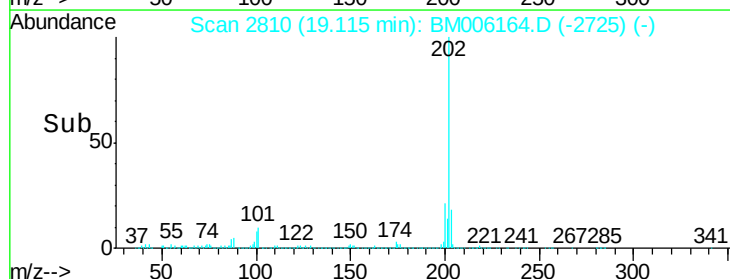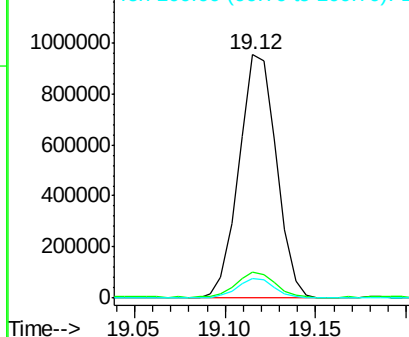







#31
Pvrene
Concen: 21.62 ng/ul
RT: 19.49 min Scan# 2873
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Instrument :
BNA_M
ClientSampleId :
D9YD5

Tot Ion	Ion	Ratio	Resp	Lower	Upper
202	100				
101	12.5		11.0	16.4	
100	9.4		8.9	13.3	




Manual Integrations
APPROVED


sohil
7/1/2016 7:15:27 PM

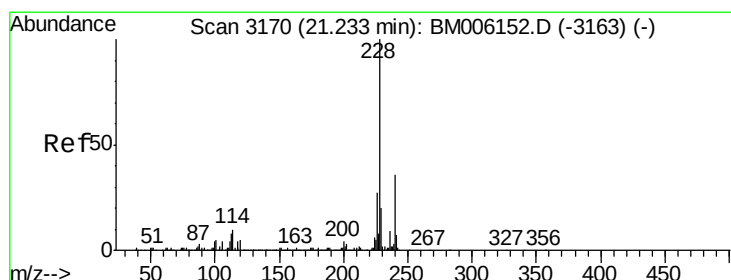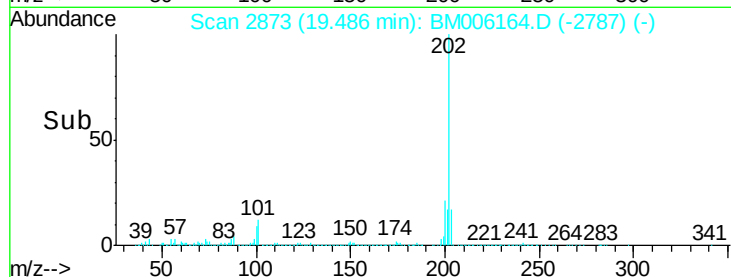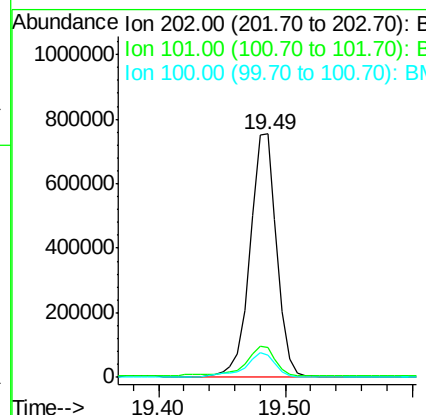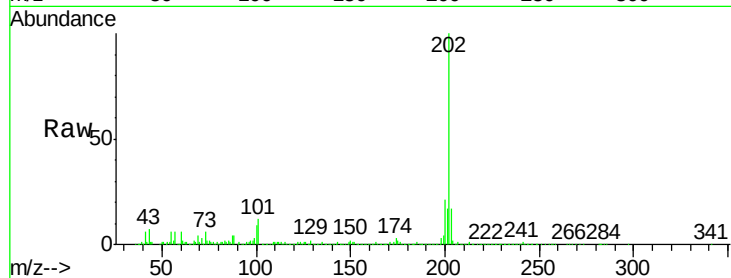

#32
Benzo(a)anthracene
Concen: 15.06 ng/ul
RT: 21.24 min Scan# 3171
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
228	100				
229	20.5		15.6	23.4	
226	28.6		21.6	32.4	

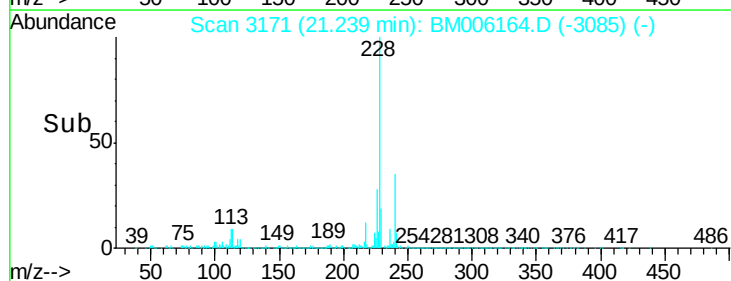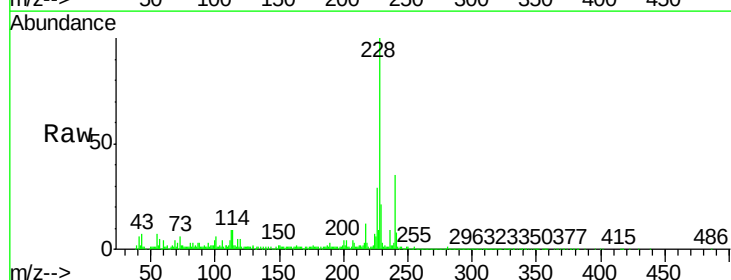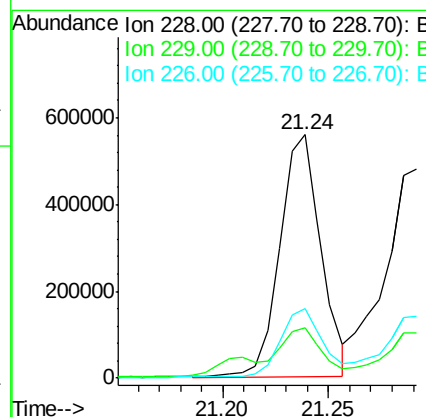







#33
Chrysene
Concen: 15.86 ng/ul
RT: 21.29 min Scan# 3180
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Instrument :
BNA_M
ClientSampleId :
D9YD5

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.6	23.8	35.6
229	21.5	15.8	23.6




Manual Integrations
APPROVED


sohil
7/1/2016 7:15:27 PM

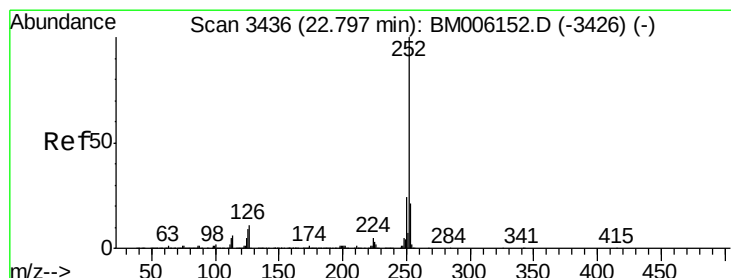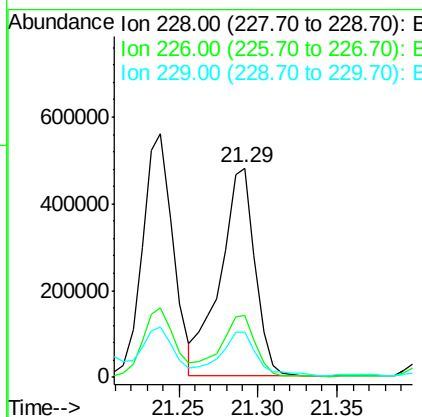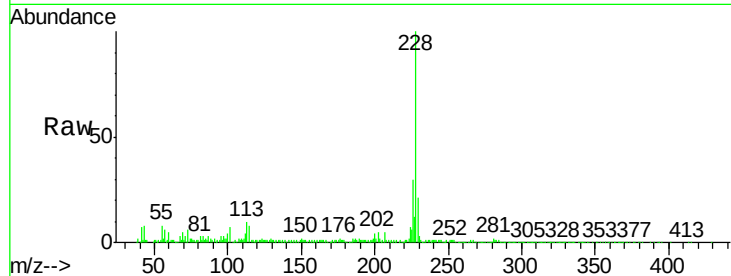

#35
Benzo(b)fluoranthene
Concen: 20.88 ng/ul
RT: 22.81 min Scan# 3438
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	17.2	25.8
125	9.8	7.8	11.6

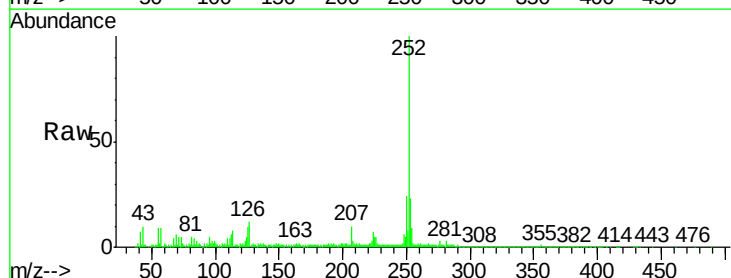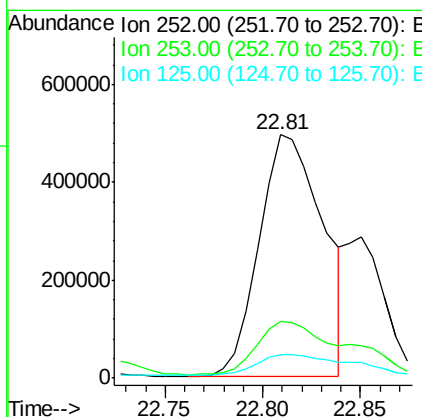







#36
Benzo(k)fluoranthene
Concen: 7.67 ng/ul m
RT: 22.85 min Scan# 3445
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Instrument :
BNA_M
ClientSampleId :
D9YD5

Tot Ion:	252	Resp:	386632
Ion Ratio	Lower	Upper	
252	100		
253	23.3	17.6	26.4
125	10.9	8.1	12.1




Manual Integrations
APPROVED


sohil
7/1/2016 7:15:27 PM

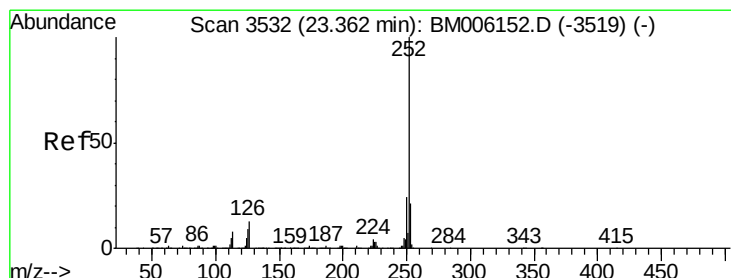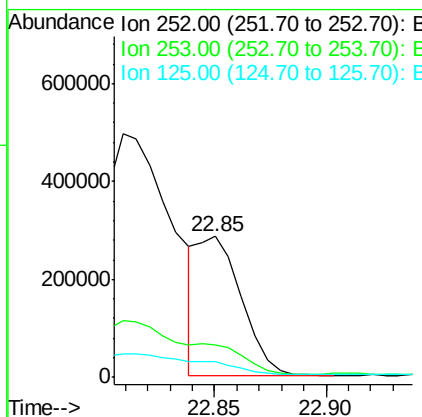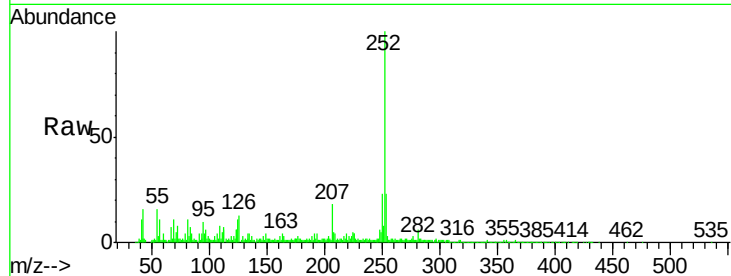

#38
Benzo(a)pyrene
Concen: 14.63 ng/ul
RT: 23.38 min Scan# 3535
Delta R.T. 0.01 min
Lab File: BM006164.D
Acq: 30 Jun 2016 19:12

Tgt Ion:	252	Resp:	743079
Ion Ratio	Lower	Upper	
252	100		
253	22.9	17.8	26.6
125	11.1	8.7	13.1

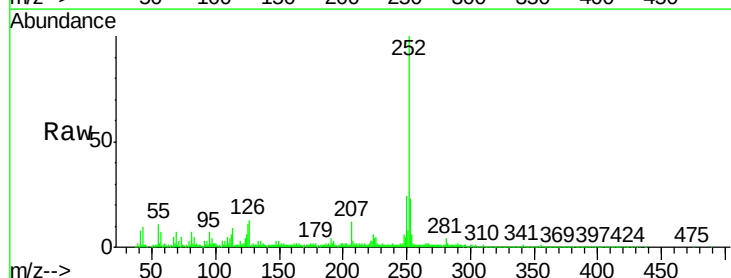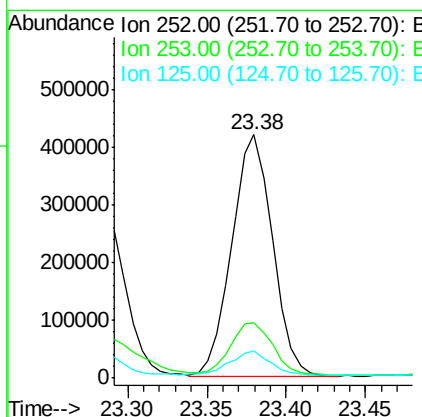




#39
 Indeno(1,2,3-cd)pyrene
 Concen: 11.18 ng/ul
 RT: 25.71 min Scan# 3931
 Delta R.T. 0.02 min
 Lab File: BM006164.D
 Acq: 30 Jun 2016 19:12

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Tot Ion	Ratio	Resp	Lower	Upper
276	100	590212		
138	18.6		20.4	30.6#
277	25.4		20.6	30.8

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:15:27 PM



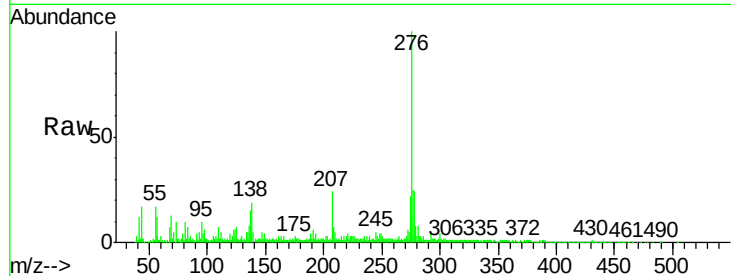


Abundance

Ion 276.00 (275.70 to 276.70): E


Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

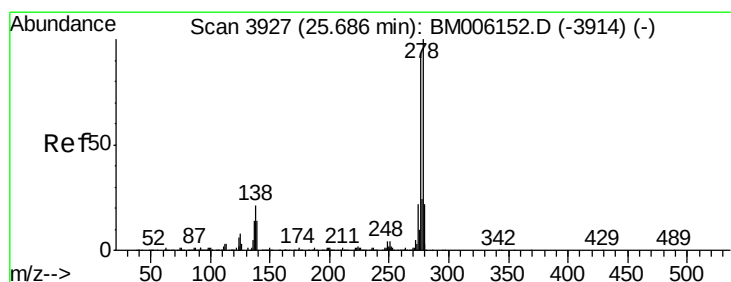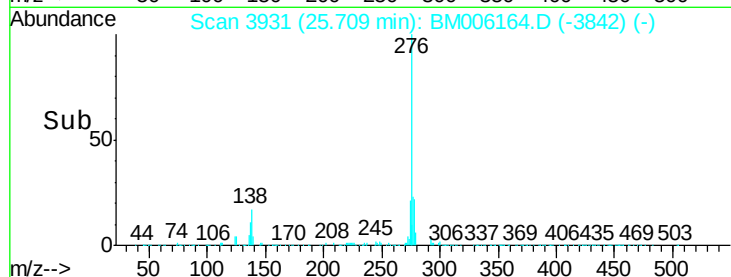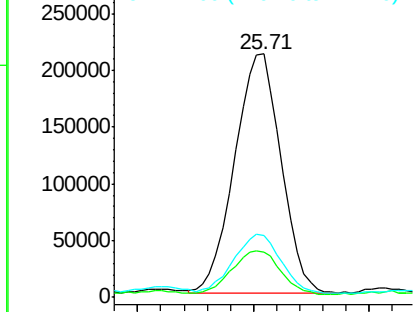

#40
 Dibenzo(a,h)anthracene
 Concen: 3.62 ng/ul
 RT: 25.70 min Scan# 3930
 Delta R.T. 0.01 min
 Lab File: BM006164.D
 Acq: 30 Jun 2016 19:12

Tgt Ion	Ratio	Resp	Lower	Upper
278	100	158099		
139	0.0		13.0	19.4#
279	33.5		18.8	28.2#


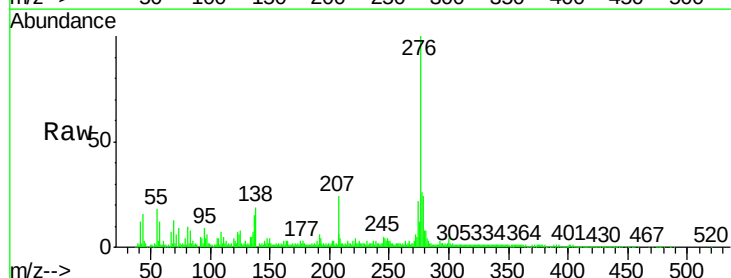



Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

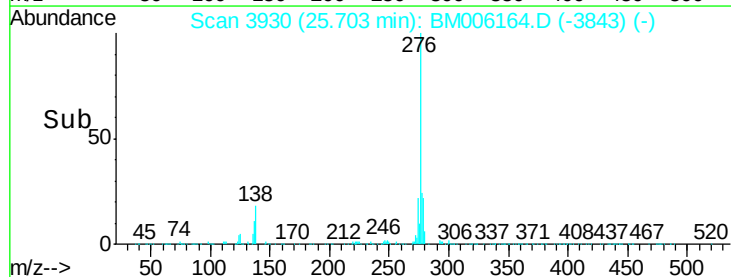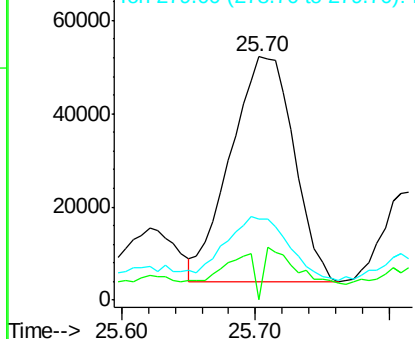



#41
 Benzo(a,h,i)perylene
 Concen: 12.23 ng/ul
 RT: 26.39 min Scan# 4047
 Delta R.T. 0.04 min
 Lab File: BM006164.D
 Acq: 30 Jun 2016 19:12

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Tot Ion:	276	Resp:	540088
Ion Ratio	Lower	Upper	
276	100		
138	19.5	16.6	25.0
277	24.6	18.9	28.3

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:15:27 PM

