
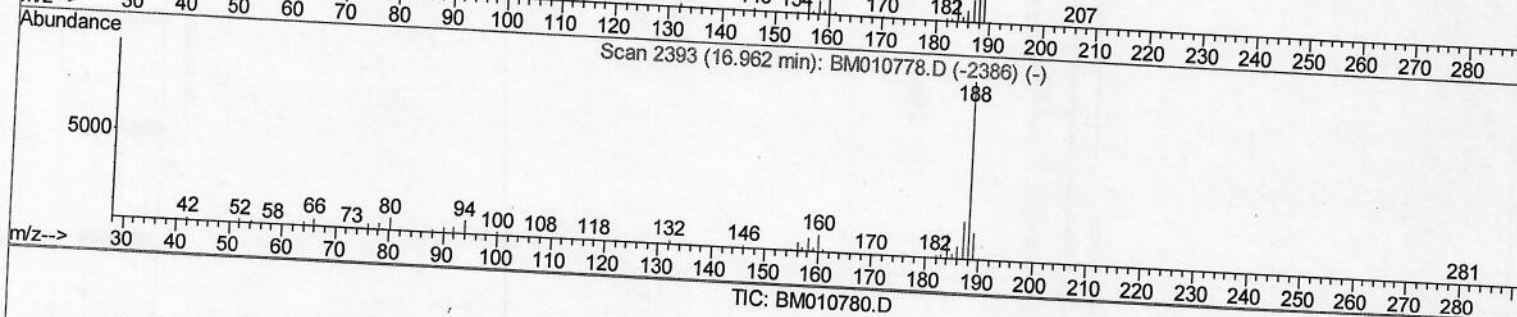


Data File : BM010780.D
Acq On : 30 Jun 2017 18:48
Operator : SJ/JU
Sample : I3942-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC79

mohammad
7/3/2017 8:08:07 AM

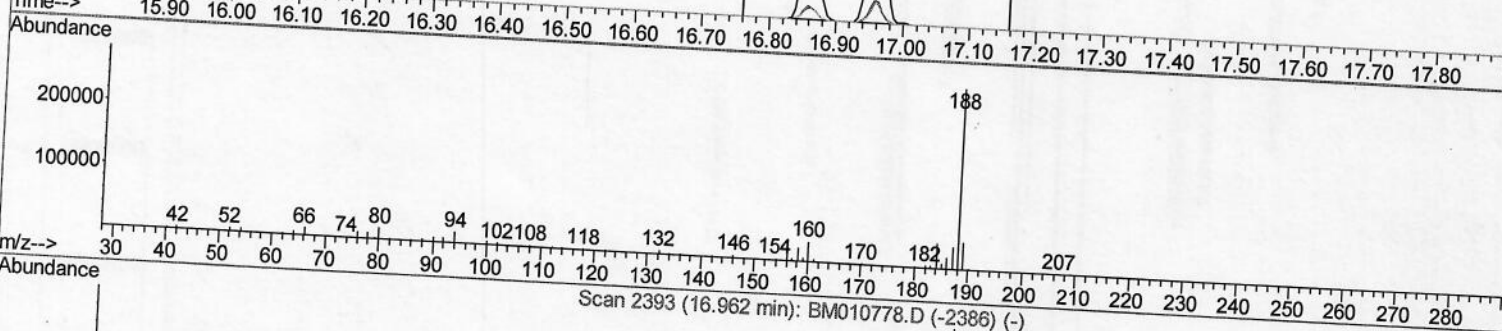

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	6.00
80.00	5.90	6.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM063017\
Quantitation Report (Qedit)


Data File : BM010780.D
Acq On : 30 Jun 2017 18:48
Operator : SJ/JU
Sample : I3942-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 01 06:44:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 01 06:43:48 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BDC79

Manual Integrations
APPROVED

mohammad
7/3/2017 8:08:07 AM

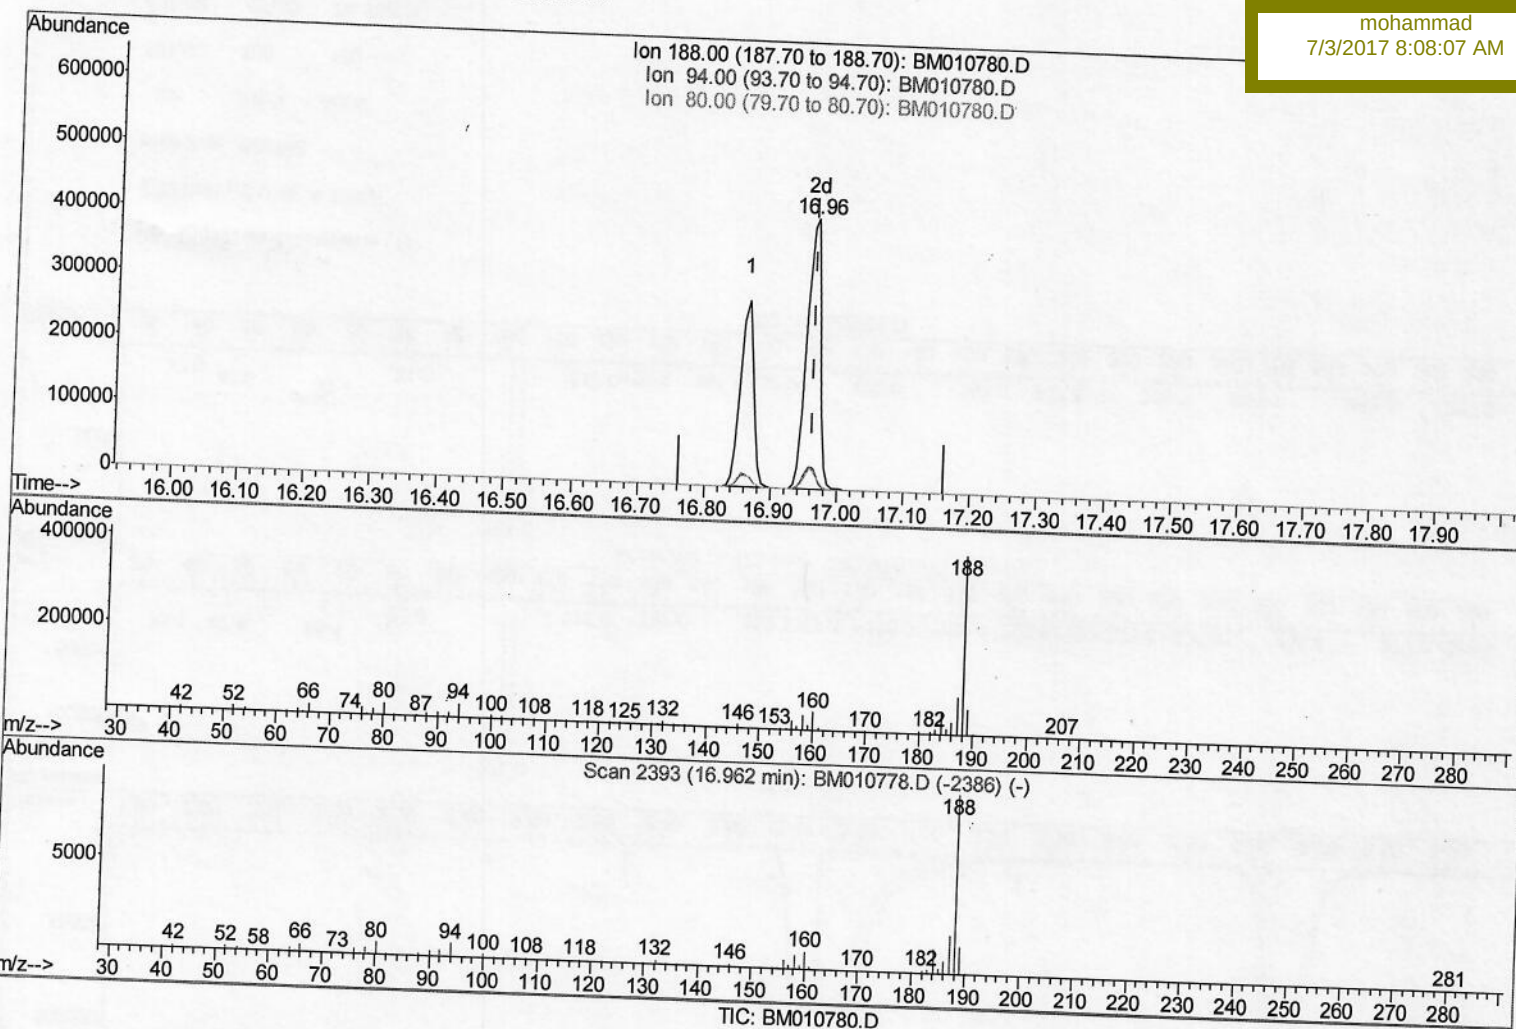

(70) Anthracene-d10 (S)

16.962min (+0.000) 31.62ng/ul m

response 588911

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	7.75#
80.00	5.90	7.04
0.00	0.00	0.00

5.9
07/03/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM063017\

Quantitation Report

(QT Reviewed)

Data File : BM010780.D

Acq On : 30 Jun 2017 18:48

Operator : SJ/JU

Sample : I3942-03

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 01 06:53:29 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Jul 01 06:43:48 2017

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

BDC79

Manual Integrations

APPROVED

mohammad

7/3/2017 8:08:07 AM

Internal Standards

	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	47712	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	216842	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	147890	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	385637	20.00	ng/ul	0.00
75) Chrysene-d12	21.07	240	437659	20.00	ng/ul	0.00
83) Perylene-d12	23.21	264	354391	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	6531	7.84	ng/uL	0.00
5) Phenol-d5	6.64	99	25433	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	71703	27.64	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	72069	22.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	50441	13.39	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	49814	32.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	57612	32.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	110557	29.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	1799	0.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	412871	31.80	ng/ul	0.00
46) Acenaphthylene-d8	13.79	160	469429	31.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	11000	4.81	ng/ul	-0.01
57) Fluorene-d10	15.11	176	359705	32.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	69221	29.23	ng/ul	0.00
70) Anthracene-d10	16.96	188	588911m	31.62	ng/ul	0.00
76) Pyrene-d10	19.27	212	729774	35.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	528636	30.86	ng/ul	0.00

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

29.9
07/03/17


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM063017\
Data File : BM010780.D Quantitation Report (QT Reviewed)
Acq On : 30 Jun 2017 18:48
Operator : SJ/JU
Sample : I3942-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jul 01 06:53:29 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 01 06:43:48 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BDC79

Manual Integrations
APPROVED

mohammad
7/3/2017 8:08:07 AM

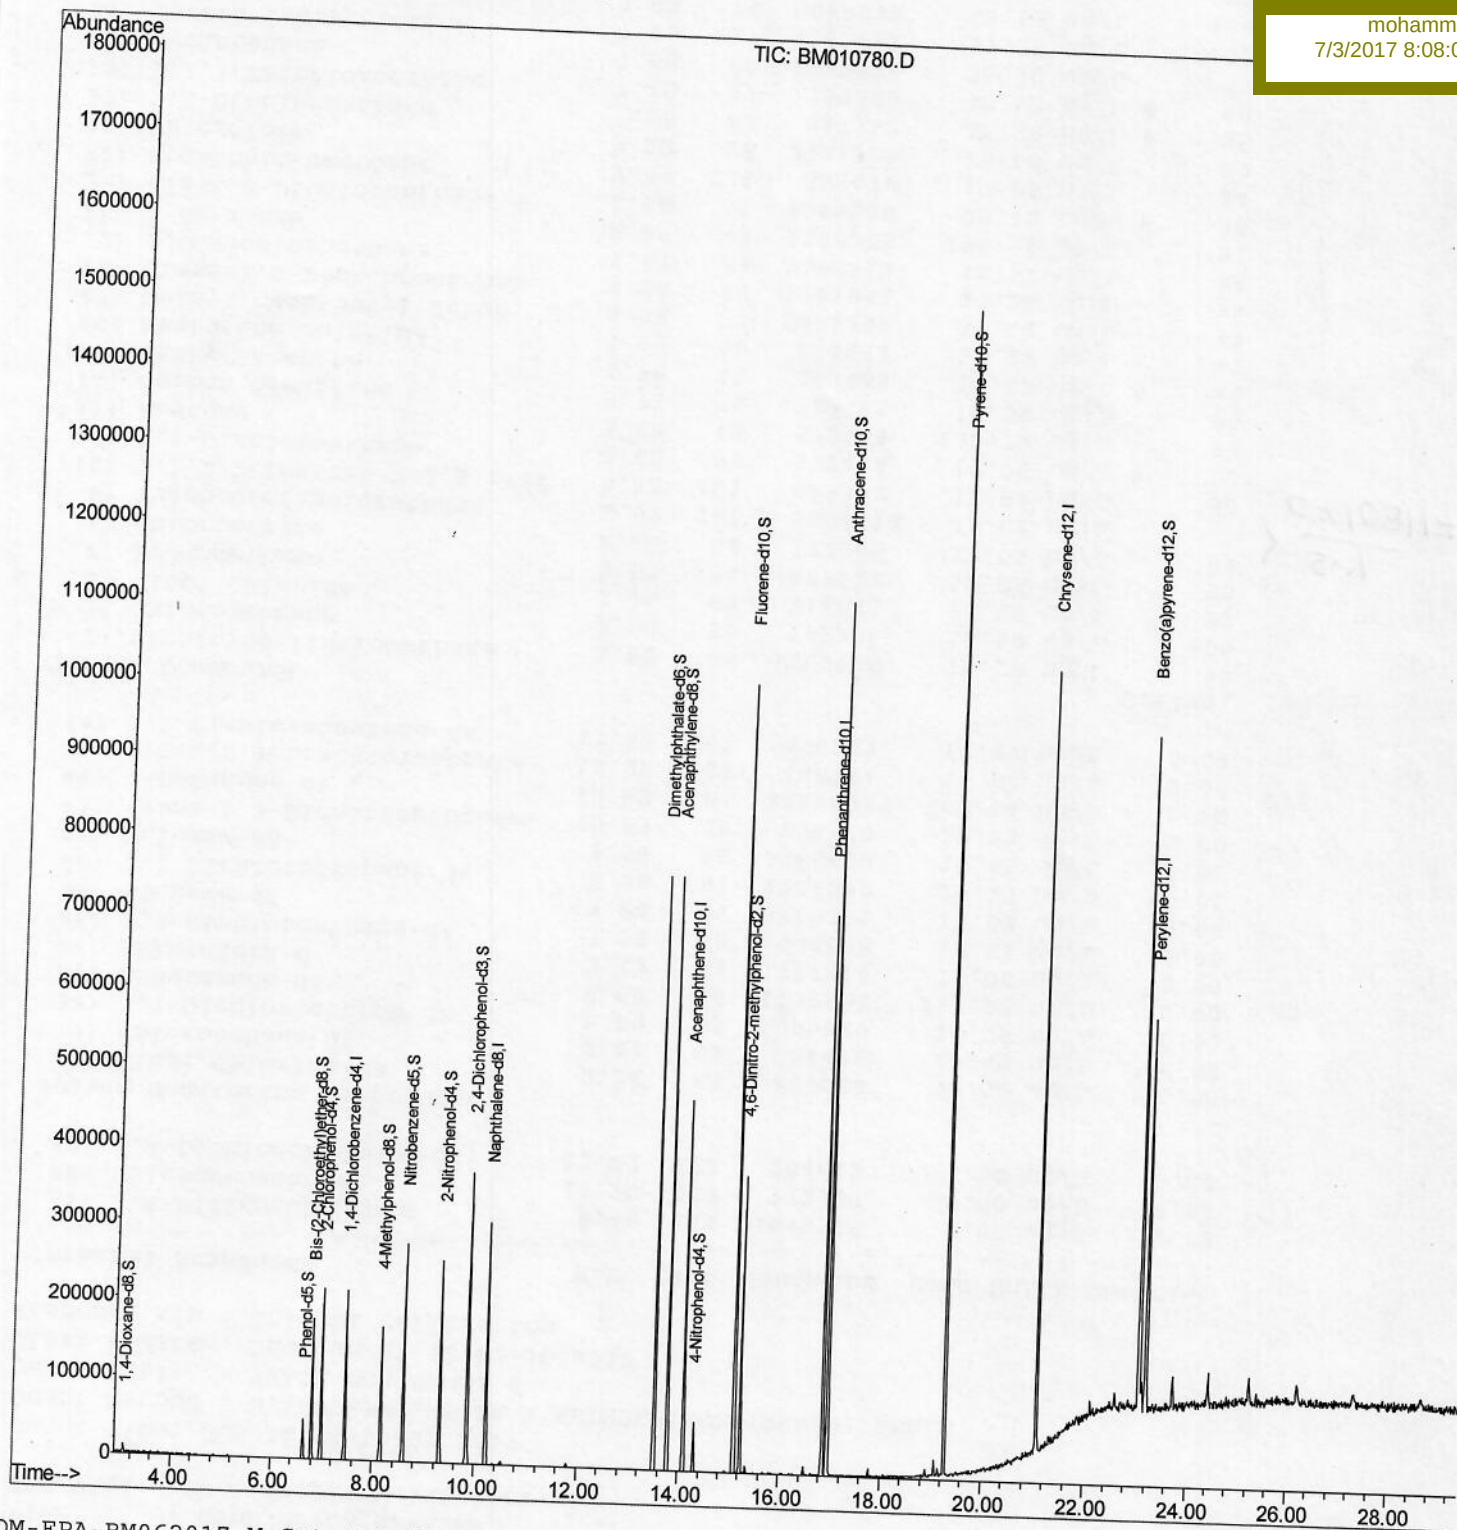

SOM-EPA-BM062017.M Sat Jul 01 06:54:02 2017