


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030765.D
Acq On : 02 Jul 2021 05:03
Operator : CG/JU
Sample : M2825-04
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ7

Manual Integrations
APPROVED

mohammad
7/2/2021 12:04:13 PM

Quant Time: Jul 02 05:44:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 04:13:39 2021
Response via : Initial Calibration

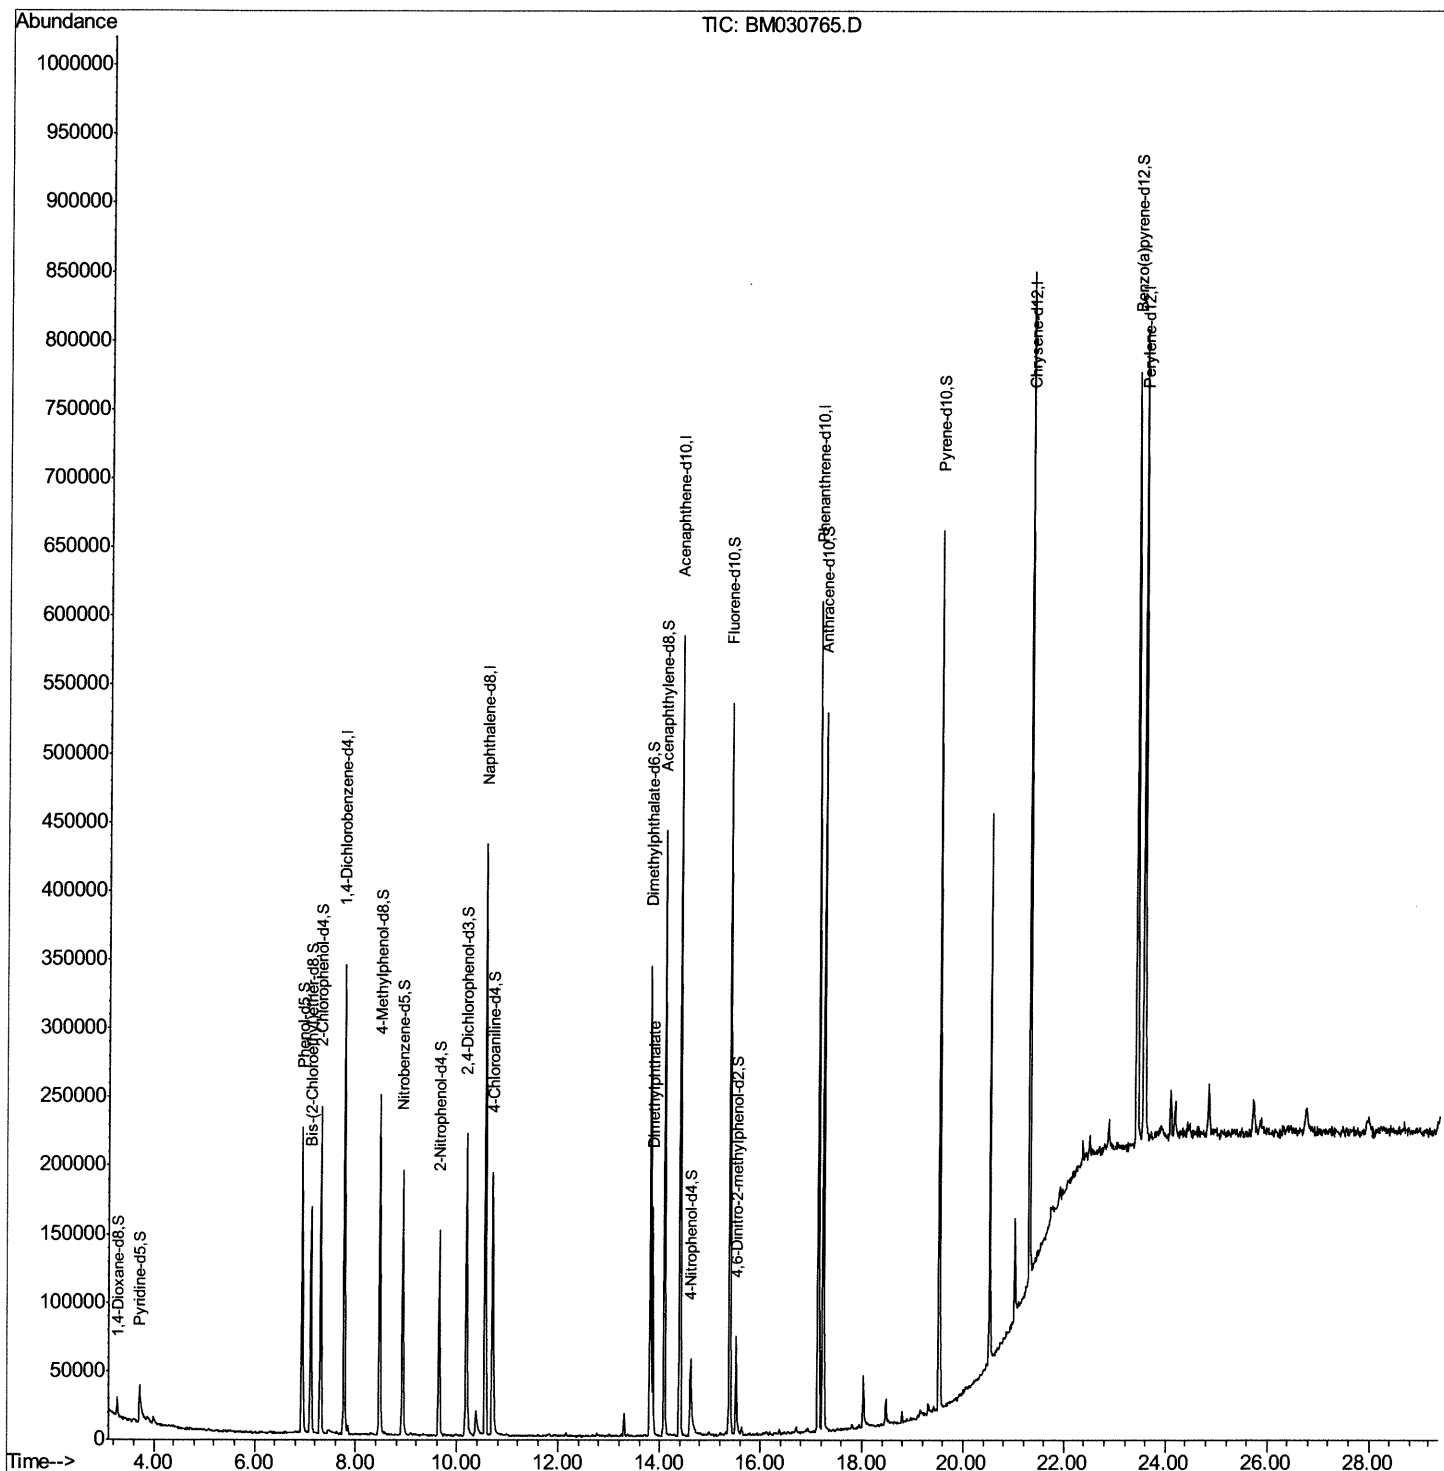

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030765.D
Acq On : 02 Jul 2021 05:03
Operator : CG/JU
Sample : M2825-04
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ7

Manual Integrations
APPROVED

mohammad
7/2/2021 12:04:13 PM




Quant Time: Jul 02 05:41:58 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jul 02 04:13:39 2021

Response via : Initial Calibration

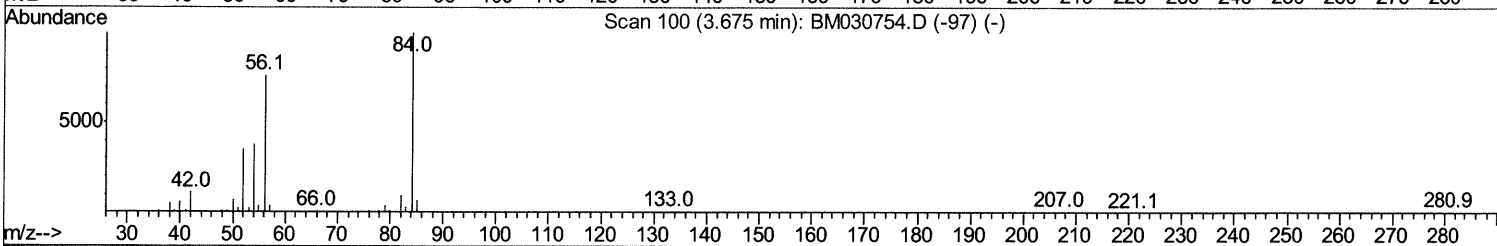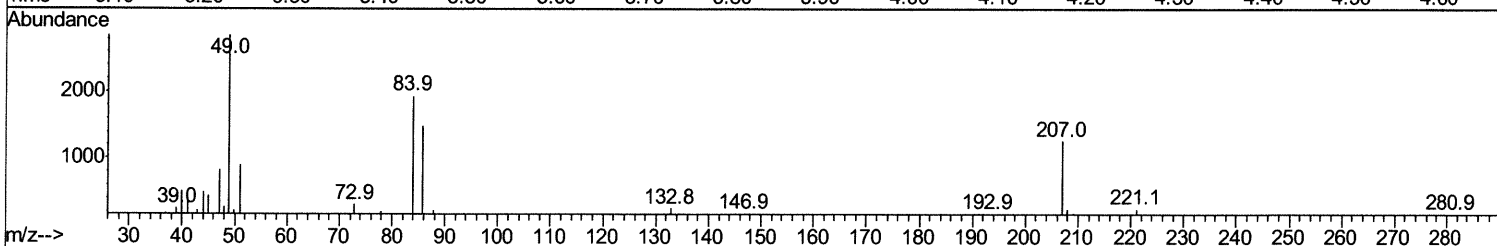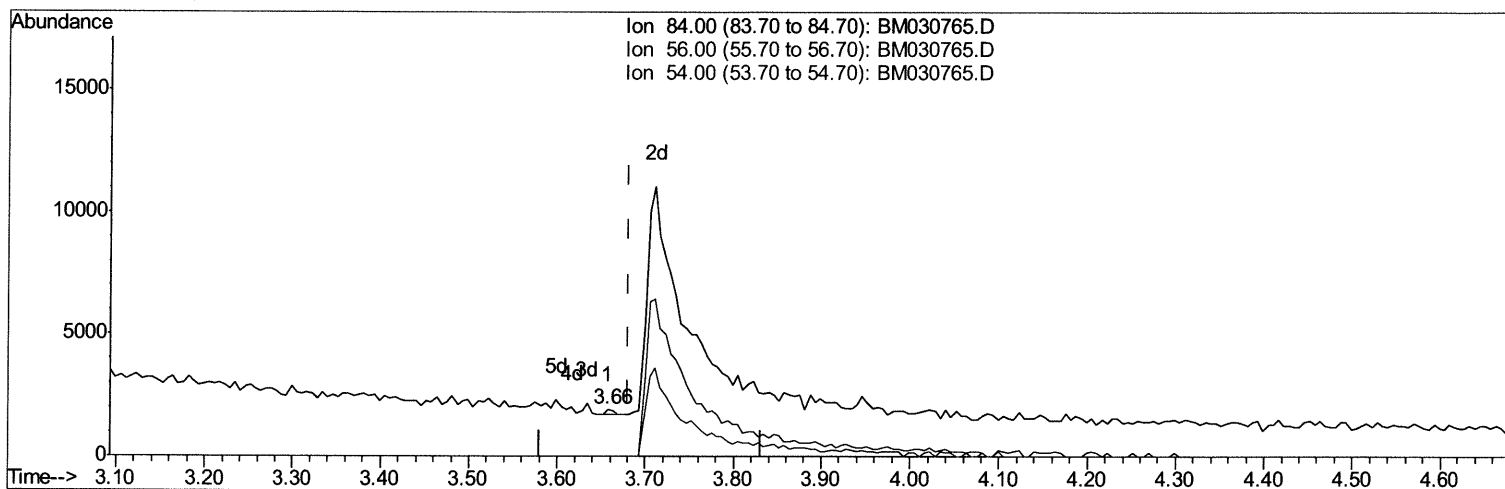

TIC: BM030765.D

(4) Pyridine-d5 (S)

3.658min (-0.023) 0.03ng/ul

response 165

Ion	Exp%	Act%
84.00	100	100
56.00	73.70	0.00#
54.00	35.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030765.D
Acq On : 02 Jul 2021 05:03
Operator : CG/JU
Sample : M2825-04
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ7

Manual Integrations
APPROVED

mohammad
7/2/2021 12:04:13 PM

Quant Time: Jul 02 05:41:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 04:13:39 2021
Response via : Initial Calibration

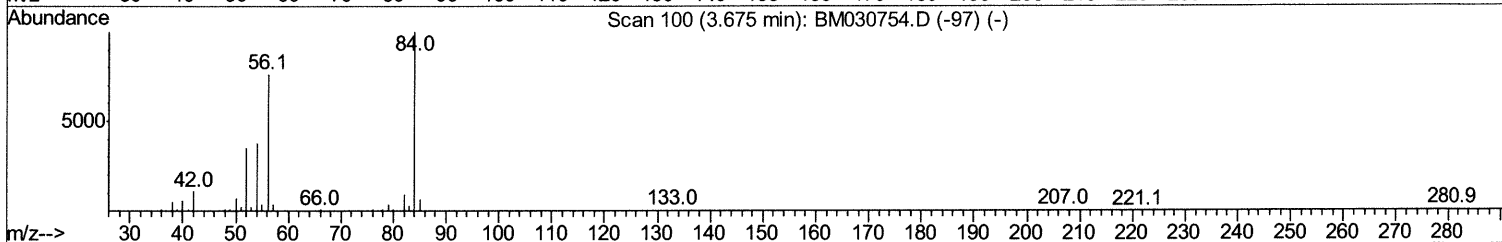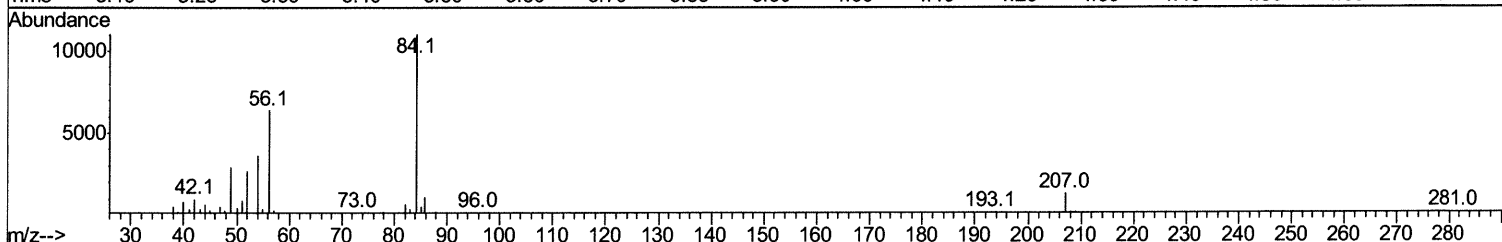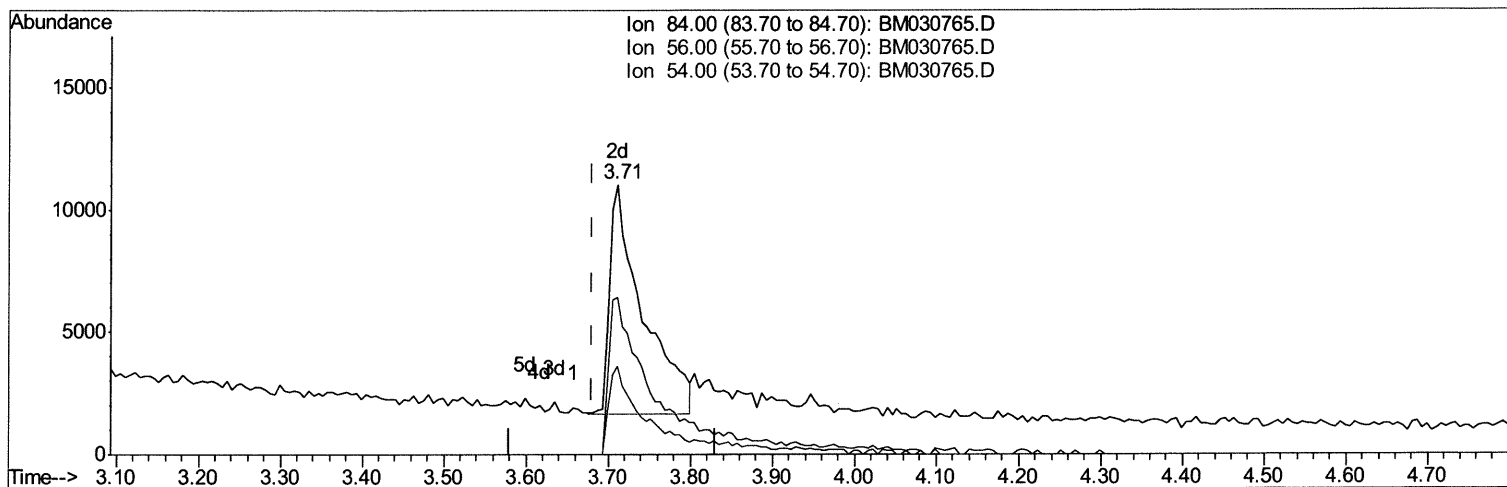

TIC: BM030765.D

(4) Pyridine-d5 (S)

3.711min (+0.030) 4.49ng/ul m

response 26375

Ion	Exp%	Act%
84.00	100	100
56.00	73.70	58.00#
54.00	35.80	32.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
 Data File : BM030765.D
 Acq On : 02 Jul 2021 05:03
 Operator : CG/JU
 Sample : M2825-04
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ7

Manual Integrations
 APPROVED

mohammad
 7/2/2021 12:04:13 PM

Quant Time: Jul 02 05:44:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 04:13:39 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	88608	20.00	ng/ul	-0.01
20) Naphthalene-d8	10.56	136	343942	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.40	164	195156	20.00	ng/ul	-0.01
64) Phenanthrene-d10	17.14	188	354109	20.00	ng/ul	0.00
79) Chrysene-d12	21.31	240	346332	20.00	ng/ul	0.00
88) Perylene-d12	23.56	264	410599	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	7066	3.23	ng/uL	0.00
4) Pyridine-d5	3.71	84	26375m	4.49	ng/ul	0.03
7) Phenol-d5	6.94	99	117619	15.39	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.11	67	79596	16.57	ng/ul	0.00
11) 2-Chlorophenol-d4	7.30	132	99853	16.93	ng/ul	0.00
15) 4-Methylphenol-d8	8.48	113	91572	15.40	ng/ul	0.00
21) Nitrobenzene-d5	8.93	128	42033	16.38	ng/ul	0.00
24) 2-Nitrophenol-d4	9.65	143	44430	15.58	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.18	165	85771	15.70	ng/ul	0.00
31) 4-Chloroaniline-d4	10.70	131	109939	14.43	ng/ul	0.00
46) Dimethylphthalate-d6	13.81	166	234150	17.38	ng/ul	-0.01
49) Acenaphthylene-d8	14.09	160	299009	17.09	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.62	143	20966	8.21	ng/ul	0.00
60) Fluorene-d10	15.39	176	205865	17.22	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.52	200	17848	7.70	ng/ul	0.00
73) Anthracene-d10	17.24	188	292924	17.72	ng/ul	0.00
81) Pyrene-d10	19.53	212	317540	17.50	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.41	264	384642	18.02	ng/ul	-0.02

Target Compounds				Ovalue	
47) Dimethylphthalate	13.86	163	107902	8.173	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed