


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030778.D
Acq On : 02 Jul 2021 16:14
Operator : CG/JU
Sample : M2825-15
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR3

Manual Integrations
APPROVED

mohammad
7/6/2021 9:24:50 AM

Quant Time: Jul 02 16:44:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

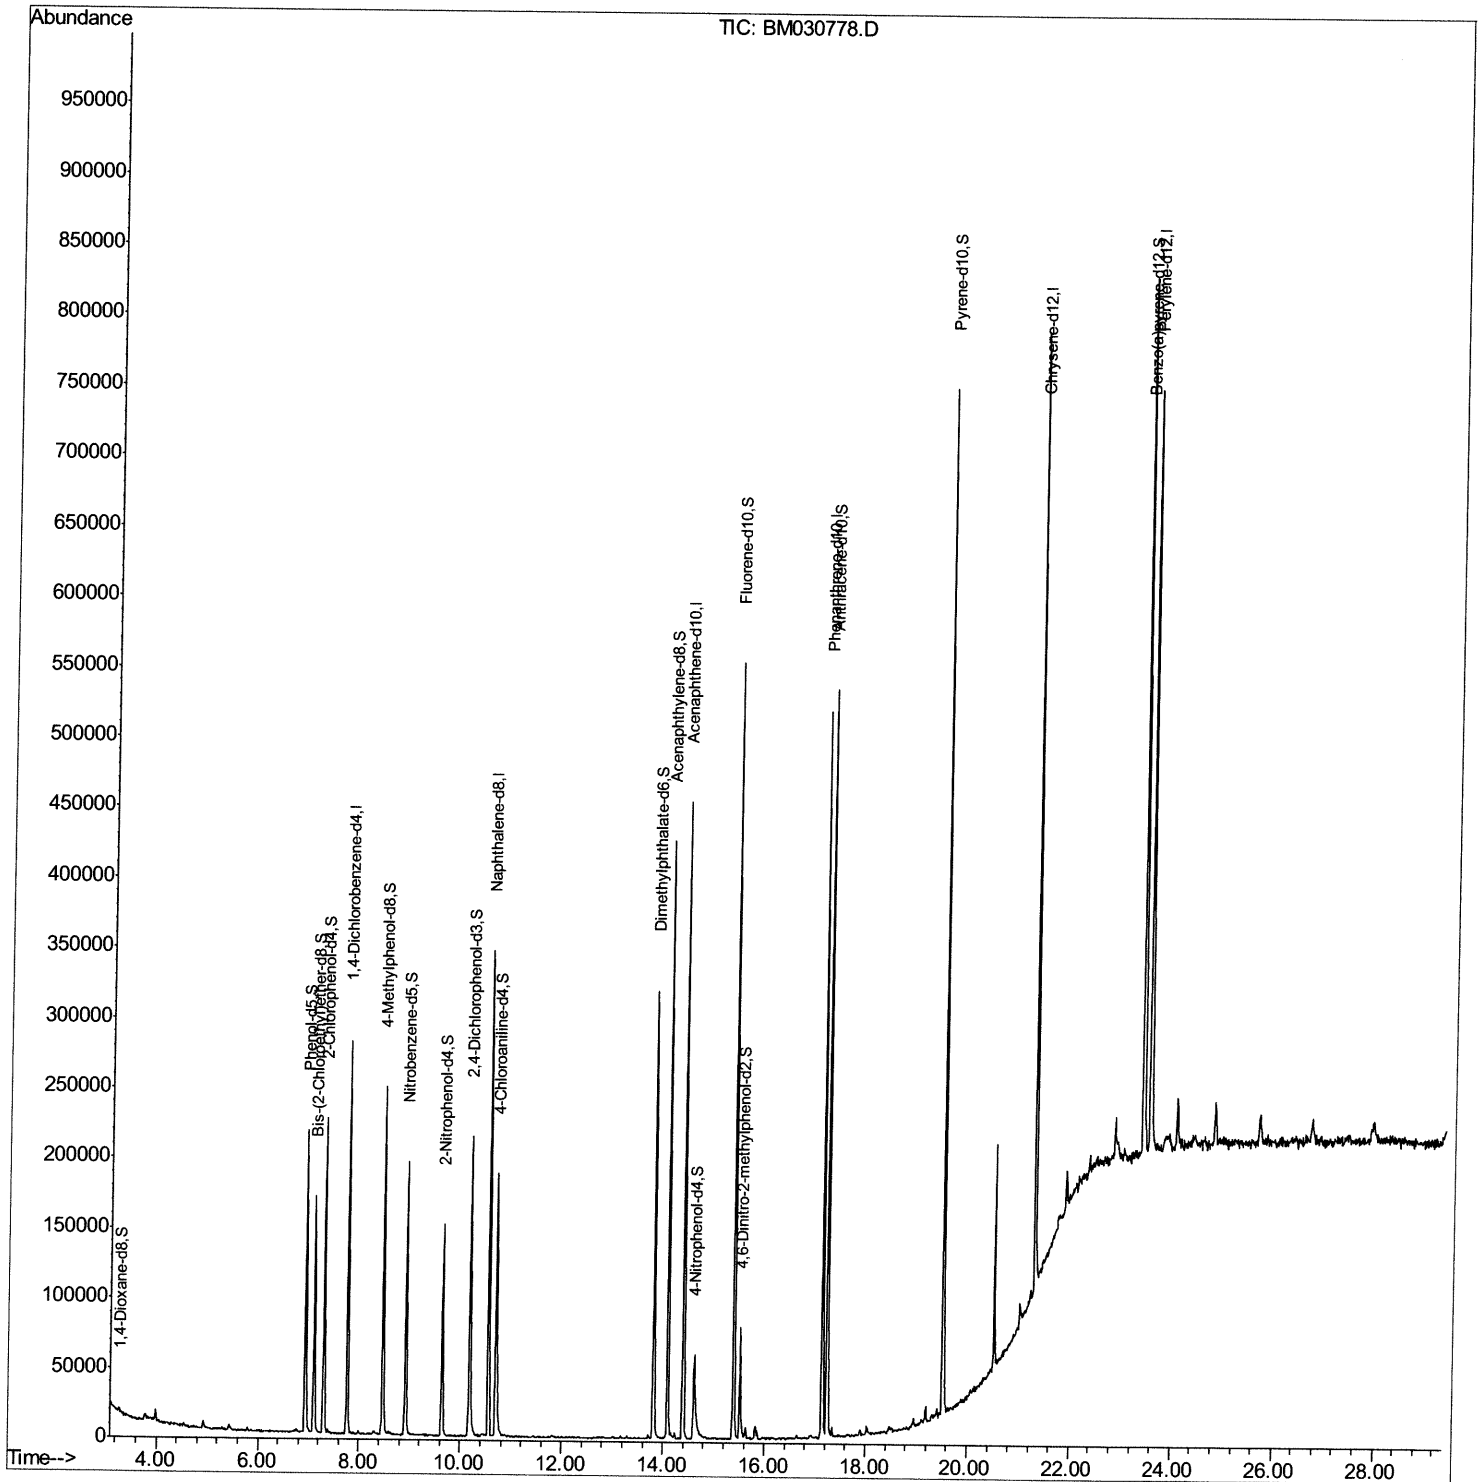




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030778.D
Acq On : 02 Jul 2021 16:14
Operator : CG/JU
Sample : M2825-15
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR3

Manual Integrations
APPROVED

mohammad
7/6/2021 9:24:50 AM

Quant Time: Jul 02 16:43:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

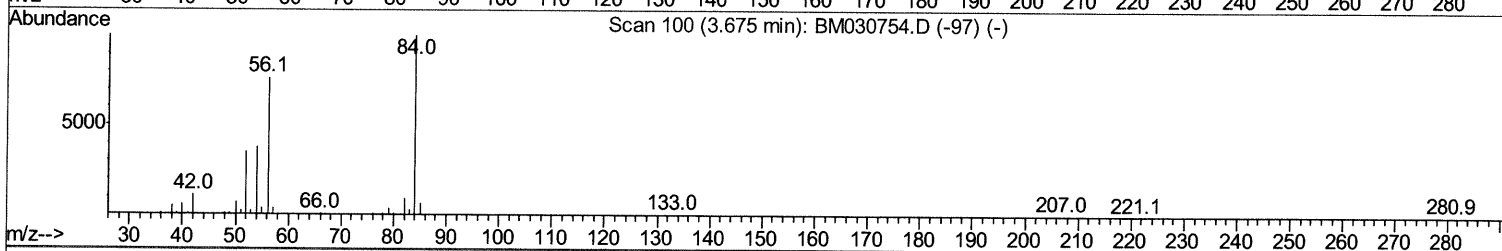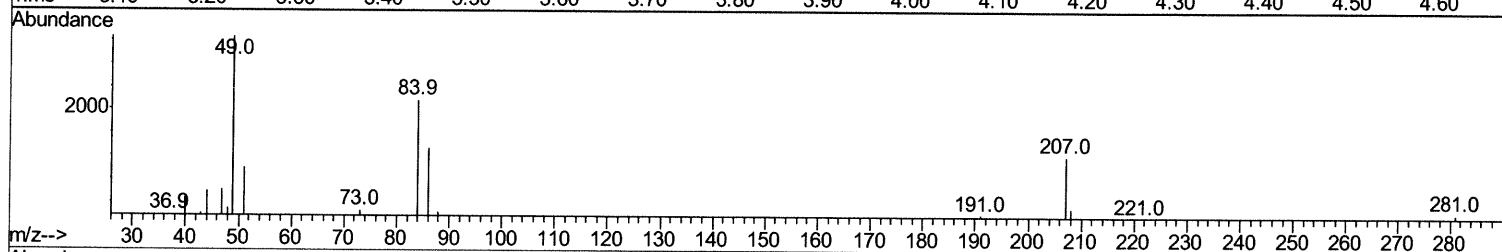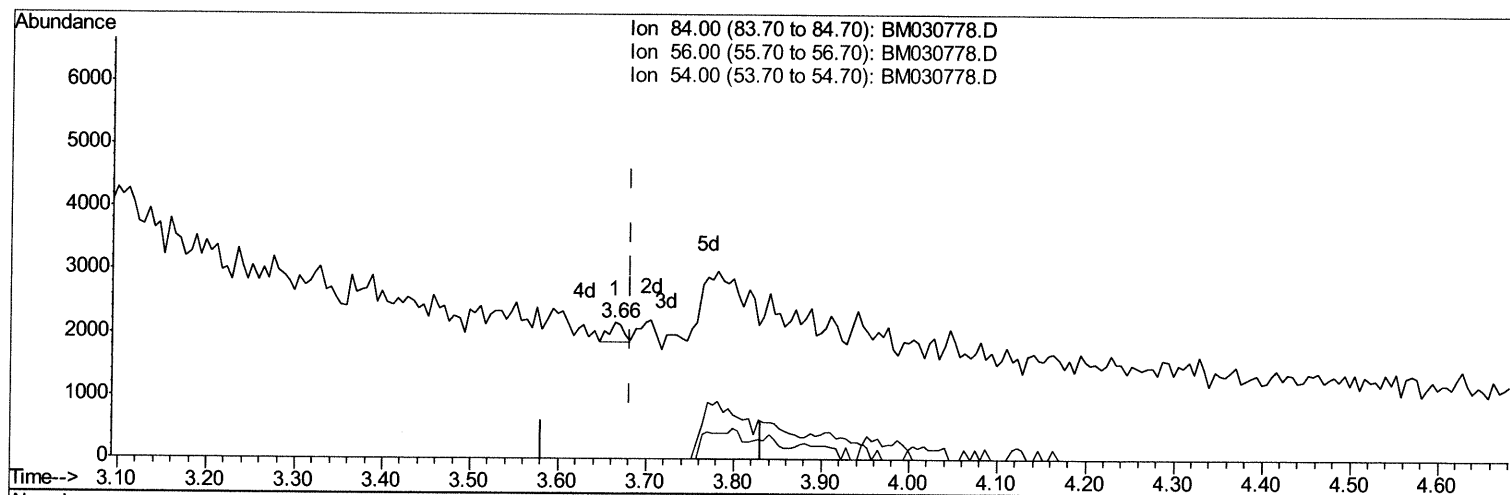

TIC: BM030778.D

(4) Pyridine-d5 (S)

3.664min (-0.017) 0.07ng/ul

response 352

Ion	Exp%	Act%
84.00	100	100
56.00	73.70	0.00#
54.00	35.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
Data File : BM030778.D
Acq On : 02 Jul 2021 16:14
Operator : CG/JU
Sample : M2825-15
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR3

Manual Integrations
APPROVED

mohammad
7/6/2021 9:24:50 AM

Quant Time: Jul 02 16:43:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

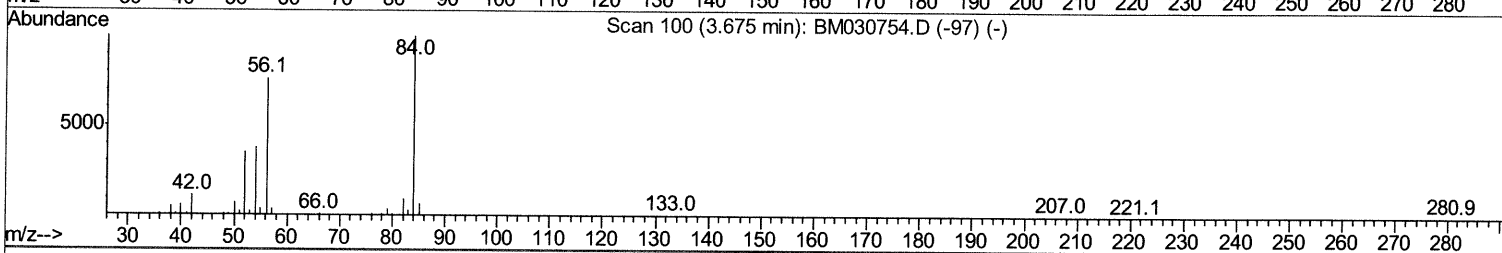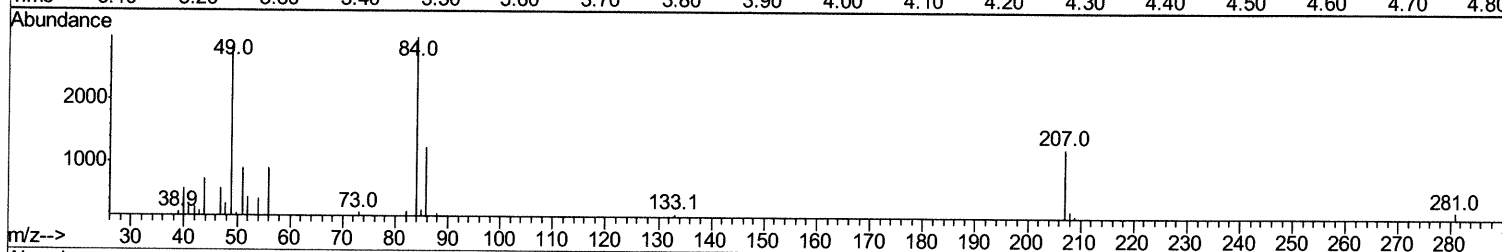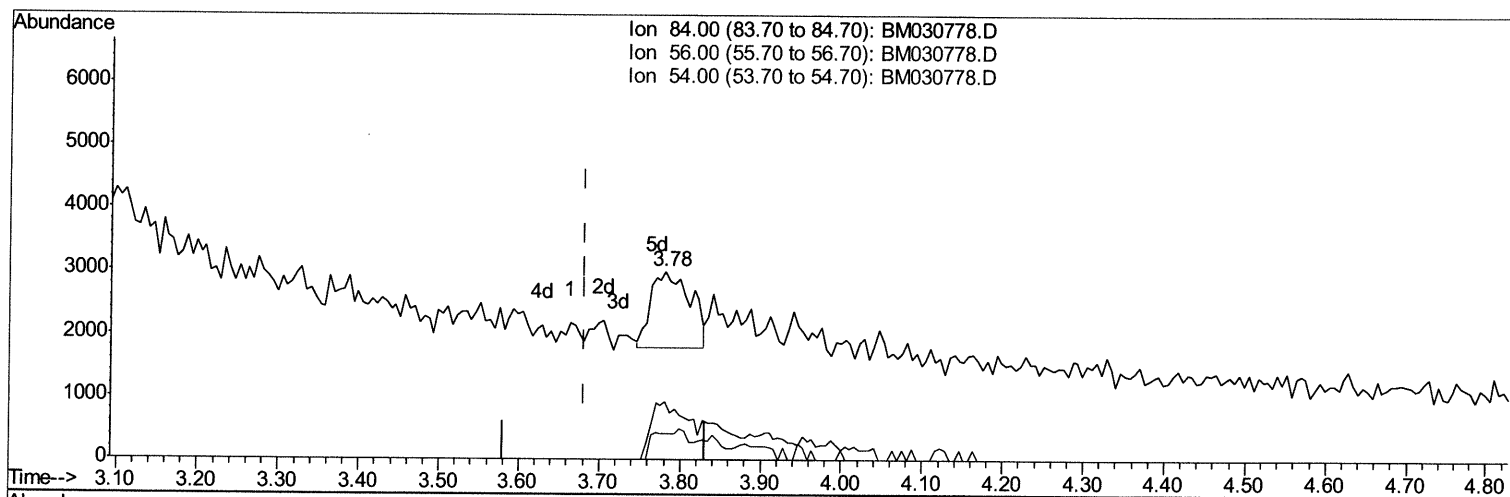

TIC: BM030778.D

(4) Pyridine-d5 (S)

3.781min (+0.100) 0.87ng/ul m

response 4161

5477/21

Ion	Exp%	Act%
84.00	100	100
56.00	73.70	30.69#
54.00	35.80	13.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM063021\
 Data File : BM030778.D
 Acq On : 02 Jul 2021 16:14
 Operator : CG/JU
 Sample : M2825-15
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR3

Manual Integrations
 APPROVED

mohammad
 7/6/2021 9:24:50 AM

Quant Time: Jul 02 16:44:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	72509	20.00	ng/ul	-0.01
20) Naphthalene-d8	10.55	136	280916	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.40	164	157489	20.00	ng/ul	-0.01
64) Phenanthrene-d10	17.14	188	302456	20.00	ng/ul	0.00
79) Chrysene-d12	21.31	240	318393	20.00	ng/ul	0.00
88) Perylene-d12	23.56	264	370784	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	1979	1.11	ng/uL	0.00
4) Pvrindine-d5	3.78	84	4161m	0.87	ng/ul	0.10
7) Phenol-d5	6.94	99	119161	19.06	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.10	67	80662	20.52	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.30	132	99045	20.52	ng/ul	0.00
15) 4-Methylphenol-d8	8.47	113	92671	19.04	ng/ul	-0.01
21) Nitrobenzene-d5	8.93	128	42221	20.14	ng/ul	0.00
24) 2-Nitrophenol-d4	9.65	143	45138	19.38	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.18	165	84574	18.95	ng/ul	0.00
31) 4-Chloroaniline-d4	10.70	131	114543	18.41	ng/ul	0.00
46) Dimethylphthalate-d6	13.82	166	234965	21.61	ng/ul	0.00
49) Acenaphthylene-d8	14.09	160	301773	21.38	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.62	143	26038	12.64	ng/ul	0.00
60) Fluorene-d10	15.39	176	209292	21.70	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.52	200	21084	10.65	ng/ul	0.00
73) Anthracene-d10	17.24	188	308652	21.87	ng/ul	0.00
81) Pyrene-d10	19.53	212	351707	21.08	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.42	264	448875	23.29	ng/ul	-0.01

ju 2/21

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed