

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030722.D
 Acq On : 01 Jul 2021 01:35
 Operator : CG/JU
 Sample : M2808-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGG09

Manual Integrations
 APPROVED

mohammad
 7/1/2021 2:55:29 PM

Quant Time: Jul 01 02:46:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 00:59:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	81422	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	333286	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	217927	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.145	188	444746	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	381377	20.000	ng/ul	0.00
88) Perylene-d12	23.562	264	356792	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	4447m	2.214	ng/uL	0.00
4) Pyridine-d5	3.716	84	20130m	3.731	ng/ul	0.04
7) Phenol-d5	6.946	99	67425	9.602	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	48142	10.907	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	58679	10.826	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	53069	9.711	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	25651	10.314	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	26665	9.648	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	50279	9.496	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	66084	8.950	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	168280	11.183	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	201069	10.294	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	10511m	3.687	ng/ul	0.02
60) Fluorene-d10	15.398	176	151466	11.349	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.527	200	10590	3.639	ng/ul	0.00
73) Anthracene-d10	17.245	188	223682	10.777	ng/ul	0.00
81) Pyrene-d10	19.527	212	231986	11.609	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.421	264	170891	9.213	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.863	163	27615	1.873	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030722.D
Acq On : 01 Jul 2021 01:35
Operator : CG/JU
Sample : M2808-03
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGG09

Manual Integrations
APPROVED

mohammad
7/1/2021 2:55:29 PM

Quant Time: Jul 01 02:46:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 00:59:58 2021
Response via : Initial Calibration

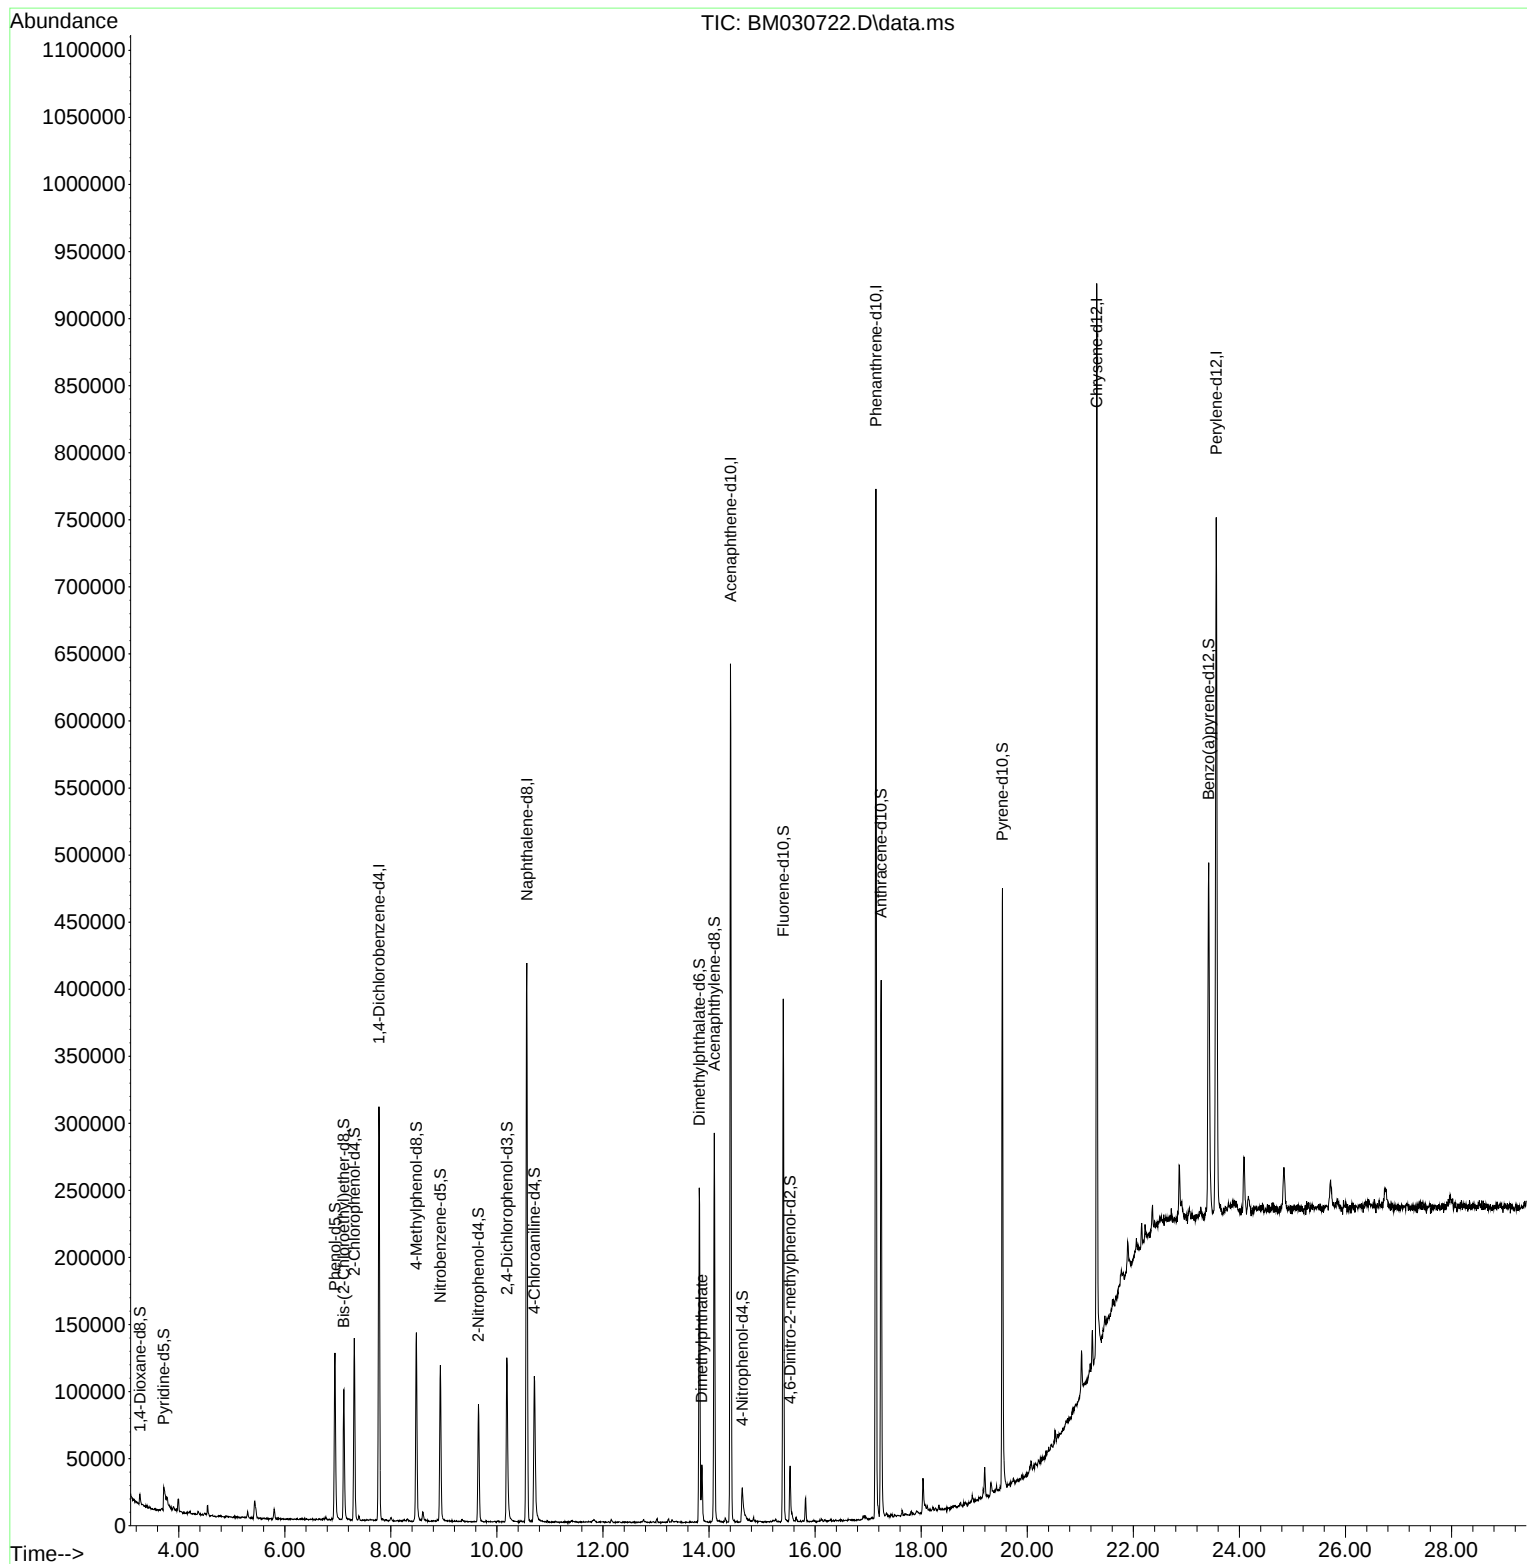

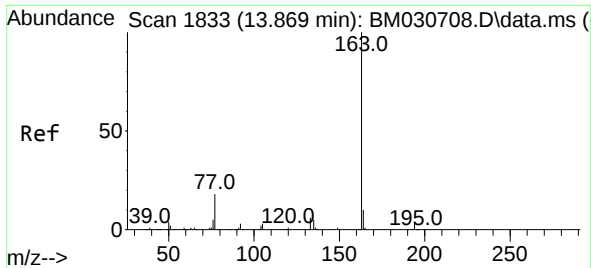

#47
 Dimethylphthalate
 Concen: 1.873 ng/ul
 RT: 13.863 min Scan# 1832
 Delta R.T. -0.006 min
 Lab File: BM030722.D
 Acq: 01 Jul 2021 01:35

Tgt Ion:	163	Resp:	27615
Ion Ratio	Lower	Upper	
163	100		
194	3.8	3.2	4.8
164	10.5	8.2	12.4

Instrument :
 BNA_M
 ClientSampleId :
 BGG09

Manual Integrations
 APPROVED

mohammad
 7/1/2021 2:55:29 PM

