

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030744.D
 Acq On : 01 Jul 2021 15:37
 Operator : CG/JU
 Sample : M2825-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR2

Quant Time: Jul 01 16:20:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	77129	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	276349	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	155064	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	308367	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	331942	20.000	ng/ul	0.00
88) Perylene-d12	23.562	264	385515	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	8405	4.418	ng/uL	0.00
4) Pyridine-d5	3.693	84	77437	15.149	ng/ul	0.01
7) Phenol-d5	6.945	99	131294	19.738	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	86187	20.614	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	110155	21.454	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	99069	19.138	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	45523	22.075	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	48539	21.180	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.186	165	90105	20.525	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	123751	20.214	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	248340	23.194	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	317098	22.816	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	27690	13.651	ng/ul	0.00
60) Fluorene-d10	15.398	176	223110	23.494	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	24780	12.283	ng/ul	0.00
73) Anthracene-d10	17.239	188	334700	23.257	ng/ul	0.00
81) Pyrene-d10	19.527	212	380679	21.887	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.415	264	468562	23.378	ng/ul	-0.01
Target Compounds						
					Qvalue	
47) Dimethylphthalate	13.863	163	121535	11.585	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030744.D
Acq On : 01 Jul 2021 15:37
Operator : CG/JU
Sample : M2825-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR2

Quant Time: Jul 01 16:20:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

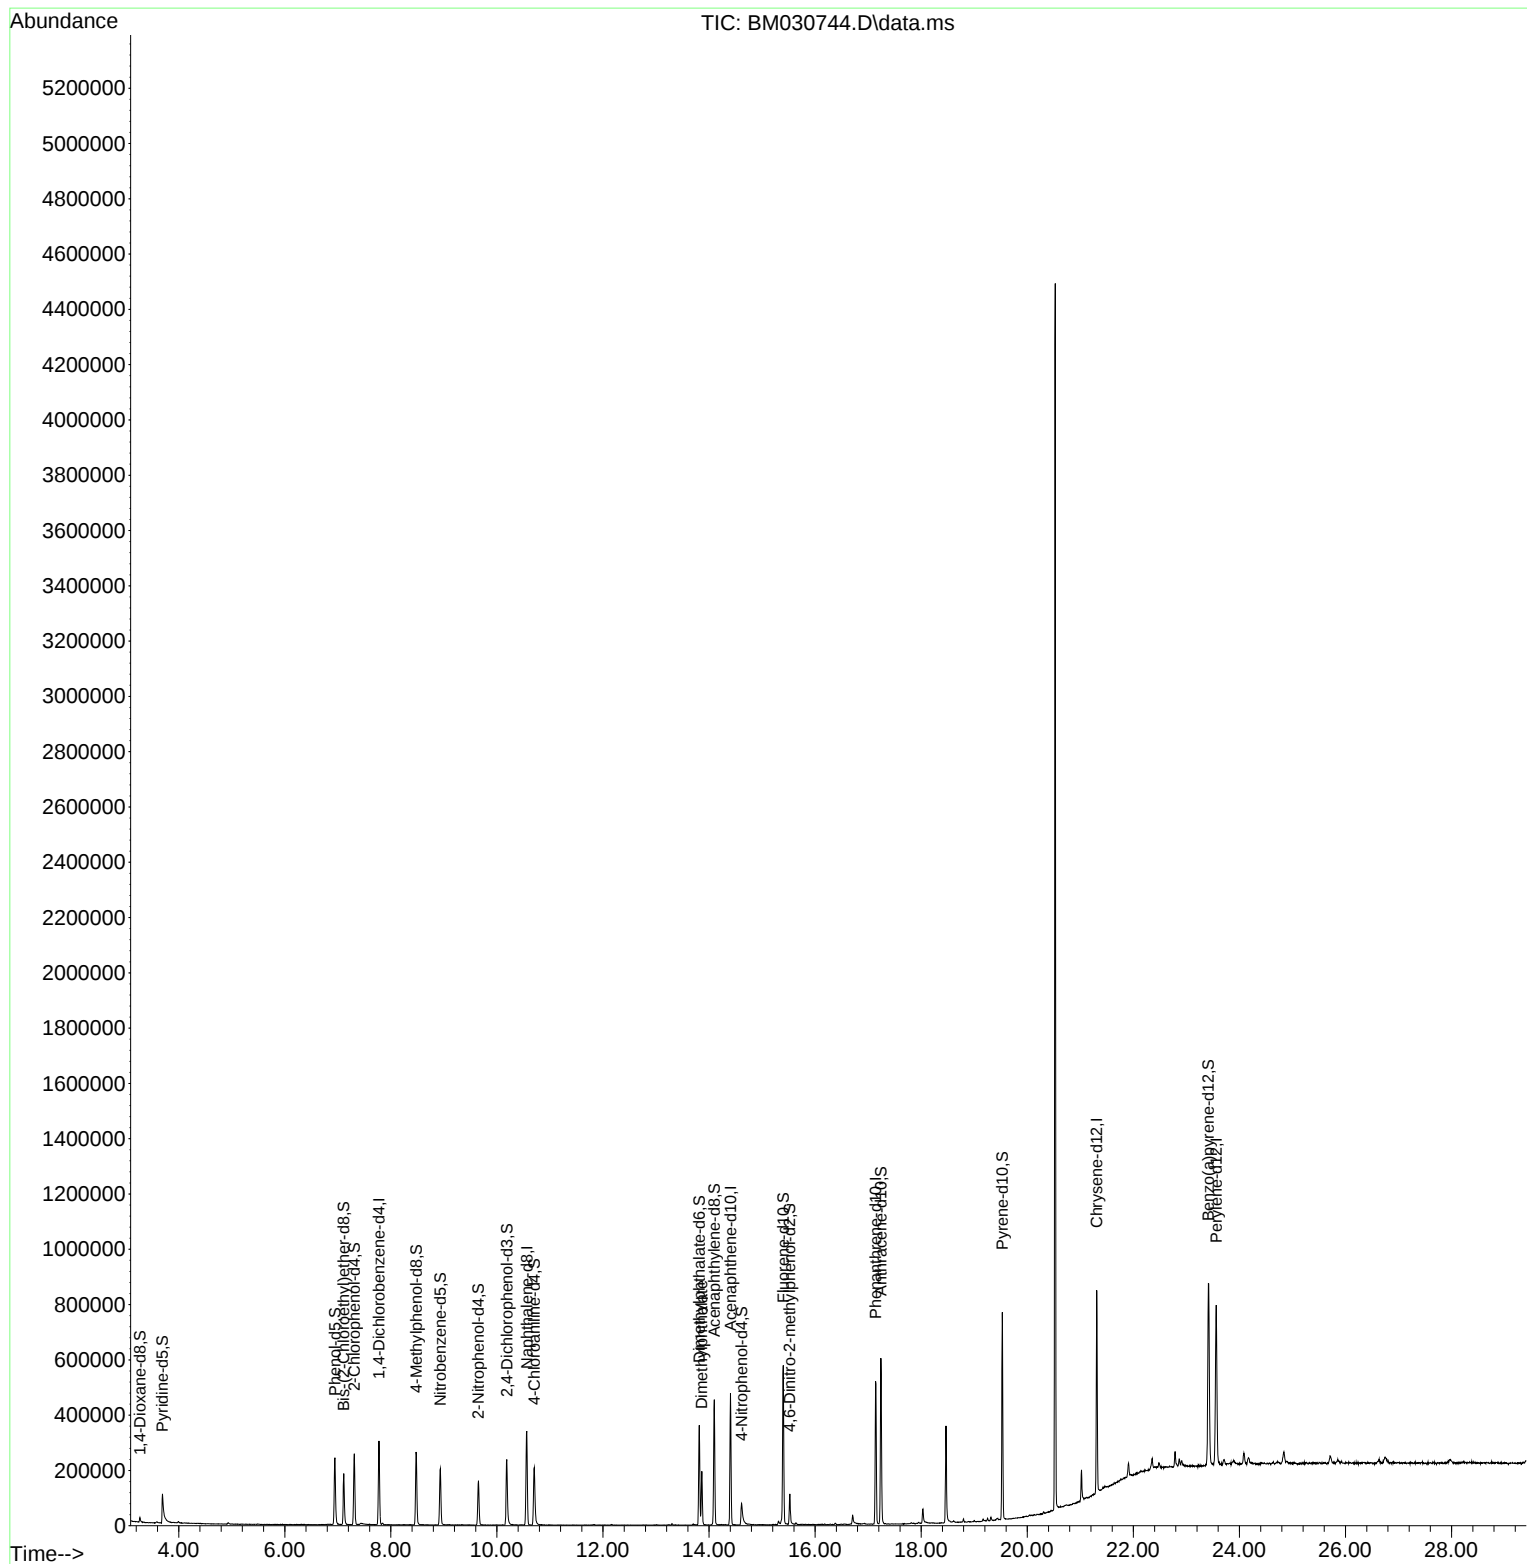

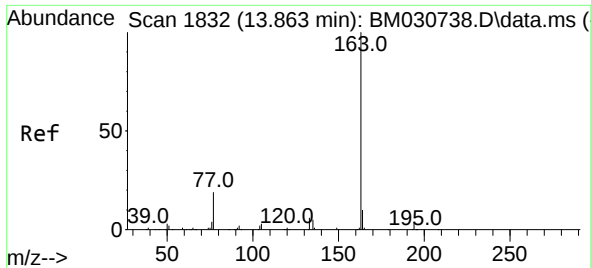

#47
 Dimethylphthalate
 Concen: 11.585 ng/ul
 RT: 13.863 min Scan# 1832
 Delta R.T. -0.006 min
 Lab File: BM030744.D
 Acq: 01 Jul 2021 15:37

Instrument :
 BNA_M
 ClientSampleId :
 BGDR2

Tgt Ion:163	Resp:	121535
Ion Ratio	Lower	Upper
163	100	
194	3.7	3.2 4.8
164	10.4	8.2 12.4

