

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030746.D
 Acq On : 01 Jul 2021 16:51
 Operator : CG/JU
 Sample : M2825-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD5

Manual Integrations
 APPROVED

mohammad
 7/2/2021 12:02:49 PM

Quant Time: Jul 01 17:22:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	76343	20.000	ng/ul	0.00
20) Naphthalene-d8	10.557	136	285665	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	157517	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.145	188	292218	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	307853	20.000	ng/ul	0.00
88) Perylene-d12	23.562	264	362978	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	4146	2.202	ng/uL	0.00
4) Pyridine-d5	3.716	84	22187m	4.385	ng/ul	0.04
7) Phenol-d5	6.945	99	64669	9.822	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	44914	10.853	ng/ul	0.00
11) 2-Chlorophenol-d4	7.310	132	54228	10.670	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	49053	9.573	ng/ul	0.00
21) Nitrobenzene-d5	8.933	128	22672	10.636	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	22999	9.709	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.186	165	42242	9.308	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	56275	8.892	ng/ul	0.00
46) Dimethylphthalate-d6	13.815	166	126326	11.615	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	152701	10.816	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	10380	5.038	ng/ul	0.02
60) Fluorene-d10	15.398	176	113279	11.743	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.527	200	8585	4.490	ng/ul	0.00
73) Anthracene-d10	17.239	188	161890	11.871	ng/ul	0.00
81) Pyrene-d10	19.527	212	181890	11.276	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.415	264	205528	10.891	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	13.863	163	61342	5.756	ng/ul#	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030746.D
Acq On : 01 Jul 2021 16:51
Operator : CG/JU
Sample : M2825-11
Misc :
ALS Vial : 49 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGDP5

Manual Integrations
APPROVED

mohammad
7/2/2021 12:02:49 PM

Quant Time: Jul 01 17:22:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

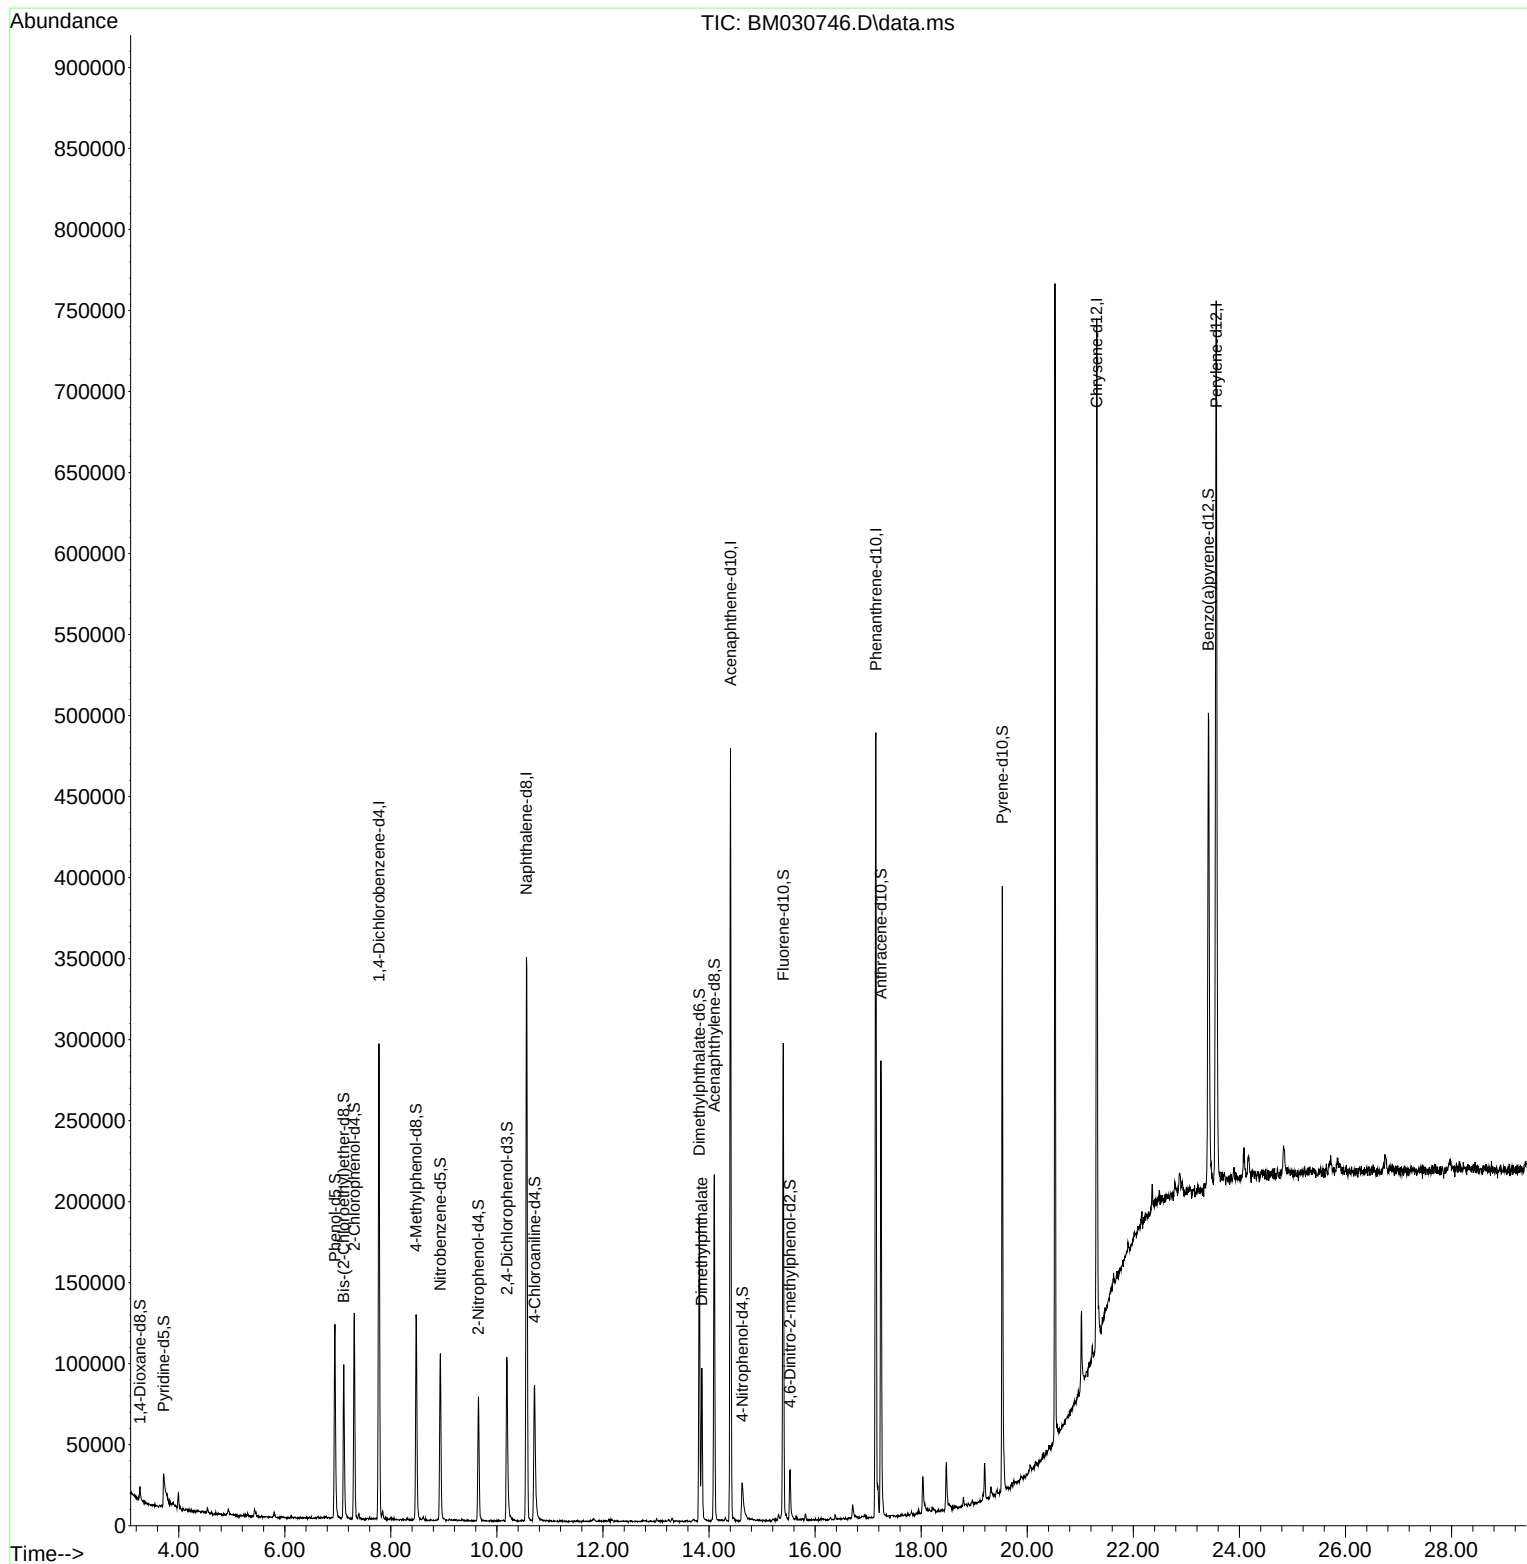

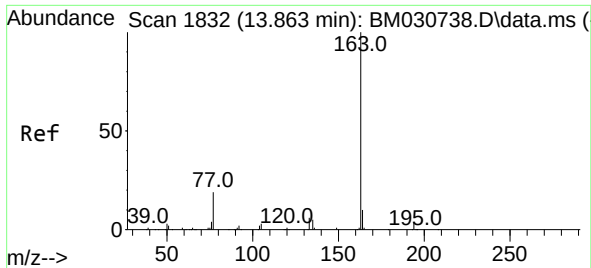

#47
 Dimethylphthalate
 Concen: 5.756 ng/ul
 RT: 13.863 min Scan# 1832
 Delta R.T. -0.006 min
 Lab File: BM030746.D
 Acq: 01 Jul 2021 16:51

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.2	3.2	4.8#
164	9.8	8.2	12.4

Instrument :
 BNA_M
 ClientSampleId :
 BGD5

Manual Integrations
 APPROVED

mohammad
 7/2/2021 12:02:49 PM

