

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030752.D
 Acq On : 01 Jul 2021 20:31
 Operator : CG/JU
 Sample : M2825-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ5

Quant Time: Jul 02 02:35:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	76637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.557	136	296840	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	166807	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	308763	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	307807	20.000	ng/ul	0.00
88) Perylene-d12	23.556	264	360455	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	10434	5.520	ng/uL	0.00
4) Pyridine-d5	3.681	84	102171	20.117	ng/ul	0.00
7) Phenol-d5	6.940	99	183688	27.791	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	122630	29.518	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	152004	29.794	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	146821	28.544	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	66781	30.149	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	71586	29.081	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	137042	29.061	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	177716	27.025	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	386076	33.520	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	494381	33.068	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.610	143	45380	20.797	ng/ul	0.00
60) Fluorene-d10	15.392	176	339772	33.261	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	40760	20.177	ng/ul	0.00
73) Anthracene-d10	17.239	188	492764	34.196	ng/ul	0.00
81) Pyrene-d10	19.527	212	531235	32.937	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.415	264	665487	35.511	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	13.863	163	172369	15.274	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030752.D
Acq On : 01 Jul 2021 20:31
Operator : CG/JU
Sample : M2825-02
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ5

Quant Time: Jul 02 02:35:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration

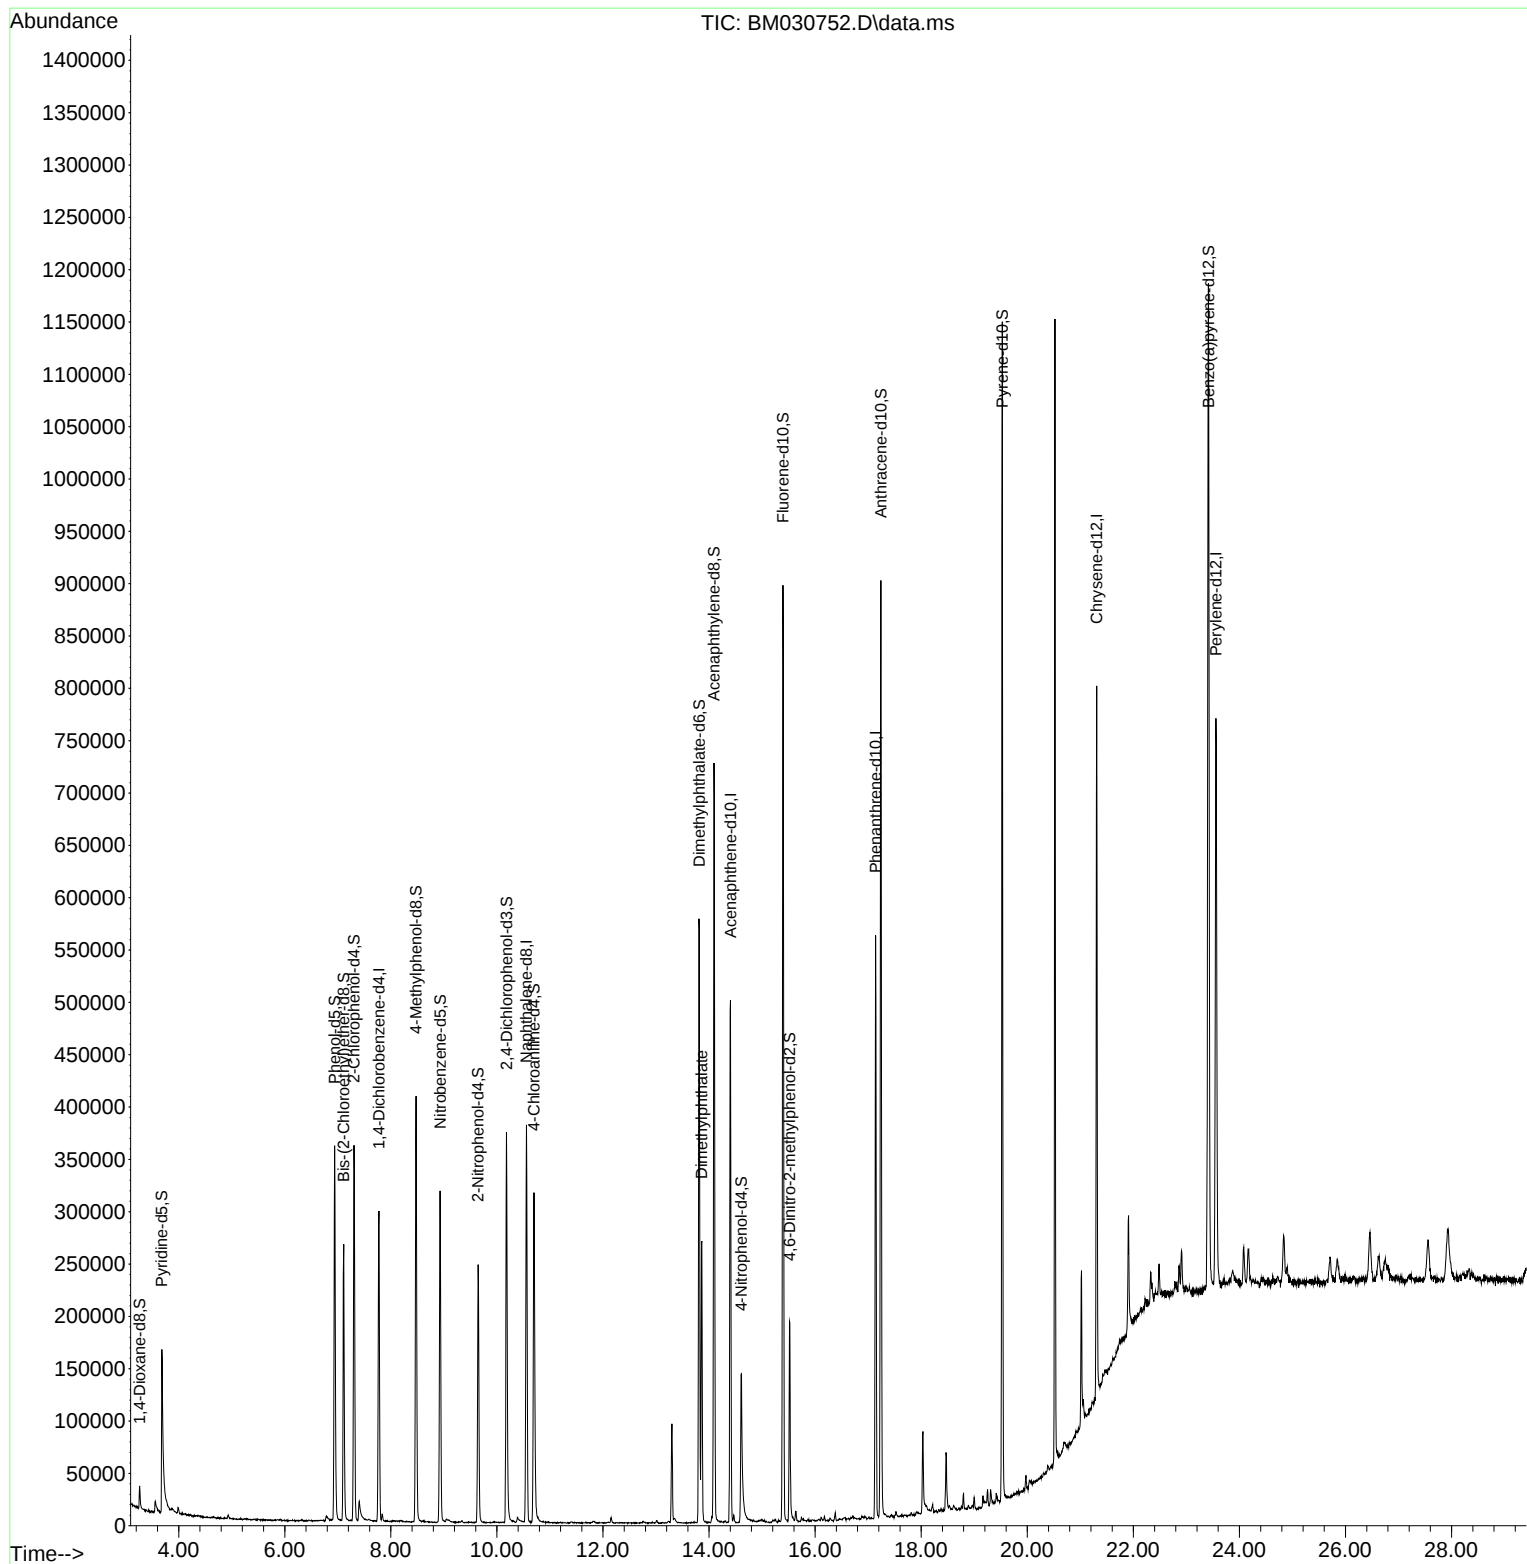

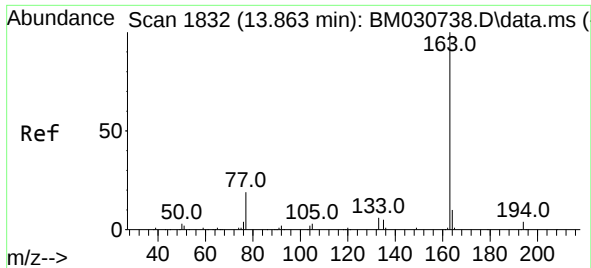

#47
 Dimethylphthalate
 Concen: 15.274 ng/ul
 RT: 13.863 min Scan# 1832
 Delta R.T. -0.006 min
 Lab File: BM030752.D
 Acq: 01 Jul 2021 20:31

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ5

Tgt Ion:163 Resp: 172369
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.2 4.8
 164 9.8 8.2 12.4

