

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030763.D
 Acq On : 02 Jul 2021 03:50
 Operator : CG/JU
 Sample : M2825-03
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ6

Quant Time: Jul 02 04:40:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 04:13:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	79047	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.557	136	301678	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	170632	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	324214	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	331108	20.000	ng/ul	0.00
88) Perylene-d12	23.556	264	382891	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	8442	4.330	ng/uL	0.00
4) Pyridine-d5	3.687	84	88380	16.871	ng/ul	0.00
7) Phenol-d5	6.940	99	143754	21.086	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	95009	22.172	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	116825	22.201	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	113049	21.308	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	50482	22.425	ng/ul	0.00
24) 2-Nitrophenol-d4	9.645	143	53432	21.358	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	103169	21.527	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	138597	20.738	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	291897	24.775	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	371298	24.279	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.610	143	32982	14.777	ng/ul	0.00
60) Fluorene-d10	15.392	176	257450	24.637	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	26556	12.520	ng/ul	0.00
73) Anthracene-d10	17.239	188	369558	24.424	ng/ul	0.00
81) Pyrene-d10	19.527	212	412180	23.757	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.415	264	503734	25.305	ng/ul	-0.01
Target Compounds						
					Qvalue	
47) Dimethylphthalate	13.863	163	138016	11.956	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030763.D
Acq On : 02 Jul 2021 03:50
Operator : CG/JU
Sample : M2825-03
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ6

Quant Time: Jul 02 04:40:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 04:13:39 2021
Response via : Initial Calibration

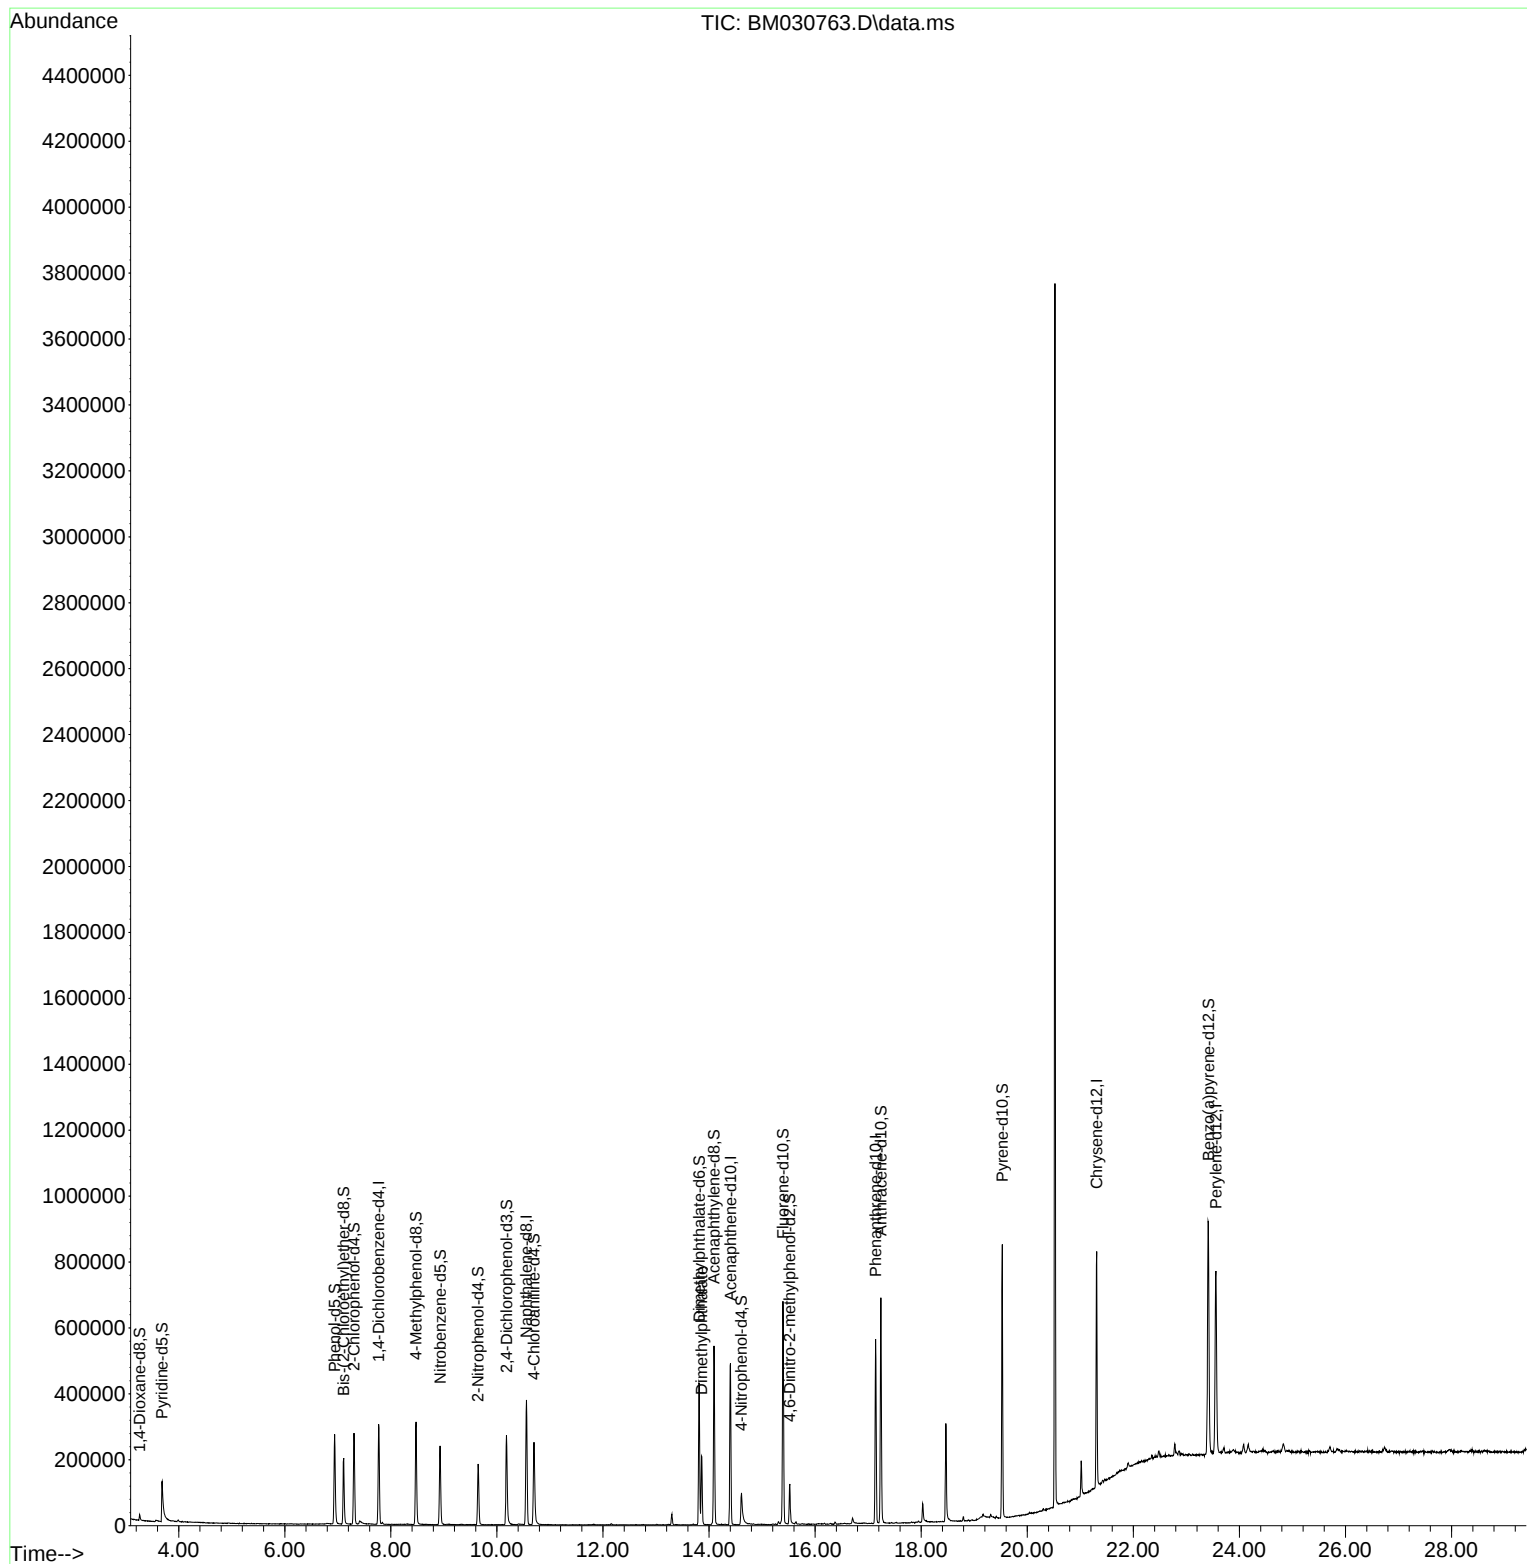

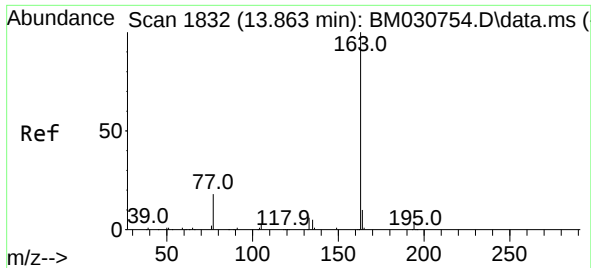

#47
 Dimethylphthalate
 Concen: 11.956 ng/ul
 RT: 13.863 min Scan# 1832
 Delta R.T. -0.006 min
 Lab File: BM030763.D
 Acq: 02 Jul 2021 03:50

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ6

Tgt Ion:163 Resp: 138016
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.2 4.8
 164 10.4 8.2 12.4

