

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030765.D
 Acq On : 02 Jul 2021 05:03
 Operator : CG/JU
 Sample : M2825-04
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ7

Manual Integrations
 APPROVED

mohammad
 7/2/2021 12:04:13 PM

Quant Time: Jul 02 05:41:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 04:13:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	88608	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.557	136	343942	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	195156	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.139	188	354109	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	346332	20.000	ng/ul	0.00
88) Perylene-d12	23.557	264	410599	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	7066	3.233	ng/uL	0.00
4) Pyridine-d5	3.711	84	26375m	4.491	ng/ul	0.03
7) Phenol-d5	6.940	99	117619	15.391	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	79596	16.571	ng/ul	0.00
11) 2-Chlorophenol-d4	7.305	132	99853	16.928	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	91572	15.398	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	42033	16.377	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	44430	15.577	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	85771	15.698	ng/ul	0.00
31) 4-Chloroaniline-d4	10.699	131	109939	14.429	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	234150	17.376	ng/ul	-0.01
49) Acenaphthylene-d8	14.092	160	299009	17.095	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.616	143	20966	8.213	ng/ul	0.00
60) Fluorene-d10	15.392	176	205865	17.225	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	17848	7.704	ng/ul	0.00
73) Anthracene-d10	17.239	188	292924	17.725	ng/ul	0.00
81) Pyrene-d10	19.527	212	317540	17.498	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	384642	18.018	ng/ul	-0.02
Target Compounds						
47) Dimethylphthalate	13.863	163	107902	8.173	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030765.D
Acq On : 02 Jul 2021 05:03
Operator : CG/JU
Sample : M2825-04
Misc :
ALS Vial : 68 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGDQ7

Manual Integrations
APPROVED


mohammad
7/2/2021 12:04:13 PM

Quant Time: Jul 02 05:41:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 04:13:39 2021
Response via : Initial Calibration


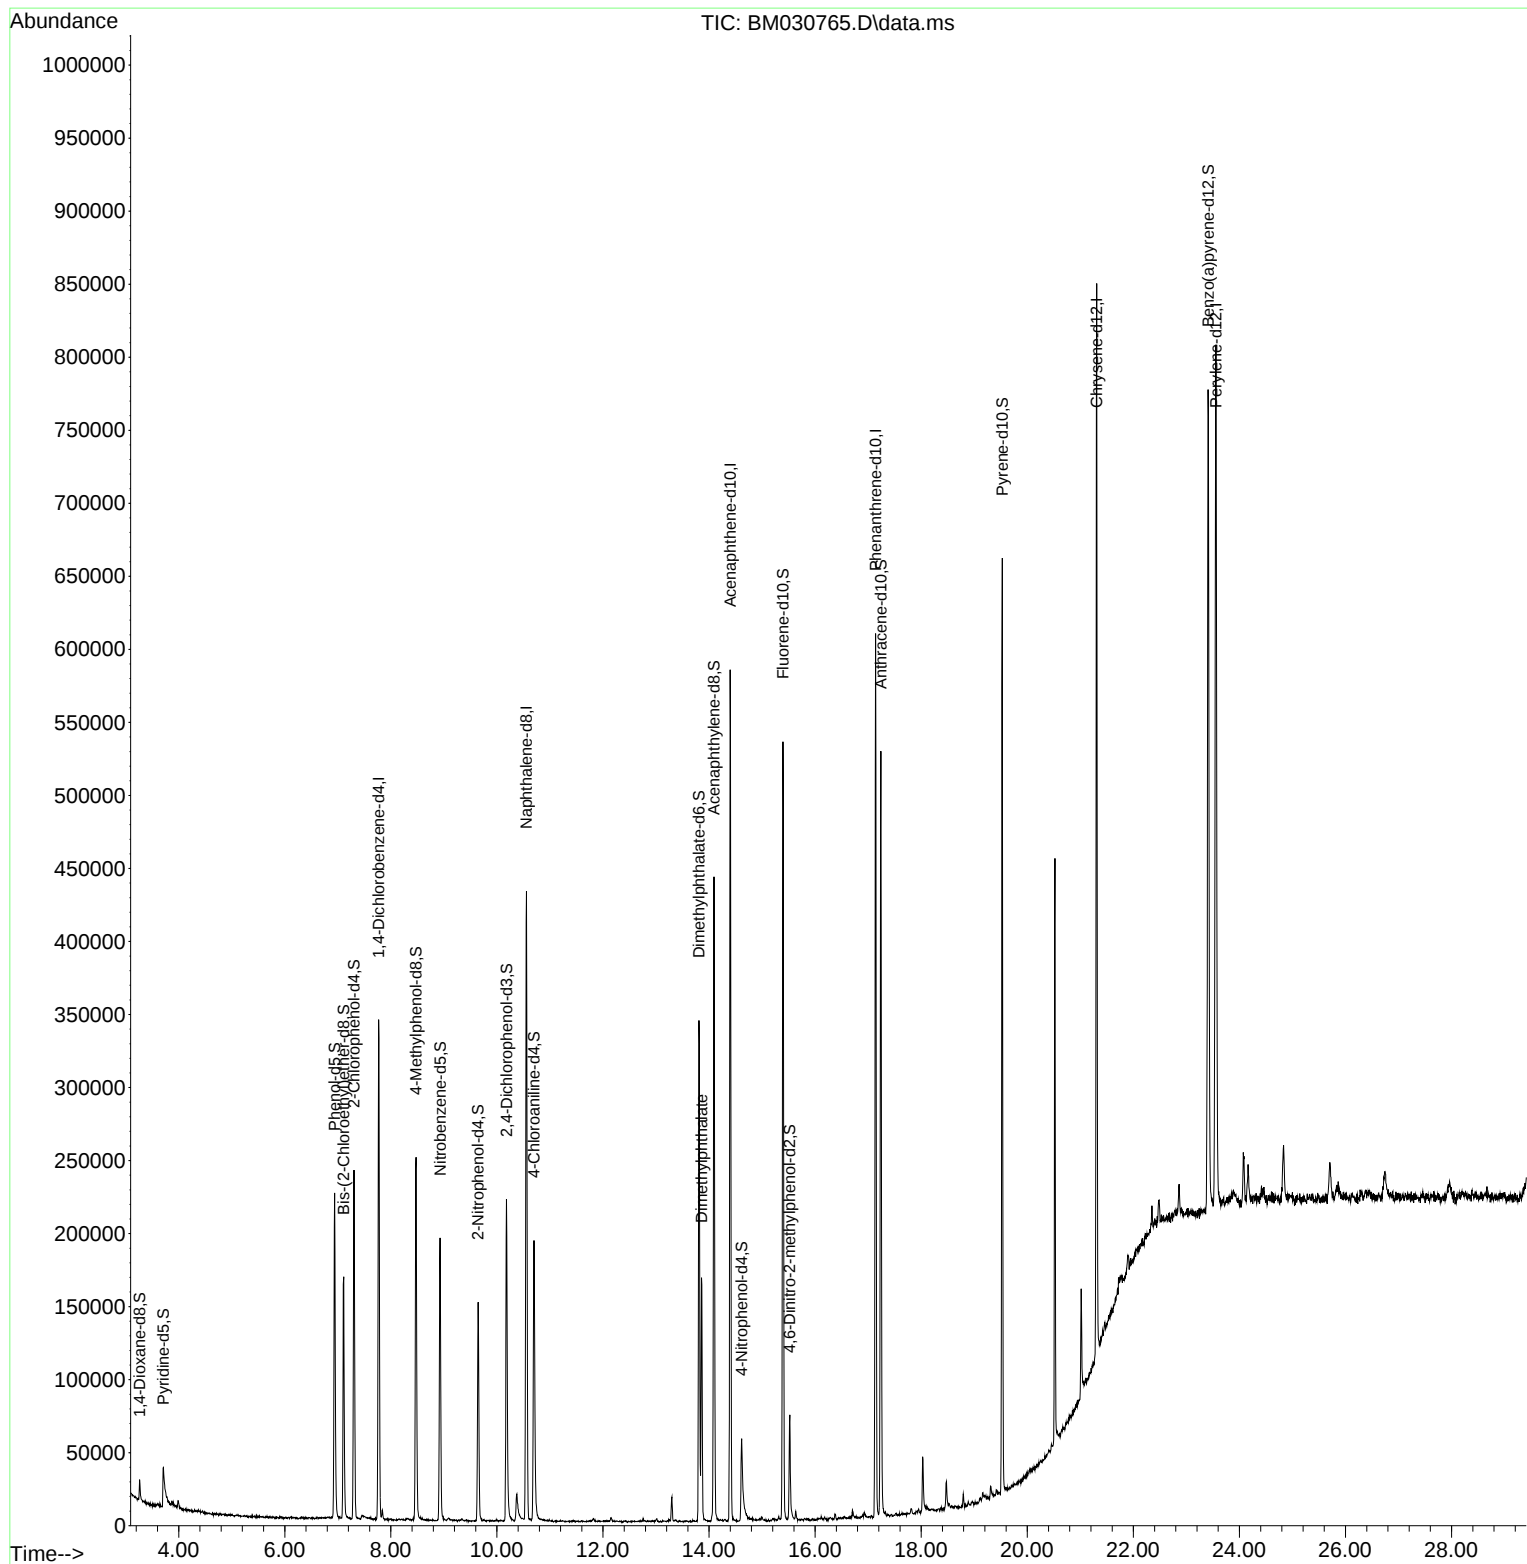


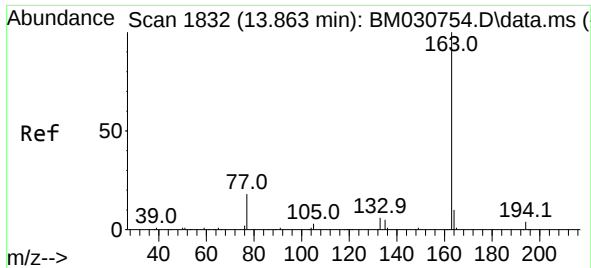

#47
Dimethylphthalate
Concen: 8.173 ng/ul
RT: 13.863 min Scan# 1832
Delta R.T. -0.006 min
Lab File: BM030765.D
Acq: 02 Jul 2021 05:03

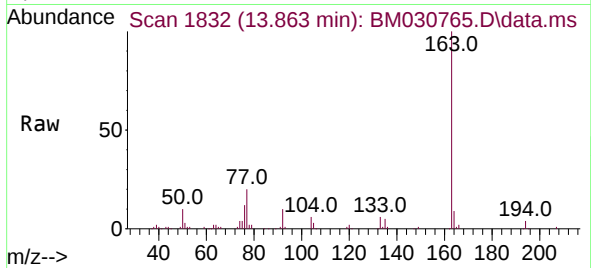

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	9.5	8.2	12.4

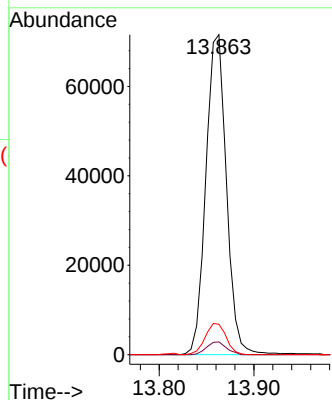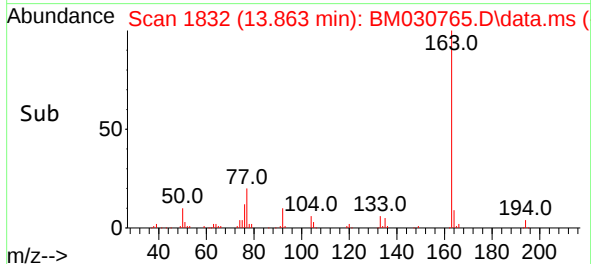

Instrument :
BNA_M
ClientSampleId :
BGDQ7

Manual Integrations
APPROVED

mohammad
7/2/2021 12:04:13 PM