

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030774.D
 Acq On : 02 Jul 2021 12:59
 Operator : CG/JU
 Sample : M2853-03DL 10X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AW1DL

Quant Time: Jul 02 13:30:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	108145	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.557	136	424874	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	252787	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.139	188	463674	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	423417	20.000	ng/ul	0.00
88) Perylene-d12	23.562	264	476795	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.940	99	3898	0.418	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	15326	2.614	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	13861	1.925	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	7553	1.041	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	7874	2.484	ng/ul	0.00
24) 2-Nitrophenol-d4	9.645	143	7464	2.118	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.192	165	14354	2.127	ng/ul	0.00
31) 4-Chloroaniline-d4	10.704	131	11829	1.257	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	57152	3.274	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	63354	2.796	ng/ul	-0.01
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.392	176	48374	3.125	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.527	200	11435	3.769	ng/ul	0.00
73) Anthracene-d10	17.239	188	75799	3.503	ng/ul	0.00
81) Pyrene-d10	19.527	212	77673	3.501	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.421	264	85098	3.433	ng/ul	0.00
Target Compounds						
					Qvalue	
42) 2,4,5-Trichlorophenol	12.916	196	5937	1.120	ng/ul	86
71) Pentachlorophenol	16.792	266	127176	37.086	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030774.D
Acq On : 02 Jul 2021 12:59
Operator : CG/JU
Sample : M2853-03DL 10X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AW1DL

Quant Time: Jul 02 13:30:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration




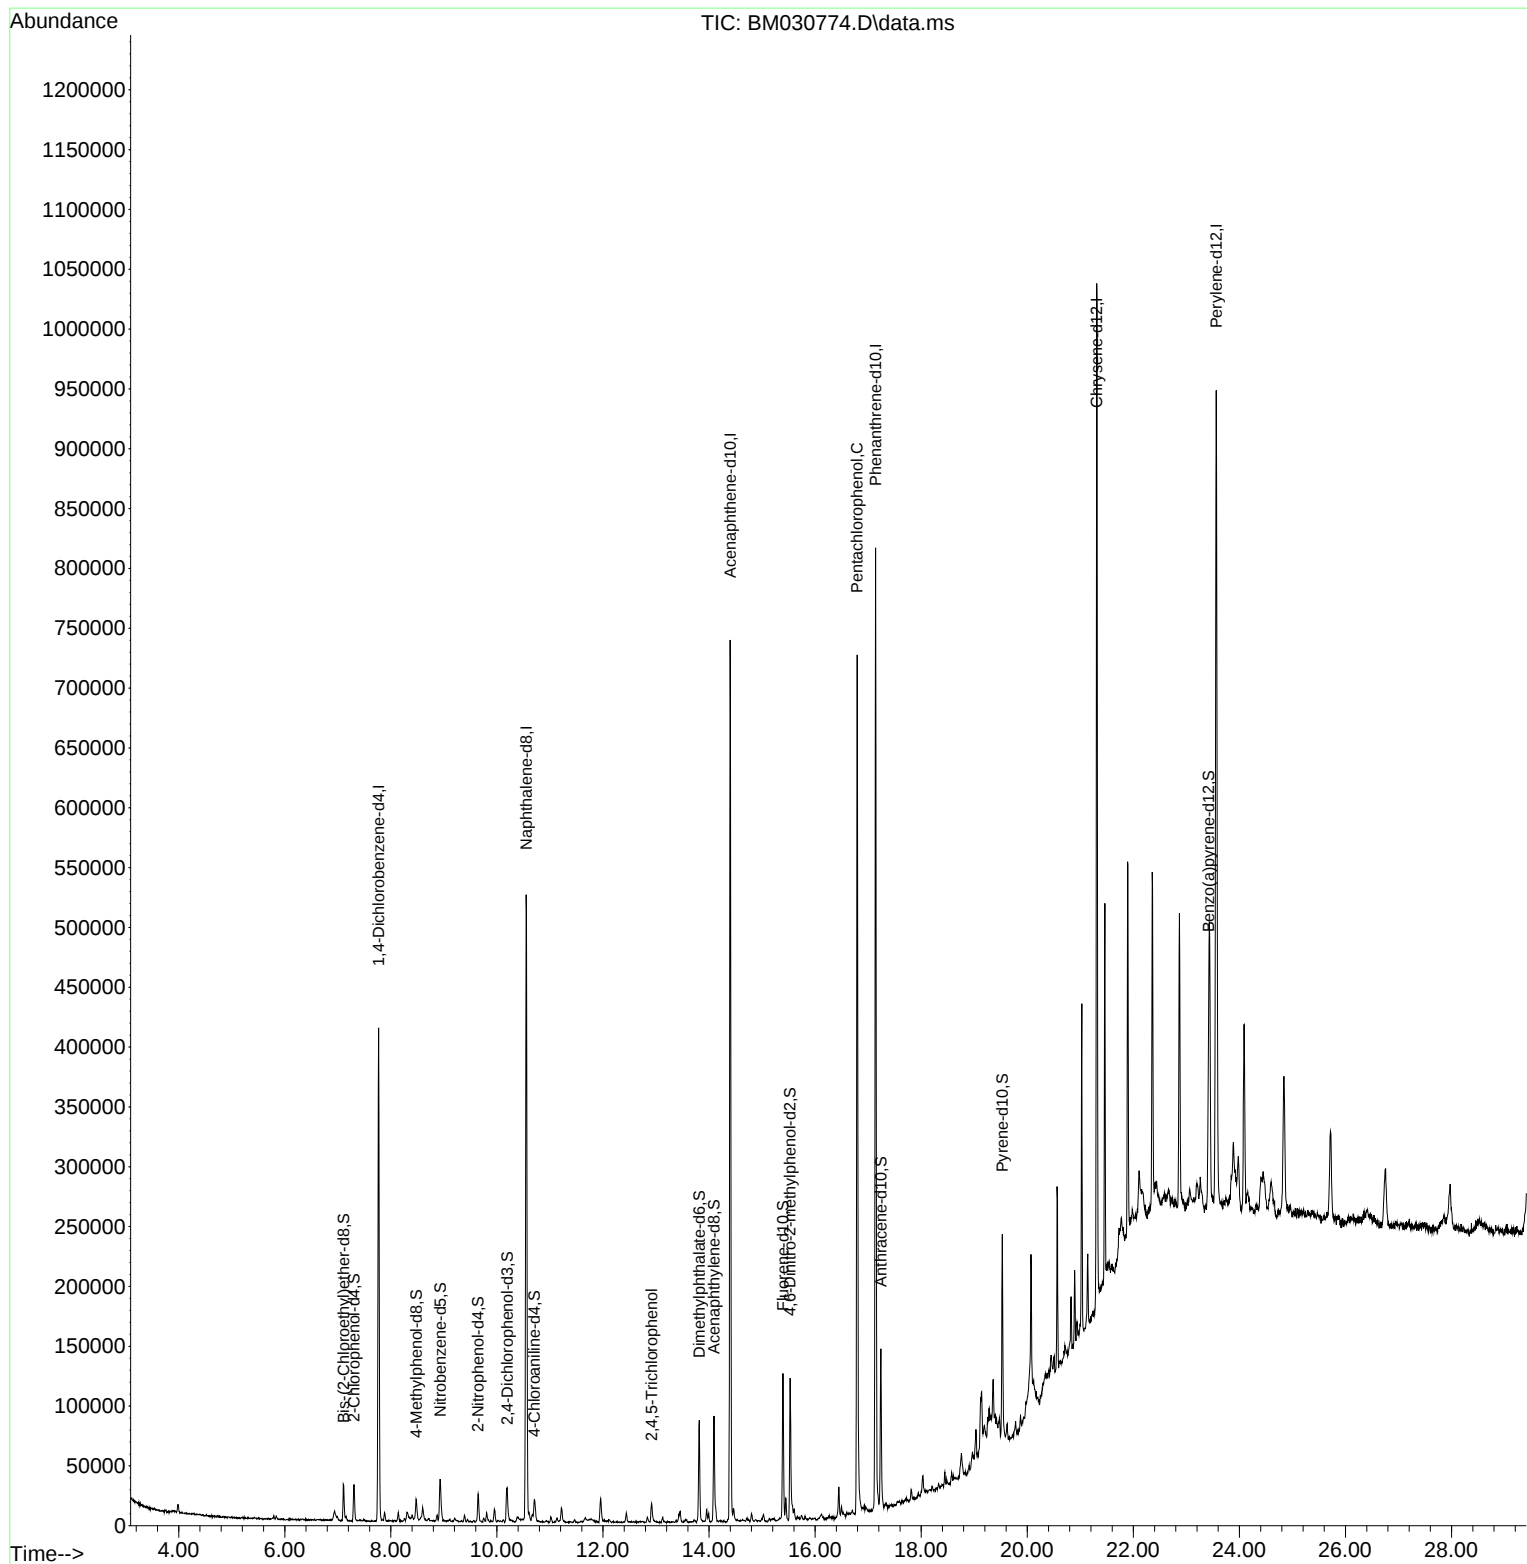


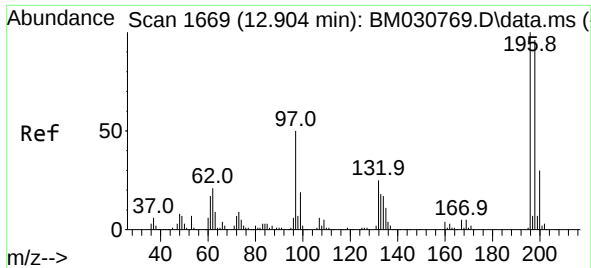

#42
2,4,5-Trichlorophenol
Concen: 1.120 ng/ul
RT: 12.916 min Scan# 1671
Delta R.T. 0.006 min
Lab File: BM030774.D
Acq: 02 Jul 2021 12:59

Instrument :
BNA_M
ClientSampled :
C0AW1DL

Tgt Ion:196 Resp: 5937
Ion Ratio Lower Upper
196 100
198 111.1 76.1 114.1
200 35.9 25.4 38.2

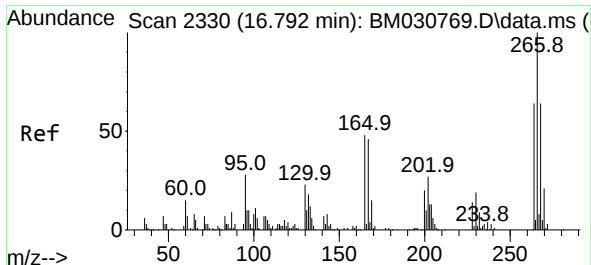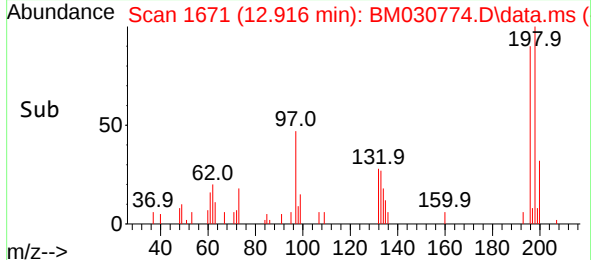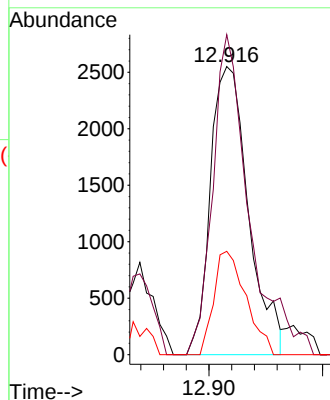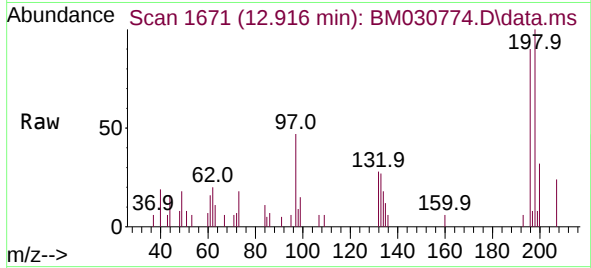

#71
Pentachlorophenol
Concen: 37.086 ng/ul
RT: 16.792 min Scan# 2330
Delta R.T. -0.012 min
Lab File: BM030774.D
Acq: 02 Jul 2021 12:59

Tgt Ion:266 Resp: 127176
Ion Ratio Lower Upper
266 100
264 62.4 48.2 72.4
268 63.7 51.6 77.4

