

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030776.D
 Acq On : 02 Jul 2021 15:01
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Manual Integrations
 APPROVED

mohammad
 7/6/2021 9:24:45 AM

Quant Time: Jul 02 15:33:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 01 05:56:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	80096	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.551	136	312792	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.398	164	178051	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.139	188	348493	20.000	ng/ul	0.00
79) Chrysene-d12	21.309	240	372451	20.000	ng/ul	0.00
88) Perylene-d12	23.562	264	421798	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	2326	1.177	ng/uL	0.00
4) Pyridine-d5	3.769	84	4361m	0.822	ng/ul	0.09
7) Phenol-d5	6.934	99	153185	22.176	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.104	67	104735	24.122	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.298	132	128808	24.157	ng/ul	-0.01
15) 4-Methylphenol-d8	8.469	113	115441	21.474	ng/ul	-0.01
21) Nitrobenzene-d5	8.922	128	56216	24.085	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.645	143	60183	23.202	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	110806	22.299	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.698	131	145871	21.051	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	304947	24.804	ng/ul	-0.01
49) Acenaphthylene-d8	14.092	160	398377	24.964	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.610	143	33584	14.419	ng/ul	0.00
60) Fluorene-d10	15.392	176	276114	25.322	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	27963	12.264	ng/ul	0.00
73) Anthracene-d10	17.239	188	405090	24.907	ng/ul	0.00
81) Pyrene-d10	19.527	212	458653	23.501	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.415	264	572712	26.116	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	13.857	163	33057	2.744	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030776.D
Acq On : 02 Jul 2021 15:01
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 79 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGDQ9

Manual Integrations
APPROVED


mohammad
7/6/2021 9:24:45 AM

Quant Time: Jul 02 15:33:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 01 05:56:56 2021
Response via : Initial Calibration


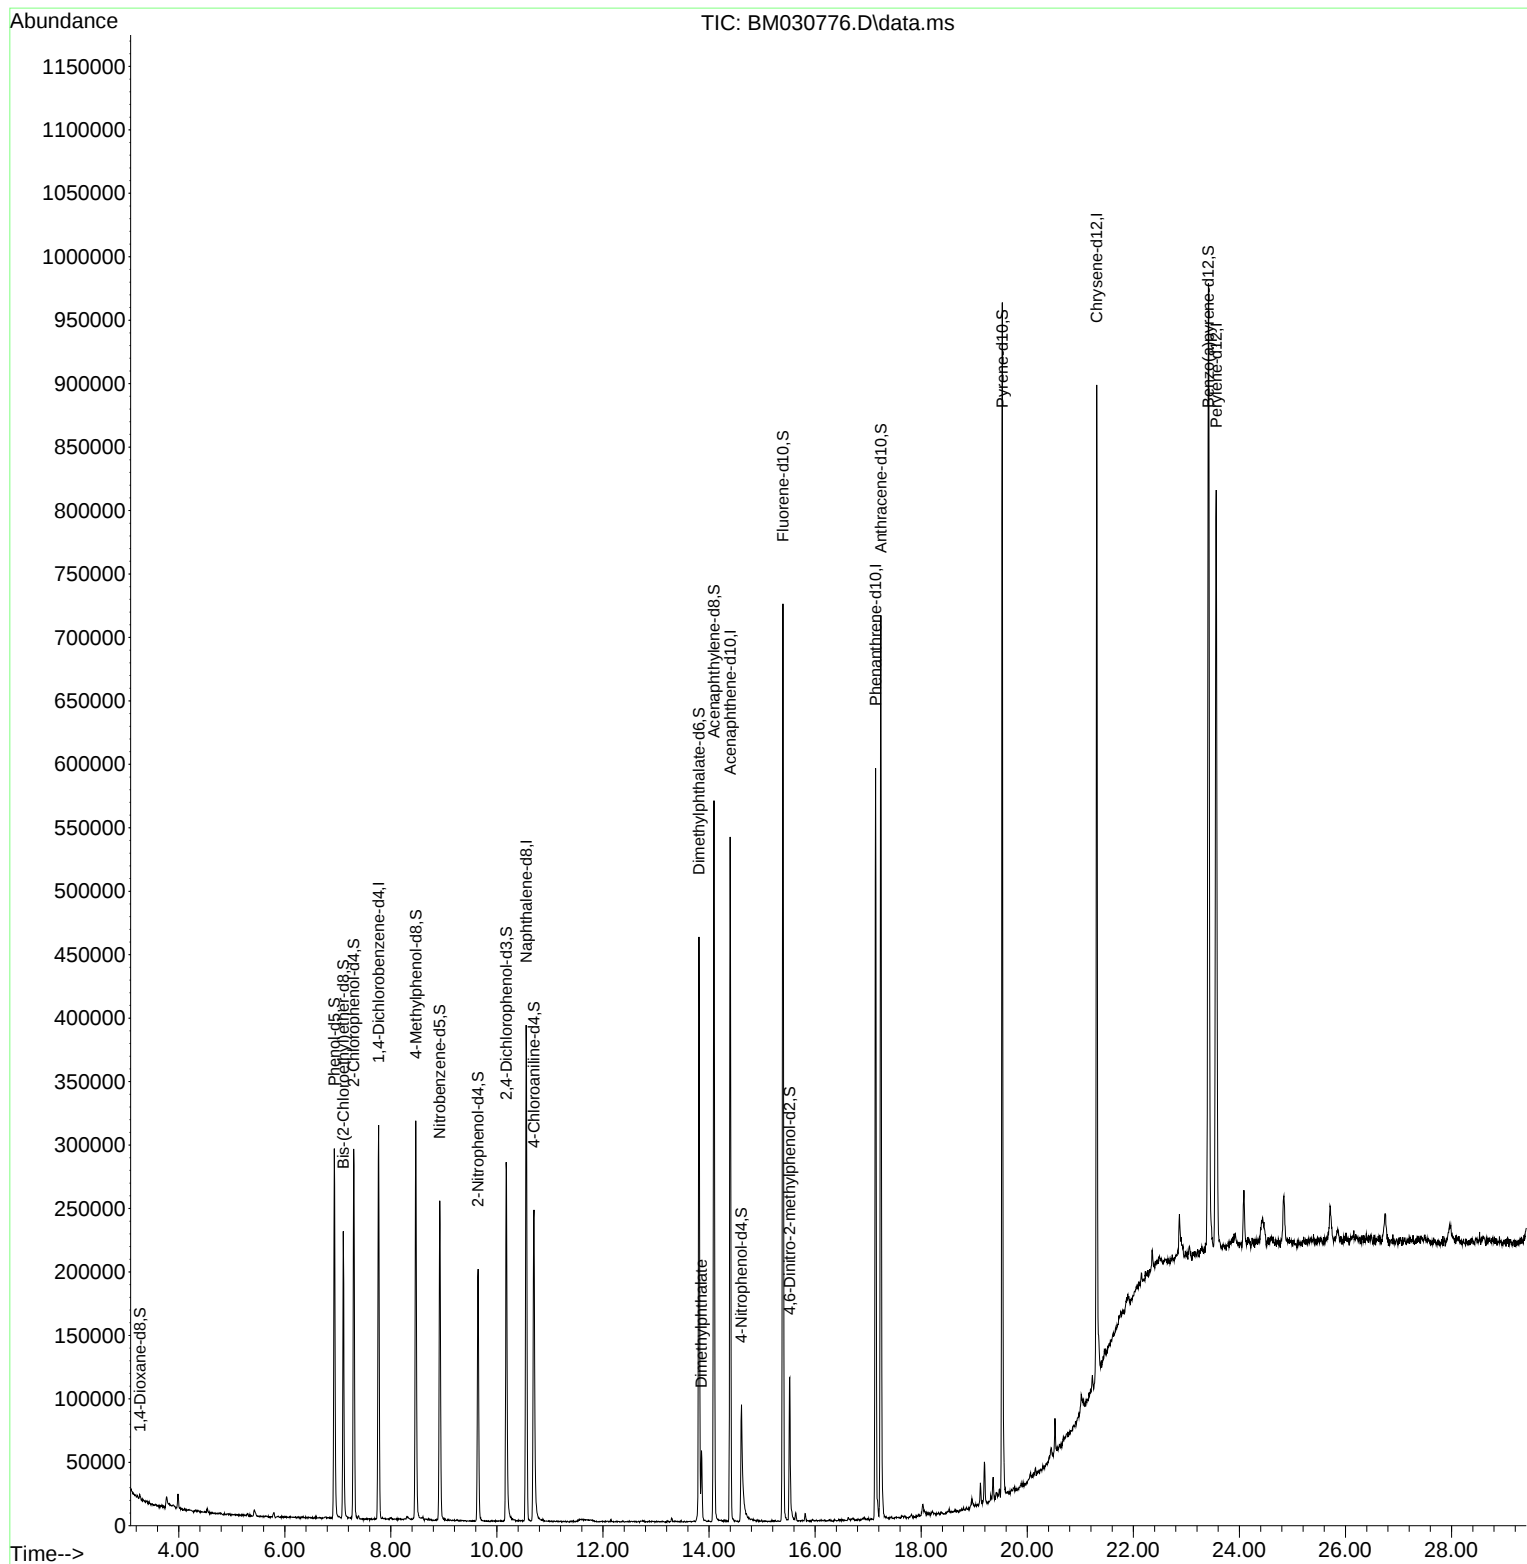


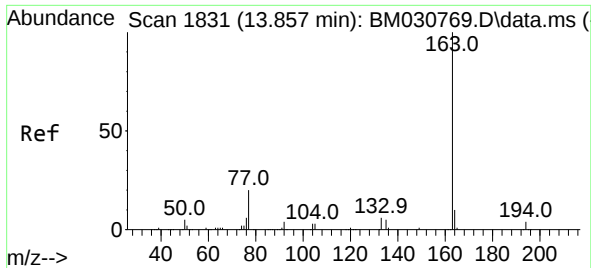

#47
 Dimethylphthalate
 Concen: 2.744 ng/ul
 RT: 13.857 min Scan# 1831
 Delta R.T. -0.012 min
 Lab File: BM030776.D
 Acq: 02 Jul 2021 15:01

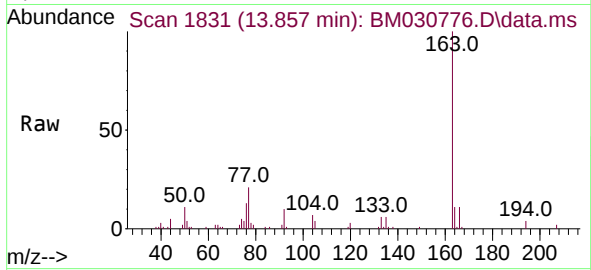

Tgt Ion:	163	Resp:	33057
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.2	4.8
164	10.7	8.2	12.4

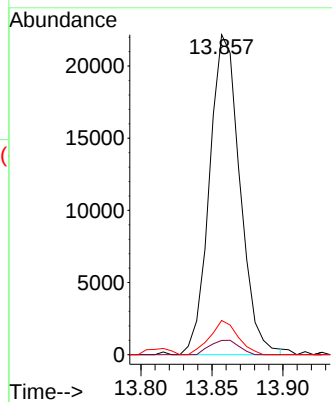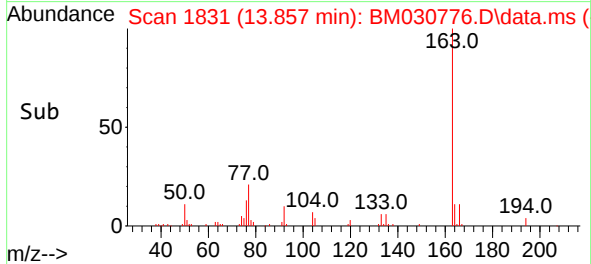

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Manual Integrations
 APPROVED

mohammad
 7/6/2021 9:24:45 AM