

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030789.D
 Acq On : 03 Jul 2021 00:10
 Operator : CG/JU
 Sample : M2869-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY5

Manual Integrations
 APPROVED

mohammad
 7/6/2021 9:25:14 AM

Quant Time: Jul 03 00:46:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 23:05:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	82971	20.00	ng/ul	0.00
20) Naphthalene-d8	10.551	136	345006	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	220146	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	435095	20.00	ng/ul	0.00
79) Chrysene-d12	21.303	240	358988	20.00	ng/ul	0.00
88) Perylene-d12	23.550	264	380869	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	8123	3.97	ng/uL	0.00
4) Pyridine-d5	3.681	84	85967	15.63	ng/ul	0.00
7) Phenol-d5	6.934	99	154494	21.59	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.104	67	103377	22.98	ng/ul	0.00
11) 2-Chlorophenol-d4	7.298	132	130185	23.57	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	127422	22.88	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	58044	22.55	ng/ul	0.00
24) 2-Nitrophenol-d4	9.645	143	63516	22.20	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	126184	23.02	ng/ul	0.00
31) 4-Chloroaniline-d4	10.692	131	150597	19.70	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	370533	24.38	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	476391	24.14	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	34145m	11.86	ng/ul	0.01
60) Fluorene-d10	15.392	176	333300	24.72	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	32960	11.58	ng/ul	0.00
73) Anthracene-d10	17.233	188	488641	24.06	ng/ul	0.00
81) Pyrene-d10	19.527	212	496537	26.40	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	485330	24.51	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.857	163	128696	8.64	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030789.D
Acq On : 03 Jul 2021 00:10
Operator : CG/JU
Sample : M2869-15
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGDY5

Manual Integrations
APPROVED


mohammad
7/6/2021 9:25:14 AM

Quant Time: Jul 03 00:46:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 23:05:33 2021
Response via : Initial Calibration


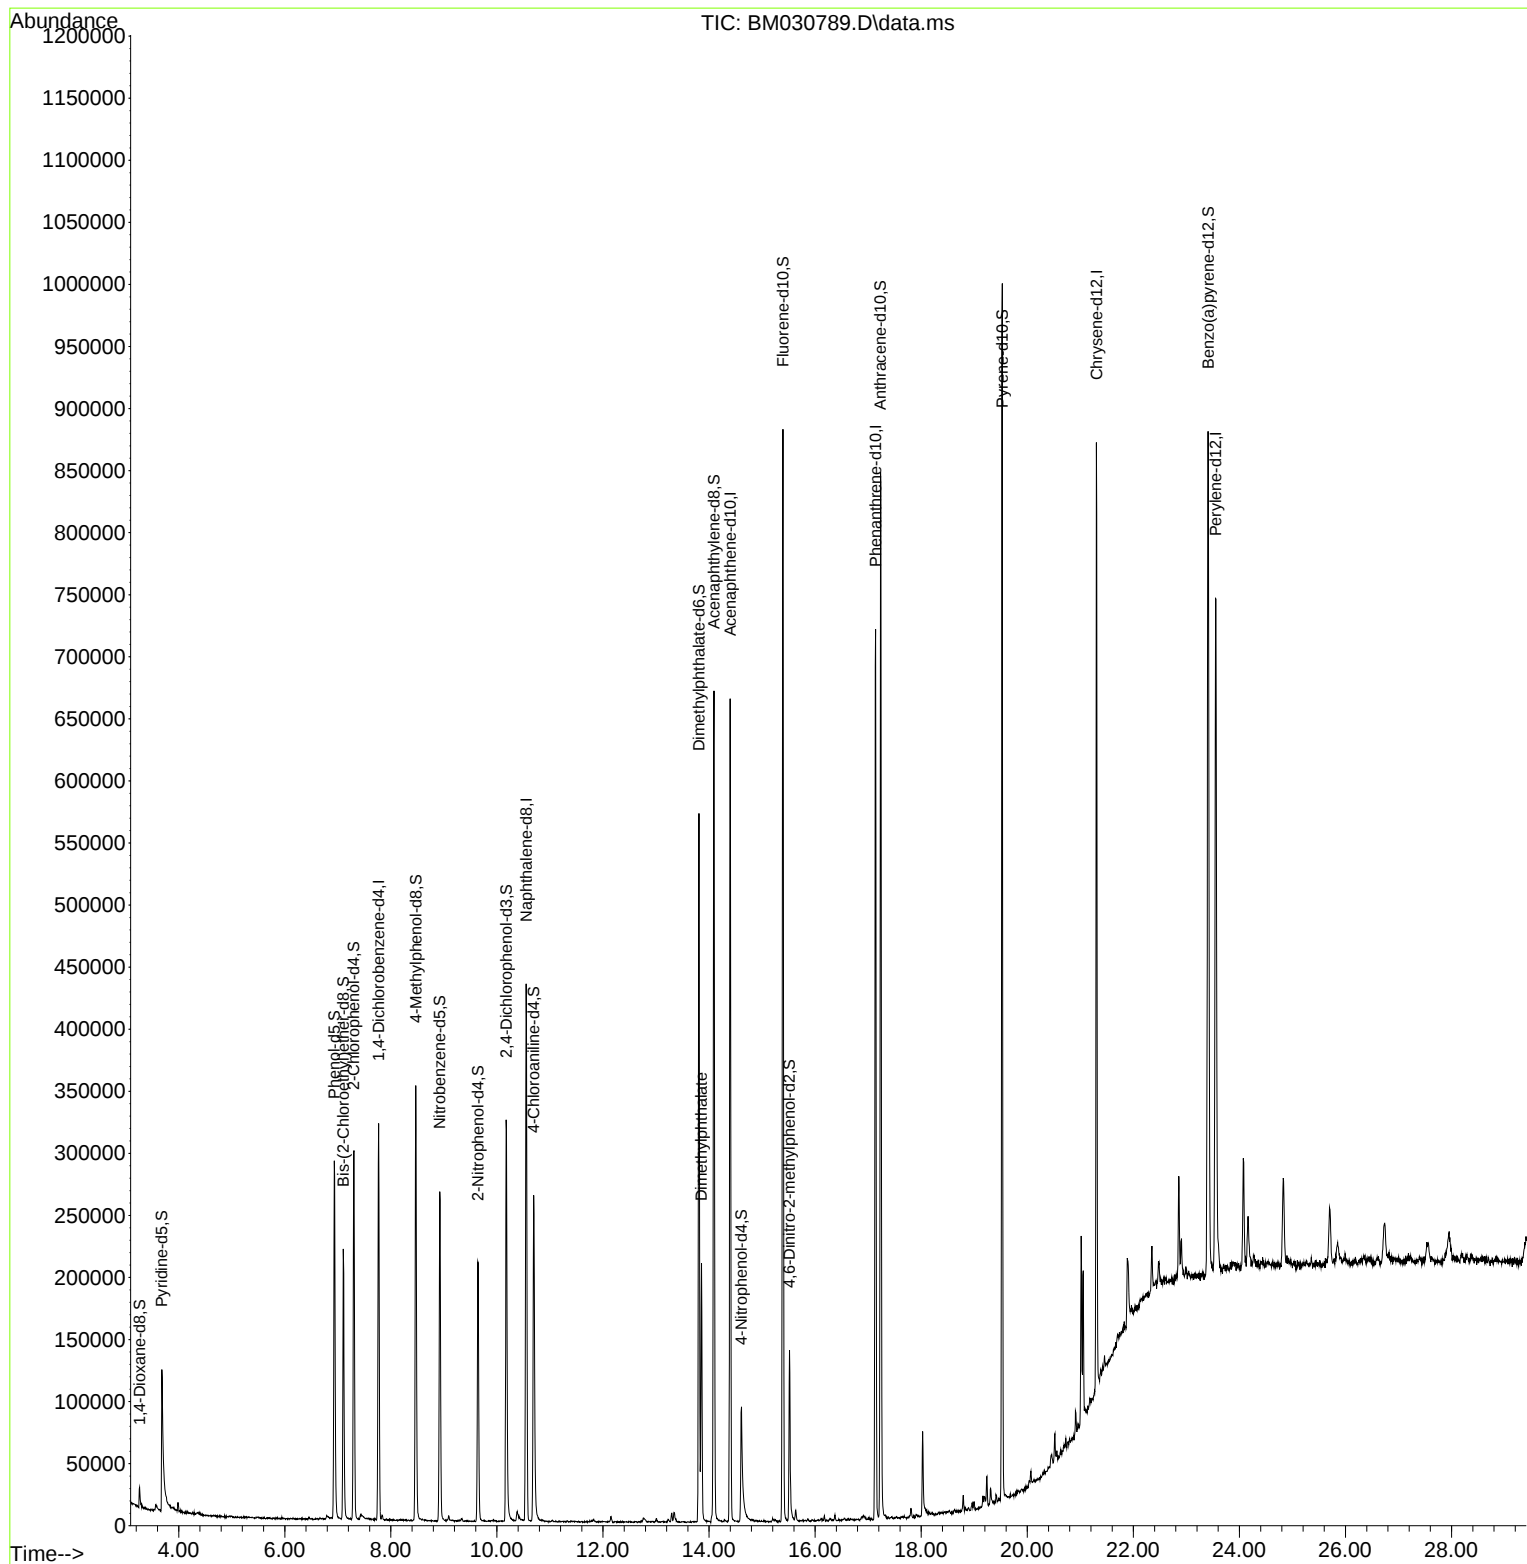


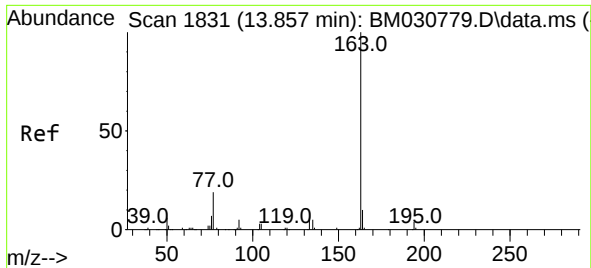

#47
 Dimethylphthalate
 Concen: 8.64 ng/ul
 RT: 13.857 min Scan# 1831
 Delta R.T. 0.000 min
 Lab File: BM030789.D
 Acq: 03 Jul 2021 00:10

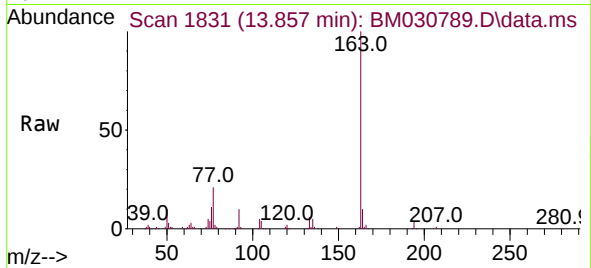

Tgt Ion:163 Resp: 128696
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.2 4.8
 164 10.0 8.2 12.4

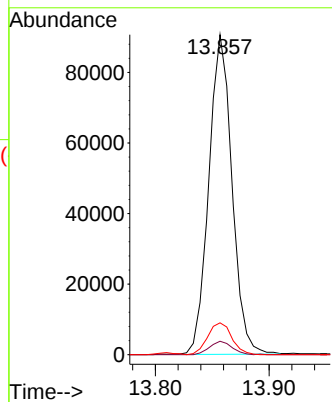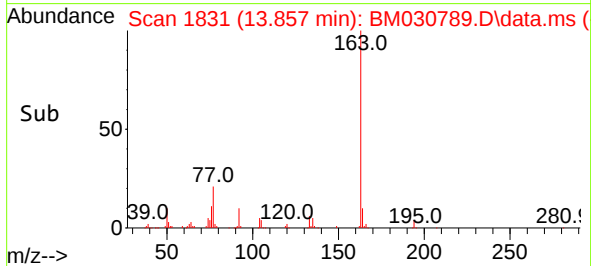

Instrument :
 BNA_M
 ClientSampleId :
 BGDY5

Manual Integrations
 APPROVED

mohammad
 7/6/2021 9:25:14 AM