

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030790.D
 Acq On : 03 Jul 2021 00:46
 Operator : CG/JU
 Sample : M2869-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY2

Quant Time: Jul 03 01:36:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 23:05:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	79450	20.00	ng/ul	0.00
20) Naphthalene-d8	10.551	136	315626	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	188472	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	349902	20.00	ng/ul	0.00
79) Chrysene-d12	21.303	240	340083	20.00	ng/ul	0.00
88) Perylene-d12	23.550	264	375879	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	9510	4.85	ng/uL	0.00
4) Pyridine-d5	3.681	84	106820	20.29	ng/ul	0.00
7) Phenol-d5	6.934	99	175194	25.57	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.104	67	115566	26.83	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	145040	27.42	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	140690	26.38	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	64702	27.47	ng/ul	0.00
24) 2-Nitrophenol-d4	9.639	143	69029	26.37	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	136485	27.22	ng/ul	0.00
31) 4-Chloroaniline-d4	10.692	131	179616	25.69	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	382552	29.40	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	490490	29.04	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	40834	16.56	ng/ul	0.00
60) Fluorene-d10	15.392	176	339642	29.43	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	34059	14.88	ng/ul	0.00
73) Anthracene-d10	17.233	188	488185	29.90	ng/ul	0.00
81) Pyrene-d10	19.521	212	524098	29.41	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	598117	30.61	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.857	163	141043	11.06	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030790.D
Acq On : 03 Jul 2021 00:46
Operator : CG/JU
Sample : M2869-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY2

Quant Time: Jul 03 01:36:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 23:05:33 2021
Response via : Initial Calibration

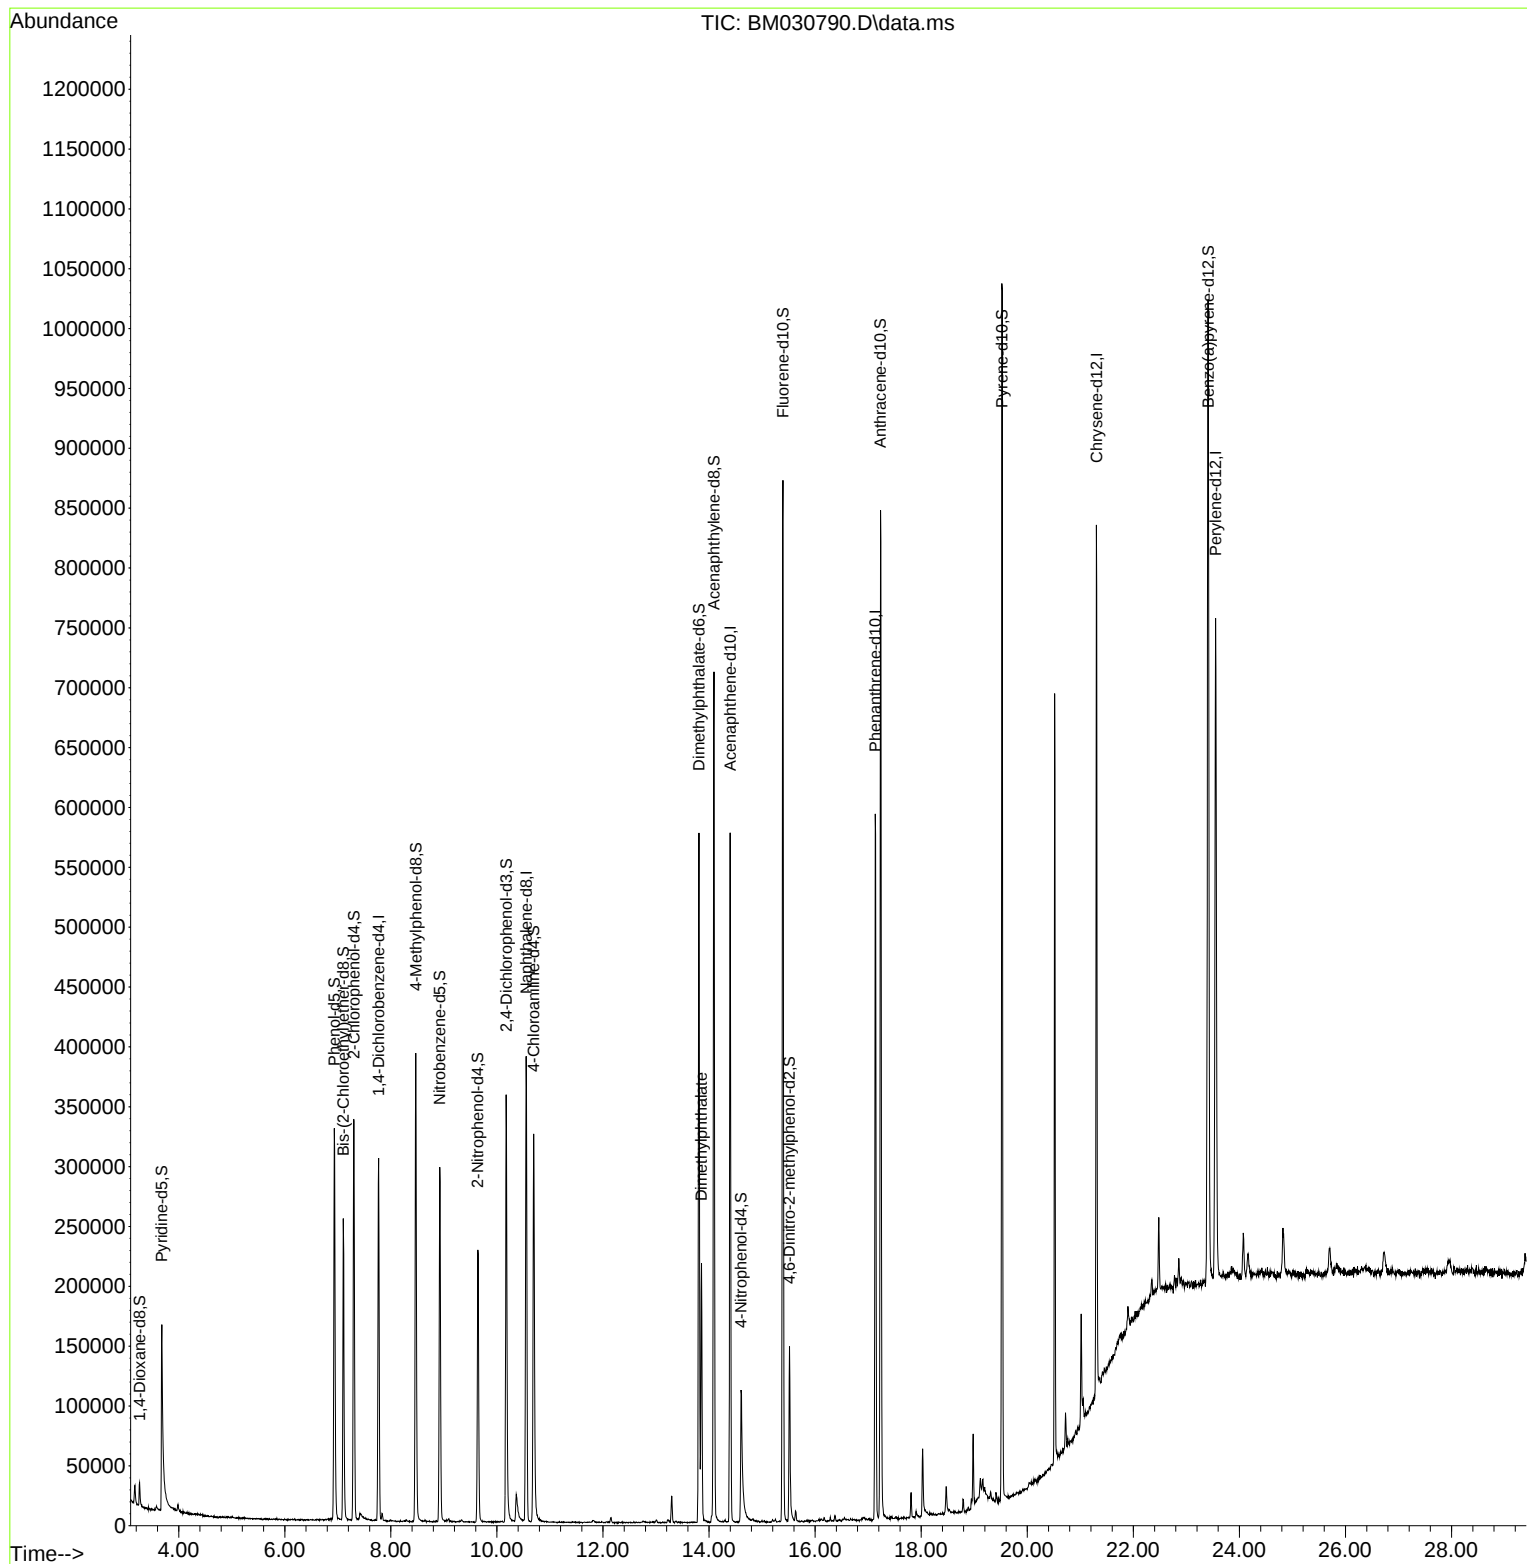

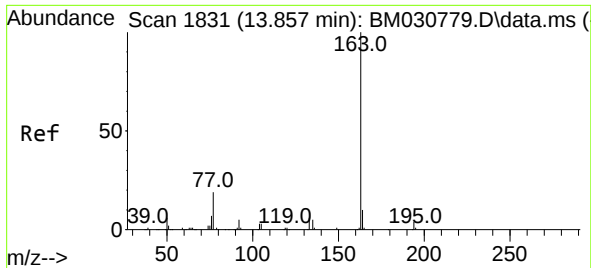

#47
 Dimethylphthalate
 Concen: 11.06 ng/ul
 RT: 13.857 min Scan# 1831
 Delta R.T. 0.000 min
 Lab File: BM030790.D
 Acq: 03 Jul 2021 00:46

Instrument :
 BNA_M
 ClientSampleId :
 BGDY2

Tgt Ion:163 Resp: 141043
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.2 4.8
 164 10.3 8.2 12.4

