

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030791.D
 Acq On : 03 Jul 2021 01:23
 Operator : CG/JU
 Sample : M2869-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDW8

Quant Time: Jul 03 02:07:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 02 23:05:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	86481	20.00	ng/ul	0.00
20) Naphthalene-d8	10.551	136	359886	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	226345	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	455295	20.00	ng/ul	0.00
79) Chrysene-d12	21.303	240	376682	20.00	ng/ul	0.00
88) Perylene-d12	23.550	264	387887	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	13678	6.41	ng/uL	0.00
4) Pyridine-d5	3.675	84	153089	26.71	ng/ul	0.00
7) Phenol-d5	6.934	99	273274	36.64	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.104	67	171187	36.52	ng/ul	0.00
11) 2-Chlorophenol-d4	7.298	132	218278	37.91	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	225103	38.78	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	101652	37.85	ng/ul	0.00
24) 2-Nitrophenol-d4	9.645	143	112969	37.85	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	218264	38.18	ng/ul	0.00
31) 4-Chloroaniline-d4	10.692	131	288117	36.14	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	653371	41.81	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	834555	41.14	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	78305	26.45	ng/ul	0.00
60) Fluorene-d10	15.392	176	586863	42.34	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	69580	23.36	ng/ul	0.00
73) Anthracene-d10	17.233	188	867859	40.84	ng/ul	0.00
81) Pyrene-d10	19.521	212	876085	44.39	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	844249	41.86	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.857	163	239721	15.65	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030791.D
Acq On : 03 Jul 2021 01:23
Operator : CG/JU
Sample : M2869-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDW8

Quant Time: Jul 03 02:07:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 02 23:05:33 2021
Response via : Initial Calibration

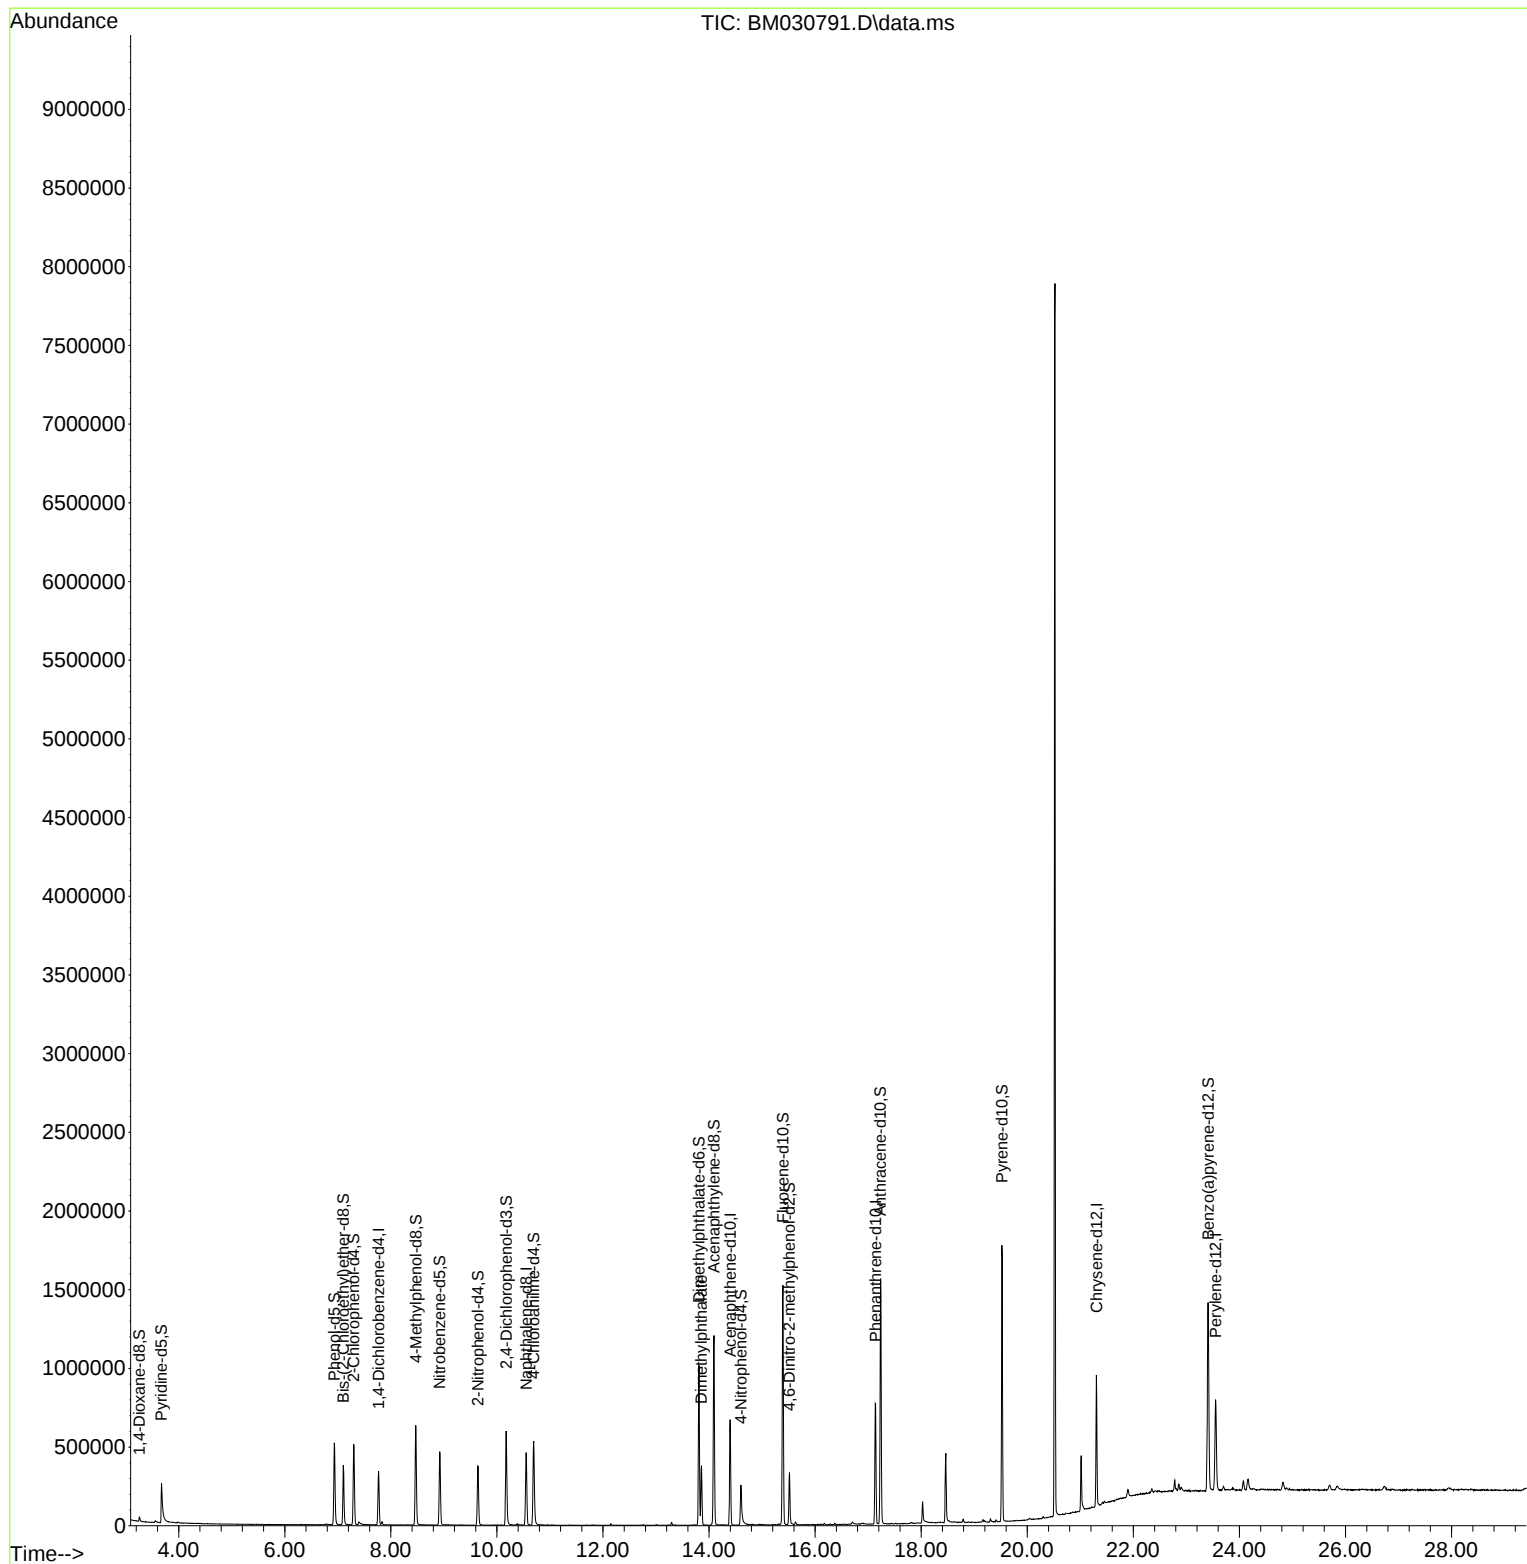

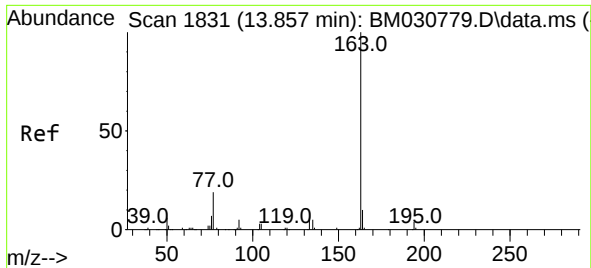

#47
 Dimethylphthalate
 Concen: 15.65 ng/ul
 RT: 13.857 min Scan# 1831
 Delta R.T. 0.000 min
 Lab File: BM030791.D
 Acq: 03 Jul 2021 01:23

Instrument :
 BNA_M
 ClientSampleId :
 BGDW8

Tgt Ion:163 Resp: 239721
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.2 4.8
 164 9.7 8.2 12.4

