

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030806.D
 Acq On : 03 Jul 2021 11:01
 Operator : CG/JU
 Sample : M2905-12
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK35

Quant Time: Jul 05 01:02:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 05 01:01:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	76254	20.00	ng/ul	0.00
20) Naphthalene-d8	10.551	136	303852	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	192383	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	404050	20.00	ng/ul	0.00
79) Chrysene-d12	21.303	240	448191	20.00	ng/ul	0.00
88) Perylene-d12	23.550	264	488137	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	11670	6.20	ng/uL	0.00
4) Pyridine-d5	3.687	84	57005	11.28	ng/ul	0.01
7) Phenol-d5	6.951	99	63673	9.68	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.104	67	141049	34.12	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	155509	30.63	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113	108213	21.14	ng/ul	0.00
21) Nitrobenzene-d5	8.922	128	85997	37.93	ng/ul	0.00
24) 2-Nitrophenol-d4	9.639	143	96016	38.10	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.180	165	179127	37.11	ng/ul	0.00
31) 4-Chloroaniline-d4	10.692	131	117087	17.39	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	564551	42.50	ng/ul	0.00
49) Acenaphthylene-d8	14.086	160	687380	39.86	ng/ul	0.00
54) 4-Nitrophenol-d4	14.615	143	25104	9.98	ng/ul	0.02
60) Fluorene-d10	15.386	176	502959	42.69	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.515	200	68616	25.96	ng/ul	0.00
73) Anthracene-d10	17.233	188	808063	42.85	ng/ul	0.00
81) Pyrene-d10	19.521	212	955264	40.68	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	1123831	44.28	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.293	88	9249	4.62	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030806.D
Acq On : 03 Jul 2021 11:01
Operator : CG/JU
Sample : M2905-12
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK35

Quant Time: Jul 05 01:02:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 05 01:01:28 2021
Response via : Initial Calibration

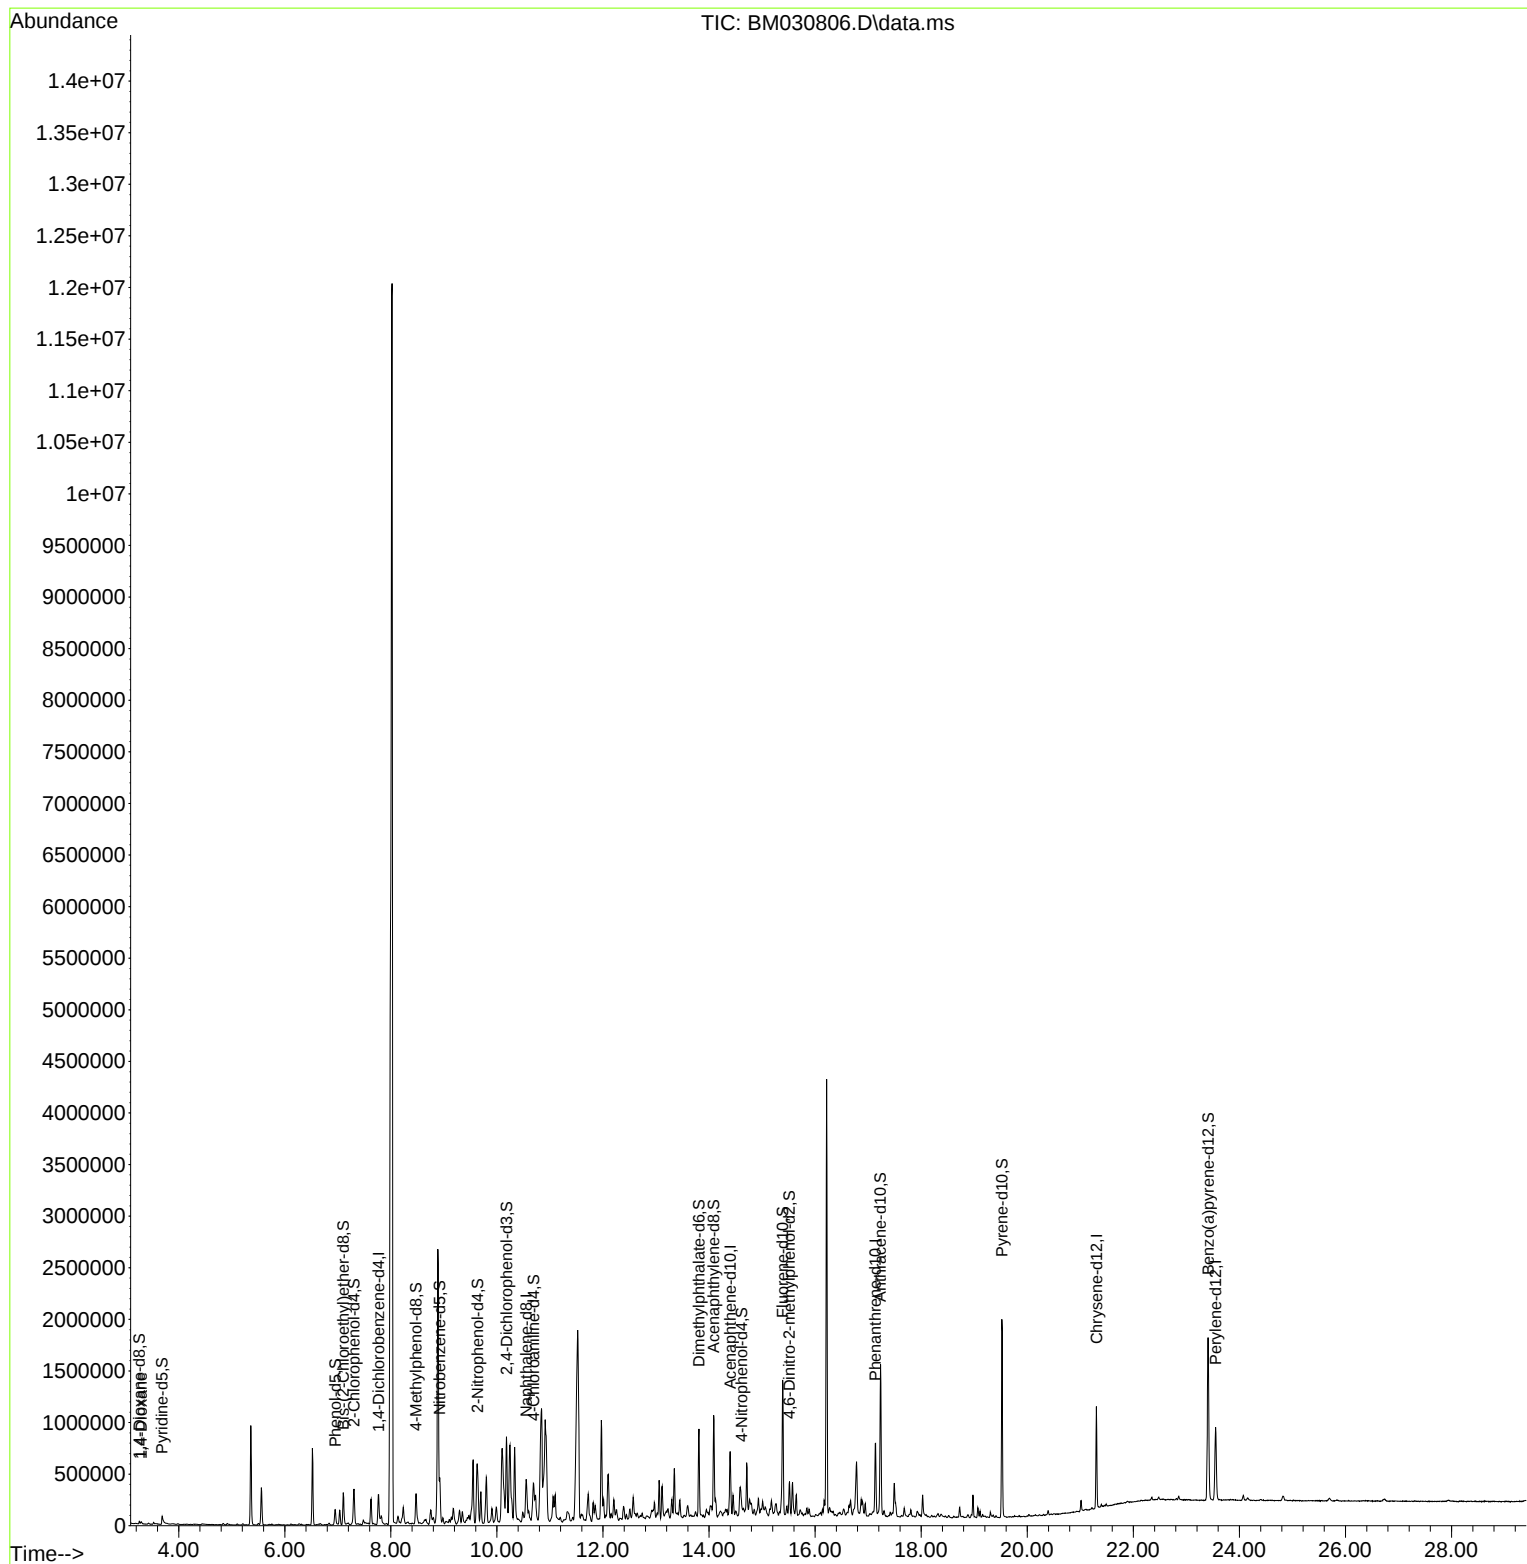

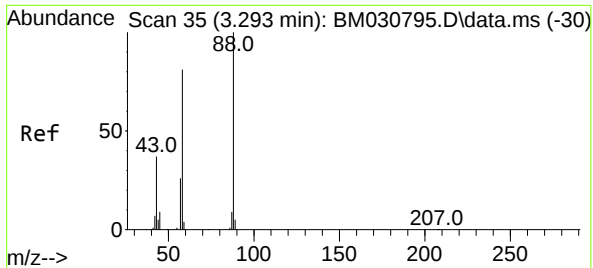

1,4-Dioxane
 Concen: 4.62 ng/uL
 RT: 3.293 min Scan# 35
 Delta R.T. -0.000 min
 Lab File: BM030806.D
 Acq: 03 Jul 2021 11:01

Instrument :
 BNA_M
 ClientSampleId :
 DBK35

Tgt Ion:	88	Resp:	9249
Ion	Ratio	Lower	Upper
88	100		
43	41.1	31.5	47.3
58	81.6	64.1	96.1

