

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030712.D
 Acq On : 30 Jun 2021 19:27
 Operator : CG/JU
 Sample : M2872-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs: 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030712.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.899	136	138	141	rVB3	1445	1522	0.11%	0.025%
2	3.993	149	154	159	rVV4	4634	8002	0.60%	0.129%
3	4.675	267	270	272	rVB3	1410	1518	0.11%	0.025%
4	7.781	791	798	811	rBV	324465	547564	41.12%	8.840%
5	7.993	830	834	836	rBV3	922	1368	0.10%	0.022%
6	10.228	1210	1214	1217	rBV2	856	1564	0.12%	0.025%
7	10.563	1264	1271	1286	rBV	425433	767063	57.60%	12.383%
8	11.810	1479	1483	1484	rBV	1996	1922	0.14%	0.031%
9	11.833	1484	1487	1490	rVB4	1936	2804	0.21%	0.045%
10	12.592	1611	1616	1621	rVB5	1021	1730	0.13%	0.028%
11	13.833	1821	1827	1837	rBV2	3349	6932	0.52%	0.112%
12	14.304	1901	1907	1908	rBV4	962	1685	0.13%	0.027%
13	14.410	1918	1925	1936	rBV	681942	1053953	79.15%	17.014%
14	15.392	2089	2092	2096	rVB3	1233	1348	0.10%	0.022%
15	16.557	2284	2290	2293	rVB4	920	2026	0.15%	0.033%
16	16.598	2293	2297	2301	rBV5	1206	2033	0.15%	0.033%
17	16.933	2351	2354	2359	rBV2	2284	3120	0.23%	0.050%
18	17.080	2376	2379	2384	rVB4	815	1333	0.10%	0.022%
19	17.145	2384	2390	2404	rBV	804032	1255846	94.31%	20.274%
20	17.451	2440	2442	2448	rVB6	1117	2345	0.18%	0.038%
21	18.045	2537	2543	2552	rBV10	6063	15099	1.13%	0.244%
22	18.168	2560	2564	2567	rVV5	1325	1835	0.14%	0.030%
23	18.262	2578	2580	2583	rBV3	1299	1372	0.10%	0.022%
24	19.321	2757	2760	2766	rBV8	4452	9526	0.72%	0.154%
25	21.315	3094	3099	3107	rBV	1029084	1331612	100.00%	21.497%
26	23.568	3476	3482	3493	rVB2	590228	1169378	87.82%	18.878%




Sum of corrected areas: 6194500

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030712.D
Acq On : 30 Jun 2021 19:27
Operator : CG/JU
Sample : M2872-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

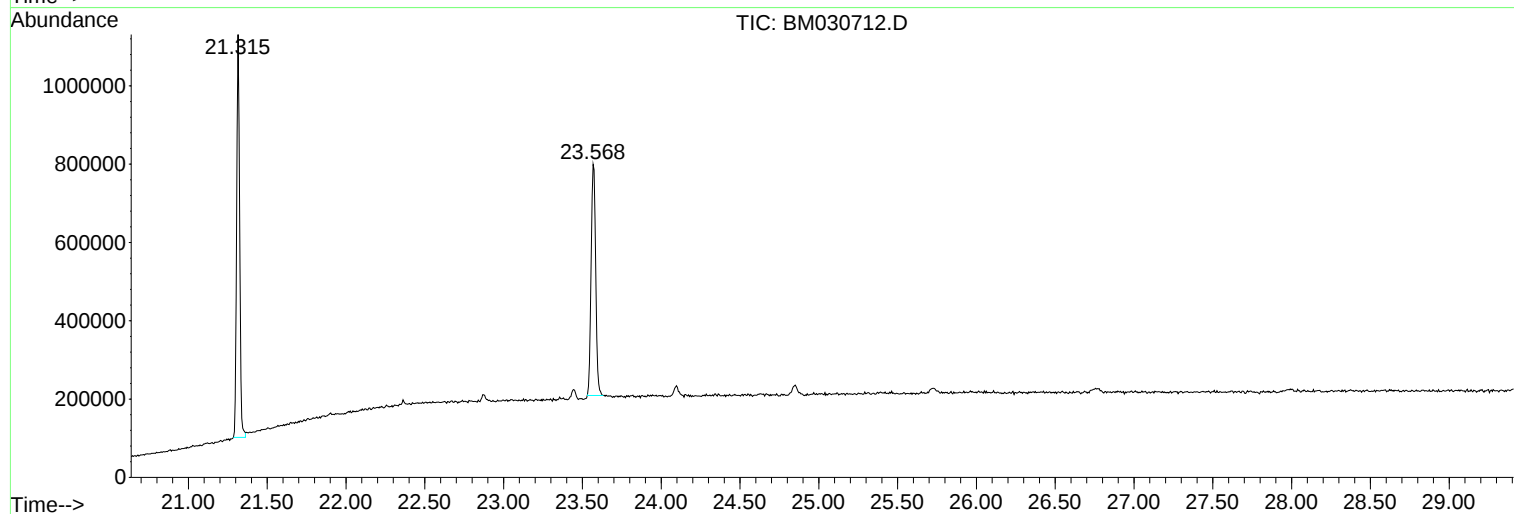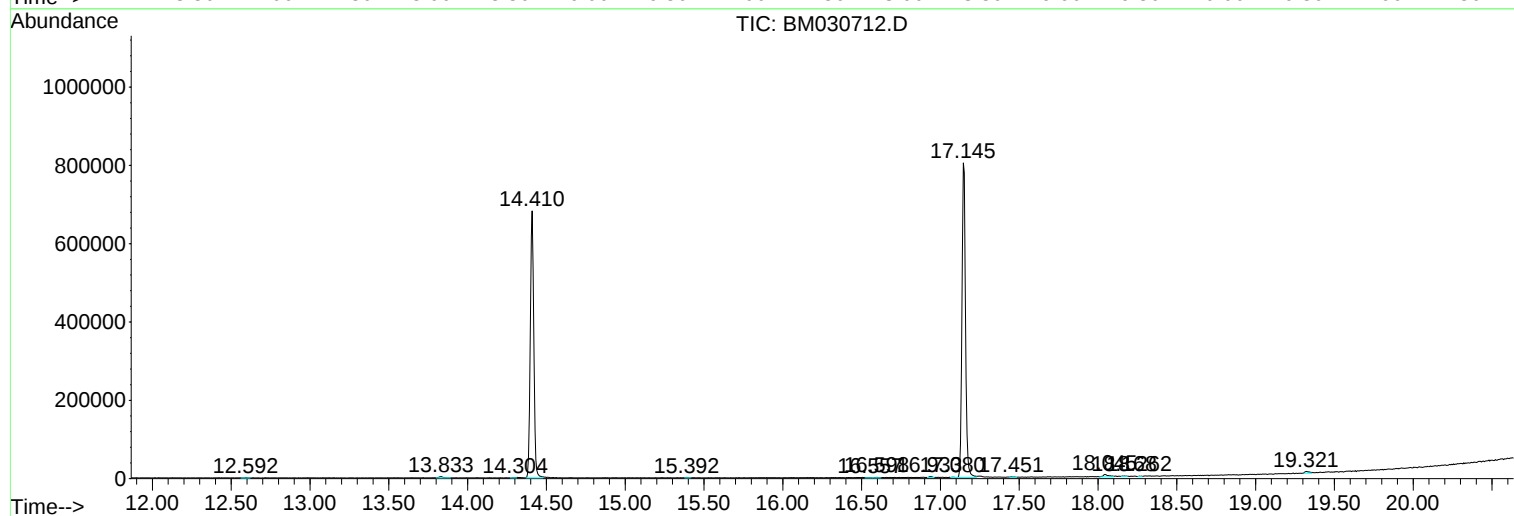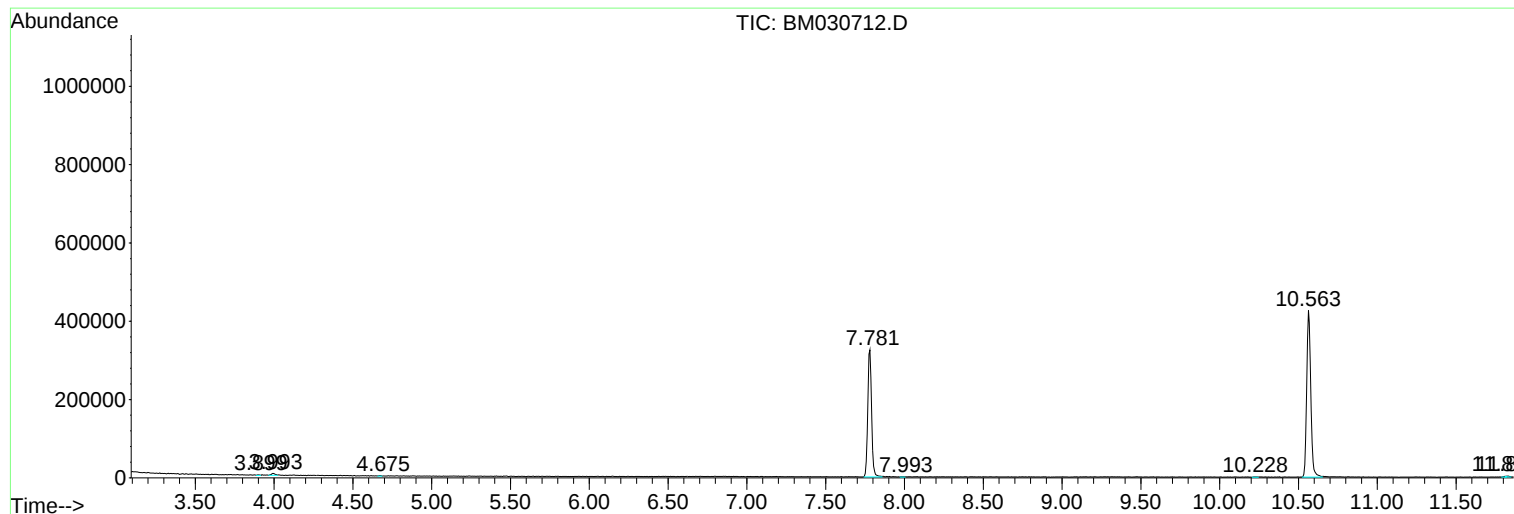

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030712.D
Acq On : 30 Jun 2021 19:27
Operator : CG/JU
Sample : M2872-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030712.D
Acq On : 30 Jun 2021 19:27
Operator : CG/JU
Sample : M2872-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
