

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030722.D
 Acq On : 01 Jul 2021 01:35
 Operator : CG/JU
 Sample : M2808-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGG09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030722.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	37	rVB3	7865	10863	0.96%	0.100%
2	3.716	105	107	115	rBV2	17512	44516	3.92%	0.408%
3	3.899	135	138	141	rBV5	2340	3209	0.28%	0.029%
4	3.993	150	154	159	rVB	9616	14574	1.28%	0.134%
5	4.216	189	192	195	rVB4	2217	2518	0.22%	0.023%
6	4.363	214	217	222	rBV6	2301	3397	0.30%	0.031%
7	4.546	245	248	255	rVB	8088	11808	1.04%	0.108%
8	4.905	307	309	315	rVB5	1146	1802	0.16%	0.017%
9	5.299	371	376	384	rVB2	5108	7335	0.65%	0.067%
10	5.434	394	399	407	rBV	13081	29080	2.56%	0.266%
11	5.799	457	461	467	rVB2	7563	11707	1.03%	0.107%
12	6.281	540	543	547	rBV3	937	1376	0.12%	0.013%
13	6.775	624	627	631	rVB4	2148	2330	0.21%	0.021%
14	6.946	649	656	671	rVB	124159	216024	19.04%	1.980%
15	7.116	678	685	693	rBV	97014	164840	14.53%	1.511%
16	7.310	711	718	728	rBV	136108	224966	19.83%	2.062%
17	7.393	729	732	737	rVB2	3346	4629	0.41%	0.042%
18	7.775	790	797	807	rBV	308330	497352	43.83%	4.558%
19	8.004	831	836	842	rVB7	2903	5257	0.46%	0.048%
20	8.316	884	889	892	rBV4	1779	2696	0.24%	0.025%
21	8.481	908	917	931	rBV	140816	247676	21.83%	2.270%
22	8.598	933	937	944	rVV2	6987	12961	1.14%	0.119%
23	8.651	944	946	948	rVB3	1290	1192	0.11%	0.011%
24	8.875	980	984	987	rBV5	1538	1892	0.17%	0.017%
25	8.934	987	994	1006	rVV	116069	198528	17.50%	1.819%
26	9.340	1061	1063	1064	rBV3	1500	1298	0.11%	0.012%
27	9.651	1110	1116	1127	rBV	87409	151078	13.31%	1.384%
28	10.016	1174	1178	1179	rBV3	1073	1491	0.13%	0.014%
29	10.187	1200	1207	1219	rBV	122588	235488	20.75%	2.158%
30	10.451	1248	1252	1253	rVV3	1206	1190	0.10%	0.011%
31	10.563	1263	1271	1279	rBV	416931	709562	62.53%	6.502%
32	10.704	1288	1295	1309	rBV	108647	233023	20.54%	2.135%
33	11.110	1359	1364	1365	rBV4	920	1224	0.11%	0.011%
34	11.398	1409	1413	1415	rBV4	1250	1725	0.15%	0.016%
35	11.828	1478	1486	1494	rBV5	2023	6659	0.59%	0.061%
36	12.151	1538	1541	1548	rVV6	2261	4255	0.37%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030722.D
 Acq On : 01 Jul 2021 01:35
 Operator : CG/JU
 Sample : M2808-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGG09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	12.304	1563	1567	1573	rVB5	791	1641	0.14%	0.015%
38	12.769	1642	1646	1648	rBV4	1734	2104	0.19%	0.019%
39	12.945	1674	1676	1681	rVV3	864	1224	0.11%	0.011%
40	13.022	1685	1689	1692	rVB2	3011	4057	0.36%	0.037%
41	13.239	1721	1726	1729	rBV3	2760	3864	0.34%	0.035%
42	13.298	1734	1736	1741	rBV4	1726	2516	0.22%	0.023%
43	13.816	1818	1824	1829	rBV	249375	365786	32.24%	3.352%
44	13.863	1829	1832	1842	rVB	42250	65503	5.77%	0.600%
45	13.963	1847	1849	1853	rVB4	941	1145	0.10%	0.010%
46	14.098	1864	1872	1882	rBV	289646	425495	37.50%	3.899%
47	14.304	1904	1907	1911	rVB3	3308	4268	0.38%	0.039%
48	14.404	1918	1924	1935	rBV	639710	962123	84.79%	8.817%
49	14.627	1955	1962	1977	rBV2	25639	70847	6.24%	0.649%
50	14.839	1995	1998	2004	rVB5	3585	4884	0.43%	0.045%
51	15.210	2056	2061	2063	rBV3	1348	2099	0.18%	0.019%
52	15.257	2066	2069	2073	rVB3	2211	2512	0.22%	0.023%
53	15.398	2087	2093	2101	rBV	389422	568318	50.08%	5.208%
54	15.527	2110	2115	2126	rBV2	41246	73204	6.45%	0.671%
55	15.645	2131	2135	2138	rBV3	2905	4053	0.36%	0.037%
56	15.769	2152	2156	2160	rBV5	1131	1689	0.15%	0.015%
57	15.821	2160	2165	2171	rVB	17763	24159	2.13%	0.221%
58	16.116	2211	2215	2219	rBV6	1958	2456	0.22%	0.023%
59	16.186	2223	2227	2229	rBV4	1600	1909	0.17%	0.017%
60	16.286	2239	2244	2246	rBV5	1210	1243	0.11%	0.011%
61	16.568	2287	2292	2296	rBV6	756	1463	0.13%	0.013%
62	16.904	2346	2349	2352	rVV5	2625	3484	0.31%	0.032%
63	16.939	2352	2355	2357	rVV2	2171	2569	0.23%	0.024%
64	17.027	2367	2370	2371	rBV2	1079	1162	0.10%	0.011%
65	17.145	2384	2390	2396	rBV	767408	1102607	97.17%	10.104%
66	17.245	2401	2407	2419	rVV	400338	591746	52.15%	5.423%
67	17.345	2421	2424	2429	rVB7	2325	3542	0.31%	0.032%
68	17.427	2436	2438	2440	rBV3	2409	2472	0.22%	0.023%
69	17.492	2447	2449	2451	rBV3	1924	1824	0.16%	0.017%
70	17.639	2469	2474	2477	rBV4	4591	6535	0.58%	0.060%
71	17.815	2500	2504	2506	rBV5	2995	4064	0.36%	0.037%
72	18.033	2536	2541	2547	rBV3	25877	43648	3.85%	0.400%
73	18.110	2552	2554	2559	rVB	3625	4498	0.40%	0.041%
74	18.221	2571	2573	2576	rVB4	2351	2271	0.20%	0.021%
75	18.333	2589	2592	2594	rBV4	3457	3986	0.35%	0.037%
76	18.962	2697	2699	2703	rVB3	4404	4179	0.37%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030722.D
 Acq On : 01 Jul 2021 01:35
 Operator : CG/JU
 Sample : M2808-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGG09

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	19.168	2732	2734	2736	rBV2	5310	5511	0.49%	0.051%
78	19.198	2736	2739	2743	rVB	21453	27203	2.40%	0.249%
79	19.315	2755	2759	2763	rBV6	10146	18340	1.62%	0.168%
80	19.533	2790	2796	2810	rBV	447443	680220	59.95%	6.233%
81	21.021	3046	3049	3056	rBV5	28732	41633	3.67%	0.382%
82	21.227	3081	3084	3088	rBV	27106	32090	2.83%	0.294%
83	21.309	3093	3098	3111	rVV	799153	1134732	100.00%	10.398%
84	23.421	3451	3457	3469	rVB	261864	539052	47.50%	4.940%
85	23.562	3475	3481	3494	rVB2	515058	987050	86.99%	9.045%




Sum of corrected areas: 10912501

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030722.D
Acq On : 01 Jul 2021 01:35
Operator : CG/JU
Sample : M2808-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGG09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

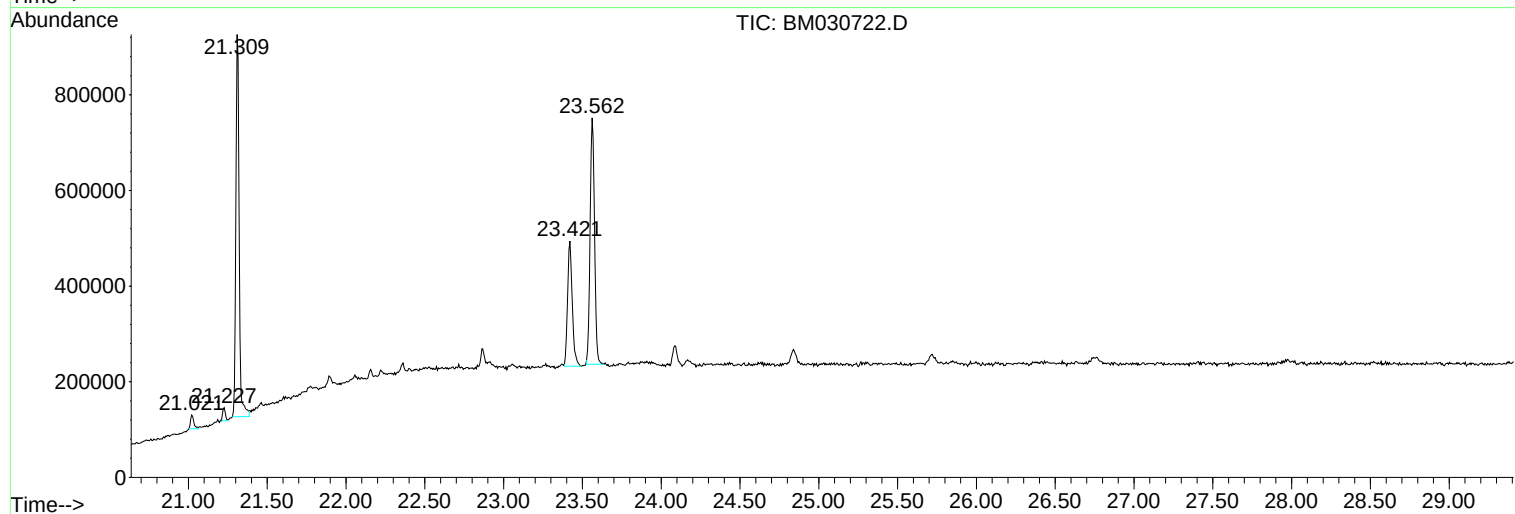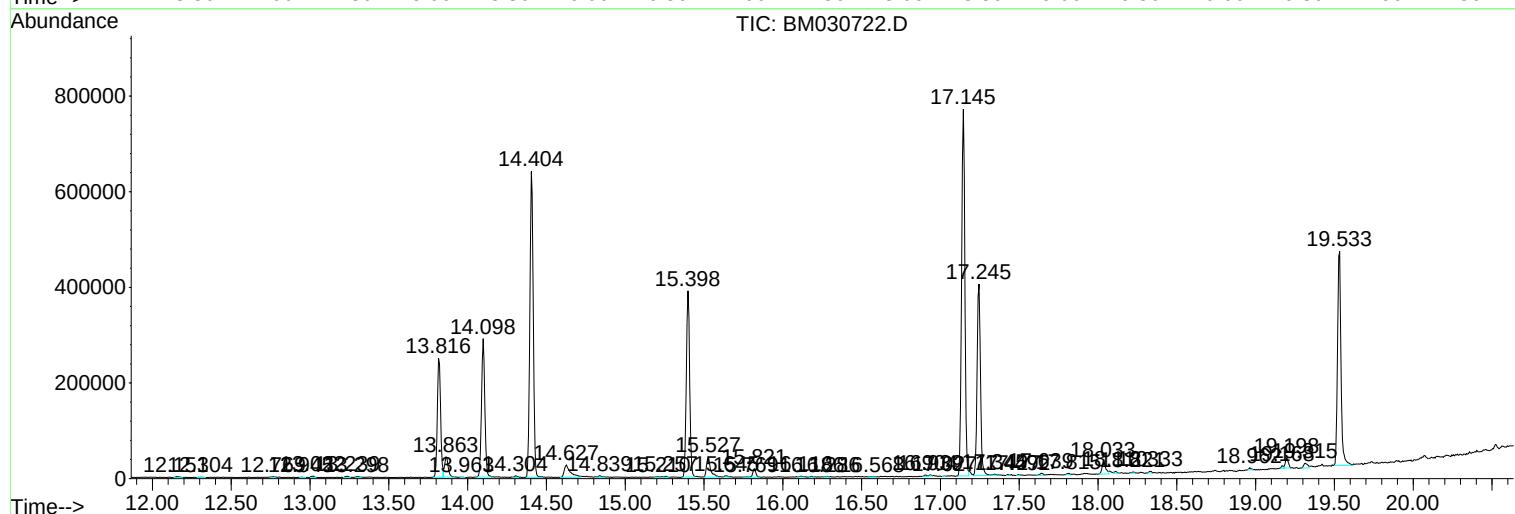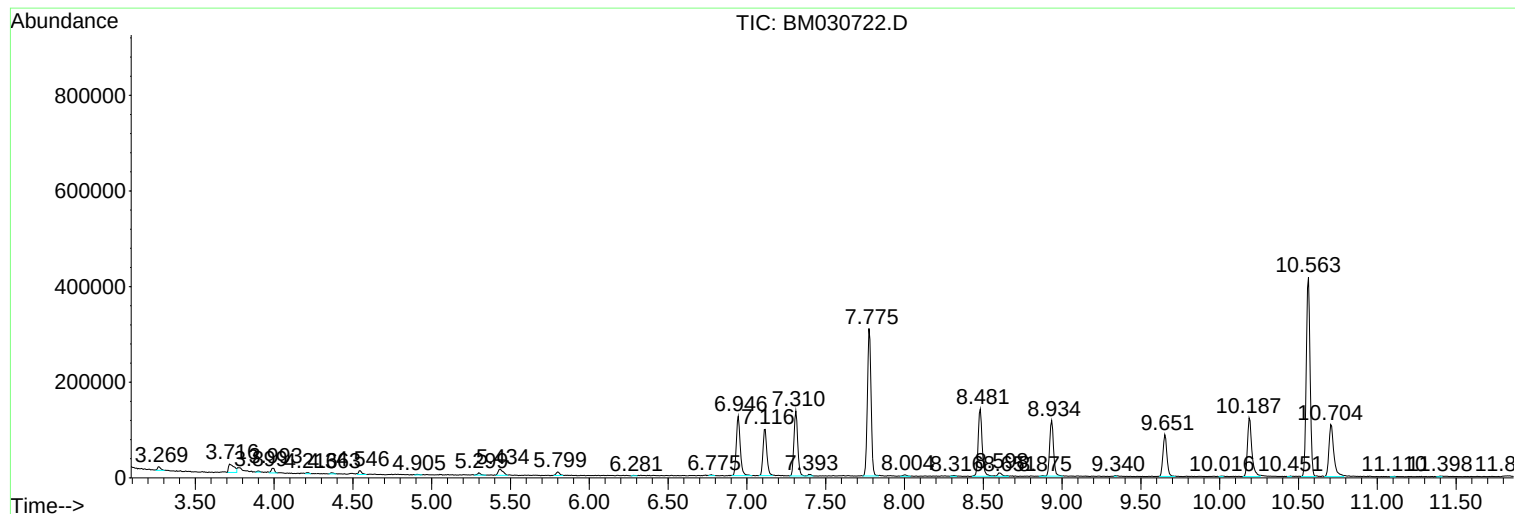

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030722.D
Acq On : 01 Jul 2021 01:35
Operator : CG/JU
Sample : M2808-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGG09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030722.D
Acq On : 01 Jul 2021 01:35
Operator : CG/JU
Sample : M2808-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGG09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
