

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030724.D
 Acq On : 01 Jul 2021 03:25
 Operator : CG/JU
 Sample : PB137380BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030724.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rBV	36544	46622	1.95%	0.168%
2	3.675	97	100	124	rBV	362900	677418	28.30%	2.438%
3	3.993	151	154	158	rVB	12724	14621	0.61%	0.053%
4	6.946	649	656	670	rBV	529940	858081	35.85%	3.089%
5	7.110	678	684	702	rBV	401010	659869	27.57%	2.375%
6	7.310	711	718	731	rVB	563127	894120	37.35%	3.218%
7	7.775	791	797	808	rVB	404521	646572	27.01%	2.327%
8	8.475	909	916	930	rBV	610018	1019482	42.59%	3.670%
9	8.934	986	994	1004	rBV	497231	826424	34.53%	2.975%
10	9.651	1107	1116	1130	rBV	410905	680830	28.44%	2.451%
11	10.181	1199	1206	1225	rBV	566615	1025182	42.83%	3.690%
12	10.563	1263	1271	1278	rBV	531859	902152	37.69%	3.247%
13	10.698	1286	1294	1313	rBV	542844	1040462	43.47%	3.745%
14	12.163	1536	1543	1551	rVB2	7613	13990	0.58%	0.050%
15	13.816	1817	1824	1840	rBV	997124	1433437	59.89%	5.160%
16	14.098	1865	1872	1888	rBV	1223780	1772361	74.04%	6.380%
17	14.404	1918	1924	1936	rVB	794989	1170623	48.91%	4.214%
18	14.604	1952	1958	1979	rBV	336117	637976	26.65%	2.296%
19	15.398	2086	2093	2106	rBV	1532098	2147097	89.70%	7.729%
20	15.522	2108	2114	2130	rVV	358205	558220	23.32%	2.009%
21	15.639	2130	2134	2138	rVB2	17062	24068	1.01%	0.087%
22	16.180	2222	2226	2230	rVB3	3747	4687	0.20%	0.017%
23	16.933	2349	2354	2360	rBV3	2600	4837	0.20%	0.017%
24	17.145	2383	2390	2400	rBV	892076	1259667	52.63%	4.534%
25	17.245	2400	2407	2419	rBV	1536372	2224493	92.93%	8.007%
26	18.051	2539	2544	2548	rBV8	2832	5982	0.25%	0.022%
27	18.633	2640	2643	2645	rBV4	1708	2461	0.10%	0.009%
28	19.169	2730	2734	2739	rVB2	13062	17786	0.74%	0.064%
29	19.421	2773	2777	2780	rVB	10515	13306	0.56%	0.048%
30	19.533	2790	2796	2804	rBV	1748370	2393638	100.00%	8.616%
31	21.310	3093	3098	3107	rBV	913185	1223239	51.10%	4.403%
32	23.421	3450	3457	3472	rVB	1199606	2321127	96.97%	8.355%
33	23.562	3475	3481	3489	rVB2	648721	1260393	52.66%	4.537%




Sum of corrected areas: 27781223

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030724.D
Acq On : 01 Jul 2021 03:25
Operator : CG/JU
Sample : PB137380BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

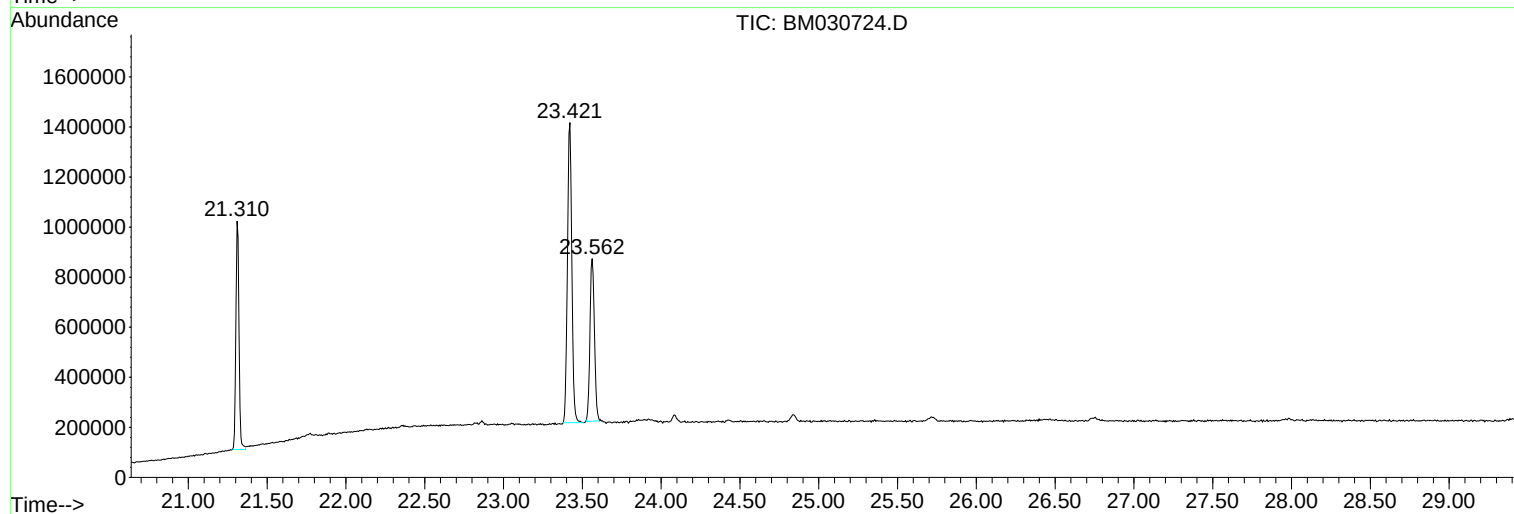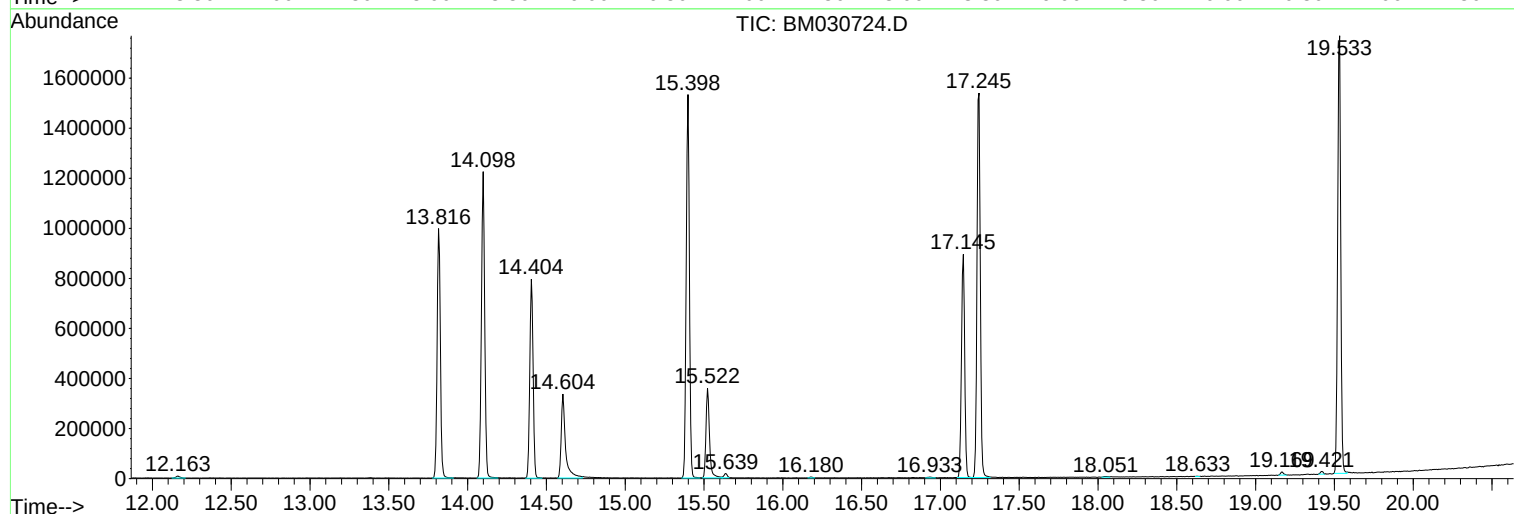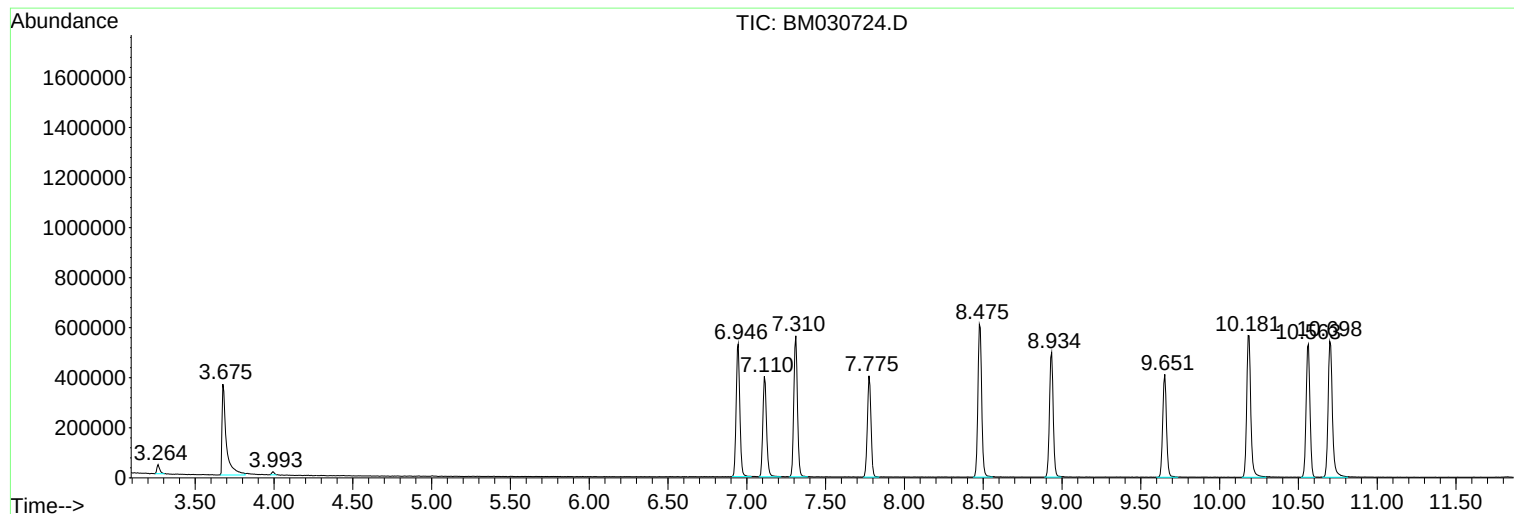

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030724.D
Acq On : 01 Jul 2021 03:25
Operator : CG/JU
Sample : PB137380BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030724.D
Acq On : 01 Jul 2021 03:25
Operator : CG/JU
Sample : PB137380BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
