

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030746.D
 Acq On : 01 Jul 2021 16:51
 Operator : CG/JU
 Sample : M2825-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030746.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	40	rVB	9388	13596	1.35%	0.137%
2	3.716	103	107	117	rBV	20182	57239	5.69%	0.576%
3	3.993	150	154	158	rBV	9286	12315	1.22%	0.124%
4	4.328	209	211	214	rBV4	1330	1168	0.12%	0.012%
5	4.357	214	216	220	rVV5	1356	1705	0.17%	0.017%
6	4.540	245	247	255	rVB6	3731	5849	0.58%	0.059%
7	4.616	258	260	263	rVB4	2040	1913	0.19%	0.019%
8	4.934	310	314	319	rVB4	3584	5845	0.58%	0.059%
9	5.428	394	398	408	rVV6	4830	10352	1.03%	0.104%
10	5.498	408	410	412	rVB3	1393	1108	0.11%	0.011%
11	5.563	419	421	423	rVB3	1407	1149	0.11%	0.012%
12	5.592	423	426	429	rBV4	865	1345	0.13%	0.014%
13	5.698	442	444	446	rBV3	1243	1306	0.13%	0.013%
14	5.798	457	461	468	rVB6	3405	5283	0.53%	0.053%
15	6.404	562	564	568	rVB4	1364	1496	0.15%	0.015%
16	6.469	573	575	578	rVV4	1242	1212	0.12%	0.012%
17	6.945	649	656	666	rBV	119539	203351	20.22%	2.048%
18	7.110	676	684	695	rBV	95135	159274	15.83%	1.604%
19	7.310	712	718	728	rVB	127129	207100	20.59%	2.086%
20	7.398	728	733	736	rBV5	3123	4463	0.44%	0.045%
21	7.598	765	767	769	rVV3	1606	1200	0.12%	0.012%
22	7.669	773	779	782	rVV6	995	1832	0.18%	0.018%
23	7.710	782	786	788	rVV5	953	1309	0.13%	0.013%
24	7.775	791	797	805	rVV	293784	469685	46.69%	4.730%
25	7.845	805	809	814	rVV3	5529	9600	0.95%	0.097%
26	7.892	816	817	821	rVB2	1699	1779	0.18%	0.018%
27	8.004	834	836	838	rVB3	1770	1545	0.15%	0.016%
28	8.181	863	866	870	rVB6	745	1253	0.12%	0.013%
29	8.310	884	888	892	rBV6	1552	2319	0.23%	0.023%
30	8.475	909	916	926	rBV	126316	217751	21.65%	2.193%
31	8.610	934	939	943	rVB3	2009	3029	0.30%	0.031%
32	8.933	987	994	1004	rBV	102498	177694	17.67%	1.789%
33	9.051	1012	1014	1018	rBV5	1032	1568	0.16%	0.016%
34	9.104	1020	1023	1028	rVV4	1113	1830	0.18%	0.018%
35	9.233	1041	1045	1048	rVB5	915	1461	0.15%	0.015%
36	9.333	1060	1062	1068	rBV4	1199	1691	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030746.D
 Acq On : 01 Jul 2021 16:51
 Operator : CG/JU
 Sample : M2825-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	9.651	1109	1116	1128	rBV	76771	132987	13.22%	1.339%
38	10.186	1201	1207	1218	rBV	101682	200342	19.92%	2.018%
39	10.257	1218	1219	1222	rVB3	1727	1227	0.12%	0.012%
40	10.557	1263	1270	1279	rBV	347533	602279	59.88%	6.065%
41	10.710	1289	1296	1311	rBV	83738	188582	18.75%	1.899%
42	10.851	1318	1320	1324	rVB5	1014	1136	0.11%	0.011%
43	11.422	1412	1417	1419	rVB4	871	1502	0.15%	0.015%
44	11.827	1482	1486	1493	rVB6	1667	3883	0.39%	0.039%
45	12.163	1539	1543	1550	rVB5	1899	3757	0.37%	0.038%
46	13.010	1684	1687	1692	rBV5	2082	3015	0.30%	0.030%
47	13.139	1706	1709	1712	rBV3	834	1145	0.11%	0.012%
48	13.239	1719	1726	1731	rVB5	1567	3099	0.31%	0.031%
49	13.304	1731	1737	1742	rVB6	2413	5179	0.51%	0.052%
50	13.698	1801	1804	1805	rBV3	1094	1116	0.11%	0.011%
51	13.715	1805	1807	1810	rVB3	1115	1213	0.12%	0.012%
52	13.815	1818	1824	1828	rBV	187375	272302	27.07%	2.742%
53	13.863	1828	1832	1844	rVB	94086	143973	14.31%	1.450%
54	14.098	1861	1872	1884	rBV	214102	331326	32.94%	3.337%
55	14.304	1903	1907	1913	rVB5	1967	2908	0.29%	0.029%
56	14.404	1917	1924	1931	rBV	477205	695410	69.13%	7.003%
57	14.462	1931	1934	1938	rVV3	1923	3013	0.30%	0.030%
58	14.515	1940	1943	1947	rBV5	1024	1638	0.16%	0.016%
59	14.621	1951	1961	1981	rBV4	23716	78262	7.78%	0.788%
60	14.810	1991	1993	1999	rVB6	1034	1266	0.13%	0.013%
61	15.198	2056	2059	2060	rBV3	1244	1290	0.13%	0.013%
62	15.251	2067	2068	2070	rBV	1477	1350	0.13%	0.014%
63	15.309	2074	2078	2082	rVV4	3978	7088	0.70%	0.071%
64	15.398	2084	2093	2101	rVV	294815	432937	43.04%	4.360%
65	15.457	2101	2103	2106	rVV4	3618	4083	0.41%	0.041%
66	15.527	2110	2115	2126	rVV2	31026	59500	5.92%	0.599%
67	15.639	2130	2134	2137	rVB4	2298	2410	0.24%	0.024%
68	15.751	2151	2153	2154	rBV2	1058	1083	0.11%	0.011%
69	15.821	2159	2165	2168	rBV4	4275	7049	0.70%	0.071%
70	16.292	2240	2245	2248	rVB4	1554	2339	0.23%	0.024%
71	16.374	2257	2259	2264	rVB3	2952	3351	0.33%	0.034%
72	16.568	2289	2292	2295	rVB4	1233	1108	0.11%	0.011%
73	16.627	2300	2302	2304	rBV3	1471	1677	0.17%	0.017%
74	16.704	2310	2315	2326	rBV	8497	19095	1.90%	0.192%
75	16.939	2351	2355	2356	rVB4	1128	1200	0.12%	0.012%
76	16.998	2361	2365	2367	rVB3	1146	1326	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030746.D
 Acq On : 01 Jul 2021 16:51
 Operator : CG/JU
 Sample : M2825-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	17.015	2367	2368	2371	rBV2	1025	1322	0.13%	0.013%
78	17.145	2383	2390	2395	rBV	484298	722902	71.87%	7.280%
79	17.180	2395	2396	2401	rVV	18807	21404	2.13%	0.216%
80	17.239	2401	2406	2419	rVB2	280323	419042	41.66%	4.220%
81	17.562	2459	2461	2463	rBV3	1657	1471	0.15%	0.015%
82	17.815	2502	2504	2508	rVB5	2615	3092	0.31%	0.031%
83	17.945	2524	2526	2529	rVB4	2535	2088	0.21%	0.021%
84	18.033	2536	2541	2546	rBV2	22584	40853	4.06%	0.411%
85	18.109	2552	2554	2557	rVB4	1923	2087	0.21%	0.021%
86	18.203	2567	2570	2572	rBV4	2736	2761	0.27%	0.028%
87	18.327	2589	2591	2592	rBV2	1704	1187	0.12%	0.012%
88	18.474	2610	2616	2622	rBV	29379	51538	5.12%	0.519%
89	18.586	2633	2635	2636	rBV2	1835	1249	0.12%	0.013%
90	18.633	2642	2643	2645	rBV2	1702	1254	0.12%	0.013%
91	18.797	2667	2671	2674	rBV3	5548	7568	0.75%	0.076%
92	19.162	2731	2733	2735	rBV3	3100	2849	0.28%	0.029%
93	19.197	2735	2739	2744	rVB	21855	29900	2.97%	0.301%
94	19.315	2755	2759	2762	rBV4	7025	10264	1.02%	0.103%
95	19.527	2790	2795	2807	rBV	373661	541644	53.85%	5.455%
96	20.521	2960	2964	2970	rBV	711856	750922	74.65%	7.562%
97	21.021	3046	3049	3056	rBV3	40847	50708	5.04%	0.511%
98	21.309	3093	3098	3103	rBV	634405	875600	87.05%	8.818%
99	23.415	3451	3456	3466	rVB	287193	562161	55.89%	5.661%
100	23.562	3475	3481	3492	rVB2	540594	1005887	100.00%	10.130%




Sum of corrected areas: 9929814

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030746.D
Acq On : 01 Jul 2021 16:51
Operator : CG/JU
Sample : M2825-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

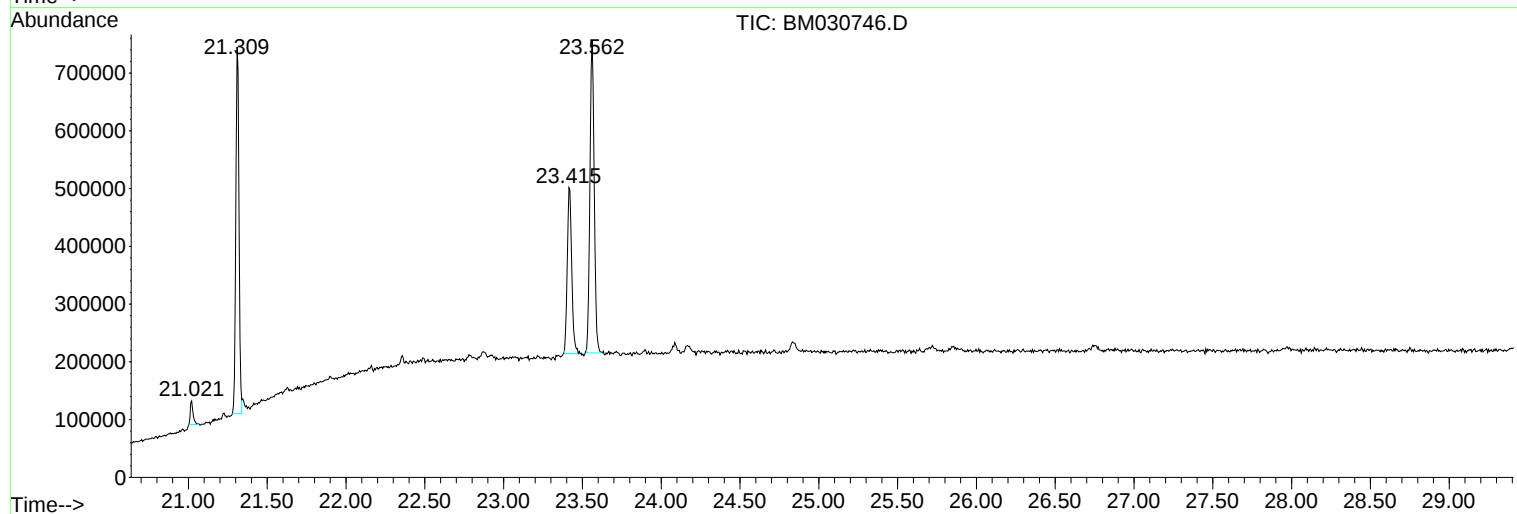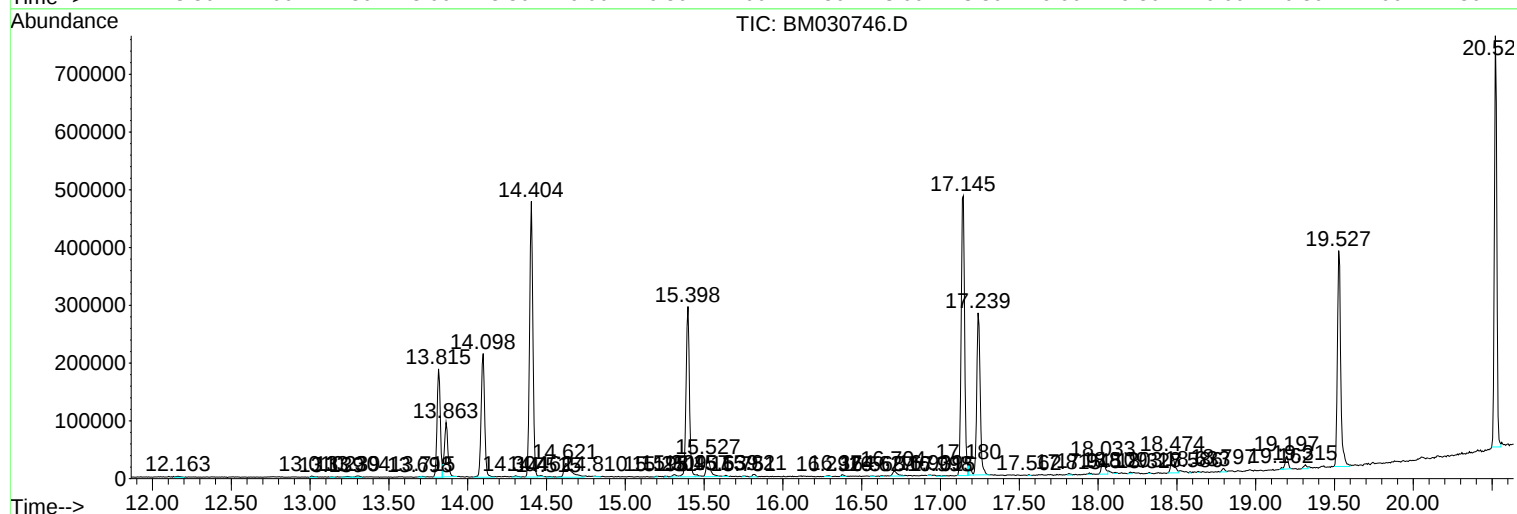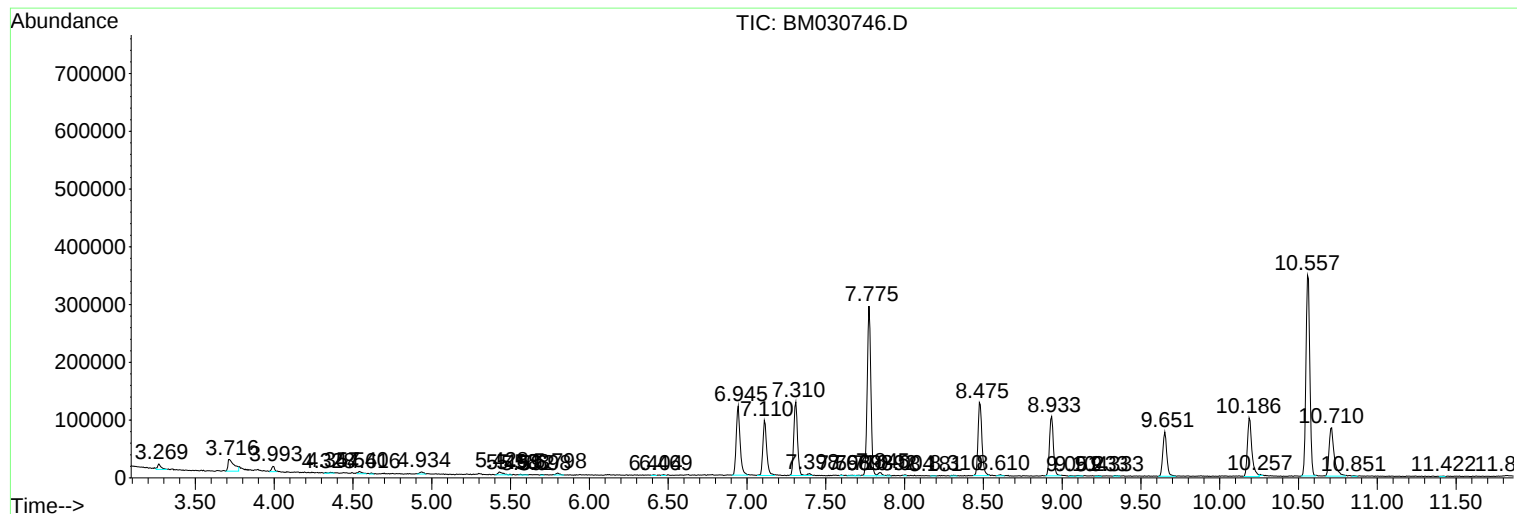

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030746.D
Acq On : 01 Jul 2021 16:51
Operator : CG/JU
Sample : M2825-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP5










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	17.15 ng/ul	750922	Chrysene-d12	21.309

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
3			Diisooctyl adipate	370	C22H42O4	001330-86-5	81
4			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	72
5			Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	68

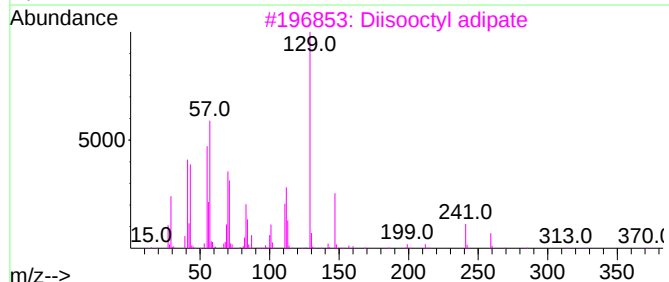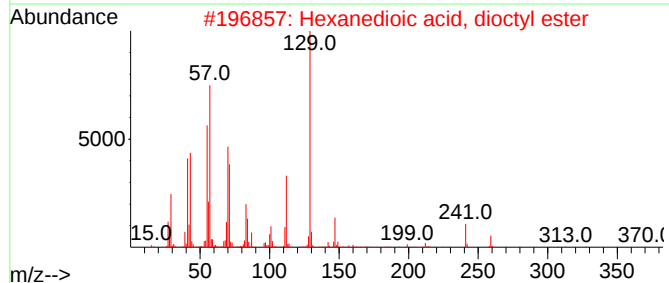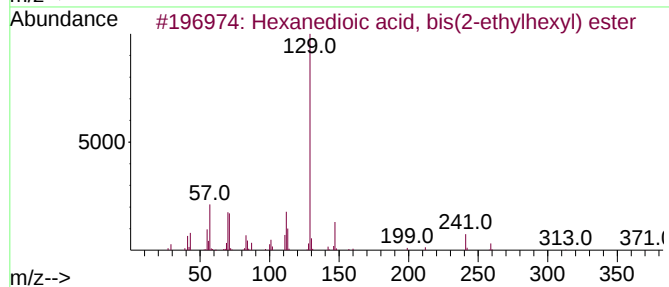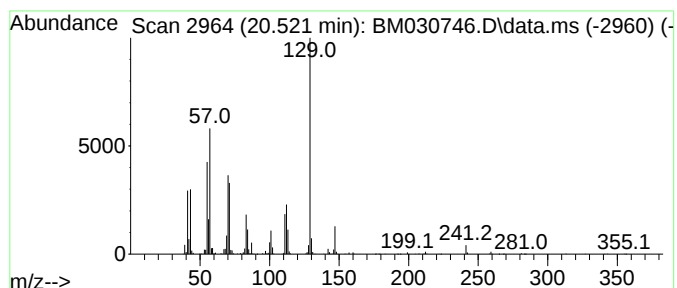

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030746.D
Acq On : 01 Jul 2021 16:51
Operator : CG/JU
Sample : M2825-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	17.1	ng/ul	750922	5	21.309	875600	20.0