

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030747.D
 Acq On : 01 Jul 2021 17:27
 Operator : CG/JU
 Sample : M2825-07
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030747.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	28	30	37	rVB3	3938	6680	0.70%	0.084%
2	3.746	108	112	113	rBV2	6630	7198	0.76%	0.090%
3	3.781	115	118	124	rVB3	9192	15305	1.61%	0.191%
4	3.993	149	154	161	rVV	9934	14851	1.56%	0.186%
5	4.545	244	248	252	rVB5	2887	4711	0.49%	0.059%
6	5.304	373	377	382	rBV6	2213	3374	0.35%	0.042%
7	5.434	394	399	405	rBV3	4327	8577	0.90%	0.107%
8	5.798	458	461	465	rVB3	2359	2886	0.30%	0.036%
9	6.769	623	626	631	rBV3	3114	4553	0.48%	0.057%
10	6.945	651	656	670	rVB	64637	115911	12.16%	1.449%
11	7.110	679	684	693	rBV	51030	89227	9.36%	1.116%
12	7.310	712	718	729	rVV	72886	119764	12.57%	1.498%
13	7.398	729	733	739	rVB6	2391	4305	0.45%	0.054%
14	7.775	789	797	806	rBV	265041	428351	44.94%	5.356%
15	7.845	806	809	812	rVV5	1828	2609	0.27%	0.033%
16	7.898	816	818	823	rVB6	1792	2766	0.29%	0.035%
17	7.998	830	835	842	rBV5	5116	8429	0.88%	0.105%
18	8.310	884	888	894	rBV4	3451	6425	0.67%	0.080%
19	8.481	907	917	926	rBV	64067	121055	12.70%	1.514%
20	8.933	988	994	1002	rBV	54171	93837	9.85%	1.173%
21	9.651	1110	1116	1128	rVV	38292	67790	7.11%	0.848%
22	10.192	1202	1208	1218	rBV	47294	100146	10.51%	1.252%
23	10.557	1263	1270	1277	rBV	318559	547976	57.50%	6.852%
24	10.716	1291	1297	1312	rVB	40907	96933	10.17%	1.212%
25	11.821	1481	1485	1488	rBV3	1647	2635	0.28%	0.033%
26	12.233	1549	1555	1559	rVB4	992	1854	0.19%	0.023%
27	12.763	1641	1645	1648	rBV4	1737	2075	0.22%	0.026%
28	13.016	1681	1688	1691	rBV4	2042	2749	0.29%	0.034%
29	13.233	1719	1725	1732	rVV6	1096	2980	0.31%	0.037%
30	13.304	1734	1737	1742	rVB4	1439	2317	0.24%	0.029%
31	13.727	1802	1809	1814	rVB3	4956	10669	1.12%	0.133%
32	13.815	1819	1824	1829	rVV	101141	152812	16.03%	1.911%
33	13.863	1829	1832	1838	rVV	48247	71886	7.54%	0.899%
34	13.904	1838	1839	1845	rVV4	1736	2584	0.27%	0.032%
35	13.963	1845	1849	1852	rVV4	2673	3505	0.37%	0.044%
36	14.098	1865	1872	1883	rBV	118730	184133	19.32%	2.303%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030747.D
 Acq On : 01 Jul 2021 17:27
 Operator : CG/JU
 Sample : M2825-07
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	14.310	1905	1908	1913	rVV5	1541	2093	0.22%	0.026%
38	14.404	1917	1924	1931	rVV	428881	631647	66.27%	7.899%
39	14.468	1931	1935	1943	rVB	30227	46602	4.89%	0.583%
40	14.633	1959	1963	1973	rVV8	8067	23652	2.48%	0.296%
41	14.804	1989	1992	1997	rVB2	3437	4940	0.52%	0.062%
42	14.880	2002	2005	2010	rBV5	1949	2729	0.29%	0.034%
43	15.198	2054	2059	2062	rVV3	1533	2562	0.27%	0.032%
44	15.310	2072	2078	2084	rBV3	2159	5373	0.56%	0.067%
45	15.398	2084	2093	2099	rVV	160309	240070	25.19%	3.002%
46	15.451	2099	2102	2109	rVV	15306	25215	2.65%	0.315%
47	15.527	2111	2115	2127	rVV4	14275	30105	3.16%	0.376%
48	15.609	2127	2129	2132	rVV4	1670	2039	0.21%	0.025%
49	15.657	2136	2137	2141	rVV3	1694	2032	0.21%	0.025%
50	15.704	2142	2145	2148	rVB3	1458	1901	0.20%	0.024%
51	15.745	2148	2152	2157	rBV2	4792	7668	0.80%	0.096%
52	15.815	2162	2164	2168	rVB5	4582	5194	0.54%	0.065%
53	15.898	2174	2178	2186	rVB	4997	10525	1.10%	0.132%
54	15.974	2190	2191	2197	rVB3	1539	2019	0.21%	0.025%
55	16.121	2212	2216	2219	rBV4	1399	2800	0.29%	0.035%
56	16.462	2270	2274	2278	rVV5	3210	5729	0.60%	0.072%
57	16.504	2278	2281	2284	rVV4	1907	2314	0.24%	0.029%
58	16.598	2294	2297	2303	rBV4	1557	2987	0.31%	0.037%
59	16.680	2308	2311	2312	rBV3	2518	2271	0.24%	0.028%
60	16.709	2312	2316	2321	rVV4	5710	9612	1.01%	0.120%
61	16.809	2331	2333	2337	rBV4	1783	1999	0.21%	0.025%
62	16.898	2341	2348	2353	rVV5	7475	15793	1.66%	0.197%
63	16.962	2355	2359	2363	rVV2	5080	7917	0.83%	0.099%
64	17.145	2383	2390	2394	rBV	431956	665520	69.83%	8.322%
65	17.186	2394	2397	2402	rVV	110113	153167	16.07%	1.915%
66	17.239	2402	2406	2410	rVV	146994	227919	23.91%	2.850%
67	17.274	2410	2412	2419	rVV	37647	52422	5.50%	0.656%
68	17.321	2419	2420	2422	rVV2	2487	2409	0.25%	0.030%
69	17.439	2433	2440	2443	rBV6	1405	3195	0.34%	0.040%
70	17.639	2470	2474	2475	rBV3	1286	1918	0.20%	0.024%
71	17.951	2524	2527	2531	rVB6	1812	3055	0.32%	0.038%
72	18.027	2534	2540	2543	rVV3	16427	31810	3.34%	0.398%
73	18.068	2543	2547	2552	rVB	16123	26057	2.73%	0.326%
74	18.150	2557	2561	2564	rVV2	8572	12332	1.29%	0.154%
75	18.215	2566	2572	2576	rVV2	21452	38391	4.03%	0.480%
76	18.245	2576	2577	2584	rVB3	8280	9484	1.00%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030747.D
 Acq On : 01 Jul 2021 17:27
 Operator : CG/JU
 Sample : M2825-07
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	18.327	2587	2591	2593	rBV5	2074	2603	0.27%	0.033%
78	18.380	2596	2600	2601	rBV4	2043	1823	0.19%	0.023%
79	18.474	2609	2616	2620	rBV	8324	15670	1.64%	0.196%
80	18.515	2621	2623	2630	rVB2	7921	11985	1.26%	0.150%
81	18.692	2650	2653	2655	rBV4	2067	2655	0.28%	0.033%
82	18.762	2660	2665	2667	rBV4	3279	4429	0.46%	0.055%
83	18.933	2691	2694	2697	rBV3	6847	8506	0.89%	0.106%
84	18.997	2702	2705	2708	rBV4	4108	5277	0.55%	0.066%
85	19.133	2727	2728	2730	rBV2	2344	2172	0.23%	0.027%
86	19.197	2734	2739	2747	rVV	126237	176879	18.56%	2.212%
87	19.256	2747	2749	2753	rVB5	3185	3099	0.33%	0.039%
88	19.292	2753	2755	2758	rBV4	3911	5736	0.60%	0.072%
89	19.527	2790	2795	2798	rBV	216125	316605	33.22%	3.959%
90	19.556	2798	2800	2810	rVB	101020	131999	13.85%	1.651%
91	19.633	2810	2813	2818	rBV5	8480	12727	1.34%	0.159%
92	19.739	2827	2831	2836	rBV2	7383	15008	1.57%	0.188%
93	19.892	2852	2857	2861	rBV4	7591	15168	1.59%	0.190%
94	20.050	2881	2884	2889	rVB	22203	30077	3.16%	0.376%
95	20.156	2898	2902	2905	rBV	21959	26174	2.75%	0.327%
96	20.521	2960	2964	2971	rBV	286837	313275	32.87%	3.917%
97	21.309	3092	3098	3102	rBV	628651	901602	94.60%	11.274%
98	21.344	3102	3104	3113	rVB	66744	95030	9.97%	1.188%
99	23.421	3452	3457	3463	rBV	141632	306094	32.12%	3.828%
100	23.562	3475	3481	3496	rVB2	487493	953076	100.00%	11.918%



Sum of corrected areas: 7996994

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030747.D
Acq On : 01 Jul 2021 17:27
Operator : CG/JU
Sample : M2825-07
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

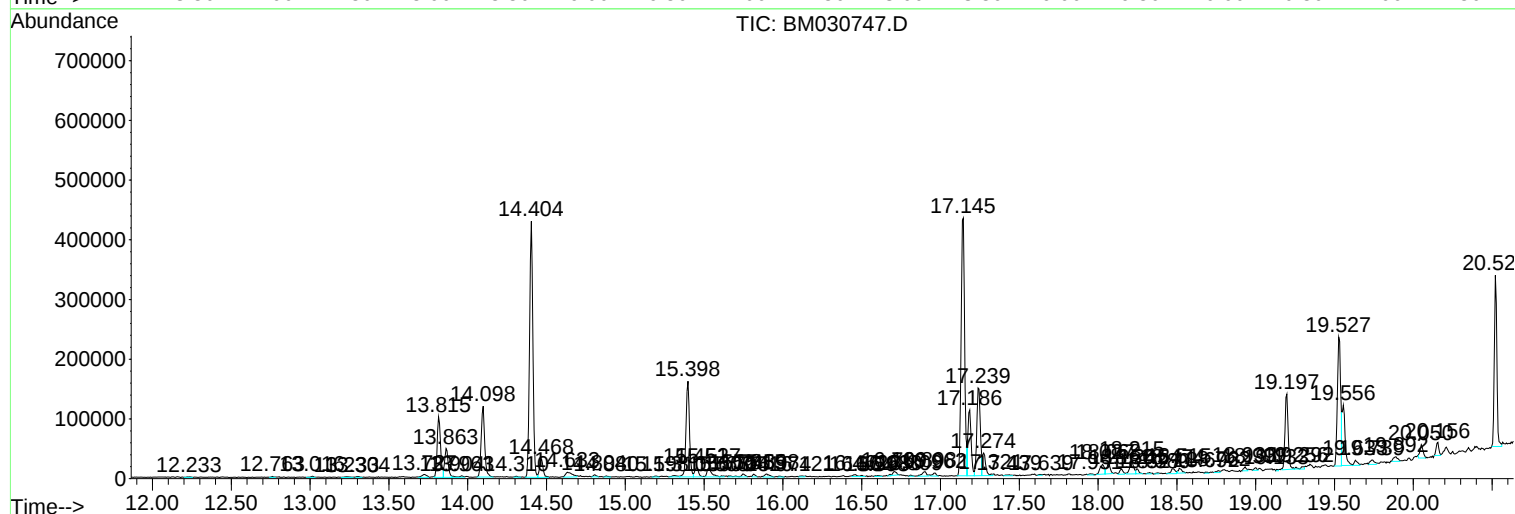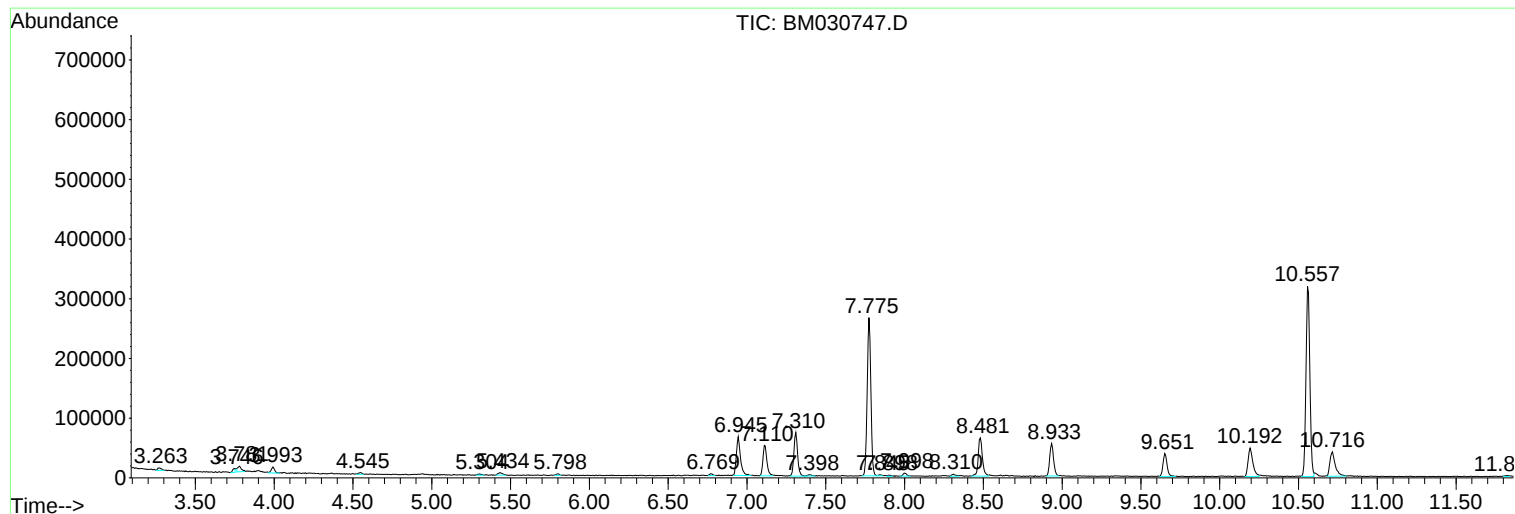

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030747.D
Acq On : 01 Jul 2021 17:27
Operator : CG/JU
Sample : M2825-07
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	6.95 ng/ul	313275	Chrysene-d12	21.309

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
4			Diisooctyl adipate	370	C22H42O4	001330-86-5	80
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	64

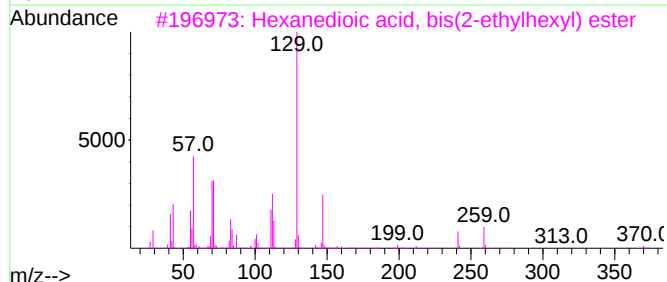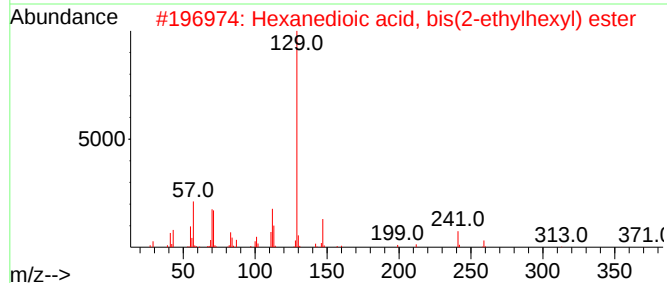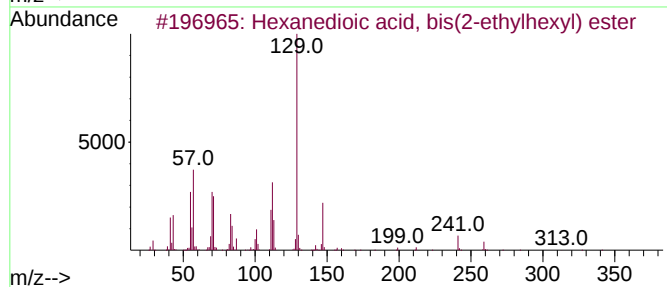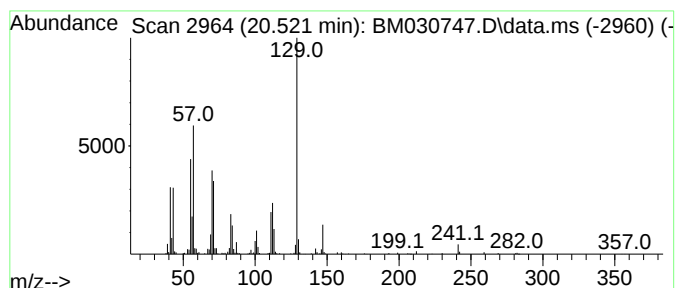

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030747.D
Acq On : 01 Jul 2021 17:27
Operator : CG/JU
Sample : M2825-07
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	7.0	ng/ul	313275	5	21.309	901602	20.0