

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030748.D
 Acq On : 01 Jul 2021 18:04
 Operator : CG/JU
 Sample : M2825-19
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030748.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	99	101	105	rBV5	2026	1539	0.16%	0.025%
2	3.781	115	118	123	rBV6	2459	3416	0.34%	0.056%
3	3.993	150	154	158	rVB	9564	12112	1.22%	0.198%
4	4.363	215	217	220	rBV4	1809	1743	0.18%	0.029%
5	4.546	244	248	251	rVB4	2627	3838	0.39%	0.063%
6	4.699	271	274	275	rBV3	1090	1298	0.13%	0.021%
7	4.758	281	284	285	rBV2	1359	1270	0.13%	0.021%
8	4.911	308	310	312	rVB3	1216	1139	0.11%	0.019%
9	5.058	331	335	337	rVB5	1212	1581	0.16%	0.026%
10	5.299	373	376	380	rBV4	2835	3536	0.36%	0.058%
11	5.428	394	398	406	rBV3	6352	13673	1.38%	0.224%
12	5.799	456	461	465	rVV5	3008	4693	0.47%	0.077%
13	6.234	533	535	539	rVV3	1018	1286	0.13%	0.021%
14	6.616	597	600	602	rBV3	1081	1015	0.10%	0.017%
15	6.775	624	627	630	rBV5	998	1140	0.11%	0.019%
16	6.946	649	656	666	rBV	26421	51197	5.16%	0.838%
17	7.052	671	674	677	rBV3	1138	1007	0.10%	0.016%
18	7.116	679	685	693	rBV	22500	40980	4.13%	0.670%
19	7.310	712	718	727	rBV	30431	51629	5.21%	0.845%
20	7.393	727	732	733	rBV5	1478	1767	0.18%	0.029%
21	7.652	773	776	778	rVB3	1160	1398	0.14%	0.023%
22	7.675	778	780	783	rBV3	884	1200	0.12%	0.020%
23	7.716	783	787	788	rBV2	922	1076	0.11%	0.018%
24	7.775	790	797	807	rBV	284865	445611	44.93%	7.290%
25	7.993	831	834	839	rBV5	1610	2530	0.26%	0.041%
26	8.128	855	857	859	rBV2	1050	1085	0.11%	0.018%
27	8.316	886	889	892	rVB4	1247	1572	0.16%	0.026%
28	8.451	908	912	913	rBV3	1079	1672	0.17%	0.027%
29	8.481	913	917	928	rVB2	24837	47552	4.79%	0.778%
30	8.934	989	994	1004	rVV	22151	42189	4.25%	0.690%
31	9.651	1111	1116	1128	rBV3	13561	26753	2.70%	0.438%
32	9.963	1167	1169	1173	rBV2	750	1030	0.10%	0.017%
33	10.210	1203	1211	1220	rBV3	14424	36059	3.64%	0.590%
34	10.563	1260	1271	1281	rBV	325285	565891	57.06%	9.257%
35	10.728	1291	1299	1310	rBV2	13404	38327	3.86%	0.627%
36	11.116	1360	1365	1368	rVB4	1170	1856	0.19%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030748.D
 Acq On : 01 Jul 2021 18:04
 Operator : CG/JU
 Sample : M2825-19
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	11.798	1477	1481	1483	rBV4	1036	1545	0.16%	0.025%
38	11.816	1483	1484	1492	rVB5	1839	3342	0.34%	0.055%
39	12.057	1520	1525	1530	rBV4	891	1816	0.18%	0.030%
40	12.334	1567	1572	1573	rBV3	973	1001	0.10%	0.016%

41	12.775	1643	1647	1649	rVB4	793	1048	0.11%	0.017%
42	13.822	1818	1825	1834	rBV	39918	68619	6.92%	1.123%
43	14.098	1866	1872	1883	rBV	50043	79349	8.00%	1.298%
44	14.404	1918	1924	1935	rBV	441610	651200	65.66%	10.653%
45	14.575	1951	1953	1956	rBV2	1192	1229	0.12%	0.020%

46	14.663	1964	1968	1969	rBV3	2214	3077	0.31%	0.050%
47	14.692	1972	1973	1977	rVB4	1432	1323	0.13%	0.022%
48	14.775	1985	1987	1990	rVB4	1014	1075	0.11%	0.018%
49	15.104	2042	2043	2048	rBV3	802	1088	0.11%	0.018%
50	15.204	2058	2060	2063	rVB4	1157	1192	0.12%	0.019%

51	15.239	2063	2066	2068	rBV3	1111	1312	0.13%	0.021%
52	15.316	2074	2079	2083	rBV4	2323	3921	0.40%	0.064%
53	15.363	2083	2087	2088	rVV4	1794	2431	0.25%	0.040%
54	15.398	2088	2093	2101	rVV	66075	105524	10.64%	1.726%
55	15.539	2113	2117	2124	rVB5	3455	5974	0.60%	0.098%

56	15.639	2131	2134	2137	rBV5	859	1231	0.12%	0.020%
57	15.816	2158	2164	2169	rBV5	4170	6684	0.67%	0.109%
58	15.927	2181	2183	2185	rBV3	1341	1049	0.11%	0.017%
59	16.251	2234	2238	2239	rBV3	960	1123	0.11%	0.018%
60	16.269	2239	2241	2244	rVV5	932	1048	0.11%	0.017%

61	16.498	2276	2280	2283	rBV3	874	1091	0.11%	0.018%
62	16.651	2305	2306	2311	rBV2	1312	1715	0.17%	0.028%
63	16.710	2311	2316	2323	rVV4	5326	11816	1.19%	0.193%
64	16.910	2347	2350	2351	rBV2	1287	1375	0.14%	0.022%
65	17.021	2366	2369	2371	rVV3	955	1144	0.12%	0.019%

66	17.063	2374	2376	2379	rVV4	977	1100	0.11%	0.018%
67	17.145	2383	2390	2400	rVV	460269	702276	70.81%	11.488%
68	17.245	2401	2407	2417	rVV2	66708	107256	10.81%	1.755%
69	17.592	2465	2466	2469	rBV3	1187	1038	0.10%	0.017%
70	17.639	2472	2474	2478	rBV4	2039	2349	0.24%	0.038%

71	17.810	2500	2503	2504	rBV3	1459	1234	0.12%	0.020%
72	18.004	2532	2536	2538	rBV4	1145	1679	0.17%	0.027%
73	18.039	2538	2542	2546	rVV7	4613	7741	0.78%	0.127%
74	18.110	2551	2554	2557	rVV4	1125	1598	0.16%	0.026%
75	18.168	2562	2564	2568	rBV3	912	1229	0.12%	0.020%

76	18.327	2587	2591	2597	rBV7	2258	5321	0.54%	0.087%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030748.D
 Acq On : 01 Jul 2021 18:04
 Operator : CG/JU
 Sample : M2825-19
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDR7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	18.380	2597	2600	2602	rVV3	1609	1703	0.17%	0.028%
78	18.474	2610	2616	2624	rBV	27145	51589	5.20%	0.844%
79	18.674	2649	2650	2652	rBV2	1665	1167	0.12%	0.019%
80	18.963	2697	2699	2701	rBV3	2093	1842	0.19%	0.030%
81	19.245	2745	2747	2749	rBV2	2390	2259	0.23%	0.037%
82	19.533	2790	2796	2805	rBV	103307	156912	15.82%	2.567%
83	20.521	2960	2964	2969	rBV	592655	615670	62.08%	10.072%
84	21.309	3093	3098	3107	rBV	684429	876809	88.41%	14.344%
85	23.421	3453	3457	3465	rVB2	97337	200356	20.20%	3.278%
86	23.562	3474	3481	3493	rVB2	498573	991794	100.00%	16.225%




Sum of corrected areas: 6112924

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030748.D
Acq On : 01 Jul 2021 18:04
Operator : CG/JU
Sample : M2825-19
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

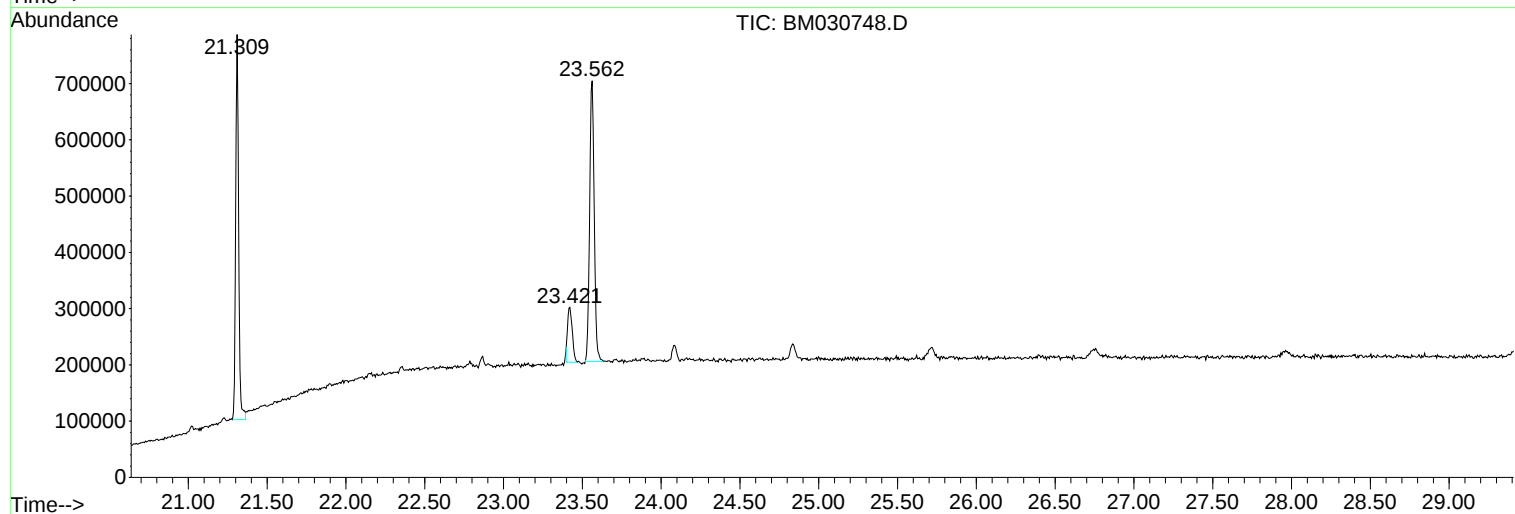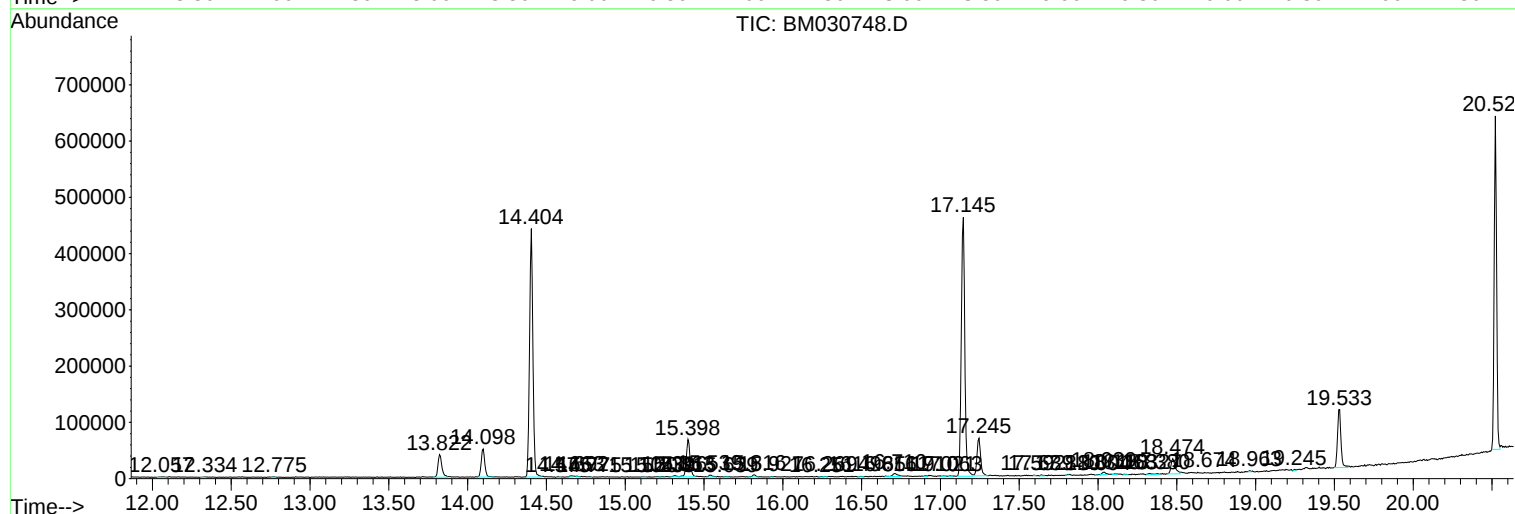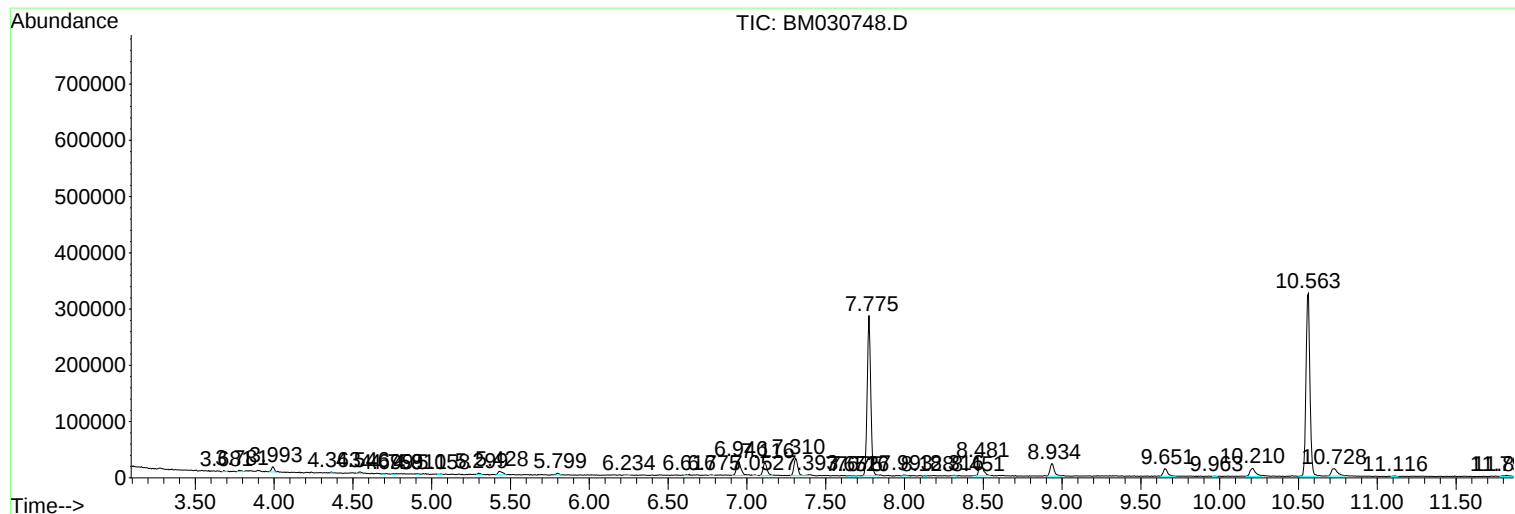

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030748.D
Acq On : 01 Jul 2021 18:04
Operator : CG/JU
Sample : M2825-19
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR7










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	14.04 ng/ul	615670	Chrysene-d12	21.309

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
3			Diisooctyl adipate	370	C22H42O4	001330-86-5	87
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	86

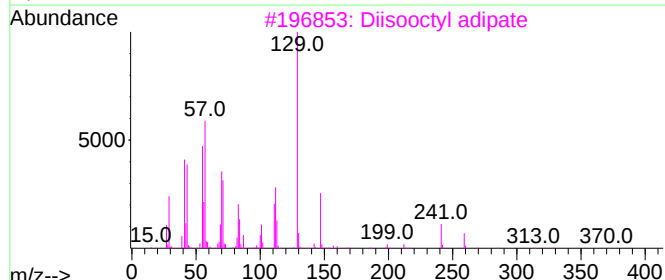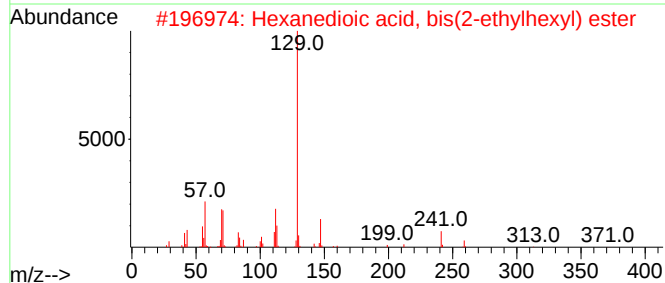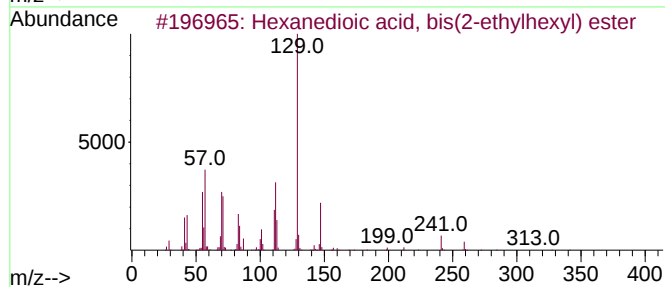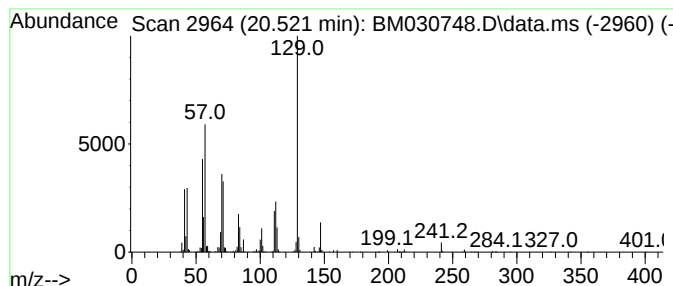

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030748.D
Acq On : 01 Jul 2021 18:04
Operator : CG/JU
Sample : M2825-19
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDR7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	14.0	ng/ul	615670	5	21.309	876809	20.0