

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030749.D
 Acq On : 01 Jul 2021 18:41
 Operator : CG/JU
 Sample : M2825-10
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030749.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.757	110	114	115	rBV3	5719	7296	0.67%	0.085%
2	3.993	150	154	157	rBV2	11440	14897	1.37%	0.173%
3	4.240	195	196	201	rBV4	1559	2454	0.23%	0.029%
4	4.363	216	217	222	rVB4	2028	1836	0.17%	0.021%
5	4.546	244	248	253	rVB4	2713	4226	0.39%	0.049%
6	4.940	313	315	320	rVB5	2440	3261	0.30%	0.038%
7	4.981	320	322	324	rBV2	1018	1149	0.11%	0.013%
8	5.304	375	377	380	rVB4	1960	1493	0.14%	0.017%
9	5.428	393	398	406	rBV4	4574	11136	1.02%	0.129%
10	5.804	456	462	465	rBV4	3607	5987	0.55%	0.070%
11	6.769	623	626	631	rVB5	2637	3246	0.30%	0.038%
12	6.898	646	648	650	rVV3	1170	1257	0.12%	0.015%
13	6.945	650	656	670	rVB	55298	105430	9.67%	1.225%
14	7.110	678	684	696	rBV	46511	81441	7.47%	0.946%
15	7.310	711	718	729	rBV	61954	104852	9.62%	1.218%
16	7.393	729	732	738	rVV5	2703	4295	0.39%	0.050%
17	7.581	760	764	767	rVB5	813	1213	0.11%	0.014%
18	7.775	789	797	805	rBV	353777	563356	51.69%	6.545%
19	7.845	805	809	815	rVV6	3874	7039	0.65%	0.082%
20	7.904	815	819	823	rVB6	1554	2971	0.27%	0.035%
21	8.004	830	836	841	rVB5	3409	6874	0.63%	0.080%
22	8.304	884	887	893	rVB3	2633	3861	0.35%	0.045%
23	8.439	905	910	911	rBV3	2403	2525	0.23%	0.029%
24	8.481	911	917	927	rVV	63242	111658	10.25%	1.297%
25	8.557	928	930	933	rVB3	1351	1531	0.14%	0.018%
26	8.610	937	939	942	rVB3	1208	1381	0.13%	0.016%
27	8.763	961	965	968	rBV4	887	1488	0.14%	0.017%
28	8.887	981	986	987	rBV3	1169	1270	0.12%	0.015%
29	8.934	987	994	1003	rVV	51880	91116	8.36%	1.059%
30	9.157	1029	1032	1034	rVB4	1183	1238	0.11%	0.014%
31	9.339	1060	1063	1066	rBV3	1078	1154	0.11%	0.013%
32	9.651	1111	1116	1125	rVV2	34460	61372	5.63%	0.713%
33	10.086	1187	1190	1193	rBV4	1316	1724	0.16%	0.020%
34	10.192	1201	1208	1224	rBV	44124	97854	8.98%	1.137%
35	10.510	1256	1262	1263	rBV3	792	1297	0.12%	0.015%
36	10.557	1263	1270	1283	rVV	450326	779747	71.55%	9.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030749.D
 Acq On : 01 Jul 2021 18:41
 Operator : CG/JU
 Sample : M2825-10
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	10.710	1290	1296	1311	rBV	42544	100178	9.19%	1.164%
38	10.881	1322	1325	1330	rVV6	976	1745	0.16%	0.020%
39	10.945	1334	1336	1339	rVB2	947	1237	0.11%	0.014%
40	11.822	1478	1485	1490	rBV5	1488	3392	0.31%	0.039%
41	12.157	1540	1542	1548	rVB5	1001	1676	0.15%	0.019%
42	12.757	1641	1644	1646	rBV3	1219	1564	0.14%	0.018%
43	13.016	1685	1688	1694	rVB4	1899	3251	0.30%	0.038%
44	13.069	1694	1697	1701	rBV6	947	1509	0.14%	0.018%
45	13.233	1721	1725	1730	rVB5	1705	2887	0.26%	0.034%
46	13.304	1733	1737	1741	rVV3	1367	2008	0.18%	0.023%
47	13.816	1818	1824	1829	rBV	109829	167390	15.36%	1.945%
48	13.863	1829	1832	1841	rVB	49780	72682	6.67%	0.844%
49	14.098	1864	1872	1883	rBV	122230	190963	17.52%	2.218%
50	14.310	1904	1908	1910	rVB3	1703	2143	0.20%	0.025%
51	14.404	1917	1924	1932	rBV	676543	974721	89.44%	11.323%
52	14.469	1932	1935	1939	rVB2	5326	7512	0.69%	0.087%
53	14.639	1959	1964	1975	rBV6	6830	20315	1.86%	0.236%
54	14.804	1987	1992	1993	rBV4	2133	2045	0.19%	0.024%
55	14.986	2017	2023	2026	rBV6	1101	1582	0.15%	0.018%
56	15.316	2073	2079	2083	rBV5	2782	4779	0.44%	0.056%
57	15.398	2087	2093	2099	rVV	164669	252107	23.13%	2.929%
58	15.445	2099	2101	2109	rVB3	5472	10394	0.95%	0.121%
59	15.527	2112	2115	2126	rVB3	11923	21541	1.98%	0.250%
60	15.751	2150	2153	2159	rVV5	1942	3152	0.29%	0.037%
61	15.815	2161	2164	2169	rVB4	4849	6555	0.60%	0.076%
62	15.904	2174	2179	2181	rBV6	2133	3699	0.34%	0.043%
63	15.986	2190	2193	2197	rVB4	1283	1351	0.12%	0.016%
64	16.057	2202	2205	2207	rVB4	1282	1352	0.12%	0.016%
65	16.339	2250	2253	2255	rVB3	1084	1152	0.11%	0.013%
66	16.380	2255	2260	2264	rBV5	1749	3707	0.34%	0.043%
67	16.433	2266	2269	2270	rBV2	1534	1731	0.16%	0.020%
68	16.445	2270	2271	2277	rBV5	1391	2187	0.20%	0.025%
69	16.710	2306	2316	2322	rBV4	4991	13566	1.24%	0.158%
70	16.874	2340	2344	2346	rBV5	2074	2938	0.27%	0.034%
71	16.933	2352	2354	2356	rVV	1814	1209	0.11%	0.014%
72	16.957	2356	2358	2364	rVB4	2687	3777	0.35%	0.044%
73	17.068	2374	2377	2379	rBV3	1012	1540	0.14%	0.018%
74	17.145	2384	2390	2394	rVV	706593	1020716	93.66%	11.858%
75	17.180	2394	2396	2401	rVV	56630	78739	7.22%	0.915%
76	17.239	2401	2406	2417	rVB	158825	263629	24.19%	3.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030749.D
 Acq On : 01 Jul 2021 18:41
 Operator : CG/JU
 Sample : M2825-10
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	17.345	2422	2424	2427	rVB3	1784	1606	0.15%	0.019%
78	17.439	2437	2440	2442	rVB3	1244	1656	0.15%	0.019%
79	17.551	2456	2459	2462	rBV5	2147	2985	0.27%	0.035%
80	17.639	2471	2474	2475	rBV2	1896	1923	0.18%	0.022%
81	17.815	2500	2504	2508	rBV6	2127	2690	0.25%	0.031%
82	17.951	2525	2527	2530	rBV4	2146	1622	0.15%	0.019%
83	18.033	2533	2541	2544	rBV5	12283	25957	2.38%	0.302%
84	18.068	2544	2547	2552	rVB2	8317	11822	1.08%	0.137%
85	18.151	2557	2561	2565	rBV3	5036	7484	0.69%	0.087%
86	18.215	2567	2572	2576	rBV2	12538	20937	1.92%	0.243%
87	18.309	2587	2588	2590	rBV2	1299	1325	0.12%	0.015%
88	18.480	2611	2617	2620	rBV2	7545	14067	1.29%	0.163%
89	18.515	2621	2623	2630	rVB5	6189	10160	0.93%	0.118%
90	18.762	2663	2665	2668	rBV4	1958	1569	0.14%	0.018%
91	18.798	2668	2671	2676	rVV5	3669	6679	0.61%	0.078%
92	18.933	2690	2694	2697	rBV6	4762	8190	0.75%	0.095%
93	19.068	2715	2717	2719	rBV3	2325	2630	0.24%	0.031%
94	19.198	2734	2739	2745	rVB	90198	126104	11.57%	1.465%
95	19.527	2790	2795	2799	rBV2	200898	310932	28.53%	3.612%
96	20.156	2899	2902	2905	rVB	13927	16001	1.47%	0.186%
97	20.521	2960	2964	2969	rBV	229461	256652	23.55%	2.982%
98	21.309	3092	3098	3102	rBV	764636	1018410	93.45%	11.831%
99	23.415	3452	3456	3471	rVB3	127315	313233	28.74%	3.639%
100	23.556	3474	3480	3496	rVB2	552592	1089818	100.00%	12.661%




Sum of corrected areas: 8607998

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030749.D
Acq On : 01 Jul 2021 18:41
Operator : CG/JU
Sample : M2825-10
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

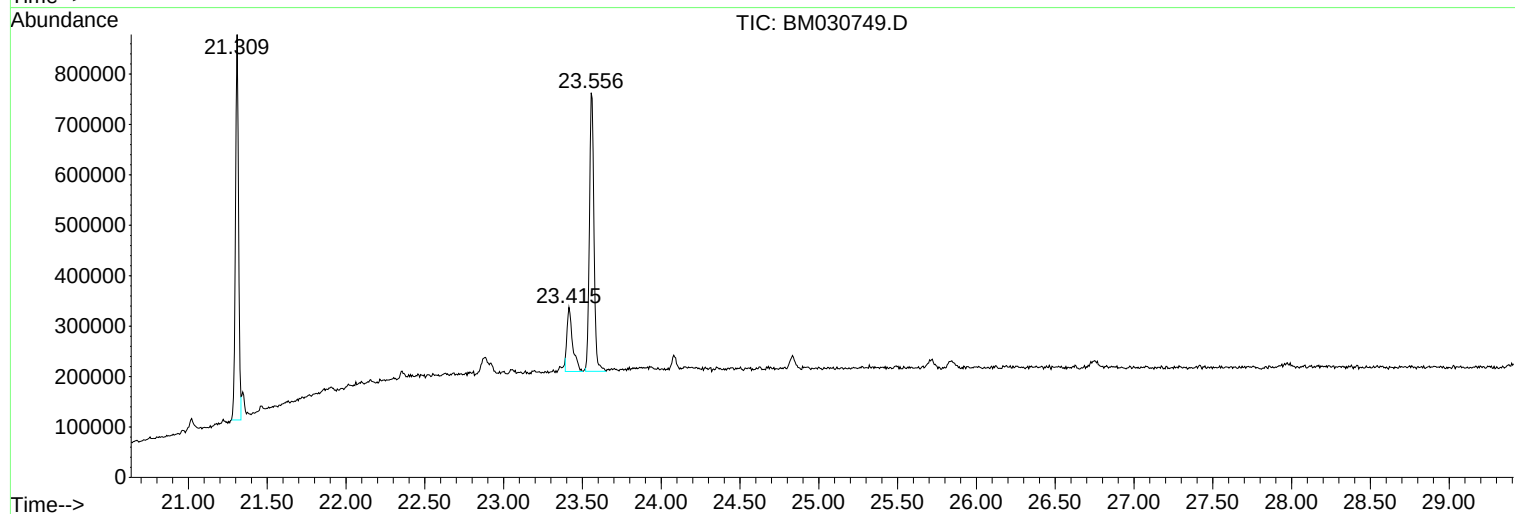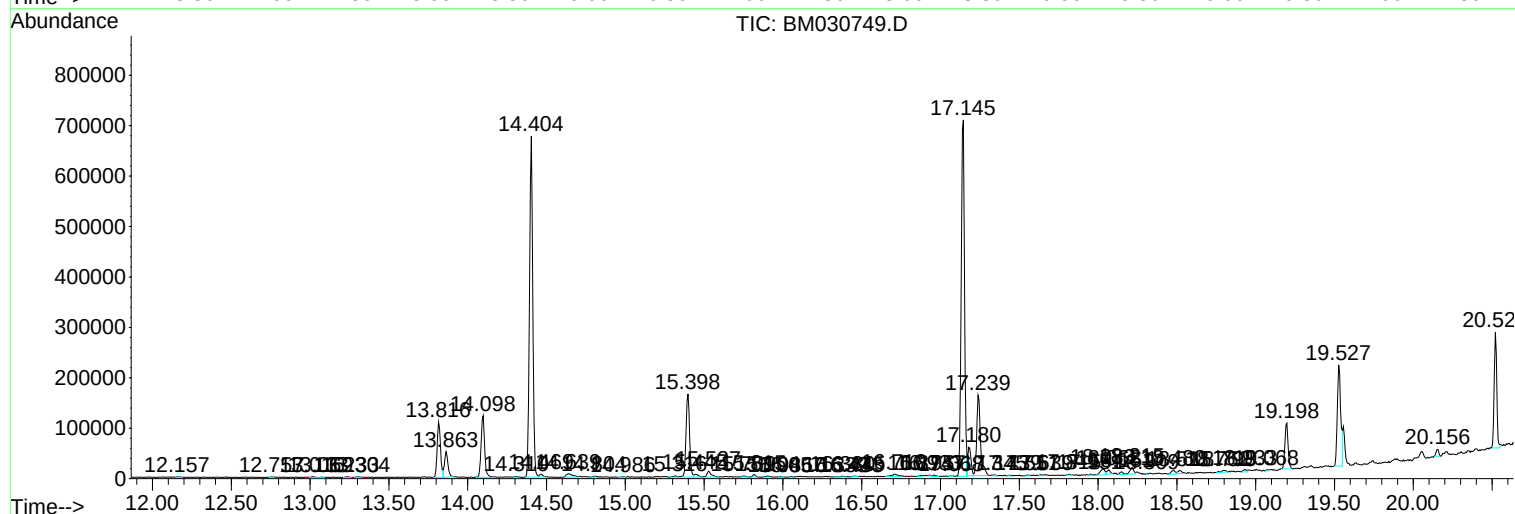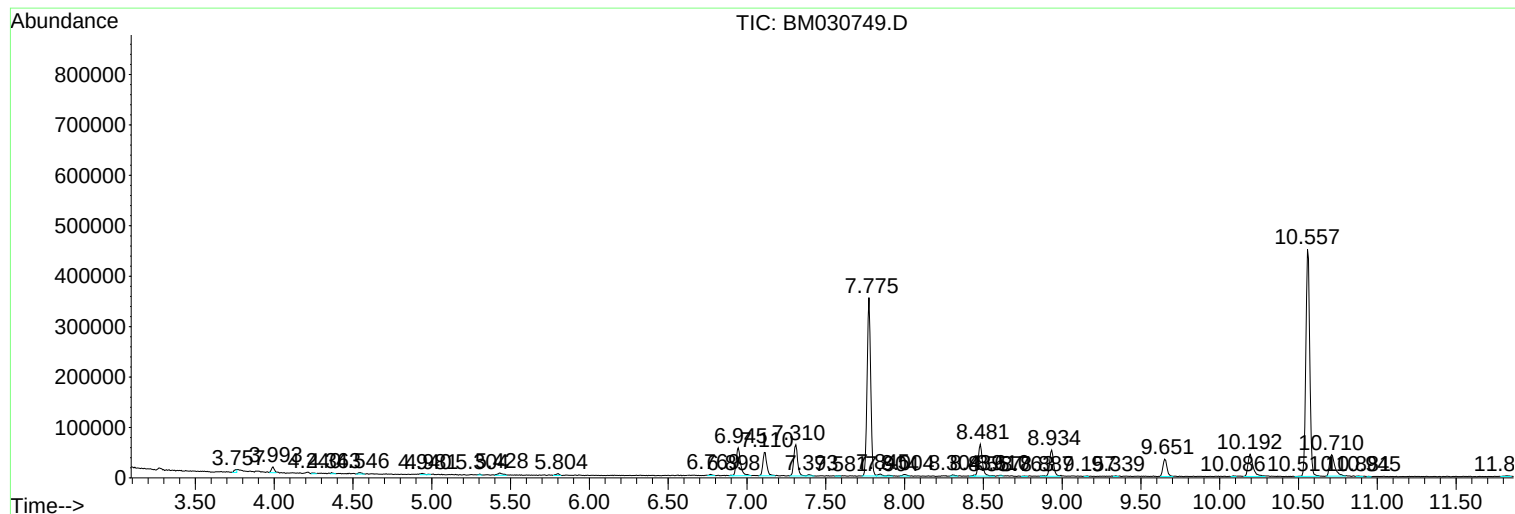

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030749.D
Acq On : 01 Jul 2021 18:41
Operator : CG/JU
Sample : M2825-10
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	5.04 ng/ul	256652	Chrysene-d12	21.309

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	86
2			Diisooctyl adipate	370	C22H42O4	001330-86-5	78
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	78
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	74
5			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	70

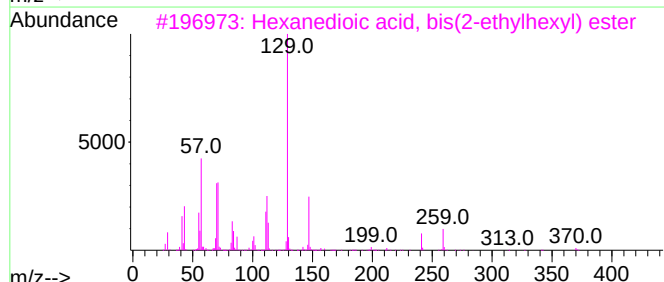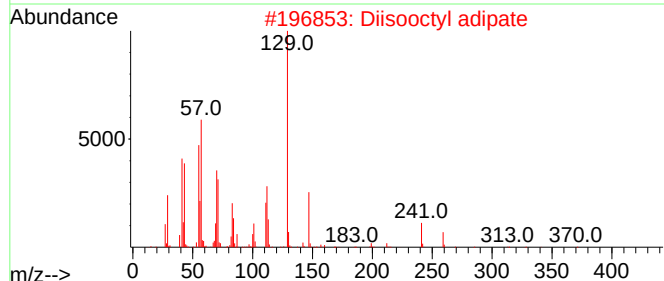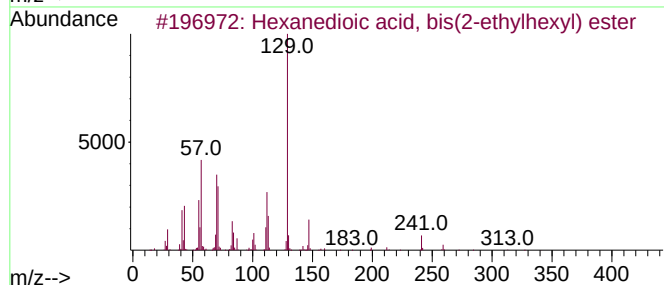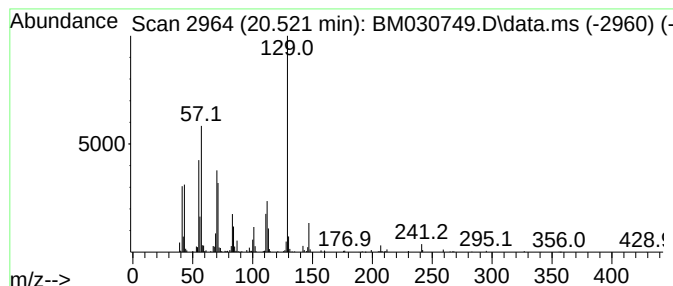

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030749.D
Acq On : 01 Jul 2021 18:41
Operator : CG/JU
Sample : M2825-10
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDP4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	5.0	ng/ul	256652	5	21.309	1018410	20.0