

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030751.D
 Acq On : 01 Jul 2021 19:55
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030751.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	29	31	36	rVB5	4372	4765	0.48%	0.061%
2	3.346	43	44	46	rBV2	2042	1012	0.10%	0.013%
3	3.775	111	117	122	rBV5	8496	17565	1.76%	0.226%
4	3.993	150	154	160	rVB	12580	18568	1.86%	0.239%
5	4.040	160	162	165	rBV4	1697	1738	0.17%	0.022%
6	4.099	170	172	174	rVB3	1611	1171	0.12%	0.015%
7	4.546	242	248	254	rVV4	3688	6357	0.64%	0.082%
8	4.610	258	259	262	rBV3	973	1213	0.12%	0.016%
9	4.916	309	311	313	rBV3	1054	1091	0.11%	0.014%
10	4.940	313	315	318	rVV2	1045	1459	0.15%	0.019%
11	5.293	372	375	379	rBV3	1800	2367	0.24%	0.030%
12	5.428	395	398	408	rVB2	6374	12794	1.28%	0.165%
13	5.799	457	461	467	rBV4	3179	4733	0.47%	0.061%
14	6.199	524	529	531	rBV3	717	1068	0.11%	0.014%
15	6.293	544	545	549	rVB4	897	1085	0.11%	0.014%
16	6.334	549	552	556	rBV4	797	1333	0.13%	0.017%
17	6.622	596	601	606	rBV6	1093	2839	0.28%	0.037%
18	6.746	619	622	624	rBV3	835	1044	0.10%	0.013%
19	6.775	624	627	629	rVB4	1223	1572	0.16%	0.020%
20	6.828	632	636	639	rBV4	770	1351	0.14%	0.017%
21	6.946	650	656	665	rBV	60963	107316	10.76%	1.380%
22	7.110	678	684	696	rBV	54943	91322	9.16%	1.174%
23	7.310	712	718	728	rVB	69164	116253	11.66%	1.495%
24	7.393	728	732	736	rBV3	3206	3902	0.39%	0.050%
25	7.545	755	758	762	rVV5	773	1186	0.12%	0.015%
26	7.587	762	765	767	rVB3	803	1029	0.10%	0.013%
27	7.651	773	776	780	rBV3	827	1135	0.11%	0.015%
28	7.775	788	797	806	rBV	303126	486044	48.73%	6.249%
29	7.957	824	828	830	rBV3	1036	1305	0.13%	0.017%
30	8.004	833	836	839	rVB4	1547	2454	0.25%	0.032%
31	8.263	877	880	883	rVB5	863	1038	0.10%	0.013%
32	8.298	883	886	888	rBV2	1793	2229	0.22%	0.029%
33	8.481	906	917	927	rBV	65397	119154	11.95%	1.532%
34	8.598	934	937	938	rBV2	1863	1913	0.19%	0.025%
35	8.834	972	977	980	rVB4	816	1283	0.13%	0.016%
36	8.875	980	984	986	rBV3	1125	1553	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030751.D
 Acq On : 01 Jul 2021 19:55
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	8.934	988	994	1003	rVV	58937	102281	10.26%	1.315%
38	9.357	1063	1066	1069	rVB3	1082	1208	0.12%	0.016%
39	9.651	1108	1116	1126	rBV2	42246	73163	7.34%	0.941%
40	9.934	1159	1164	1168	rVB4	724	1245	0.12%	0.016%

41	10.192	1201	1208	1221	rBV	51220	112369	11.27%	1.445%
42	10.310	1226	1228	1232	rVB5	1346	1310	0.13%	0.017%
43	10.410	1242	1245	1248	rVB4	1138	1442	0.14%	0.019%
44	10.557	1263	1270	1280	rBV	400103	683207	68.50%	8.785%
45	10.710	1290	1296	1311	rVV	46810	114528	11.48%	1.473%

46	10.828	1313	1316	1322	rVB5	1042	1486	0.15%	0.019%
47	11.616	1447	1450	1454	rVB4	902	1480	0.15%	0.019%
48	11.822	1483	1485	1491	rVB5	2025	2695	0.27%	0.035%
49	12.069	1523	1527	1531	rBV5	829	1380	0.14%	0.018%
50	12.157	1540	1542	1544	rBV3	875	1028	0.10%	0.013%

51	12.310	1565	1568	1572	rBV4	536	1011	0.10%	0.013%
52	12.751	1638	1643	1644	rBV4	601	1028	0.10%	0.013%
53	13.233	1724	1725	1729	rVV4	1183	1077	0.11%	0.014%
54	13.304	1732	1737	1742	rVB2	3412	5690	0.57%	0.073%
55	13.475	1763	1766	1768	rVB3	1182	999	0.10%	0.013%

56	13.816	1818	1824	1829	rBV	133247	197398	19.79%	2.538%
57	13.863	1829	1832	1846	rVB	63604	95392	9.56%	1.227%
58	14.098	1864	1872	1882	rBV	141212	221291	22.19%	2.845%
59	14.304	1904	1907	1910	rVB4	1597	1562	0.16%	0.020%
60	14.404	1917	1924	1936	rBV	590242	904693	90.71%	11.632%

61	14.639	1957	1964	1977	rBV4	7095	24629	2.47%	0.317%
62	14.927	2011	2013	2015	rBV2	890	1001	0.10%	0.013%
63	15.257	2066	2069	2073	rVB4	1084	1147	0.12%	0.015%
64	15.304	2073	2077	2079	rBV4	1359	2180	0.22%	0.028%
65	15.398	2082	2093	2102	rBV	203479	301427	30.22%	3.876%

66	15.527	2111	2115	2122	rBV3	11927	21914	2.20%	0.282%
67	15.574	2122	2123	2125	rVV	1623	1126	0.11%	0.014%
68	15.627	2129	2132	2139	rBV6	1587	2677	0.27%	0.034%
69	15.733	2149	2150	2152	rBV2	1442	1017	0.10%	0.013%
70	15.816	2160	2164	2168	rBV3	6585	8871	0.89%	0.114%

71	16.121	2214	2216	2220	rVB4	1157	1192	0.12%	0.015%
72	16.345	2252	2254	2258	rVV4	1003	1101	0.11%	0.014%
73	16.386	2258	2261	2264	rVB4	1662	1599	0.16%	0.021%
74	16.527	2281	2285	2290	rVB6	800	1548	0.16%	0.020%
75	16.704	2308	2315	2323	rBV5	3765	9421	0.94%	0.121%

76	16.886	2343	2346	2348	rBV3	1028	1188	0.12%	0.015%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030751.D
 Acq On : 01 Jul 2021 19:55
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	16.910	2348	2350	2351	rVV2	1687	1445	0.14%	0.019%
78	16.927	2351	2353	2361	rVB5	2230	4116	0.41%	0.053%
79	17.010	2364	2367	2371	rBV4	1197	1919	0.19%	0.025%
80	17.139	2383	2389	2401	rBV	658934	997339	100.00%	12.824%
81	17.239	2401	2406	2418	rVV2	190628	298815	29.96%	3.842%
82	17.345	2420	2424	2427	rVV4	1872	2140	0.21%	0.028%
83	17.433	2435	2439	2445	rVB3	2258	3425	0.34%	0.044%
84	17.639	2471	2474	2477	rVB5	1542	1690	0.17%	0.022%
85	17.810	2501	2503	2505	rBV3	1411	1180	0.12%	0.015%
86	17.921	2520	2522	2524	rBV2	1556	1544	0.15%	0.020%
87	18.033	2535	2541	2545	rBV7	7901	15897	1.59%	0.204%
88	18.110	2552	2554	2556	rVB3	2308	1924	0.19%	0.025%
89	18.145	2558	2560	2562	rBV3	1700	1282	0.13%	0.016%
90	18.215	2568	2572	2574	rBV5	3076	5324	0.53%	0.068%
91	18.486	2617	2618	2621	rBV3	1493	1035	0.10%	0.013%
92	18.521	2622	2624	2625	rVV2	1575	1069	0.11%	0.014%
93	18.792	2668	2670	2676	rBV6	2886	4894	0.49%	0.063%
94	18.962	2696	2699	2702	rBV4	7030	6915	0.69%	0.089%
95	19.198	2735	2739	2745	rVB	31623	42578	4.27%	0.547%
96	19.527	2790	2795	2805	rBV2	229566	359349	36.03%	4.620%
97	20.521	2961	2964	2968	rBV	32878	33899	3.40%	0.436%
98	21.309	3093	3098	3103	rBV	656619	861614	86.39%	11.078%
99	23.415	3451	3456	3468	rVB2	141108	321630	32.25%	4.135%
100	23.562	3475	3481	3491	rVB2	450656	871121	87.34%	11.201%




Sum of corrected areas: 7777386

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030751.D
Acq On : 01 Jul 2021 19:55
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

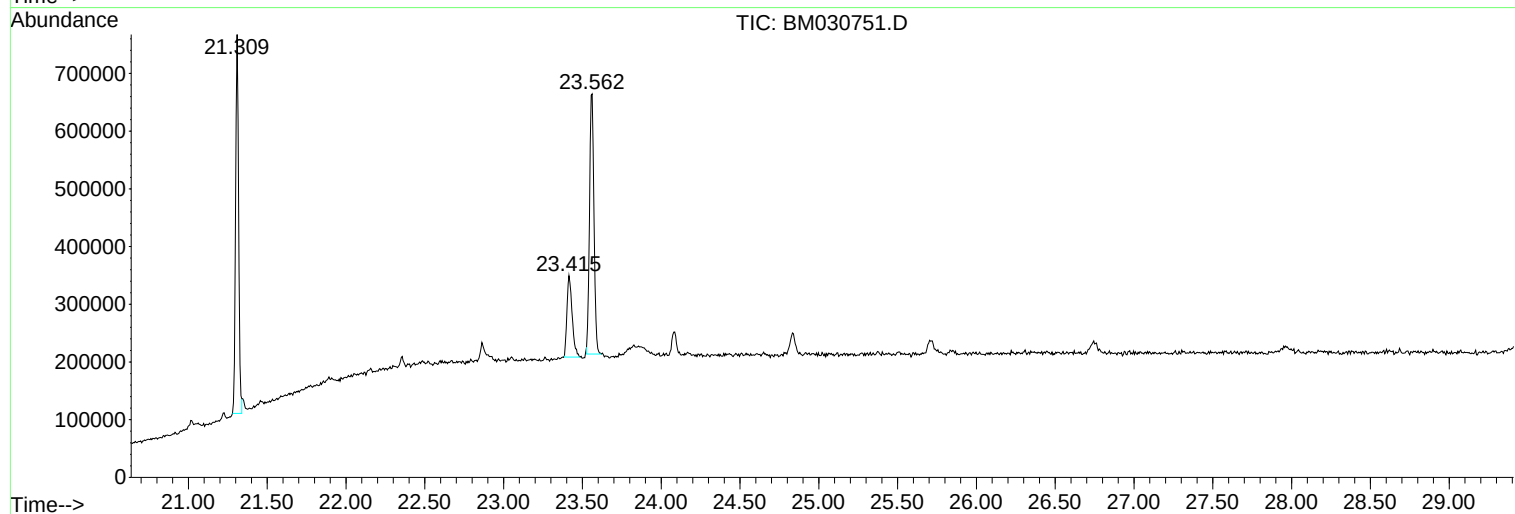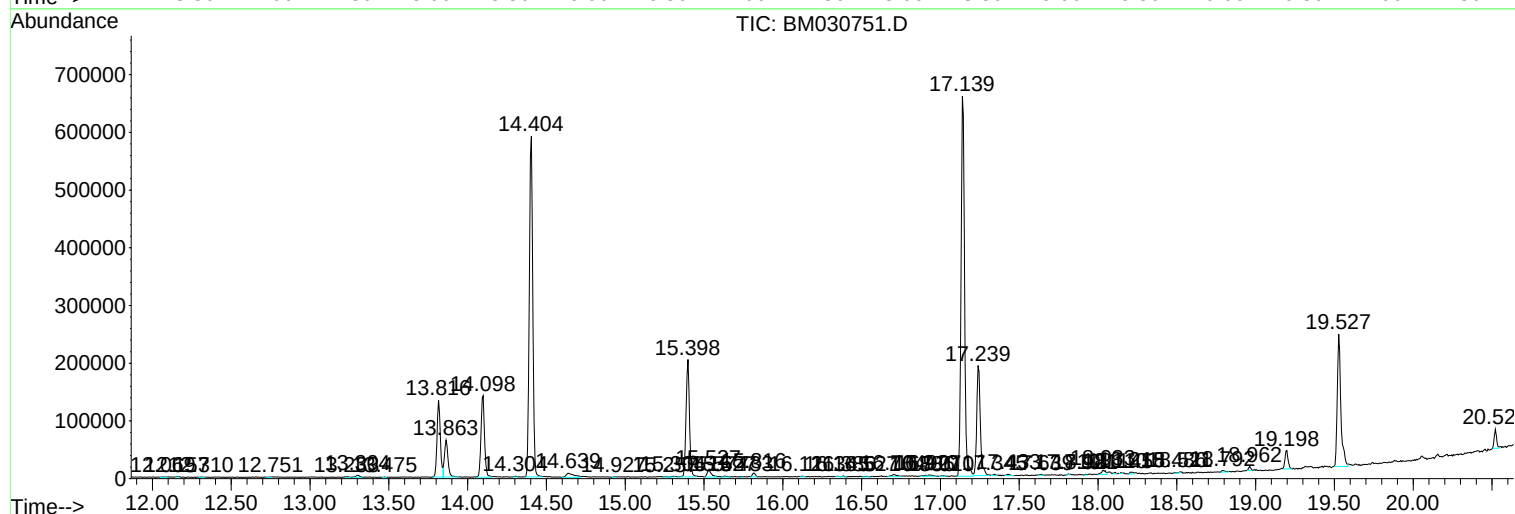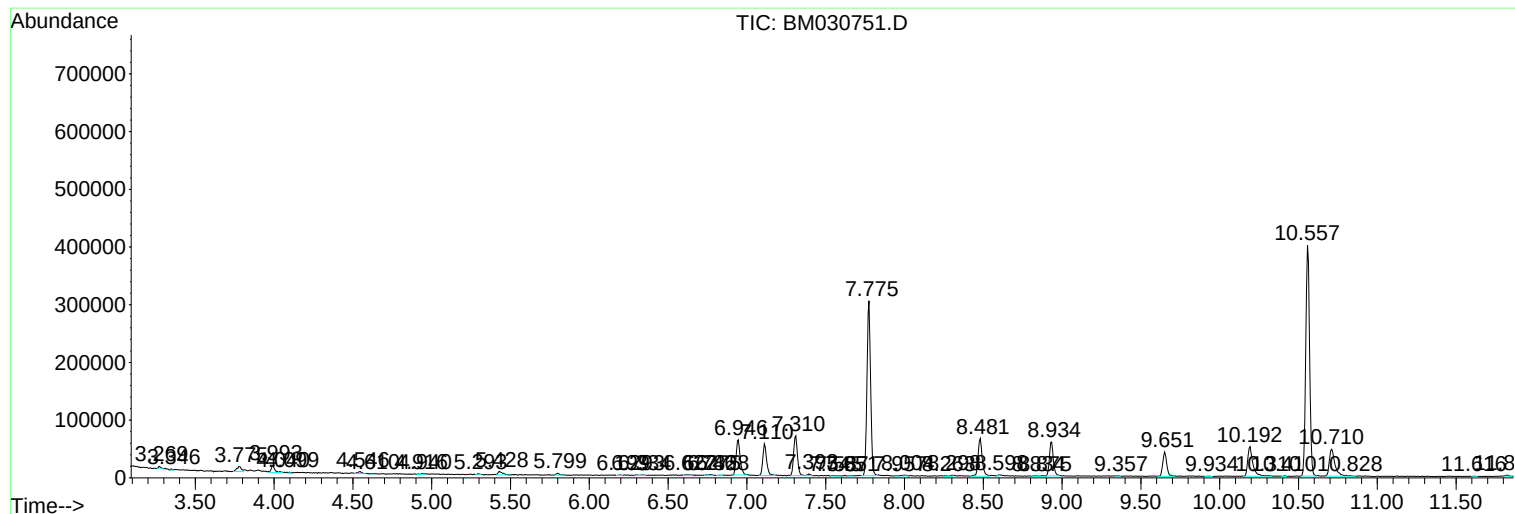

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030751.D
Acq On : 01 Jul 2021 19:55
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030751.D
Acq On : 01 Jul 2021 19:55
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
