

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030755.D
 Acq On : 01 Jul 2021 22:58
 Operator : CG/JU
 Sample : PB137426BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030755.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	39	rVB	38187	54278	1.86%	0.169%
2	3.675	96	100	120	rBV	410252	765623	26.27%	2.380%
3	3.993	150	154	162	rVB	12518	21365	0.73%	0.066%
4	6.940	649	655	668	rBV	628754	997706	34.23%	3.101%
5	7.110	677	684	696	rBV	463036	736480	25.27%	2.289%
6	7.304	710	717	729	rBV	630676	1013107	34.76%	3.149%
7	7.775	786	797	810	rBV	413676	673990	23.12%	2.095%
8	8.475	908	916	934	rBV	730878	1205491	41.36%	3.747%
9	8.928	985	993	1012	rBV	581372	959948	32.93%	2.984%
10	9.645	1108	1115	1128	rBV	478730	792422	27.19%	2.463%
11	10.181	1198	1206	1220	rBV	702080	1226836	42.09%	3.813%
12	10.557	1262	1270	1280	rVB	573479	969971	33.28%	3.015%
13	10.698	1287	1294	1316	rBV	661255	1233659	42.33%	3.835%
14	11.822	1483	1485	1492	rVB3	2777	5222	0.18%	0.016%
15	12.157	1535	1542	1550	rBV	8706	17349	0.60%	0.054%
16	13.816	1817	1824	1837	rBV	1221613	1738817	59.66%	5.405%
17	14.092	1864	1871	1884	rBV	1404305	2152349	73.84%	6.690%
18	14.404	1917	1924	1932	rBV	885943	1300764	44.63%	4.043%
19	14.604	1949	1958	1981	rBV	387082	767186	26.32%	2.385%
20	15.398	2085	2093	2103	rBV	1791167	2648245	90.86%	8.232%
21	15.521	2108	2114	2128	rVV	404740	607973	20.86%	1.890%
22	15.633	2129	2133	2139	rVB	20711	31792	1.09%	0.099%
23	16.180	2222	2226	2230	rVB4	5345	7030	0.24%	0.022%
24	16.933	2345	2354	2358	rBV5	3519	8193	0.28%	0.025%
25	17.139	2383	2389	2398	rBV	1037316	1460339	50.10%	4.539%
26	17.239	2400	2406	2422	rVV	2047696	2808475	96.35%	8.730%
27	18.045	2537	2543	2549	rBV8	2195	5400	0.19%	0.017%
28	19.168	2730	2734	2740	rBV	16570	22916	0.79%	0.071%
29	19.415	2772	2776	2783	rBV2	15432	21117	0.72%	0.066%
30	19.527	2789	2795	2803	rBV	2193255	2914723	100.00%	9.060%
31	21.309	3093	3098	3106	rBV	956363	1234037	42.34%	3.836%
32	23.415	3449	3456	3469	rBV	1302243	2525967	86.66%	7.852%
33	23.562	3474	3481	3492	rVB2	619290	1242809	42.64%	3.863%




Sum of corrected areas: 32171579

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030755.D
Acq On : 01 Jul 2021 22:58
Operator : CG/JU
Sample : PB137426BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

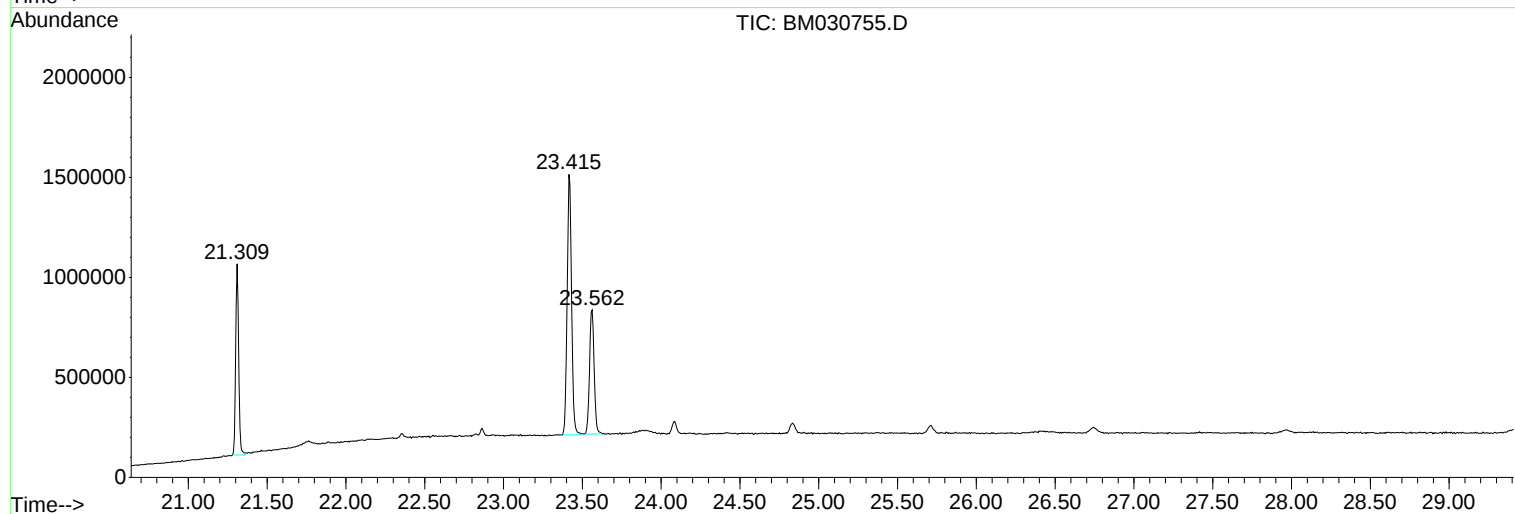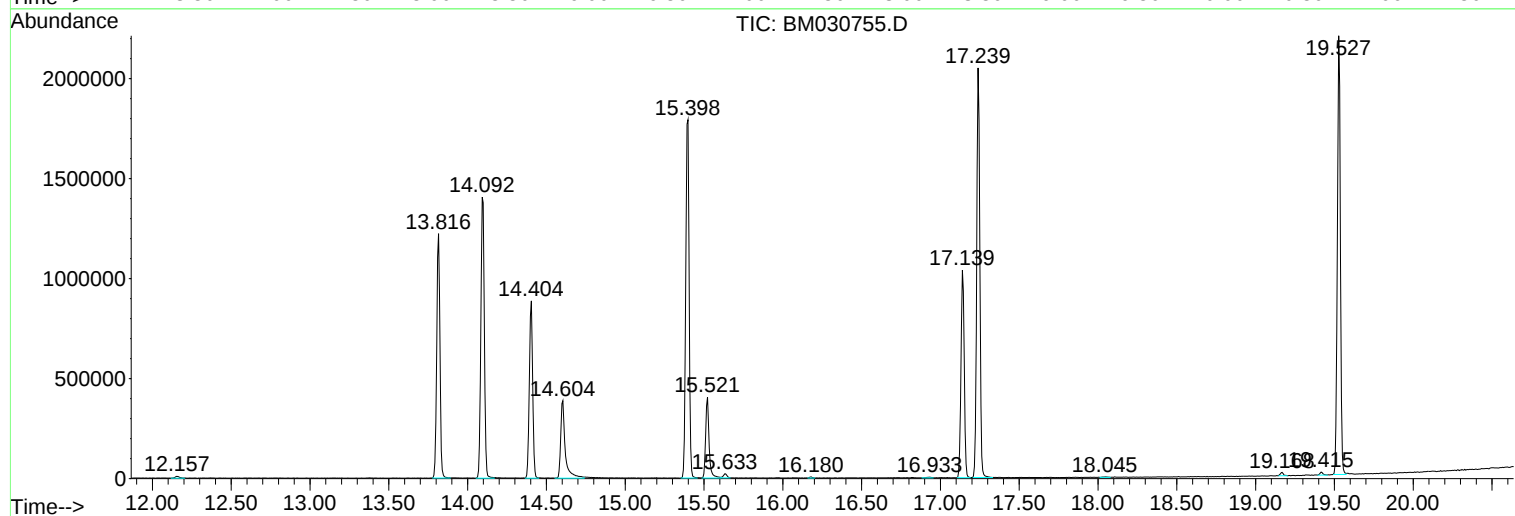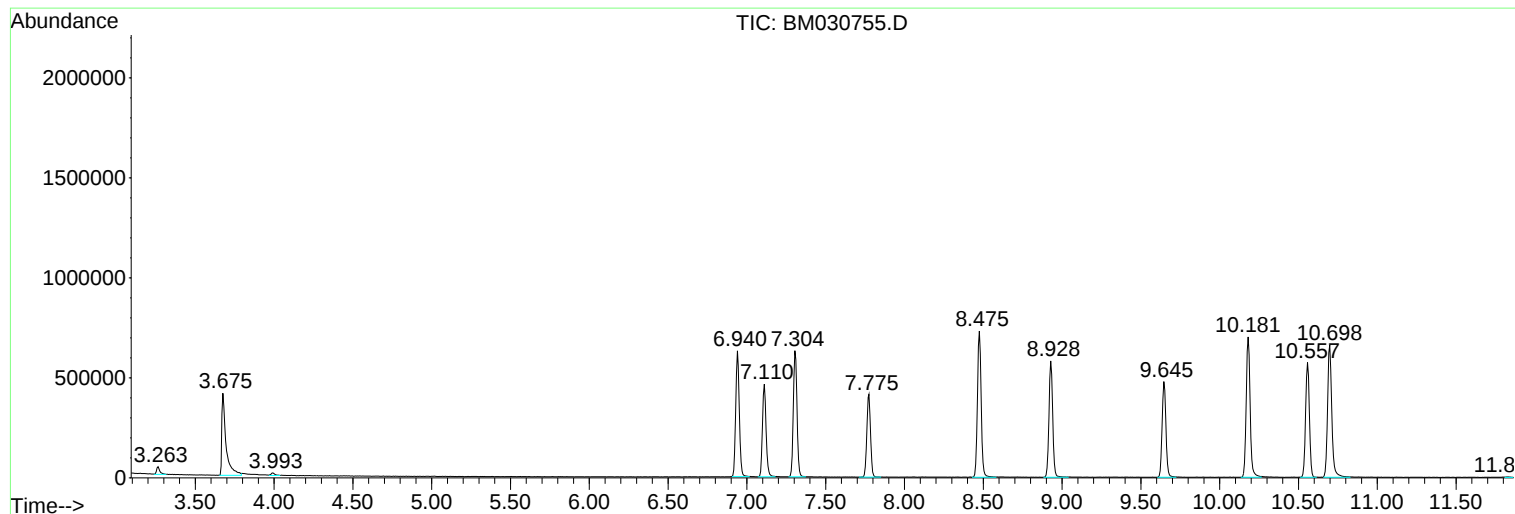

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030755.D
Acq On : 01 Jul 2021 22:58
Operator : CG/JU
Sample : PB137426BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030755.D
Acq On : 01 Jul 2021 22:58
Operator : CG/JU
Sample : PB137426BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
