

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030770.D
 Acq On : 02 Jul 2021 08:41
 Operator : CG/JU
 Sample : PB137472BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK472

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030770.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	40	rVB	33268	47373	2.24%	0.209%
2	3.675	97	100	128	rBV	335293	634069	29.93%	2.803%
3	3.987	151	153	158	rVB	6572	8306	0.39%	0.037%
4	4.404	222	224	228	rVB4	1761	2297	0.11%	0.010%
5	5.004	322	326	331	rBV5	1932	3120	0.15%	0.014%
6	6.940	648	655	668	rBV	498733	802767	37.90%	3.549%
7	7.104	675	683	699	rBV	355628	598232	28.24%	2.645%
8	7.222	701	703	710	rVB7	1437	2283	0.11%	0.010%
9	7.304	710	717	725	rBV	523454	827629	39.07%	3.659%
10	7.769	789	796	805	rVB	328836	521547	24.62%	2.306%
11	8.469	908	915	927	rBV	563948	933669	44.08%	4.128%
12	8.545	927	928	933	rVB4	1895	2161	0.10%	0.010%
13	8.928	985	993	1008	rBV	442160	741754	35.02%	3.279%
14	9.645	1106	1115	1127	rBV	357471	602032	28.42%	2.662%
15	10.181	1198	1206	1226	rBV	510041	924879	43.66%	4.089%
16	10.557	1261	1270	1280	rBV	430064	722460	34.11%	3.194%
17	10.692	1286	1293	1309	rBV	459081	894879	42.25%	3.956%
18	11.816	1482	1484	1492	rVB4	1699	3135	0.15%	0.014%
19	12.157	1537	1542	1550	rVB	6330	11874	0.56%	0.052%
20	13.810	1817	1823	1837	rBV	755456	1122693	53.00%	4.964%
21	14.092	1863	1871	1882	rBV	1002948	1455630	68.72%	6.436%
22	14.398	1917	1923	1931	rBV	578161	852552	40.25%	3.769%
23	14.604	1951	1958	1982	rBV	190358	451844	21.33%	1.998%
24	15.392	2085	2092	2104	rBV	1195898	1706753	80.57%	7.546%
25	15.516	2108	2113	2125	rBV	211455	339382	16.02%	1.500%
26	15.633	2129	2133	2138	rVB2	12307	17213	0.81%	0.076%
27	16.174	2221	2225	2230	rVV3	2694	3942	0.19%	0.017%
28	16.257	2232	2239	2241	rBV7	1125	2686	0.13%	0.012%
29	16.710	2312	2316	2320	rBV5	2368	4817	0.23%	0.021%
30	16.927	2348	2353	2354	rBV5	1978	2518	0.12%	0.011%
31	17.139	2383	2389	2399	rBV	599116	846034	39.94%	3.740%
32	17.239	2399	2406	2420	rBV2	1130216	1669469	78.81%	7.381%
33	18.362	2594	2597	2598	rBV3	2176	2170	0.10%	0.010%
34	19.115	2723	2725	2727	rBV3	2308	2174	0.10%	0.010%
35	19.162	2729	2733	2738	rBV	11373	15509	0.73%	0.069%
36	19.415	2772	2776	2780	rBV	8709	13680	0.65%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030770.D
Acq On : 02 Jul 2021 08:41
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Title : SVOA CALIBRATION

37	19.527	2789	2795	2804	rBV	1337782	1797937	84.88%	7.949%
38	21.309	3093	3098	3105	rBV	679668	891510	42.09%	3.942%
39	23.415	3449	3456	3468	rBV	1109824	2118299	100.00%	9.365%
40	23.556	3474	3480	3490	rVB2	520623	1017116	48.02%	4.497%




Sum of corrected areas: 22618394

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030770.D
Acq On : 02 Jul 2021 08:41
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

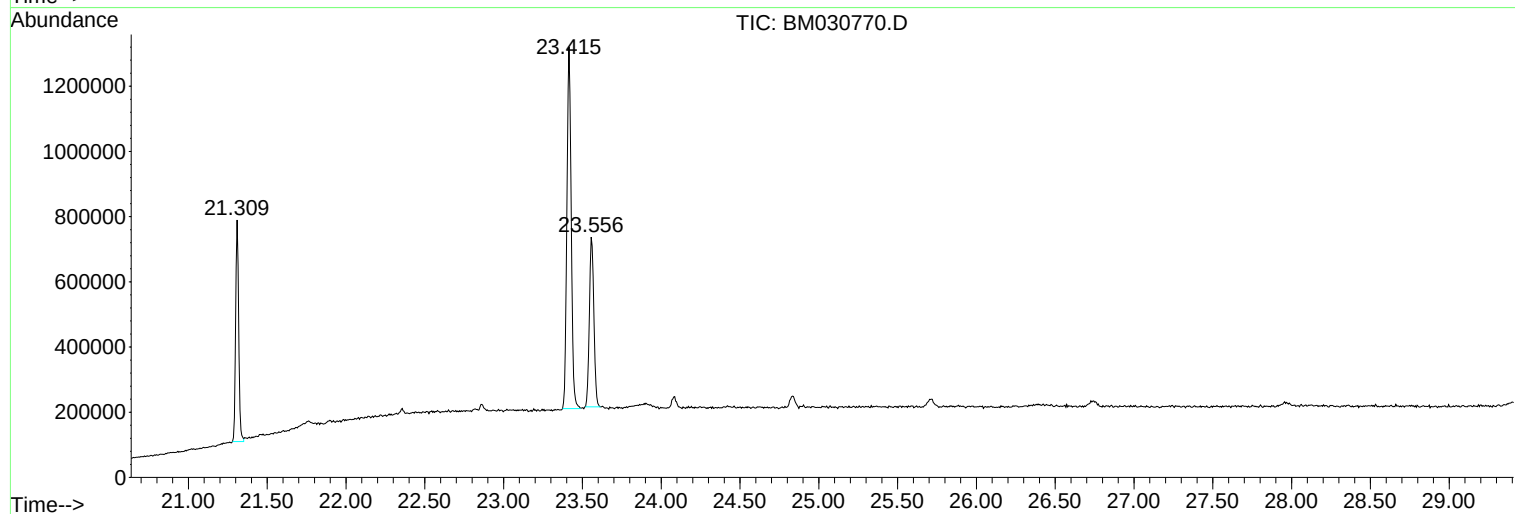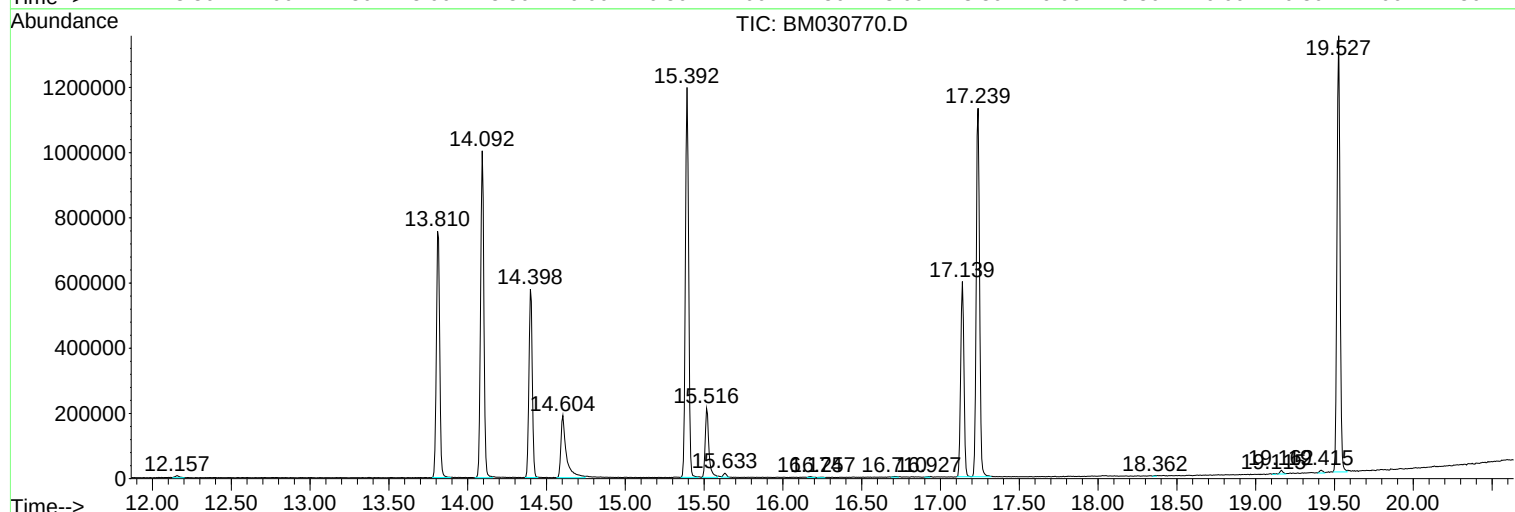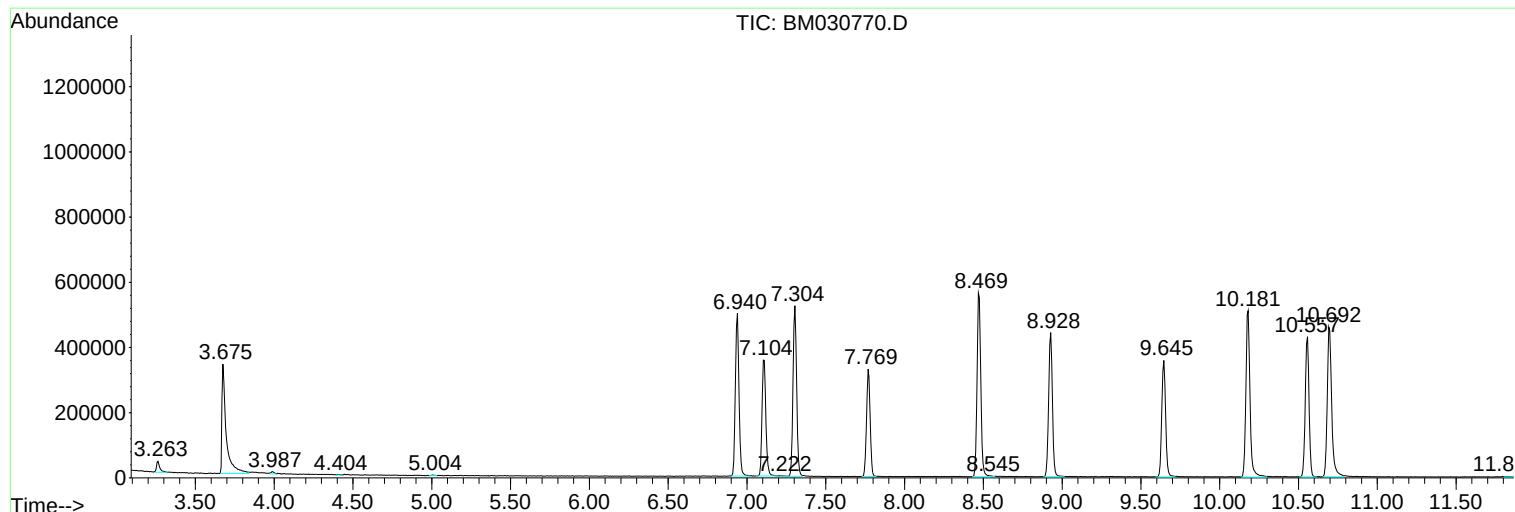

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030770.D
Acq On : 02 Jul 2021 08:41
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030770.D
Acq On : 02 Jul 2021 08:41
Operator : CG/JU
Sample : PB137472BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK472

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc