

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030776.D
 Acq On : 02 Jul 2021 15:01
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030776.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.769	112	116	122	rBV5	8413	17950	1.15%	0.112%
2	3.987	149	153	157	rVB	11036	13648	0.87%	0.085%
3	4.540	243	247	251	rVB4	3415	4556	0.29%	0.029%
4	5.428	394	398	405	rVB5	4788	9440	0.60%	0.059%
5	5.793	455	460	465	rVB5	4165	7974	0.51%	0.050%
6	6.716	614	617	620	rBV5	1069	1711	0.11%	0.011%
7	6.934	647	654	668	rBV	291537	471260	30.19%	2.950%
8	7.104	676	683	697	rVB	226058	358110	22.94%	2.242%
9	7.298	709	716	725	rBV	291639	478542	30.66%	2.996%
10	7.393	728	732	736	rVB4	2754	3911	0.25%	0.024%
11	7.769	789	796	805	rBV	310335	490992	31.46%	3.074%
12	7.987	831	833	836	rBV3	1552	2128	0.14%	0.013%
13	8.251	875	878	881	rBV3	1011	1597	0.10%	0.010%
14	8.304	884	887	889	rBV3	2003	2571	0.16%	0.016%
15	8.469	908	915	927	rBV	313165	514785	32.98%	3.223%
16	8.604	937	938	942	rVB4	2778	2120	0.14%	0.013%
17	8.922	985	992	1003	rBV	251457	432343	27.70%	2.707%
18	9.645	1106	1115	1127	rBV	198819	342903	21.97%	2.147%
19	10.175	1199	1205	1219	rBV	282453	519082	33.26%	3.250%
20	10.551	1262	1269	1279	rBV	390798	655117	41.97%	4.101%
21	10.698	1286	1294	1308	rBV	245004	498978	31.97%	3.124%
22	12.710	1632	1636	1638	rBV3	1266	1966	0.13%	0.012%
23	13.292	1730	1735	1739	rBV2	3001	4579	0.29%	0.029%
24	13.810	1811	1823	1828	rBV	460956	669980	42.93%	4.194%
25	13.857	1828	1831	1839	rVV	55953	84280	5.40%	0.528%
26	13.922	1839	1842	1848	rVB5	1204	2178	0.14%	0.014%
27	14.092	1863	1871	1883	rBV	568188	852021	54.59%	5.334%
28	14.298	1904	1906	1909	rVB3	1393	1635	0.10%	0.010%
29	14.398	1917	1923	1932	rBV	539483	789288	50.57%	4.941%
30	14.610	1950	1959	1973	rBV	92429	233718	14.97%	1.463%
31	15.392	2084	2092	2101	rBV	723129	1045821	67.01%	6.547%
32	15.521	2108	2114	2130	rBV	112366	192626	12.34%	1.206%
33	15.633	2130	2133	2139	rVB4	6623	9330	0.60%	0.058%
34	15.810	2159	2163	2169	rVB4	5983	8626	0.55%	0.054%
35	15.951	2183	2187	2193	rBV6	1870	3812	0.24%	0.024%
36	16.621	2298	2301	2305	rBV3	2414	3344	0.21%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030776.D
 Acq On : 02 Jul 2021 15:01
 Operator : CG/JU
 Sample : M2825-05
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDQ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	16.710	2313	2316	2321	rVB5	1488	2479	0.16%	0.016%
38	16.927	2350	2353	2356	rVB4	1591	1655	0.11%	0.010%
39	17.139	2383	2389	2395	rBV	591493	859235	55.05%	5.379%
40	17.239	2400	2406	2417	rVB	710584	1062374	68.07%	6.651%
41	17.427	2435	2438	2440	rBV3	1117	1596	0.10%	0.010%
42	17.510	2449	2452	2453	rBV2	1428	1580	0.10%	0.010%
43	17.815	2499	2504	2508	rVB5	2831	4694	0.30%	0.029%
44	18.033	2534	2541	2544	rBV5	9063	18182	1.16%	0.114%
45	18.104	2551	2553	2557	rBV2	2909	3354	0.21%	0.021%
46	18.145	2558	2560	2564	rVB2	2658	3197	0.20%	0.020%
47	18.292	2583	2585	2587	rBV3	2024	1783	0.11%	0.011%
48	18.327	2589	2591	2594	rVB4	1952	1882	0.12%	0.012%
49	18.374	2596	2599	2601	rBV4	2336	2759	0.18%	0.017%
50	18.527	2623	2625	2627	rVB3	2706	1677	0.11%	0.010%
51	18.733	2657	2660	2661	rBV3	1869	2146	0.14%	0.013%
52	18.798	2669	2671	2674	rVB4	2252	1858	0.12%	0.012%
53	18.851	2678	2680	2684	rBV5	1788	1584	0.10%	0.010%
54	18.957	2690	2698	2703	rBV8	8548	20049	1.28%	0.126%
55	19.115	2722	2725	2729	rVB	15619	16660	1.07%	0.104%
56	19.192	2734	2738	2746	rVB	32525	46721	2.99%	0.293%
57	19.309	2756	2758	2762	rBV5	4449	4433	0.28%	0.028%
58	19.356	2762	2766	2770	rVB3	17970	23270	1.49%	0.146%
59	19.474	2783	2786	2789	rVB3	6598	8104	0.52%	0.051%
60	19.527	2789	2795	2804	rBV	941629	1308458	83.84%	8.192%
61	20.521	2961	2964	2968	rBV2	25954	27424	1.76%	0.172%
62	21.309	3093	3098	3110	rBV	777654	1086929	69.64%	6.805%
63	23.415	3450	3456	3472	rVB	759185	1560742	100.00%	9.771%
64	23.562	3475	3481	3490	rVB2	592113	1165238	74.66%	7.295%




Sum of corrected areas: 15972985

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030776.D
Acq On : 02 Jul 2021 15:01
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

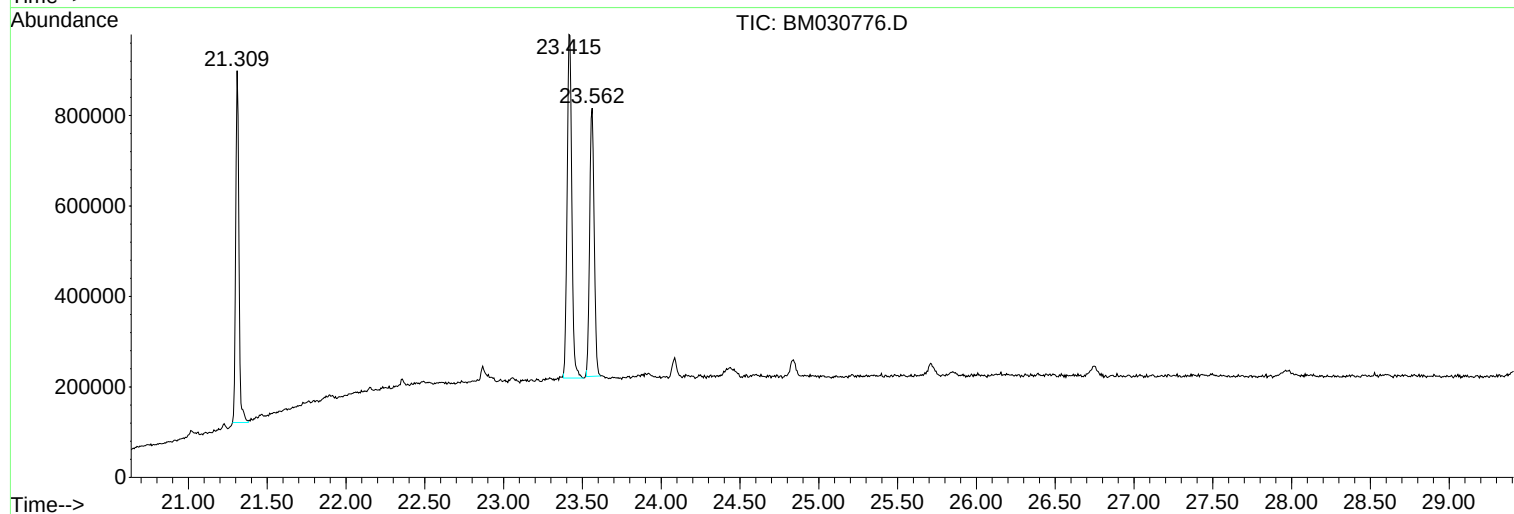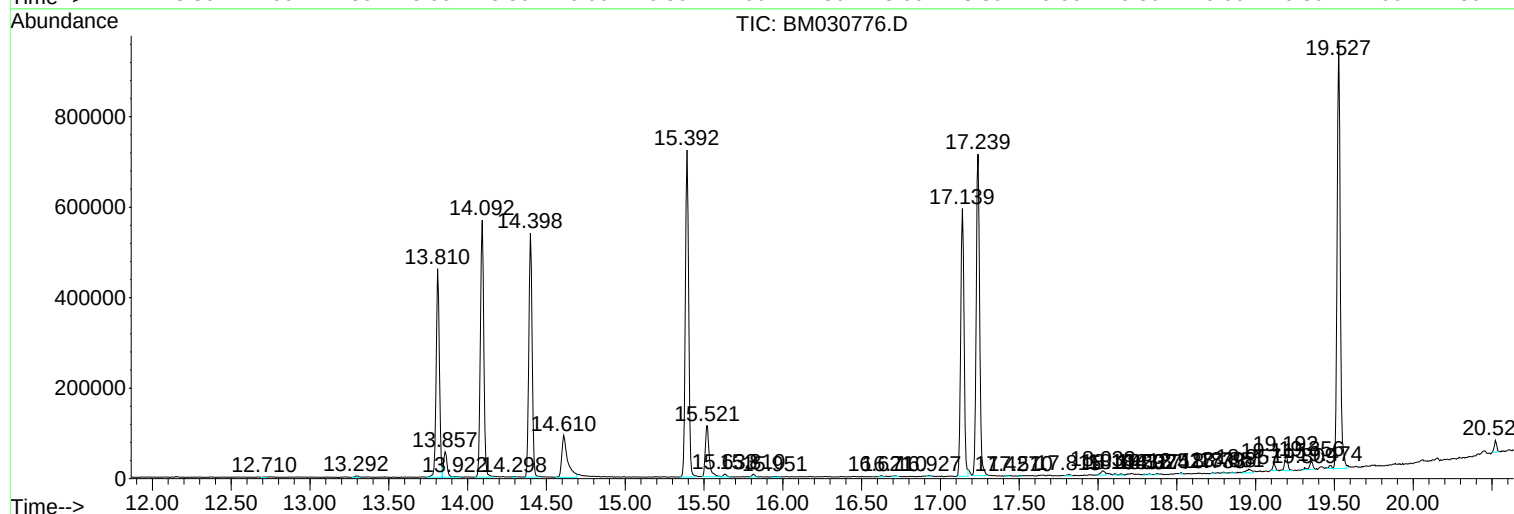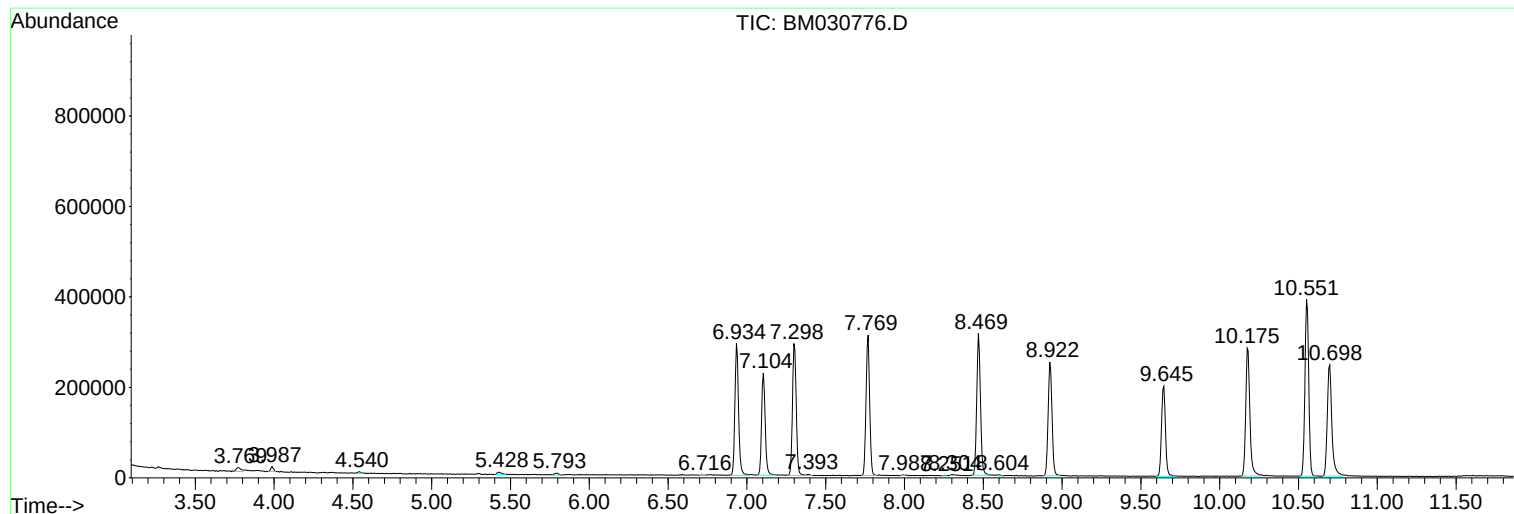

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030776.D
Acq On : 02 Jul 2021 15:01
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030776.D
Acq On : 02 Jul 2021 15:01
Operator : CG/JU
Sample : M2825-05
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDQ9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
