

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030787.D
 Acq On : 02 Jul 2021 22:57
 Operator : CG/JU
 Sample : M2869-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030787.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	35	rVB2	9123	10773	1.02%	0.097%
2	3.728	105	109	113	rBV2	11135	21900	2.08%	0.197%
3	3.987	150	153	161	rVB	8109	11658	1.11%	0.105%
4	4.540	244	247	254	rVB3	3156	4883	0.46%	0.044%
5	4.793	289	290	292	rBV2	1765	1157	0.11%	0.010%
6	5.140	346	349	352	rBV3	1144	1668	0.16%	0.015%
7	5.293	372	375	378	rVB5	1601	1913	0.18%	0.017%
8	5.428	393	398	404	rBV	4758	8958	0.85%	0.080%
9	5.722	444	448	449	rBV3	1626	1607	0.15%	0.014%
10	5.793	457	460	463	rBV5	2917	2801	0.27%	0.025%
11	6.763	621	625	628	rBV5	1822	2449	0.23%	0.022%
12	6.940	648	655	668	rVB	141025	245038	23.24%	2.199%
13	7.104	677	683	694	rBV	115530	192300	18.24%	1.726%
14	7.304	710	717	726	rBV	156885	263107	24.95%	2.362%
15	7.392	729	732	736	rVV3	3143	4827	0.46%	0.043%
16	7.540	753	757	762	rBV6	1072	2525	0.24%	0.023%
17	7.722	785	788	789	rBV3	1393	1258	0.12%	0.011%
18	7.769	789	796	805	rVV	296175	476023	45.15%	4.273%
19	7.834	805	807	812	rVB5	1319	1819	0.17%	0.016%
20	7.992	831	834	840	rVB4	2779	4619	0.44%	0.041%
21	8.304	883	887	895	rVB7	2001	3765	0.36%	0.034%
22	8.469	909	915	925	rBV	155538	262195	24.87%	2.353%
23	8.598	933	937	942	rVV5	2194	3837	0.36%	0.034%
24	8.651	944	946	948	rVB3	1487	1237	0.12%	0.011%
25	8.928	986	993	1001	rBV	131347	229574	21.77%	2.061%
26	9.334	1059	1062	1068	rVB5	1534	2818	0.27%	0.025%
27	9.645	1109	1115	1125	rBV	100764	173940	16.50%	1.561%
28	10.181	1196	1206	1220	rBV	138588	275855	26.16%	2.476%
29	10.386	1237	1241	1255	rBV4	5149	18095	1.72%	0.162%
30	10.481	1255	1257	1260	rVB4	1390	1446	0.14%	0.013%
31	10.551	1260	1269	1277	rBV	379036	649176	61.57%	5.827%
32	10.698	1287	1294	1310	rVV	114512	247506	23.47%	2.222%
33	11.428	1417	1418	1426	rVB4	850	1263	0.12%	0.011%
34	11.827	1479	1486	1492	rVB5	1502	4119	0.39%	0.037%
35	11.980	1510	1512	1515	rVB4	1162	1454	0.14%	0.013%
36	12.151	1535	1541	1547	rVB6	1988	3630	0.34%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030787.D
 Acq On : 02 Jul 2021 22:57
 Operator : CG/JU
 Sample : M2869-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG DY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	12.369	1575	1578	1581	rVB2	907	1230	0.12%	0.011%
38	12.757	1641	1644	1647	rVB3	998	1516	0.14%	0.014%
39	13.004	1683	1686	1692	rVB5	2630	4494	0.43%	0.040%
40	13.222	1719	1723	1727	rVB4	2440	3591	0.34%	0.032%
41	13.298	1730	1736	1742	rVV	18327	29356	2.78%	0.263%
42	13.374	1745	1749	1754	rBV4	1347	2907	0.28%	0.026%
43	13.810	1817	1823	1834	rBV	251360	381670	36.20%	3.426%
44	14.092	1863	1871	1879	rBV	297888	462297	43.84%	4.149%
45	14.298	1902	1906	1911	rVB3	2540	3925	0.37%	0.035%
46	14.398	1916	1923	1933	rBV	560327	811537	76.97%	7.284%
47	14.621	1954	1961	1968	rBV3	24035	61708	5.85%	0.554%
48	14.751	1982	1983	1987	rVB3	1554	1334	0.13%	0.012%
49	14.833	1994	1997	2001	rBV5	1326	1831	0.17%	0.016%
50	15.192	2053	2058	2060	rBV5	1622	2311	0.22%	0.021%
51	15.251	2065	2068	2072	rVB4	1886	2728	0.26%	0.024%
52	15.310	2076	2078	2083	rVB4	1261	1267	0.12%	0.011%
53	15.392	2085	2092	2105	rBV	397270	601667	57.06%	5.400%
54	15.521	2109	2114	2129	rVB	38699	71818	6.81%	0.645%
55	15.639	2129	2134	2136	rBV2	3406	4318	0.41%	0.039%
56	15.810	2159	2163	2167	rBV4	4608	6407	0.61%	0.058%
57	16.104	2211	2213	2217	rVV5	1889	3036	0.29%	0.027%
58	16.174	2221	2225	2229	rVB4	3119	4848	0.46%	0.044%
59	16.286	2240	2244	2247	rVV2	1652	2367	0.22%	0.021%
60	16.374	2254	2259	2265	rBV5	2879	4673	0.44%	0.042%
61	16.457	2270	2273	2275	rBV2	1460	1316	0.12%	0.012%
62	16.527	2280	2285	2289	rBV4	1496	2878	0.27%	0.026%
63	16.592	2293	2296	2300	rBV4	1548	1815	0.17%	0.016%
64	16.668	2306	2309	2311	rBV3	1733	2009	0.19%	0.018%
65	16.810	2331	2333	2337	rBV5	868	1262	0.12%	0.011%
66	16.874	2339	2344	2347	rBV5	3644	5395	0.51%	0.048%
67	16.898	2347	2348	2351	rVV2	2962	2680	0.25%	0.024%
68	16.927	2351	2353	2356	rVB2	1077	1275	0.12%	0.011%
69	17.139	2382	2389	2395	rBV	570135	850815	80.69%	7.637%
70	17.233	2400	2405	2419	rVB	383849	599122	56.82%	5.378%
71	17.427	2434	2438	2440	rBV4	1873	2706	0.26%	0.024%
72	17.574	2461	2463	2467	rBV5	1971	2327	0.22%	0.021%
73	17.633	2470	2473	2476	rVV4	1889	2455	0.23%	0.022%
74	17.686	2480	2482	2485	rVV3	1321	1316	0.12%	0.012%
75	17.809	2498	2503	2508	rBV2	11482	16352	1.55%	0.147%
76	17.886	2514	2516	2519	rBV4	1885	2347	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030787.D
 Acq On : 02 Jul 2021 22:57
 Operator : CG/JU
 Sample : M2869-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	18.027	2534	2540	2543	rVV4	13056	22765	2.16%	0.204%
78	18.062	2543	2546	2550	rVV2	9635	15414	1.46%	0.138%
79	18.104	2550	2553	2556	rVV	5588	7143	0.68%	0.064%
80	18.145	2556	2560	2565	rVV3	5599	8905	0.84%	0.080%
81	18.209	2565	2571	2575	rVV3	10295	18483	1.75%	0.166%
82	18.251	2575	2578	2586	rVB7	4314	7067	0.67%	0.063%
83	18.321	2589	2590	2594	rVB4	1818	1375	0.13%	0.012%
84	18.515	2620	2623	2626	rVB	4269	5673	0.54%	0.051%
85	18.609	2637	2639	2640	rBV2	1522	1245	0.12%	0.011%
86	18.951	2690	2697	2698	rBV5	8566	14490	1.37%	0.130%
87	18.980	2698	2702	2706	rVB2	43003	51315	4.87%	0.461%
88	19.115	2721	2725	2729	rVB	11488	14116	1.34%	0.127%
89	19.192	2730	2738	2746	rVV	97988	140181	13.29%	1.258%
90	19.309	2756	2758	2760	rBV3	3331	3954	0.38%	0.035%
91	19.339	2760	2763	2769	rVB3	7084	9497	0.90%	0.085%
92	19.527	2789	2795	2809	rBV3	480984	797737	75.66%	7.160%
93	19.739	2828	2831	2835	rBV2	7034	9007	0.85%	0.081%
94	20.050	2881	2884	2891	rVB3	20008	33522	3.18%	0.301%
95	20.150	2898	2901	2905	rVB	19676	23257	2.21%	0.209%
96	20.515	2961	2963	2967	rVB	12092	12691	1.20%	0.114%
97	20.686	2990	2992	2996	rVB4	16485	16420	1.56%	0.147%
98	21.303	3091	3097	3102	rBV	708442	1054395	100.00%	9.464%
99	23.409	3450	3455	3471	rVB	338634	753554	71.47%	6.764%
100	23.556	3474	3480	3488	rVB	547813	1008738	95.67%	9.054%




Sum of corrected areas: 11141043

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030787.D
Acq On : 02 Jul 2021 22:57
Operator : CG/JU
Sample : M2869-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

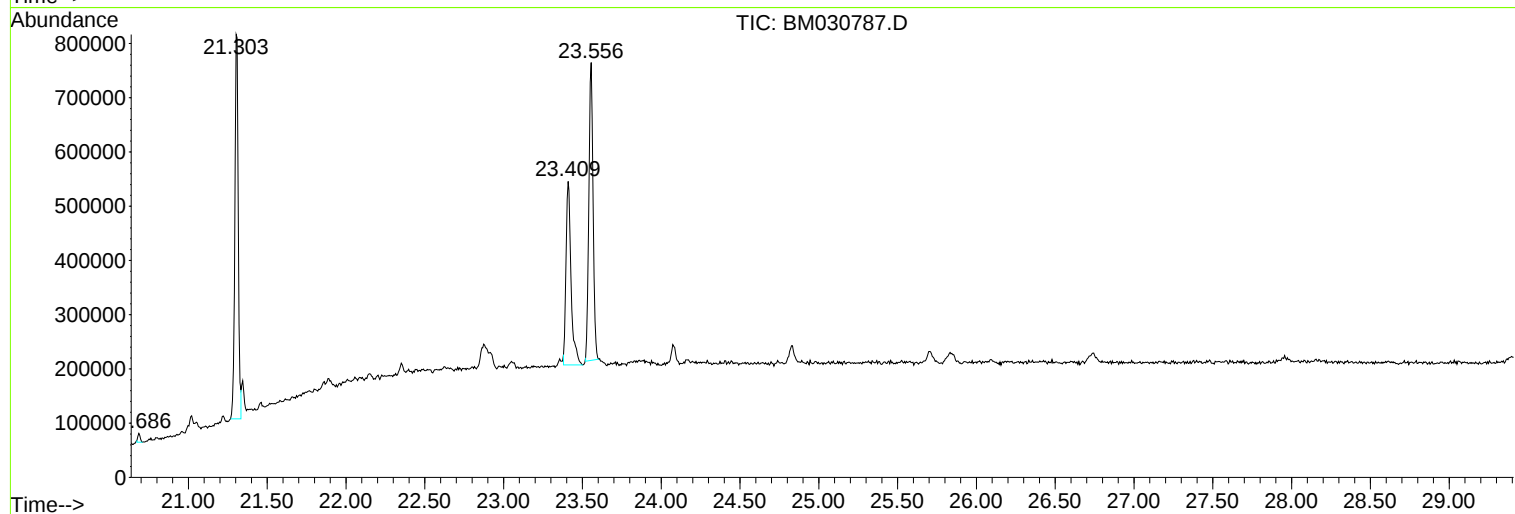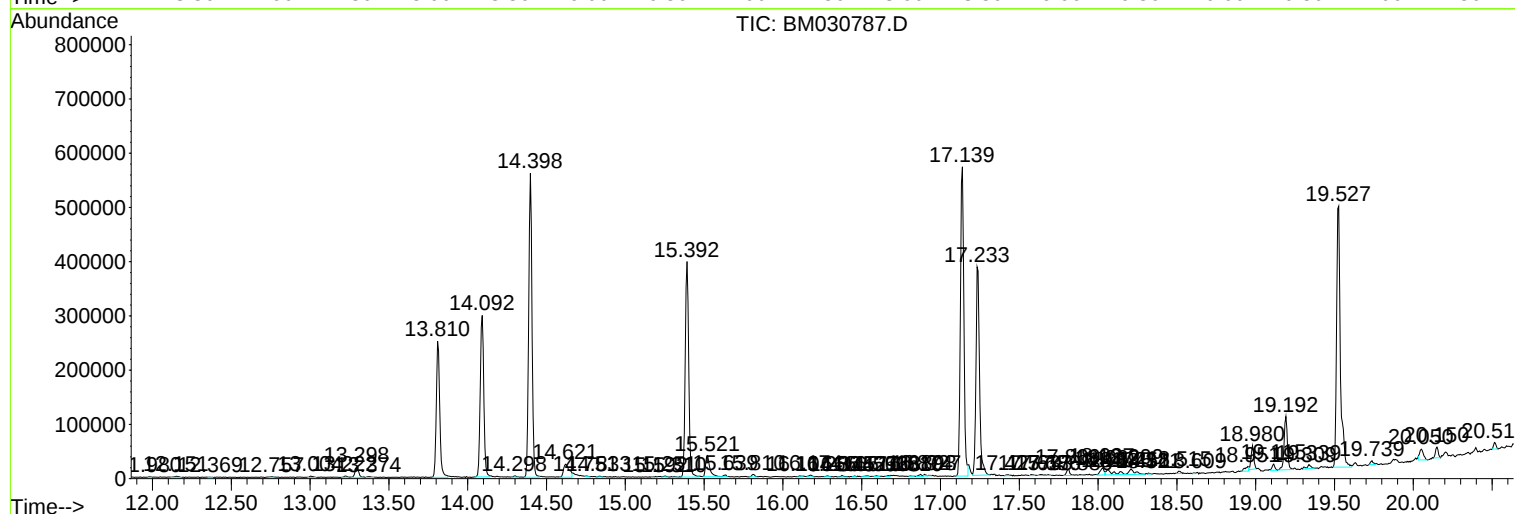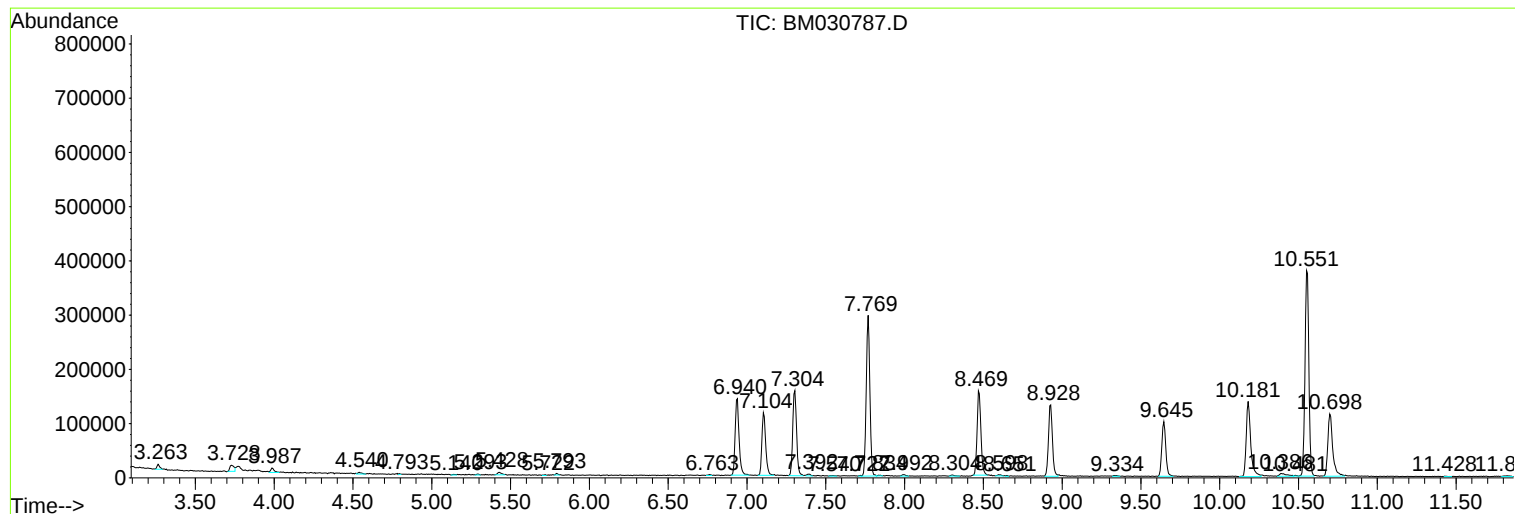

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030787.D
Acq On : 02 Jul 2021 22:57
Operator : CG/JU
Sample : M2869-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030787.D
Acq On : 02 Jul 2021 22:57
Operator : CG/JU
Sample : M2869-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
