

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030788.D
 Acq On : 02 Jul 2021 23:34
 Operator : CG/JU
 Sample : M2869-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY3

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030788.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB5	4960	9502	0.94%	0.114%
2	3.746	108	112	114	rBV2	6664	11569	1.14%	0.139%
3	3.987	150	153	157	rVV2	5940	7561	0.74%	0.091%
4	4.169	181	184	186	rVB3	1449	1341	0.13%	0.016%
5	4.546	244	248	253	rVB4	2685	3956	0.39%	0.047%
6	4.899	305	308	310	rBV4	2045	2647	0.26%	0.032%
7	4.969	317	320	322	rBV3	1225	1477	0.15%	0.018%
8	5.187	356	357	361	rBV3	979	1079	0.11%	0.013%
9	5.422	393	397	404	rBV4	4742	9576	0.94%	0.115%
10	5.640	432	434	438	rVB4	1229	1098	0.11%	0.013%
11	5.793	456	460	466	rVB3	3861	5309	0.52%	0.064%
12	5.846	466	469	474	rVB5	905	1411	0.14%	0.017%
13	6.011	495	497	501	rVB5	1672	2203	0.22%	0.026%
14	6.040	501	502	506	rBV3	1215	1582	0.16%	0.019%
15	6.722	615	618	621	rVB4	930	1185	0.12%	0.014%
16	6.763	621	625	630	rBV4	2335	3708	0.37%	0.044%
17	6.940	649	655	665	rVV	69759	126394	12.45%	1.514%
18	7.105	678	683	694	rBV	62259	106161	10.46%	1.272%
19	7.305	710	717	727	rBV	81797	138176	13.61%	1.656%
20	7.393	729	732	734	rBV4	2018	2384	0.23%	0.029%
21	7.487	746	748	754	rVB5	1071	1893	0.19%	0.023%
22	7.769	788	796	807	rBV	304030	489372	48.21%	5.864%
23	7.840	807	808	813	rVV4	1694	1916	0.19%	0.023%
24	7.993	830	834	838	rBV3	2787	3762	0.37%	0.045%
25	8.305	883	887	889	rBV3	2147	2324	0.23%	0.028%
26	8.434	905	909	910	rBV3	2444	2983	0.29%	0.036%
27	8.475	910	916	926	rVB2	80860	141089	13.90%	1.691%
28	8.599	934	937	939	rBV3	2029	2665	0.26%	0.032%
29	8.640	943	944	949	rVV3	1579	1516	0.15%	0.018%
30	8.675	949	950	954	rVB3	1062	1030	0.10%	0.012%
31	8.928	987	993	1002	rVV	67482	117458	11.57%	1.407%
32	9.334	1058	1062	1064	rBV4	1492	1556	0.15%	0.019%
33	9.646	1109	1115	1123	rBV	48469	84644	8.34%	1.014%
34	10.187	1200	1207	1220	rBV	63424	136922	13.49%	1.641%
35	10.281	1222	1223	1227	rVV2	1498	1757	0.17%	0.021%
36	10.416	1243	1246	1248	rBV4	1062	1340	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030788.D
 Acq On : 02 Jul 2021 23:34
 Operator : CG/JU
 Sample : M2869-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	10.446	1248	1251	1255	rVV5	972	1474	0.15%	0.018%
38	10.551	1262	1269	1277	rBV	394133	673471	66.34%	8.070%
39	10.704	1289	1295	1309	rBV	55920	127038	12.51%	1.522%
40	10.957	1337	1338	1341	rVB3	1801	1492	0.15%	0.018%
41	11.087	1358	1360	1366	rVB4	859	1371	0.14%	0.016%
42	11.804	1478	1482	1483	rVV4	1510	1855	0.18%	0.022%
43	11.822	1483	1485	1489	rVB2	1406	1856	0.18%	0.022%
44	12.157	1539	1542	1546	rBV5	1039	1565	0.15%	0.019%
45	12.757	1637	1644	1649	rBV4	1834	3056	0.30%	0.037%
46	13.010	1682	1687	1690	rVB4	2486	3595	0.35%	0.043%
47	13.222	1719	1723	1725	rBV4	1375	1500	0.15%	0.018%
48	13.298	1732	1736	1739	rBV4	2152	2731	0.27%	0.033%
49	13.363	1744	1747	1750	rVB2	924	1066	0.11%	0.013%
50	13.745	1810	1812	1814	rBV3	1003	1088	0.11%	0.013%
51	13.810	1817	1823	1828	rBV	139438	212786	20.96%	2.550%
52	13.857	1828	1831	1842	rVB	56321	89942	8.86%	1.078%
53	13.998	1853	1855	1862	rVB4	1130	1085	0.11%	0.013%
54	14.092	1862	1871	1881	rBV	163028	251411	24.77%	3.012%
55	14.304	1901	1907	1909	rBV5	1831	2542	0.25%	0.030%
56	14.398	1916	1923	1931	rBV	565721	846441	83.38%	10.142%
57	14.634	1958	1963	1971	rBV6	7440	22747	2.24%	0.273%
58	14.792	1987	1990	1995	rVB2	1076	1614	0.16%	0.019%
59	14.863	1999	2002	2004	rVB4	1153	1261	0.12%	0.015%
60	15.198	2054	2059	2061	rBV4	1633	2537	0.25%	0.030%
61	15.228	2061	2064	2067	rVV2	1311	1709	0.17%	0.020%
62	15.257	2067	2069	2071	rVB3	1642	1400	0.14%	0.017%
63	15.392	2086	2092	2101	rBV	215327	334464	32.95%	4.008%
64	15.528	2111	2115	2121	rVV2	13092	22303	2.20%	0.267%
65	15.810	2158	2163	2167	rVB4	5263	7338	0.72%	0.088%
66	16.104	2211	2213	2216	rBV2	856	1026	0.10%	0.012%
67	16.286	2241	2244	2245	rBV2	889	1052	0.10%	0.013%
68	16.375	2255	2259	2263	rBV3	2292	3507	0.35%	0.042%
69	16.528	2283	2285	2289	rVB3	916	1187	0.12%	0.014%
70	16.675	2304	2310	2312	rBV3	1692	2823	0.28%	0.034%
71	16.716	2313	2317	2319	rVV5	2254	3380	0.33%	0.041%
72	16.733	2319	2320	2325	rVV4	1364	2134	0.21%	0.026%
73	16.869	2342	2343	2345	rBV2	1274	1107	0.11%	0.013%
74	16.904	2345	2349	2352	rVV5	1681	2980	0.29%	0.036%
75	17.139	2382	2389	2399	rBV	593719	900498	88.70%	10.790%
76	17.239	2399	2406	2417	rVB	201745	327136	32.22%	3.920%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030788.D
 Acq On : 02 Jul 2021 23:34
 Operator : CG/JU
 Sample : M2869-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	17.427	2435	2438	2446	rVB6	2953	5225	0.51%	0.063%
78	17.633	2471	2473	2478	rVB5	1675	2165	0.21%	0.026%
79	17.810	2499	2503	2508	rVB4	4791	6237	0.61%	0.075%
80	17.922	2521	2522	2525	rVB2	1153	1176	0.12%	0.014%
81	18.027	2535	2540	2544	rBV6	12407	20398	2.01%	0.244%
82	18.104	2549	2553	2557	rVB	7405	10343	1.02%	0.124%
83	18.151	2557	2561	2562	rBV5	1636	1536	0.15%	0.018%
84	18.210	2567	2571	2575	rBV6	4013	5964	0.59%	0.071%
85	18.322	2588	2590	2595	rVB5	2777	3935	0.39%	0.047%
86	18.369	2597	2598	2601	rBV3	1804	1988	0.20%	0.024%
87	18.451	2610	2612	2615	rBV3	2103	1843	0.18%	0.022%
88	18.522	2620	2624	2629	rVV4	2879	5118	0.50%	0.061%
89	18.610	2636	2639	2644	rBV7	3141	3366	0.33%	0.040%
90	18.786	2665	2669	2672	rBV5	4433	6312	0.62%	0.076%
91	18.921	2690	2692	2694	rBV3	2524	2344	0.23%	0.028%
92	18.980	2700	2702	2707	rVB5	5714	7393	0.73%	0.089%
93	19.163	2731	2733	2734	rBV2	2958	2530	0.25%	0.030%
94	19.192	2734	2738	2743	rVV	37226	51994	5.12%	0.623%
95	19.316	2754	2759	2761	rBV6	5222	8465	0.83%	0.101%
96	19.527	2789	2795	2805	rBV2	259801	423224	41.69%	5.071%
97	21.015	3045	3048	3053	rBV5	27521	34464	3.39%	0.413%
98	21.304	3092	3097	3108	rBV	708372	1000267	98.53%	11.986%
99	23.409	3450	3455	3471	rVB2	188088	424024	41.77%	5.081%
100	23.551	3473	3479	3488	rVV2	503737	1015185	100.00%	12.164%




Sum of corrected areas: 8345610

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030788.D
Acq On : 02 Jul 2021 23:34
Operator : CG/JU
Sample : M2869-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

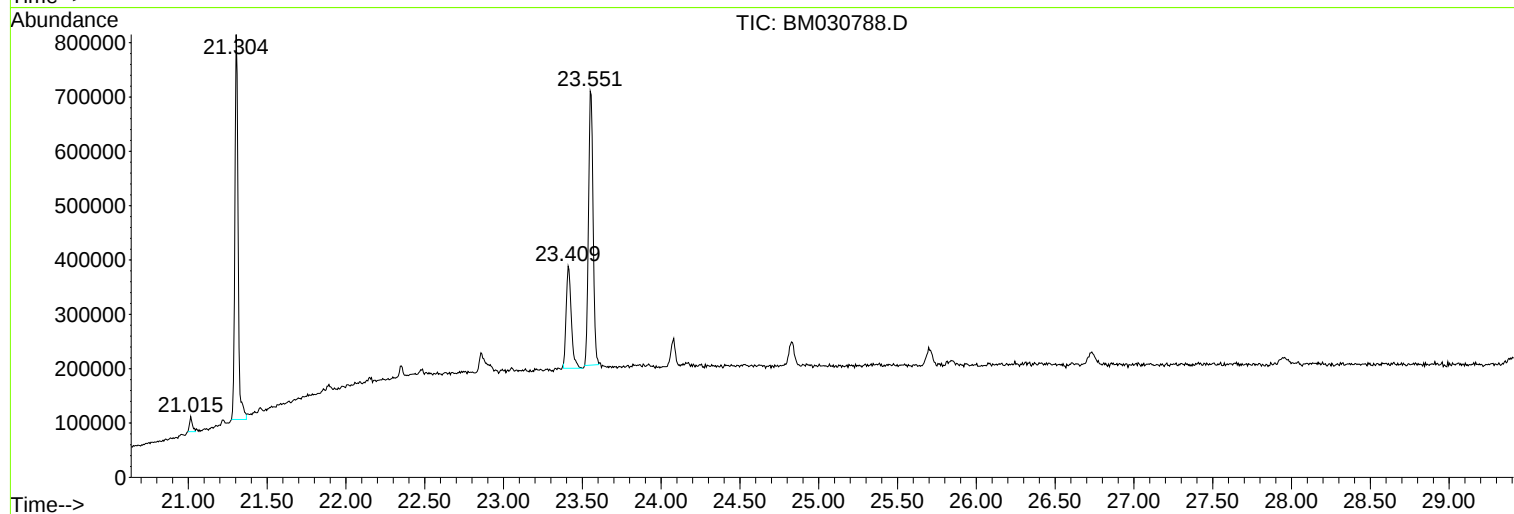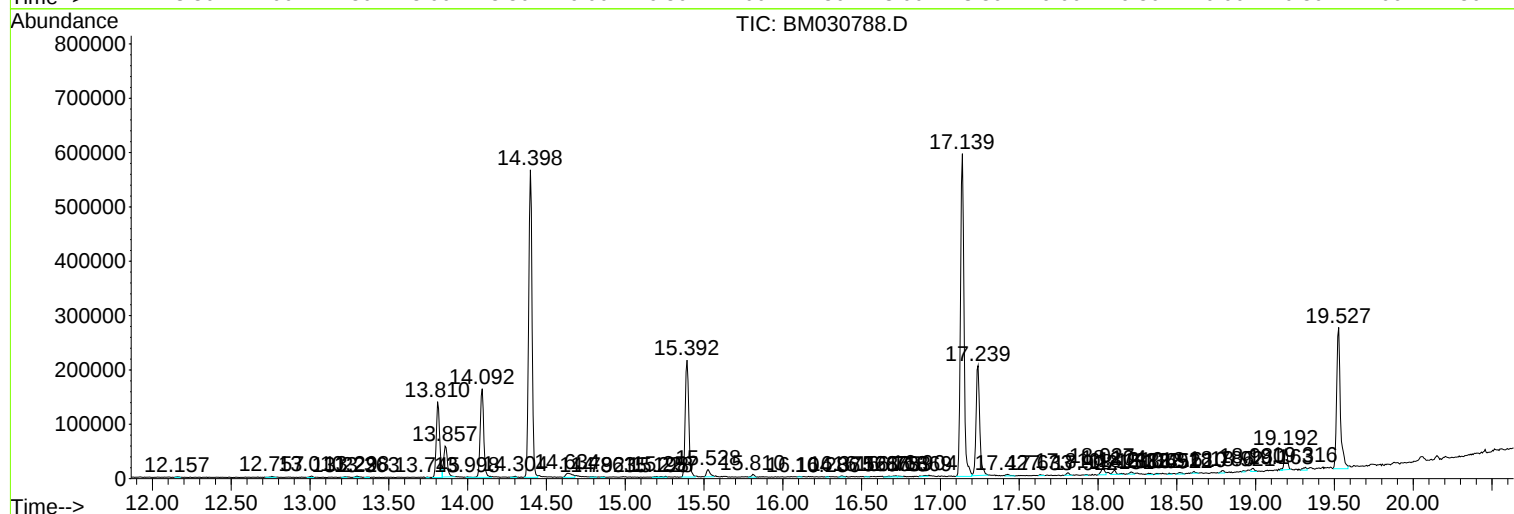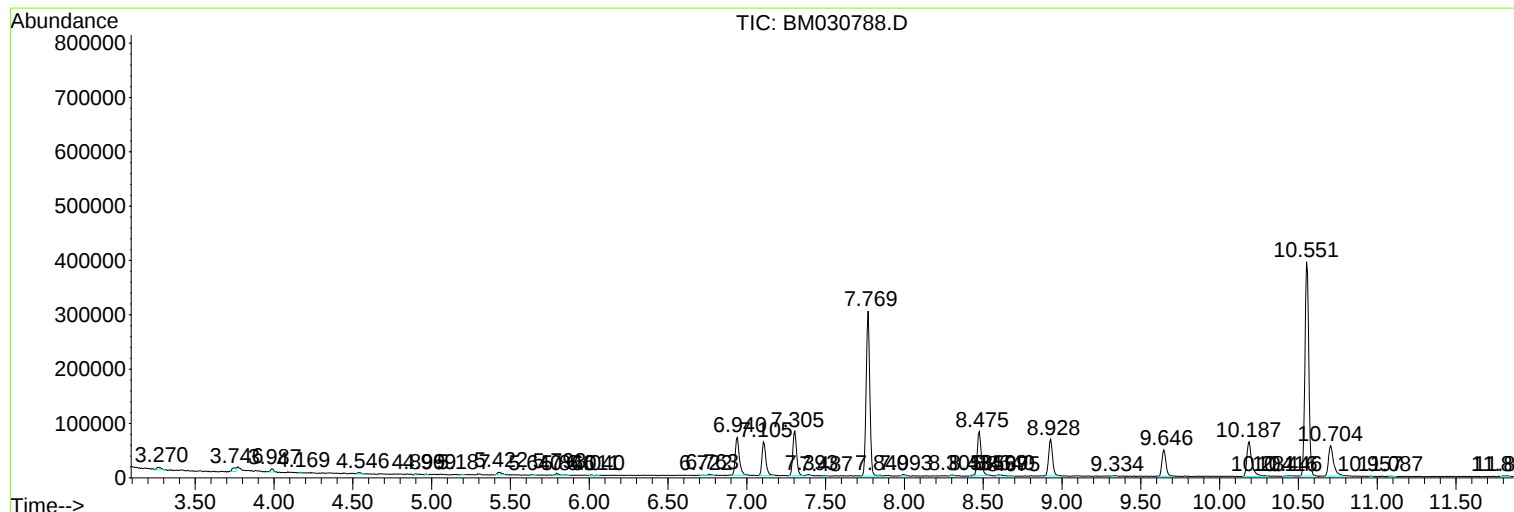

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030788.D
Acq On : 02 Jul 2021 23:34
Operator : CG/JU
Sample : M2869-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030788.D
Acq On : 02 Jul 2021 23:34
Operator : CG/JU
Sample : M2869-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
