

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030792.D
 Acq On : 03 Jul 2021 01:59
 Operator : CG/JU
 Sample : M2869-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY0

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030792.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	28	30	35	rVB2	4028	4801	0.40%	0.052%
2	3.740	108	111	113	rBV3	7358	10390	0.86%	0.112%
3	3.775	114	117	121	rVB2	9433	14371	1.19%	0.155%
4	3.987	150	153	158	rVB2	8126	11147	0.92%	0.120%
5	4.199	188	189	194	rVB5	2073	2179	0.18%	0.023%
6	4.234	194	195	199	rBV3	1477	1615	0.13%	0.017%
7	4.534	242	246	251	rBV5	3377	5544	0.46%	0.060%
8	5.422	394	397	402	rBV2	5235	8627	0.71%	0.093%
9	5.793	456	460	463	rBV3	3507	4558	0.38%	0.049%
10	5.957	484	488	491	rVB4	1017	1773	0.15%	0.019%
11	6.769	622	626	631	rVB6	1914	3666	0.30%	0.039%
12	6.940	649	655	668	rVB	75039	135243	11.16%	1.455%
13	7.104	677	683	693	rBV	61648	105001	8.66%	1.130%
14	7.304	709	717	724	rBV	82449	140317	11.58%	1.510%
15	7.387	729	731	734	rVB2	2230	2028	0.17%	0.022%
16	7.769	789	796	804	rBV	271393	431856	35.64%	4.648%
17	7.898	813	818	822	rVB4	952	1798	0.15%	0.019%
18	7.998	831	835	841	rVB5	2765	4525	0.37%	0.049%
19	8.298	882	886	894	rBV6	2428	5483	0.45%	0.059%
20	8.475	909	916	925	rVV	79215	139035	11.47%	1.496%
21	8.592	933	936	937	rBV3	1996	1723	0.14%	0.019%
22	8.928	986	993	1005	rBV	66784	118068	9.74%	1.271%
23	9.086	1015	1020	1022	rBV5	1907	2746	0.23%	0.030%
24	9.345	1060	1064	1066	rBV5	1022	1673	0.14%	0.018%
25	9.645	1109	1115	1125	rVB	47314	84024	6.93%	0.904%
26	10.186	1198	1207	1219	rBV	60979	130635	10.78%	1.406%
27	10.416	1241	1246	1248	rBV5	1998	3404	0.28%	0.037%
28	10.551	1262	1269	1277	rBV	329465	568041	46.88%	6.113%
29	10.704	1289	1295	1309	rBV	50146	114579	9.46%	1.233%
30	11.798	1478	1481	1483	rBV3	1444	1759	0.15%	0.019%
31	11.916	1494	1501	1504	rBV3	1200	2183	0.18%	0.023%
32	11.980	1507	1512	1514	rBV3	1550	2079	0.17%	0.022%
33	12.033	1517	1521	1524	rBV6	1106	1601	0.13%	0.017%
34	12.751	1640	1643	1647	rVB5	1475	2023	0.17%	0.022%
35	13.016	1684	1688	1690	rVB4	1790	2198	0.18%	0.024%
36	13.233	1719	1725	1727	rBV3	1967	3004	0.25%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030792.D
 Acq On : 03 Jul 2021 01:59
 Operator : CG/JU
 Sample : M2869-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	13.292	1731	1735	1742	rVB5	2058	3500	0.29%	0.038%
38	13.710	1800	1806	1809	rBV4	1309	2556	0.21%	0.028%
39	13.810	1815	1823	1828	rBV	126492	195584	16.14%	2.105%
40	13.857	1828	1831	1841	rVB	52069	81625	6.74%	0.878%

41	14.092	1862	1871	1882	rBV	149237	240868	19.88%	2.592%
42	14.304	1903	1907	1910	rVB5	2112	3019	0.25%	0.032%
43	14.398	1914	1923	1931	rBV	470183	684392	56.48%	7.365%
44	14.457	1931	1933	1939	rVB4	3625	5692	0.47%	0.061%
45	14.633	1957	1963	1976	rBV6	11227	37810	3.12%	0.407%

46	14.798	1989	1991	1994	rBV3	1581	1775	0.15%	0.019%
47	14.839	1994	1998	2002	rVB4	1842	2629	0.22%	0.028%
48	14.868	2002	2003	2008	rBV4	1587	1802	0.15%	0.019%
49	15.304	2074	2077	2082	rVV3	3043	5337	0.44%	0.057%
50	15.392	2082	2092	2099	rVV	211833	322008	26.57%	3.465%

51	15.439	2099	2100	2108	rVV5	4897	7877	0.65%	0.085%
52	15.521	2110	2114	2127	rVB2	20174	36085	2.98%	0.388%
53	15.627	2127	2132	2135	rBV7	1757	3327	0.27%	0.036%
54	15.745	2147	2152	2153	rBV3	1908	2337	0.19%	0.025%
55	15.810	2160	2163	2168	rVB4	5013	5889	0.49%	0.063%

56	16.115	2210	2215	2216	rBV4	2069	2770	0.23%	0.030%
57	16.280	2241	2243	2248	rVB5	1499	2391	0.20%	0.026%
58	16.551	2287	2289	2295	rVB4	1224	2016	0.17%	0.022%
59	16.627	2298	2302	2303	rBV4	1687	2401	0.20%	0.026%
60	16.680	2305	2311	2312	rVV3	3335	5870	0.48%	0.063%

61	16.704	2312	2315	2321	rVV2	7604	13118	1.08%	0.141%
62	16.868	2340	2343	2346	rVV5	2332	3531	0.29%	0.038%
63	16.892	2346	2347	2350	rVV3	2641	2540	0.21%	0.027%
64	16.933	2350	2354	2356	rVV3	1633	2467	0.20%	0.027%
65	17.139	2382	2389	2394	rBV	498145	765704	63.19%	8.240%

66	17.180	2394	2396	2400	rVV	40737	48110	3.97%	0.518%
67	17.233	2400	2405	2418	rVV2	206263	346347	28.58%	3.727%
68	17.333	2418	2422	2426	rVB6	3855	4941	0.41%	0.053%
69	17.433	2437	2439	2443	rVB4	1358	1586	0.13%	0.017%
70	17.580	2460	2464	2465	rBV4	1560	1895	0.16%	0.020%

71	17.733	2485	2490	2492	rBV5	1632	1837	0.15%	0.020%
72	17.809	2498	2503	2507	rBV5	7439	11950	0.99%	0.129%
73	17.898	2516	2518	2523	rBV5	1537	2394	0.20%	0.026%
74	17.939	2523	2525	2528	rVV3	1966	2169	0.18%	0.023%
75	18.027	2533	2540	2543	rBV3	18808	36524	3.01%	0.393%

76	18.062	2543	2546	2552	rVB	13663	18874	1.56%	0.203%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030792.D
 Acq On : 03 Jul 2021 01:59
 Operator : CG/JU
 Sample : M2869-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	18.145	2556	2560	2563	rBV2	8039	11520	0.95%	0.124%
78	18.209	2565	2571	2575	rBV4	14943	27370	2.26%	0.295%
79	18.321	2589	2590	2594	rVB4	2101	1966	0.16%	0.021%
80	18.468	2610	2615	2617	rBV4	4713	7092	0.59%	0.076%
81	18.509	2619	2622	2627	rVB2	6534	10464	0.86%	0.113%
82	18.604	2636	2638	2640	rBV3	2553	2974	0.25%	0.032%
83	18.756	2661	2664	2666	rBV4	3713	3494	0.29%	0.038%
84	18.792	2668	2670	2672	rBV3	3095	3346	0.28%	0.036%
85	18.927	2689	2693	2696	rBV5	9617	14691	1.21%	0.158%
86	18.956	2696	2698	2700	rVV3	3875	3341	0.28%	0.036%
87	19.192	2733	2738	2744	rBV	163650	224091	18.49%	2.412%
88	19.345	2760	2764	2767	rVB	12603	16646	1.37%	0.179%
89	19.521	2789	2794	2798	rBV	310270	481952	39.77%	5.187%
90	19.551	2798	2799	2808	rVV	125428	126236	10.42%	1.359%
91	19.627	2809	2812	2815	rVV2	7635	10331	0.85%	0.111%
92	19.733	2827	2830	2835	rVB2	10766	15233	1.26%	0.164%
93	19.880	2851	2855	2863	rVB5	12828	30277	2.50%	0.326%
94	20.050	2880	2884	2890	rVB	34981	53014	4.37%	0.571%
95	20.145	2897	2900	2904	rBV	33657	41772	3.45%	0.450%
96	20.515	2959	2963	2968	rBV	142363	153747	12.69%	1.655%
97	21.303	3090	3097	3101	rBV2	857910	1211794	100.00%	13.041%
98	21.339	3101	3103	3112	rVB	112450	151166	12.47%	1.627%
99	23.409	3450	3455	3471	rVB3	209113	560644	46.27%	6.034%
100	23.550	3473	3479	3494	rVB2	588230	1131696	93.39%	12.179%




Sum of corrected areas: 9292101

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030792.D
Acq On : 03 Jul 2021 01:59
Operator : CG/JU
Sample : M2869-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

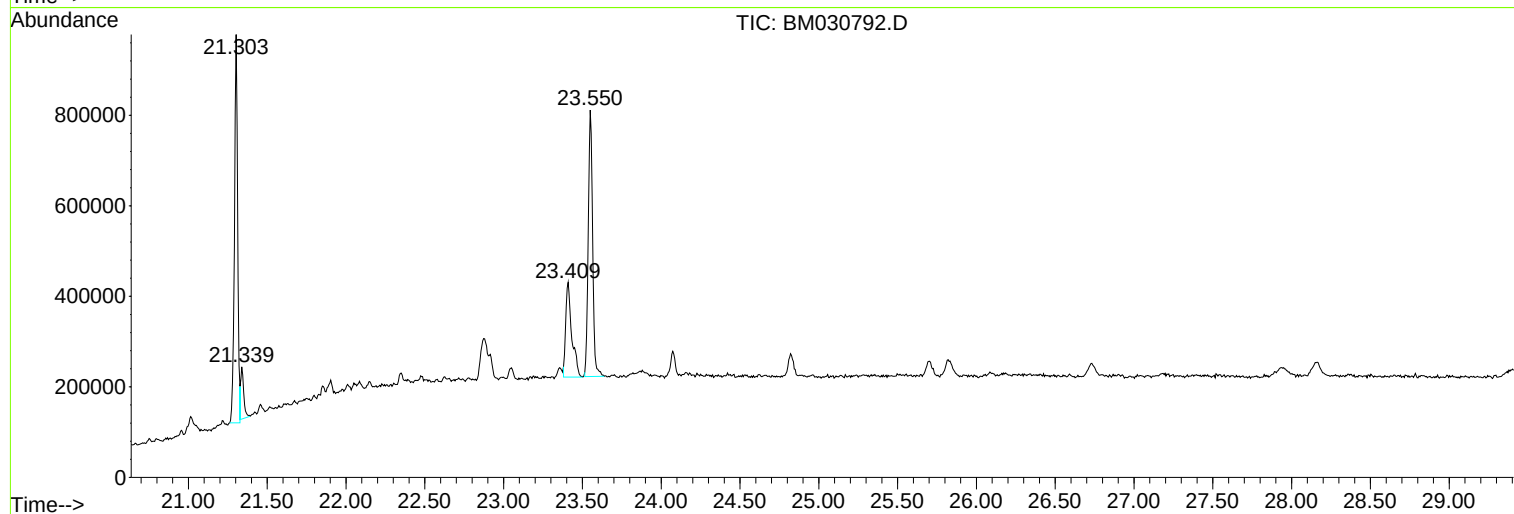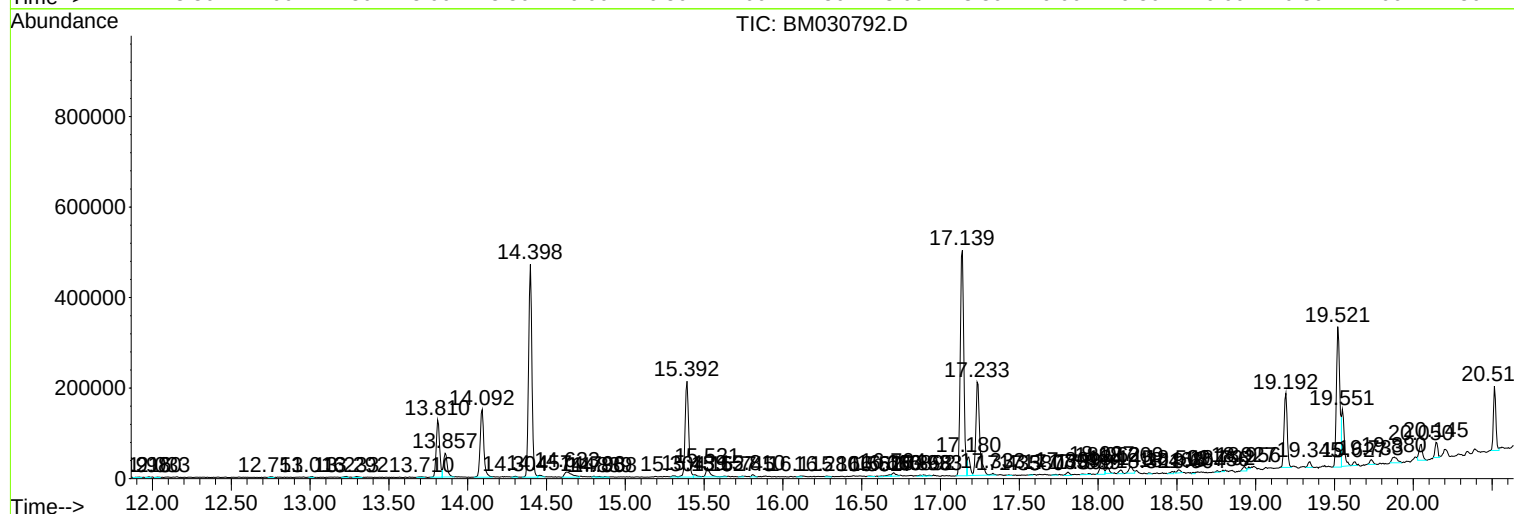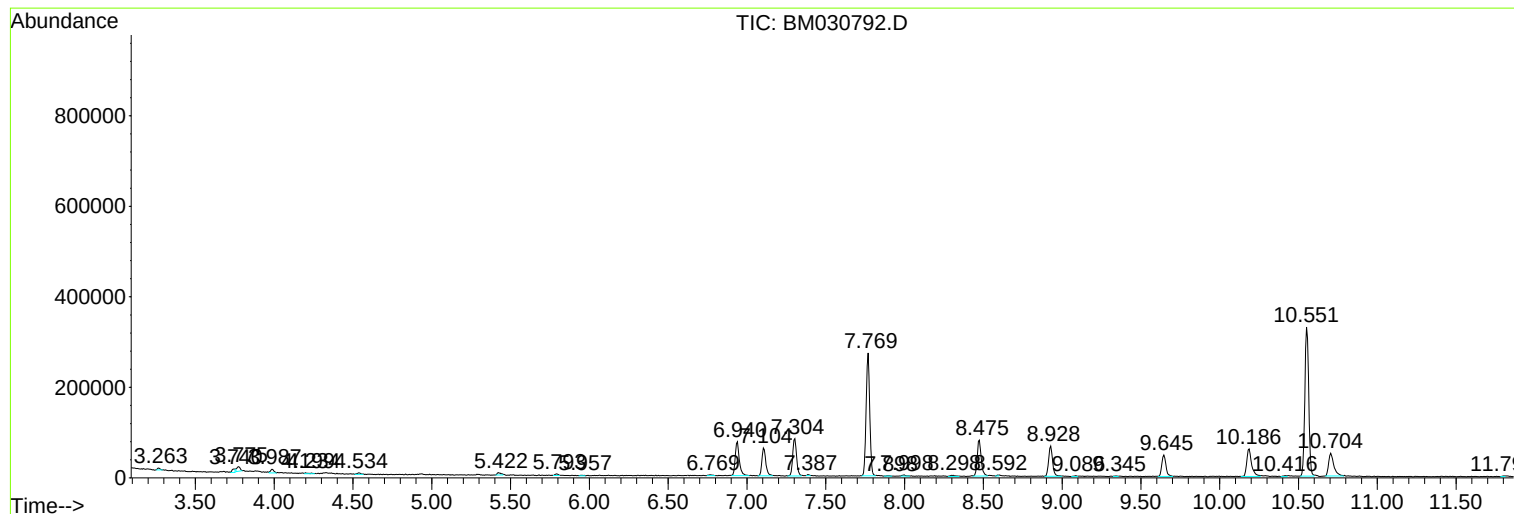

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030792.D
Acq On : 03 Jul 2021 01:59
Operator : CG/JU
Sample : M2869-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY0










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	2.54 ng/ul	153747	Chrysene-d12	21.303

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
3			Diisooctyl adipate	370	C22H42O4	001330-86-5	87
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
5			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	87

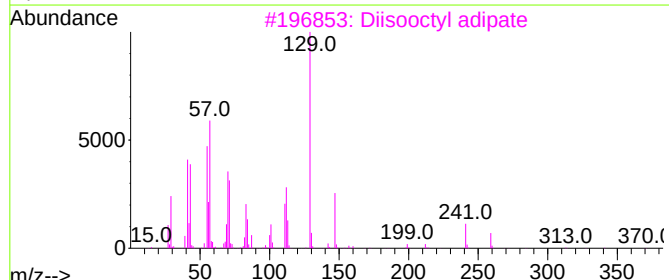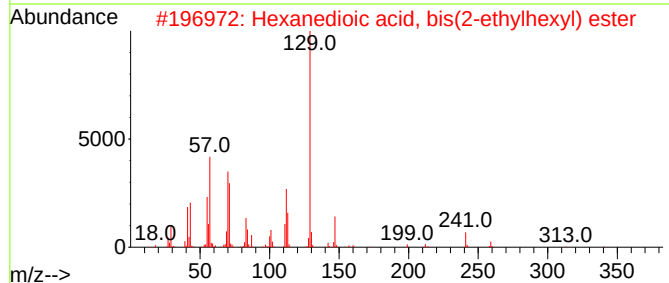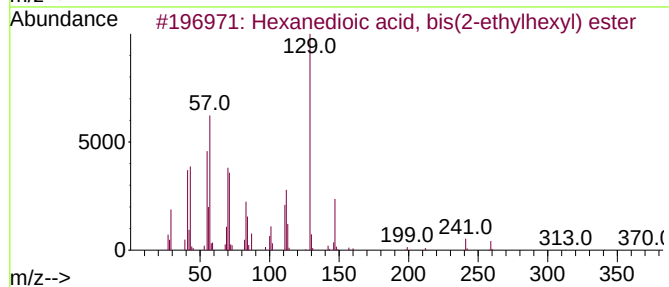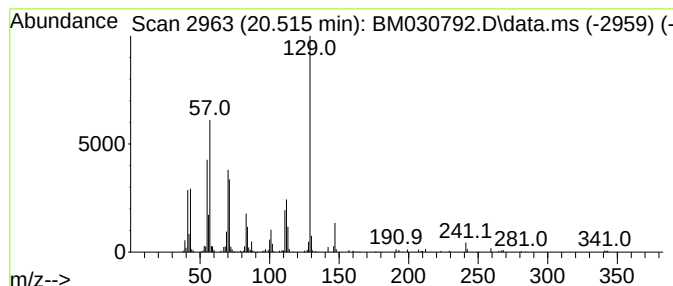

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030792.D
Acq On : 03 Jul 2021 01:59
Operator : CG/JU
Sample : M2869-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	2.5	ng/ul	153747	5	21.303	1211790	20.0