

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030794.D
 Acq On : 03 Jul 2021 03:11
 Operator : CG/JU
 Sample : M2869-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDx2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030794.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	36	rVB	9780	13361	1.27%	0.115%
2	3.704	102	105	116	rBV	28763	78686	7.50%	0.678%
3	3.987	150	153	157	rVB2	6951	10859	1.04%	0.094%
4	4.546	243	248	250	rBV	2994	4342	0.41%	0.037%
5	4.904	308	309	312	rBV3	1678	1448	0.14%	0.012%
6	5.263	366	370	371	rBV3	1227	1268	0.12%	0.011%
7	5.422	393	397	405	rBV3	4441	10436	1.00%	0.090%
8	5.787	456	459	464	rVV4	3162	4906	0.47%	0.042%
9	6.757	618	624	625	rBV5	1964	2962	0.28%	0.026%
10	6.769	625	626	628	rVV2	2382	1811	0.17%	0.016%
11	6.934	648	654	667	rVV	152597	260186	24.81%	2.242%
12	7.104	676	683	695	rBV	122768	203401	19.40%	1.753%
13	7.298	710	716	727	rVV	158969	265805	25.35%	2.291%
14	7.392	727	732	736	rVB5	2985	4890	0.47%	0.042%
15	7.769	788	796	803	rBV	287943	467956	44.63%	4.033%
16	7.834	803	807	815	rVV2	9912	17912	1.71%	0.154%
17	7.892	815	817	820	rVB4	1443	1664	0.16%	0.014%
18	7.992	830	834	841	rBV5	2982	5506	0.53%	0.047%
19	8.298	882	886	890	rBV5	1964	2629	0.25%	0.023%
20	8.469	906	915	928	rBV	169824	292552	27.90%	2.521%
21	8.598	933	937	942	rVB6	2558	3615	0.34%	0.031%
22	8.669	948	949	953	rVB4	1587	1890	0.18%	0.016%
23	8.875	980	984	986	rBV4	954	1414	0.13%	0.012%
24	8.922	986	992	1009	rVB	131800	231427	22.07%	1.994%
25	9.104	1020	1023	1027	rVB5	1478	2203	0.21%	0.019%
26	9.334	1059	1062	1069	rVB7	2090	3227	0.31%	0.028%
27	9.528	1092	1095	1100	rBV6	1075	1731	0.17%	0.015%
28	9.645	1107	1115	1131	rBV	95692	170627	16.27%	1.470%
29	10.181	1198	1206	1221	rBV	137963	274380	26.17%	2.365%
30	10.551	1262	1269	1281	rBV	373051	628883	59.97%	5.420%
31	10.698	1287	1294	1314	rBV	120539	267209	25.48%	2.303%
32	10.822	1314	1315	1318	rVV3	1549	1591	0.15%	0.014%
33	10.851	1318	1320	1323	rVB5	1589	1404	0.13%	0.012%
34	11.798	1477	1481	1482	rBV2	3573	3873	0.37%	0.033%
35	12.151	1537	1541	1546	rVB4	1912	3373	0.32%	0.029%
36	12.751	1638	1643	1647	rBV5	1750	2909	0.28%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030794.D
 Acq On : 03 Jul 2021 03:11
 Operator : CG/JU
 Sample : M2869-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDX2

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	12.798	1649	1651	1655	rVB3	1000	1363	0.13%	0.012%
38	12.922	1670	1672	1675	rBV3	930	1251	0.12%	0.011%
39	13.010	1683	1687	1691	rVB3	2514	2945	0.28%	0.025%
40	13.222	1721	1723	1726	rBV3	1645	1924	0.18%	0.017%
41	13.292	1728	1735	1742	rBV4	2862	5541	0.53%	0.048%
42	13.810	1817	1823	1827	rVV	254770	366878	34.99%	3.162%
43	13.857	1827	1831	1839	rVB	95805	148720	14.18%	1.282%
44	14.092	1860	1871	1884	rBV	281305	448514	42.77%	3.865%
45	14.298	1902	1906	1912	rVB7	2214	3257	0.31%	0.028%
46	14.398	1916	1923	1930	rVV	514908	746912	71.23%	6.437%
47	14.457	1930	1933	1940	rVB	17309	27000	2.57%	0.233%
48	14.621	1955	1961	1975	rBV2	29807	90621	8.64%	0.781%
49	14.739	1980	1981	1986	rVV5	2960	4183	0.40%	0.036%
50	14.798	1989	1991	1994	rVV4	2501	3072	0.29%	0.026%
51	14.833	1994	1997	2001	rVV5	2084	3353	0.32%	0.029%
52	14.886	2004	2006	2009	rVB4	1632	1402	0.13%	0.012%
53	15.068	2035	2037	2040	rBV3	1172	1250	0.12%	0.011%
54	15.192	2054	2058	2060	rBV3	2078	2529	0.24%	0.022%
55	15.210	2060	2061	2066	rVB4	1369	1842	0.18%	0.016%
56	15.251	2066	2068	2073	rVB5	1579	1747	0.17%	0.015%
57	15.304	2073	2077	2079	rBV4	2041	2589	0.25%	0.022%
58	15.392	2084	2092	2100	rBV	368691	563970	53.78%	4.860%
59	15.521	2109	2114	2121	rBV2	37357	65042	6.20%	0.561%
60	15.633	2129	2133	2134	rBV3	2054	2294	0.22%	0.020%
61	15.745	2147	2152	2158	rBV4	4121	7024	0.67%	0.061%
62	15.810	2160	2163	2169	rVB3	4966	7105	0.68%	0.061%
63	15.874	2173	2174	2177	rBV3	932	1275	0.12%	0.011%
64	15.910	2177	2180	2186	rVB5	2616	3997	0.38%	0.034%
65	16.110	2208	2214	2216	rBV4	1881	3385	0.32%	0.029%
66	16.168	2222	2224	2227	rBV3	975	1412	0.13%	0.012%
67	16.286	2242	2244	2248	rVB5	1611	1710	0.16%	0.015%
68	16.374	2256	2259	2263	rVB4	2589	2566	0.24%	0.022%
69	16.445	2265	2271	2275	rBV4	2838	5387	0.51%	0.046%
70	16.557	2287	2290	2295	rBV6	1273	1927	0.18%	0.017%
71	16.674	2306	2310	2312	rBV4	2216	3194	0.30%	0.028%
72	16.710	2312	2316	2320	rVB4	3498	6400	0.61%	0.055%
73	16.874	2339	2344	2346	rBV5	2115	3110	0.30%	0.027%
74	16.898	2346	2348	2351	rVV3	2412	2965	0.28%	0.026%
75	16.927	2351	2353	2355	rVV3	2349	2621	0.25%	0.023%
76	16.951	2355	2357	2362	rVB2	2194	3074	0.29%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030794.D
 Acq On : 03 Jul 2021 03:11
 Operator : CG/JU
 Sample : M2869-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	17.133	2382	2388	2393	rBV	526925	797921	76.09%	6.877%
78	17.180	2393	2396	2400	rVV	64509	91404	8.72%	0.788%
79	17.233	2400	2405	2418	rVB	370620	568697	54.23%	4.901%
80	17.398	2431	2433	2435	rBV3	2106	2121	0.20%	0.018%
81	17.609	2465	2469	2471	rBV3	1434	2166	0.21%	0.019%
82	17.633	2471	2473	2474	rBV2	2653	1614	0.15%	0.014%
83	17.809	2500	2503	2508	rVB6	3137	3814	0.36%	0.033%
84	17.898	2516	2518	2520	rBV3	1794	1943	0.19%	0.017%
85	17.951	2523	2527	2529	rVB5	1876	2408	0.23%	0.021%
86	18.027	2534	2540	2545	rBV4	33699	63367	6.04%	0.546%
87	18.098	2550	2552	2557	rVB2	3543	4005	0.38%	0.035%
88	18.209	2566	2571	2575	rBV3	11279	17490	1.67%	0.151%
89	18.368	2596	2598	2601	rVB4	1925	1797	0.17%	0.015%
90	18.468	2611	2615	2621	rBV	12670	21801	2.08%	0.188%
91	18.792	2665	2670	2674	rBV5	5194	8615	0.82%	0.074%
92	19.156	2730	2732	2733	rBV2	3768	3060	0.29%	0.026%
93	19.192	2733	2738	2746	rVB	49084	69138	6.59%	0.596%
94	19.309	2754	2758	2762	rBV6	9073	13719	1.31%	0.118%
95	19.521	2789	2794	2809	rBV	449008	690370	65.84%	5.950%
96	20.515	2959	2963	2968	rBV	644355	673794	64.25%	5.807%
97	21.015	3045	3048	3051	rBV4	25907	30098	2.87%	0.259%
98	21.303	3092	3097	3109	rBV	720915	971635	92.66%	8.374%
99	23.409	3449	3455	3469	rVB	339912	706044	67.33%	6.085%
100	23.550	3473	3479	3493	rVB2	523134	1048630	100.00%	9.037%




Sum of corrected areas: 11603338

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030794.D
Acq On : 03 Jul 2021 03:11
Operator : CG/JU
Sample : M2869-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDX2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

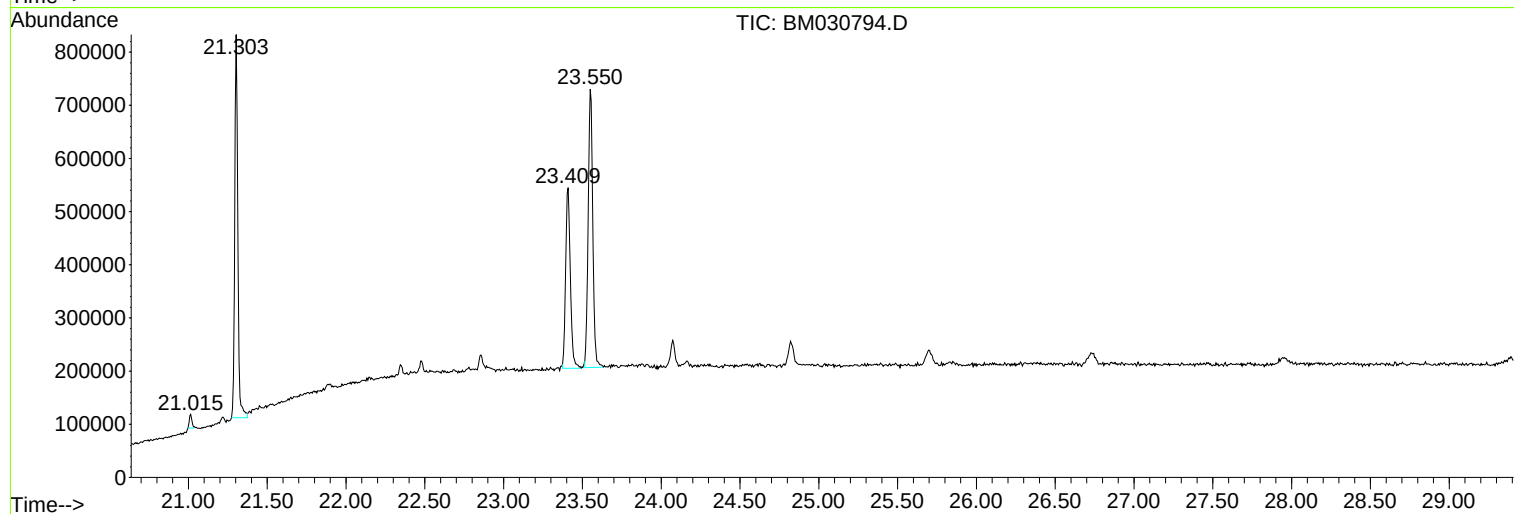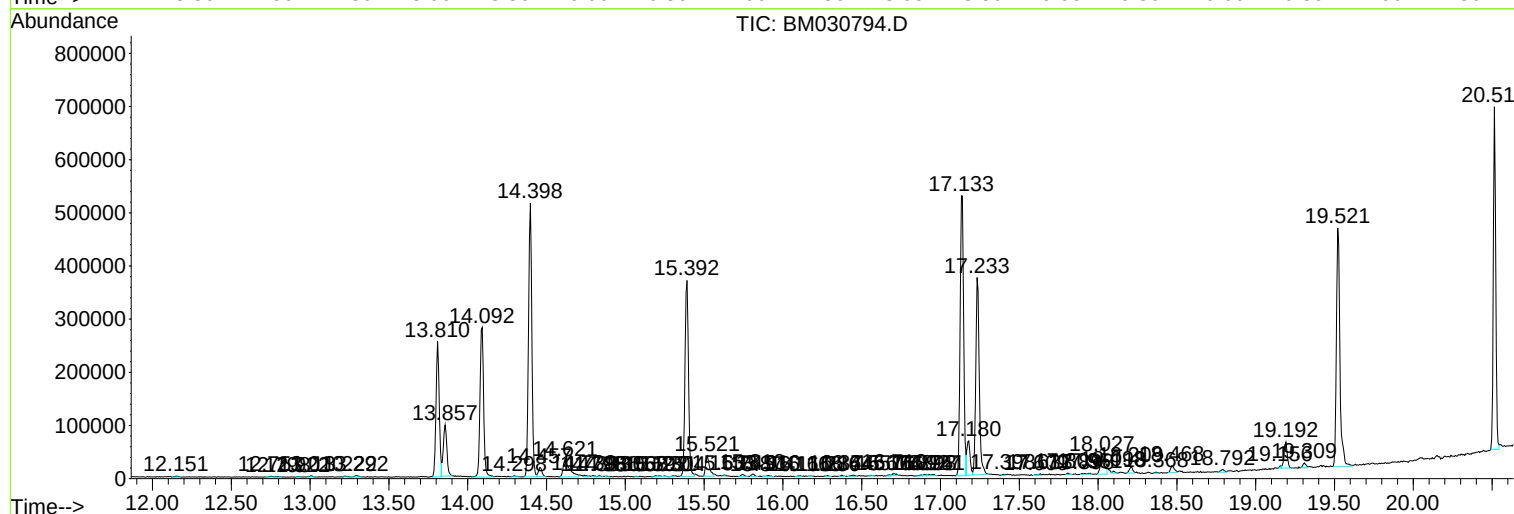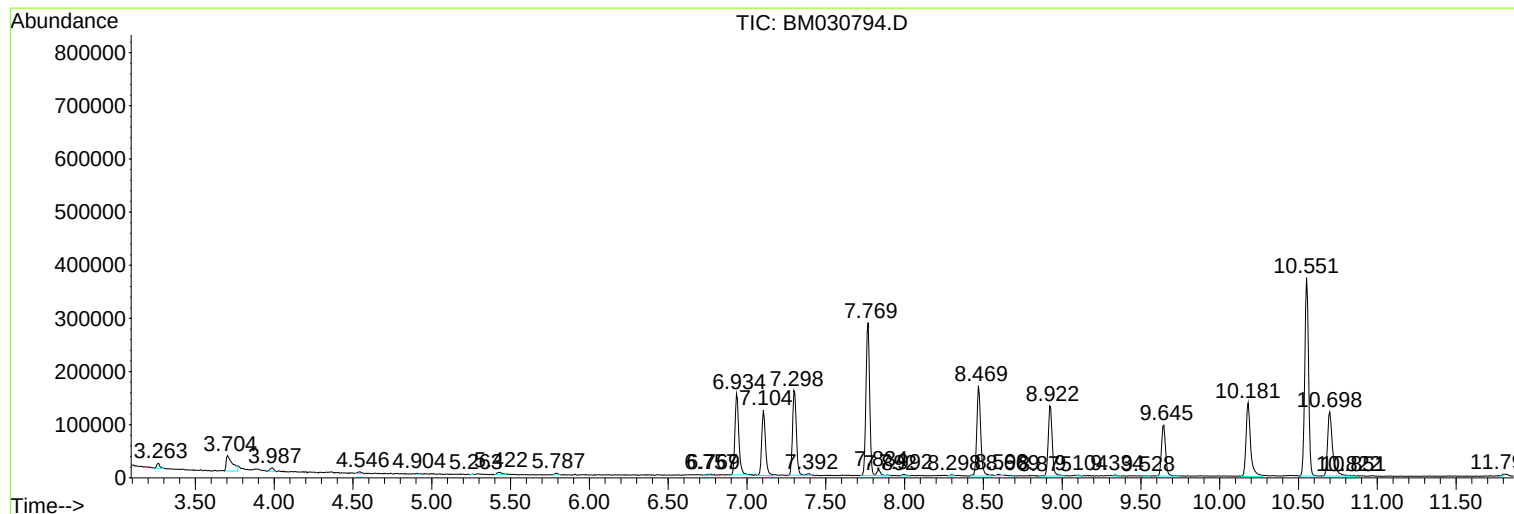

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030794.D
Acq On : 03 Jul 2021 03:11
Operator : CG/JU
Sample : M2869-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDX2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.520	13.87 ng/ul	673794	Chrysene-d12	21.303

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	90
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	81
5			Diisooctyl adipate	370	C22H42O4	001330-86-5	78

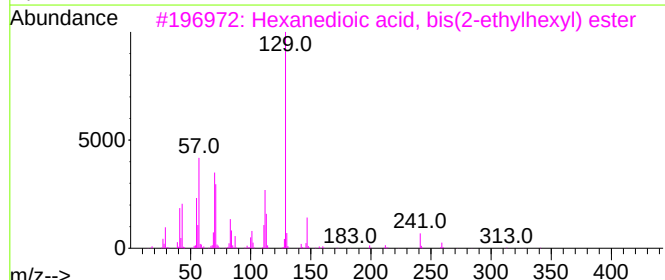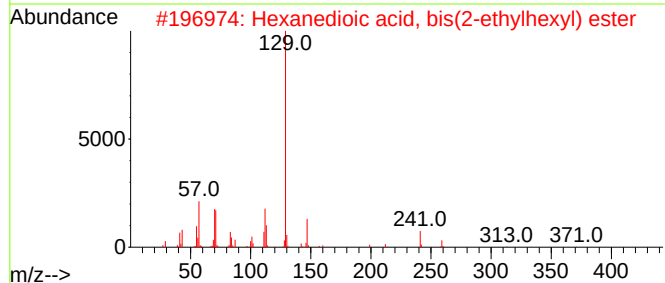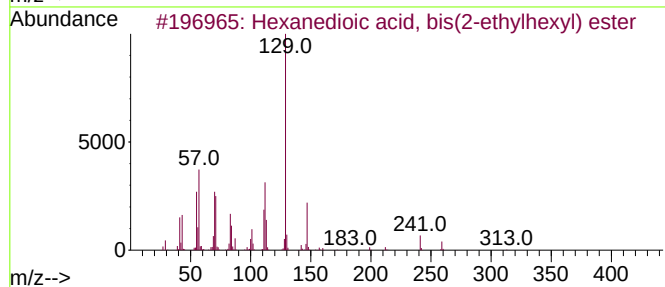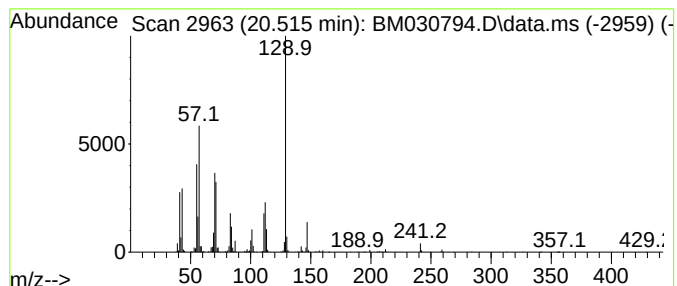

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030794.D
Acq On : 03 Jul 2021 03:11
Operator : CG/JU
Sample : M2869-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDX2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.520	13.9	ng/ul	673794	5	21.303	971635	20.0