

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030796.D
 Acq On : 03 Jul 2021 05:00
 Operator : CG/JU
 Sample : PB137473BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK473

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030796.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	38	rVB	36378	47653	1.85%	0.186%
2	3.669	96	99	119	rBV	366630	671868	26.05%	2.628%
3	3.987	150	153	157	rVB	6400	7220	0.28%	0.028%
4	6.934	647	654	667	rBV	529265	854058	33.11%	3.341%
5	7.105	677	683	700	rVB	394854	635985	24.66%	2.488%
6	7.299	709	716	734	rBV	549132	880058	34.12%	3.443%
7	7.769	787	796	805	rBV	355483	576398	22.35%	2.255%
8	8.469	908	915	928	rBV	601955	977748	37.91%	3.825%
9	8.922	984	992	1006	rBV	477602	783539	30.38%	3.065%
10	9.640	1108	1114	1127	rBV	375844	628422	24.37%	2.458%
11	10.175	1198	1205	1223	rBV	542186	967745	37.52%	3.786%
12	10.551	1261	1269	1278	rBV	462875	775097	30.05%	3.032%
13	10.693	1285	1293	1315	rBV	490062	965298	37.43%	3.776%
14	12.157	1536	1542	1551	rVB2	6230	12588	0.49%	0.049%
15	13.810	1816	1823	1839	rBV	830639	1211853	46.99%	4.741%
16	14.086	1863	1870	1884	rBV	1027134	1567115	60.76%	6.131%
17	14.398	1916	1923	1935	rBV	628934	937628	36.35%	3.668%
18	14.598	1951	1957	1978	rBV	221685	528396	20.49%	2.067%
19	15.386	2084	2091	2104	rBV	1245266	1866720	72.38%	7.303%
20	15.516	2108	2113	2125	rVV	263816	404437	15.68%	1.582%
21	15.628	2128	2132	2137	rVB	13809	20925	0.81%	0.082%
22	16.169	2220	2224	2233	rBV6	3785	5302	0.21%	0.021%
23	16.927	2349	2353	2356	rBV5	3032	4456	0.17%	0.017%
24	17.133	2382	2388	2398	rBV	688787	1001007	38.81%	3.916%
25	17.233	2398	2405	2418	rBV2	1315252	1933762	74.98%	7.565%
26	19.098	2718	2722	2723	rBV4	2111	2684	0.10%	0.010%
27	19.163	2729	2733	2738	rBV	11945	15928	0.62%	0.062%
28	19.410	2772	2775	2780	rVB3	8995	12470	0.48%	0.049%
29	19.521	2788	2794	2804	rBV	1622669	2233887	86.61%	8.739%
30	21.304	3092	3097	3104	rBV	886332	1151388	44.64%	4.504%
31	23.409	3448	3455	3467	rVB	1364034	2579170	100.00%	10.090%
32	23.551	3473	3479	3491	rVB2	676942	1301547	50.46%	5.092%




Sum of corrected areas: 25562352

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030796.D
Acq On : 03 Jul 2021 05:00
Operator : CG/JU
Sample : PB137473BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK473

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

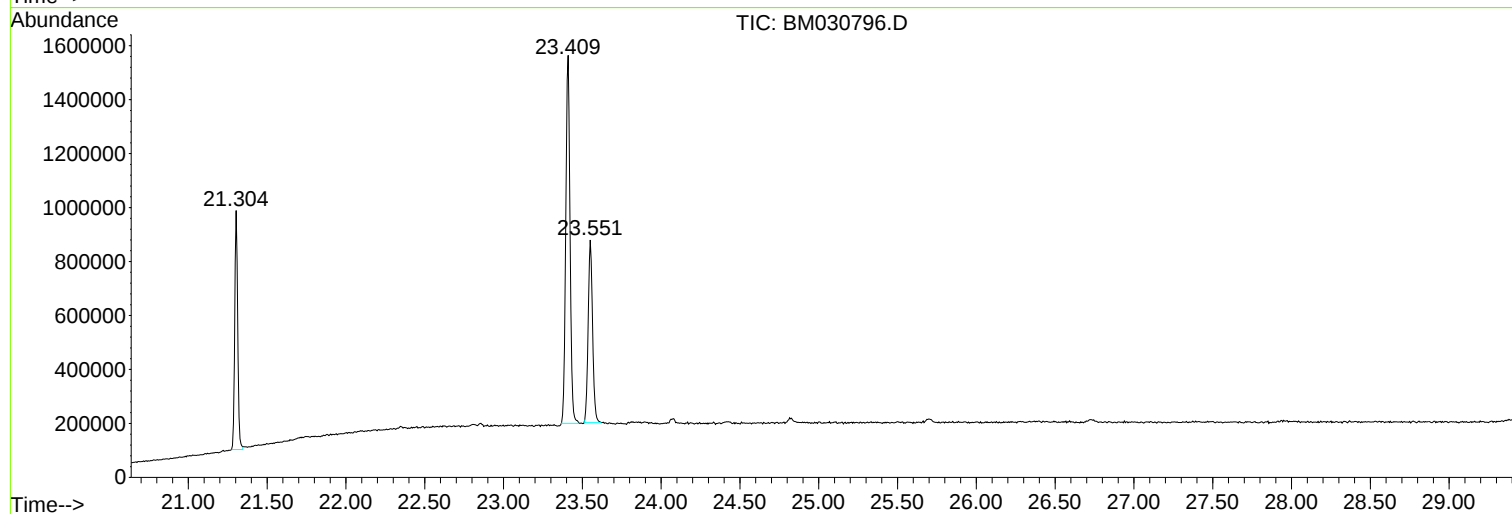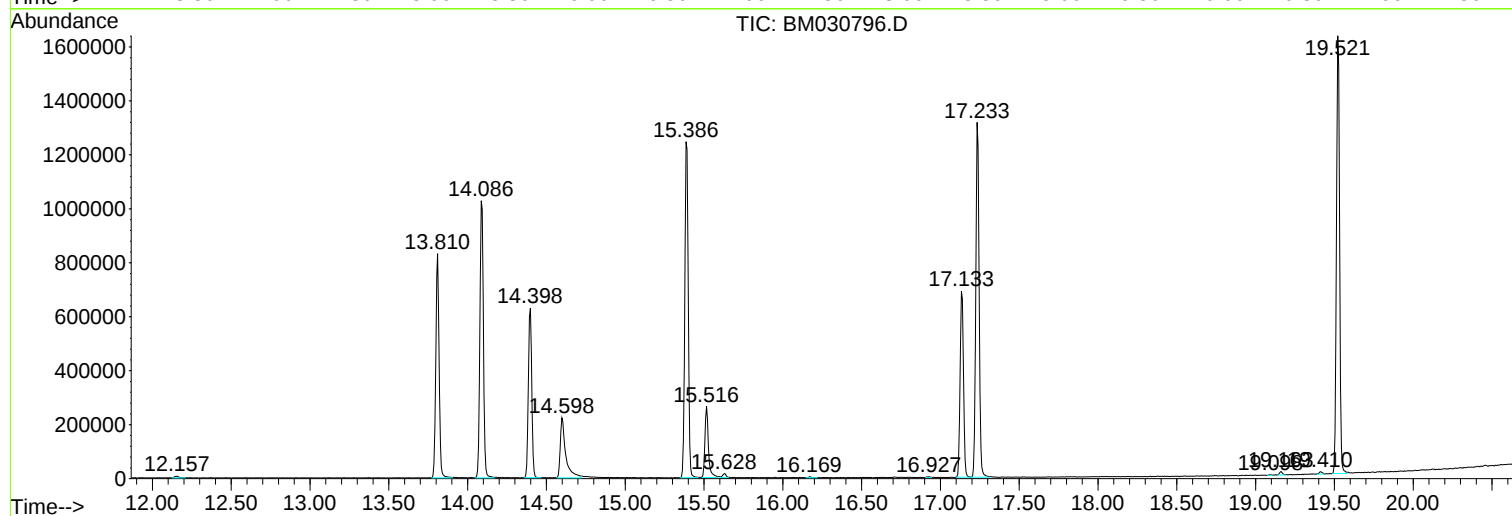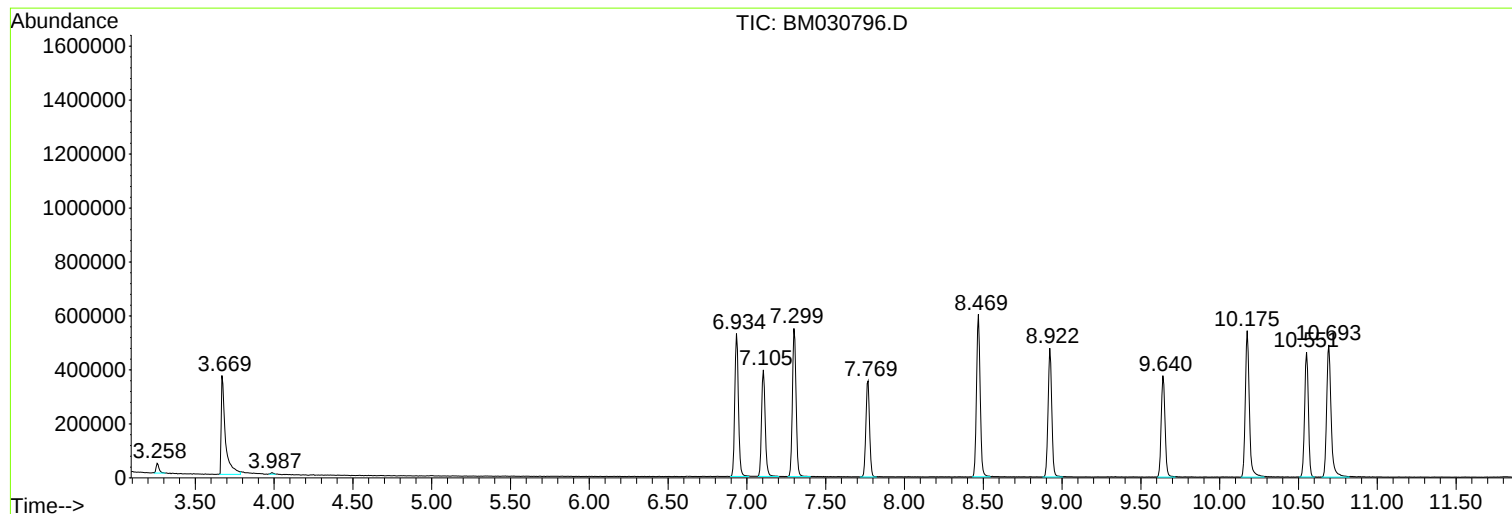

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030796.D
Acq On : 03 Jul 2021 05:00
Operator : CG/JU
Sample : PB137473BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK473

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030796.D
Acq On : 03 Jul 2021 05:00
Operator : CG/JU
Sample : PB137473BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK473

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
