

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030803.D
 Acq On : 03 Jul 2021 09:12
 Operator : CG/JU
 Sample : M2869-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030803.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	38	rVB3	7982	12130	0.93%	0.108%
2	3.693	101	103	106	rBV3	2032	1352	0.10%	0.012%
3	3.746	110	112	114	rBV3	5330	5975	0.46%	0.053%
4	3.987	149	153	159	rVB	7535	11290	0.86%	0.100%
5	4.128	173	177	180	rBV4	1449	2219	0.17%	0.020%
6	4.251	196	198	203	rVB6	1407	1605	0.12%	0.014%
7	4.351	213	215	219	rBV5	1840	2736	0.21%	0.024%
8	4.534	243	246	250	rBV2	2482	3405	0.26%	0.030%
9	5.293	373	375	380	rVB2	1837	1806	0.14%	0.016%
10	5.428	393	398	405	rVB	6177	11802	0.90%	0.105%
11	5.569	418	422	426	rBV4	1045	1668	0.13%	0.015%
12	5.787	455	459	465	rBV5	4454	8193	0.63%	0.073%
13	5.851	466	470	474	rVB6	1155	1872	0.14%	0.017%
14	6.022	495	499	504	rVB5	1097	1830	0.14%	0.016%
15	6.075	504	508	512	rVB4	1199	1844	0.14%	0.016%
16	6.651	604	606	610	rVB4	1628	2018	0.15%	0.018%
17	6.763	621	625	629	rVB5	2854	3865	0.30%	0.034%
18	6.810	629	633	635	rBV3	1206	1802	0.14%	0.016%
19	6.934	647	654	668	rBV	132177	226761	17.31%	2.013%
20	7.104	677	683	694	rVV	102177	167610	12.79%	1.488%
21	7.298	709	716	728	rBV	140976	235053	17.94%	2.087%
22	7.387	728	731	738	rVB3	3963	5683	0.43%	0.050%
23	7.769	788	796	804	rBV	340464	554419	42.32%	4.922%
24	7.834	804	807	812	rVB5	2166	3506	0.27%	0.031%
25	7.892	812	817	821	rBV5	1227	2265	0.17%	0.020%
26	7.992	828	834	840	rVB4	2775	5675	0.43%	0.050%
27	8.251	874	878	881	rBV4	981	1576	0.12%	0.014%
28	8.304	881	887	890	rBV3	1772	2775	0.21%	0.025%
29	8.469	905	915	925	rBV	150898	262484	20.04%	2.330%
30	8.592	932	936	941	rVV4	2586	4596	0.35%	0.041%
31	8.634	941	943	946	rVB2	1570	1651	0.13%	0.015%
32	8.922	985	992	1001	rBV	119774	204305	15.60%	1.814%
33	9.092	1018	1021	1026	rVB4	1743	2397	0.18%	0.021%
34	9.316	1056	1059	1060	rBV3	1243	1327	0.10%	0.012%
35	9.639	1107	1114	1122	rBV	90230	159801	12.20%	1.419%
36	10.181	1198	1206	1221	rBV	118674	244615	18.67%	2.171%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030803.D
 Acq On : 03 Jul 2021 09:12
 Operator : CG/JU
 Sample : M2869-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	10.275	1221	1222	1227	rVB5	1406	1572	0.12%	0.014%
38	10.386	1235	1241	1250	rBV5	5931	18389	1.40%	0.163%
39	10.551	1262	1269	1278	rVB	447456	756593	57.75%	6.716%
40	10.698	1287	1294	1309	rBV	97335	215892	16.48%	1.916%
41	11.039	1347	1352	1353	rBV3	1394	1818	0.14%	0.016%
42	11.816	1478	1484	1490	rVB5	2070	4303	0.33%	0.038%
43	11.986	1509	1513	1516	rVB5	1276	1837	0.14%	0.016%
44	12.145	1537	1540	1547	rVB5	1953	3295	0.25%	0.029%
45	12.751	1640	1643	1647	rVB4	2206	2461	0.19%	0.022%
46	12.792	1647	1650	1655	rBV5	1587	2434	0.19%	0.022%
47	13.004	1683	1686	1693	rVB4	2817	4191	0.32%	0.037%
48	13.227	1718	1724	1727	rBV5	1852	3686	0.28%	0.033%
49	13.363	1742	1747	1750	rVV5	2357	4428	0.34%	0.039%
50	13.498	1768	1770	1774	rBV3	991	1311	0.10%	0.012%
51	13.810	1816	1823	1834	rBV	229417	350029	26.72%	3.107%
52	14.086	1859	1870	1882	rBV	277552	427575	32.64%	3.796%
53	14.186	1885	1887	1890	rVB3	1652	1542	0.12%	0.014%
54	14.298	1901	1906	1909	rVB5	2248	3498	0.27%	0.031%
55	14.398	1916	1923	1934	rBV	611900	946004	72.21%	8.398%
56	14.568	1947	1952	1954	rVB4	1673	2474	0.19%	0.022%
57	14.621	1954	1961	1974	rBV3	25950	79577	6.07%	0.706%
58	14.833	1994	1997	2005	rVB7	2749	4979	0.38%	0.044%
59	14.980	2021	2022	2029	rVB4	1471	2050	0.16%	0.018%
60	15.045	2029	2033	2037	rBV4	1121	2077	0.16%	0.018%
61	15.121	2043	2046	2048	rBV3	1747	1651	0.13%	0.015%
62	15.198	2054	2059	2061	rBV3	1633	2718	0.21%	0.024%
63	15.221	2061	2063	2065	rVV2	1656	1797	0.14%	0.016%
64	15.251	2065	2068	2072	rVB4	1893	2455	0.19%	0.022%
65	15.392	2084	2092	2105	rBV	351304	544124	41.54%	4.830%
66	15.521	2109	2114	2129	rVV2	31269	59803	4.57%	0.531%
67	15.627	2129	2132	2136	rVB3	4043	4788	0.37%	0.043%
68	15.810	2159	2163	2167	rBV2	6794	9025	0.69%	0.080%
69	16.110	2210	2214	2216	rBV5	1637	2632	0.20%	0.023%
70	16.174	2221	2225	2229	rBV3	3384	5028	0.38%	0.045%
71	16.210	2229	2231	2235	rVB3	1707	1559	0.12%	0.014%
72	16.280	2238	2243	2244	rBV4	1956	2976	0.23%	0.026%
73	16.368	2255	2258	2263	rBV5	1678	2287	0.17%	0.020%
74	16.486	2275	2278	2281	rVB5	1060	1537	0.12%	0.014%
75	16.533	2281	2286	2289	rBV3	2424	4070	0.31%	0.036%
76	16.874	2338	2344	2346	rBV5	3926	4816	0.37%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030803.D
 Acq On : 03 Jul 2021 09:12
 Operator : CG/JU
 Sample : M2869-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDY6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

77	17.051	2373	2374	2378	rVB4	1539	1432	0.11%	0.013%
78	17.133	2382	2388	2399	rVV	641024	1011212	77.19%	8.977%
79	17.233	2399	2405	2416	rVB	370607	559798	42.73%	4.969%
80	17.427	2436	2438	2441	rVB3	1269	1524	0.12%	0.014%
81	17.574	2461	2463	2466	rVB4	1519	1337	0.10%	0.012%
82	17.639	2470	2474	2475	rVV4	1829	2016	0.15%	0.018%
83	17.809	2498	2503	2507	rBV3	7853	11062	0.84%	0.098%
84	17.921	2519	2522	2523	rBV3	1801	1382	0.11%	0.012%
85	18.027	2536	2540	2549	rBV10	9986	17703	1.35%	0.157%
86	18.098	2550	2552	2556	rVB3	3479	3616	0.28%	0.032%
87	18.321	2587	2590	2591	rBV3	2821	3053	0.23%	0.027%
88	18.704	2654	2655	2657	rBV2	1816	1703	0.13%	0.015%
89	18.821	2673	2675	2678	rBV4	2144	1970	0.15%	0.017%
90	18.956	2695	2698	2701	rBV5	8777	11523	0.88%	0.102%
91	18.992	2702	2704	2709	rVB5	6661	6662	0.51%	0.059%
92	19.086	2719	2720	2721	rBV	3710	2268	0.17%	0.020%
93	19.233	2742	2745	2749	rVB5	9713	11982	0.91%	0.106%
94	19.521	2789	2794	2802	rBV2	447528	635006	48.47%	5.637%
95	20.515	2960	2963	2968	rVB2	26965	28624	2.19%	0.254%
96	21.015	3044	3048	3051	rBV	58934	79011	6.03%	0.701%
97	21.303	3092	3097	3105	rBV	907971	1179913	90.07%	10.474%
98	23.409	3449	3455	3465	rVB	345042	724956	55.34%	6.435%
99	23.550	3473	3479	3492	rVB	667286	1310014	100.00%	11.629%



Sum of corrected areas: 11264959

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030803.D
Acq On : 03 Jul 2021 09:12
Operator : CG/JU
Sample : M2869-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

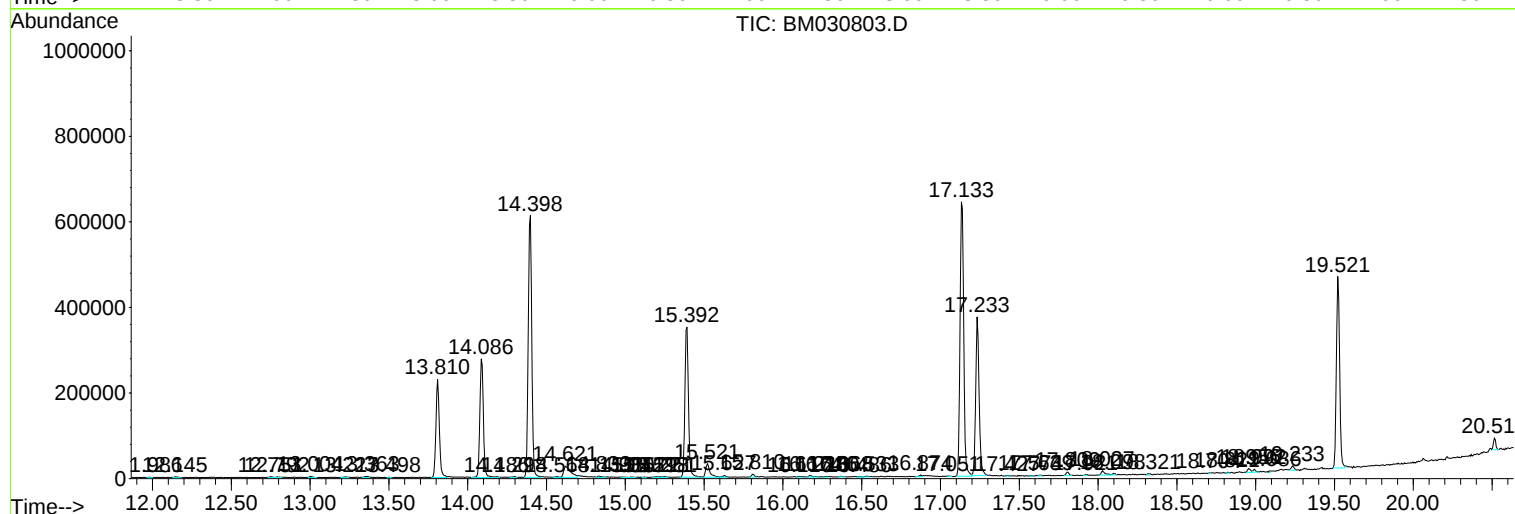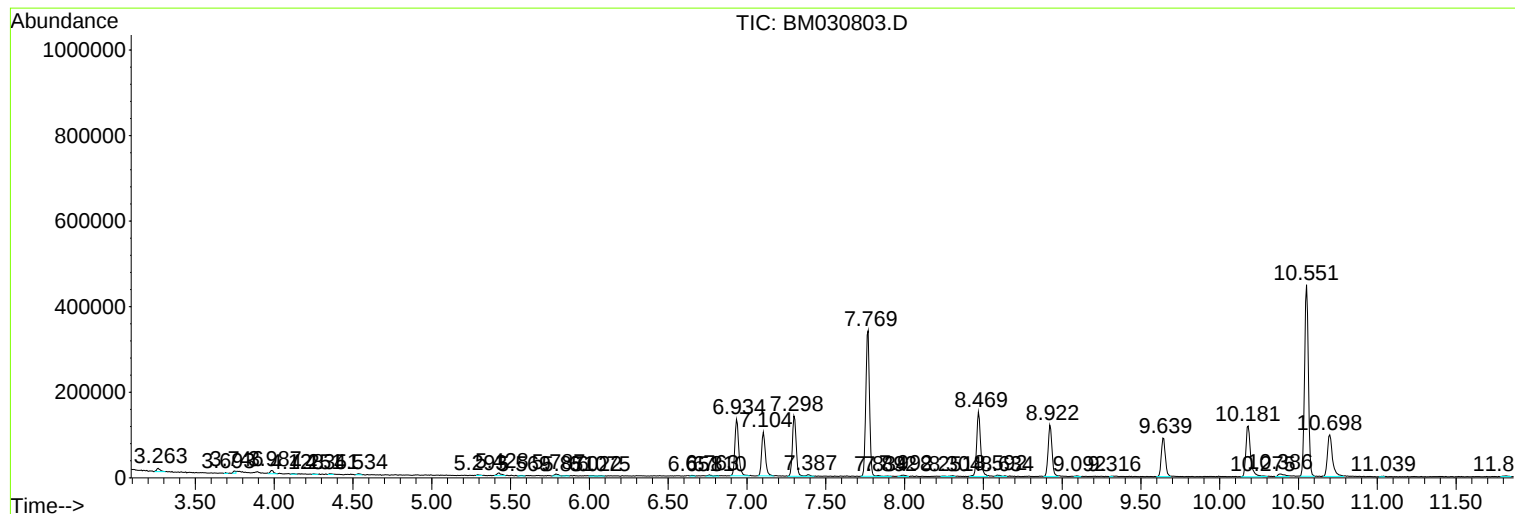

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030803.D
Acq On : 03 Jul 2021 09:12
Operator : CG/JU
Sample : M2869-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030803.D
Acq On : 03 Jul 2021 09:12
Operator : CG/JU
Sample : M2869-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDY6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
